

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012121\
 Data File : P0075027.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jan 2021 10:01
 Operator : AJ/MA
 Sample : M1086-11DL 5X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DUP-10DL

Manual Integrations
 APPROVED

Ankita
 1/22/2021 12:11:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 14:27:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.927	4.000	458195	238715	4.342	4.244
2) SA Decachlor...	10.944	9.250	282894	241593	2.787	4.400m#
Target Compounds						
26) L6 AR-1254-1	7.163	6.109	1193180	815230	271.292	225.700
27) L6 AR-1254-2	7.392	6.268	2304143	1094168	338.309	351.085
28) L6 AR-1254-3	7.776	6.684	3293542	2143949	469.545	437.191
29) L6 AR-1254-4	8.074	6.923	3205151	1587201	528.495	457.700
30) L6 AR-1254-5	8.503	7.348	5443740	4377569	937.132	967.217

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012121\
Data File : PO075027.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jan 2021 10:01
Operator : AJ/MA
Sample : M1086-11DL 5X
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
DUP-10DL


Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 14:27:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

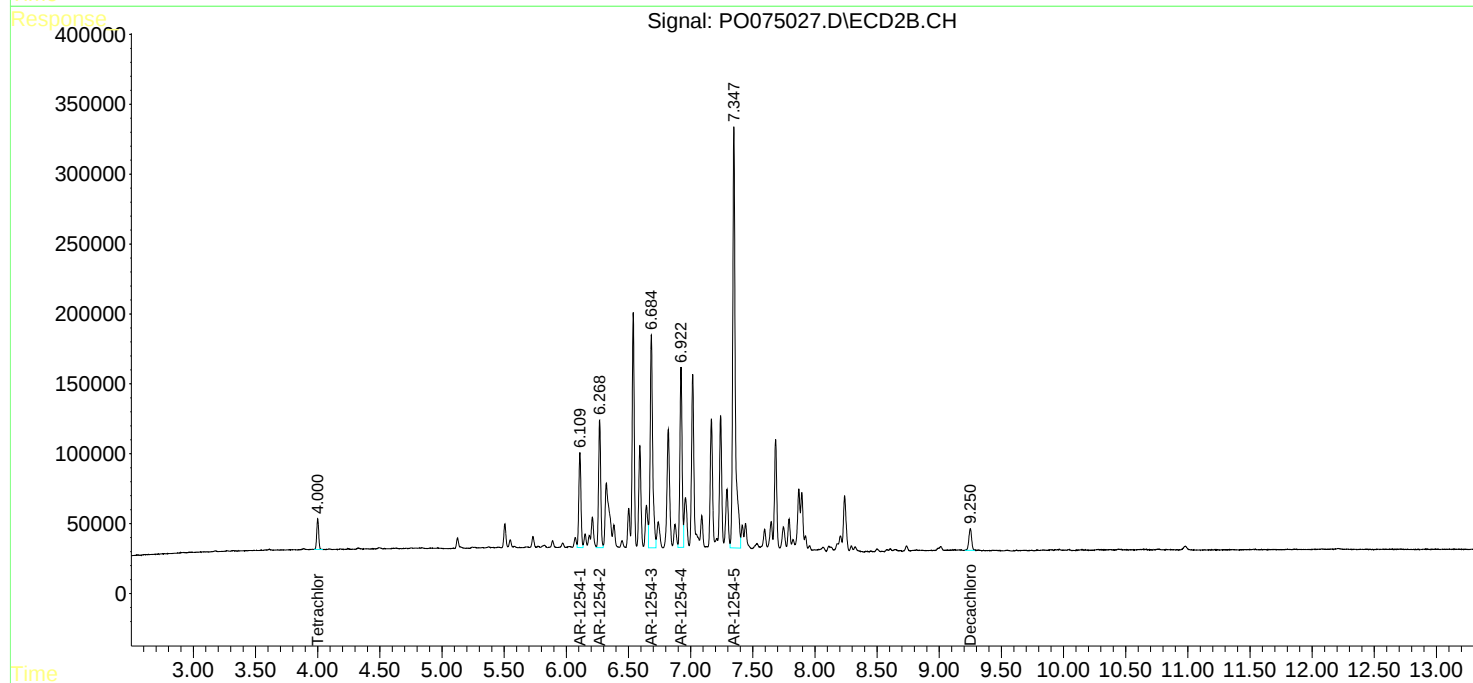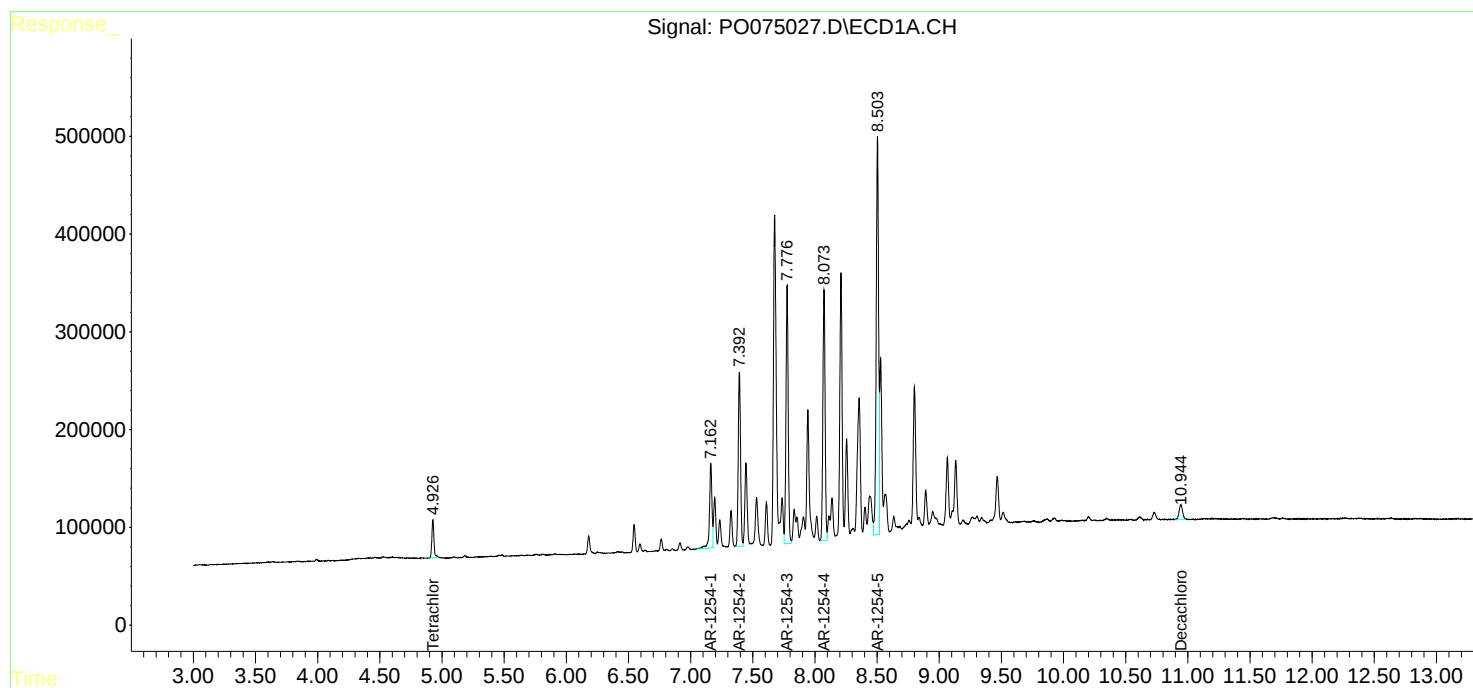

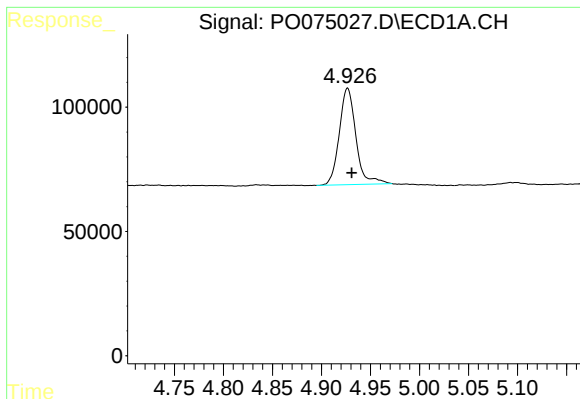


#1 Tetrachloro-m-xylene

R.T.: 4.927 min
Delta R.T.: -0.004 min
Response: 458195
Conc: 4.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-10DL


Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:36 PM

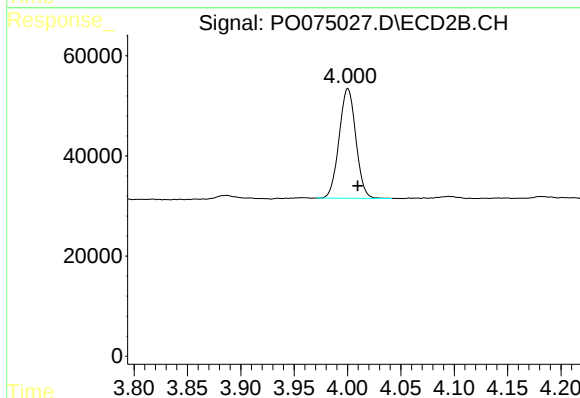


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.009 min
Response: 238715
Conc: 4.24 ng/ml

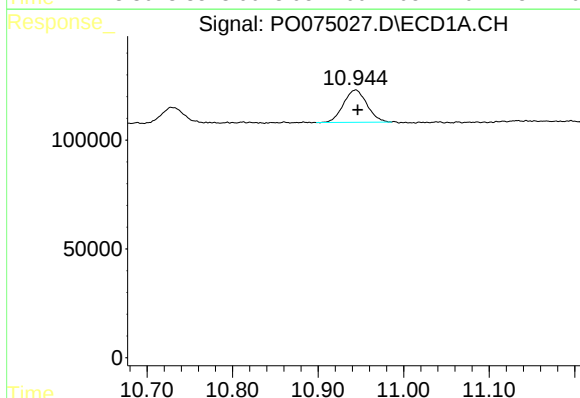


#2 Decachlorobiphenyl

R.T.: 10.944 min
Delta R.T.: -0.002 min
Response: 282894
Conc: 2.79 ng/ml

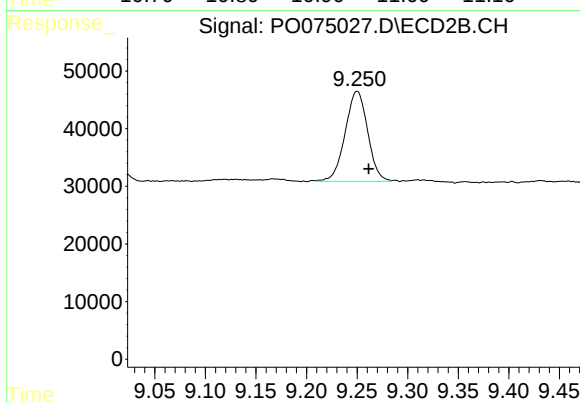

#2 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.012 min
Response: 241593
Conc: 4.40 ng/ml m

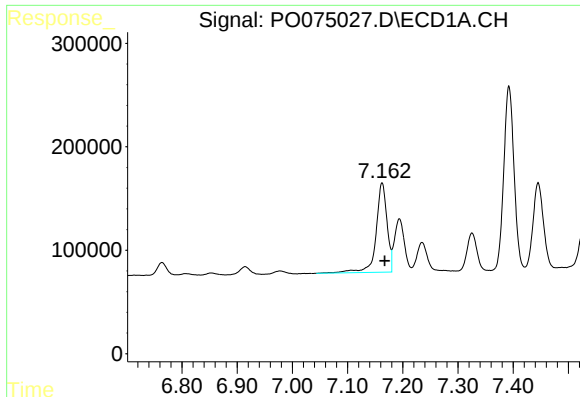


#26 AR-1254-1

R.T.: 7.163 min
Delta R.T.: -0.005 min
Response: 1193180
Conc: 271.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-10DL


Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:36 PM

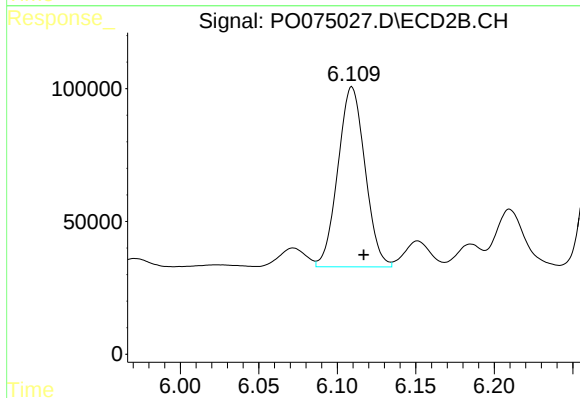


#26 AR-1254-1

R.T.: 6.109 min
Delta R.T.: -0.008 min
Response: 815230
Conc: 225.70 ng/ml

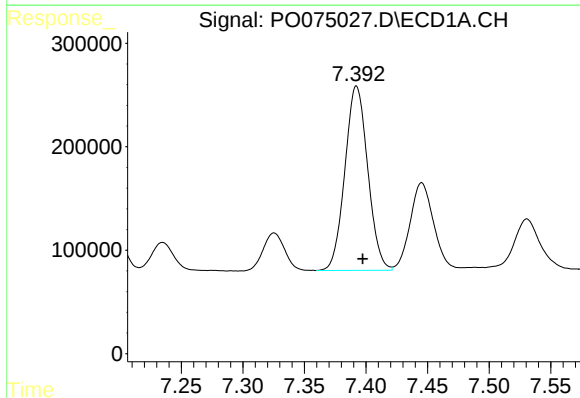


#27 AR-1254-2

R.T.: 7.392 min
Delta R.T.: -0.005 min
Response: 2304143
Conc: 338.31 ng/ml

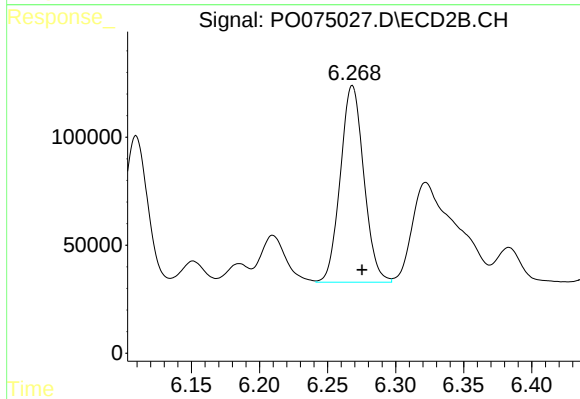

#27 AR-1254-2

R.T.: 6.268 min
Delta R.T.: -0.007 min
Response: 1094168
Conc: 351.08 ng/ml

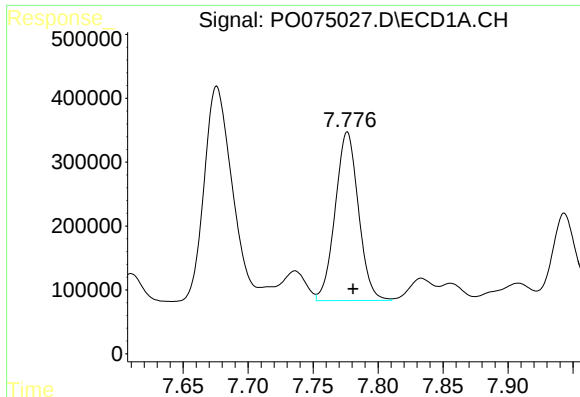


#28 AR-1254-3

R.T.: 7.776 min
Delta R.T.: -0.005 min
Response: 3293542
Conc: 469.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-10DL


Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:36 PM

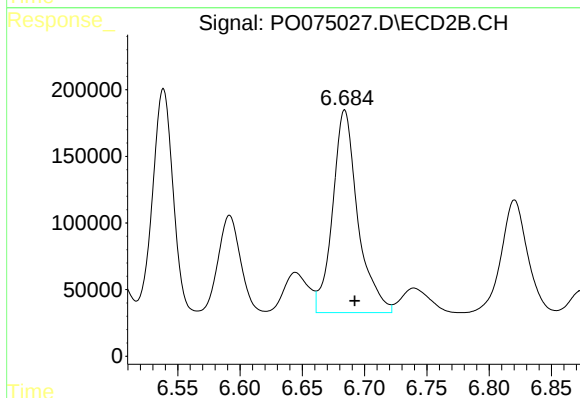


#28 AR-1254-3

R.T.: 6.684 min
Delta R.T.: -0.008 min
Response: 2143949
Conc: 437.19 ng/ml

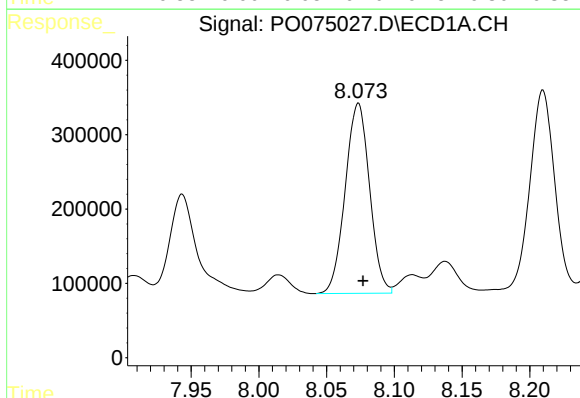


#29 AR-1254-4

R.T.: 8.074 min
Delta R.T.: -0.004 min
Response: 3205151
Conc: 528.50 ng/ml

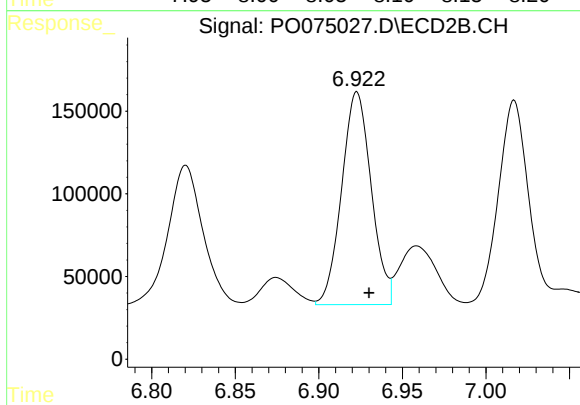

#29 AR-1254-4

R.T.: 6.923 min
Delta R.T.: -0.007 min
Response: 1587201
Conc: 457.70 ng/ml

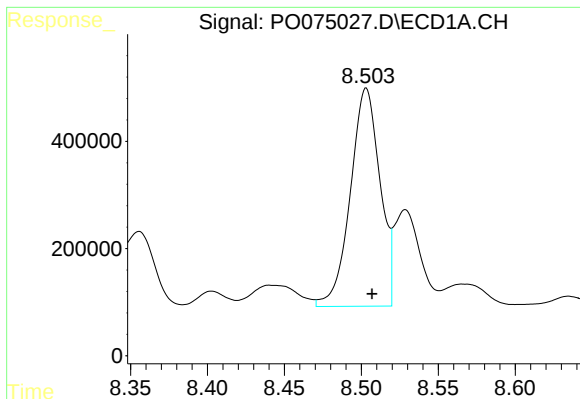


#30 AR-1254-5

R.T.: 8.503 min
Delta R.T.: -0.004 min
Response: 5443740
Conc: 937.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-10DL

Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:36 PM

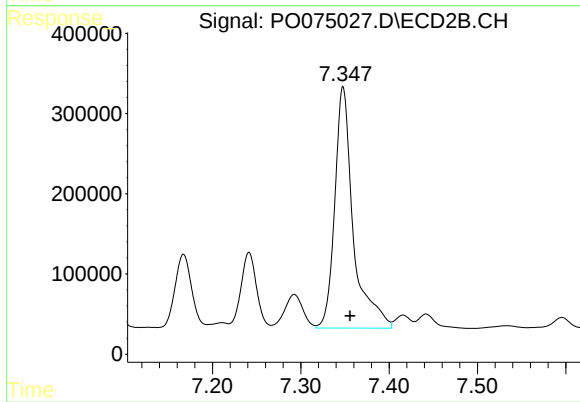

#30 AR-1254-5

R.T.: 7.348 min
Delta R.T.: -0.008 min
Response: 4377569
Conc: 967.22 ng/ml