

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012121\
 Data File : P0075029.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jan 2021 10:35
 Operator : AJ/MA
 Sample : M1084-15DL 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S1-03-DDL

Manual Integrations
 APPROVED

Ankita
 1/22/2021 12:11:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 14:28:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.927	4.001	190149	105062	1.802m	1.868
2) SA Decachlor...	10.945	9.252	95844	64126	0.944	1.168
Target Compounds						
26) L6 AR-1254-1	7.163	6.110	1288775	965327	293.027	267.255
27) L6 AR-1254-2	7.393	6.268	2692391	1230278	395.314	394.758
28) L6 AR-1254-3	7.777	6.684	3492820	2267121	497.955	462.308
29) L6 AR-1254-4	8.074	6.922	3423520	1686187	564.502	486.244
30) L6 AR-1254-5	8.503	7.348	5035828	3903503	866.910	862.473

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012121\
Data File : PO075029.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jan 2021 10:35
Operator : AJ/MA
Sample : M1084-15DL 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S1-03-DDL


Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 14:28:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

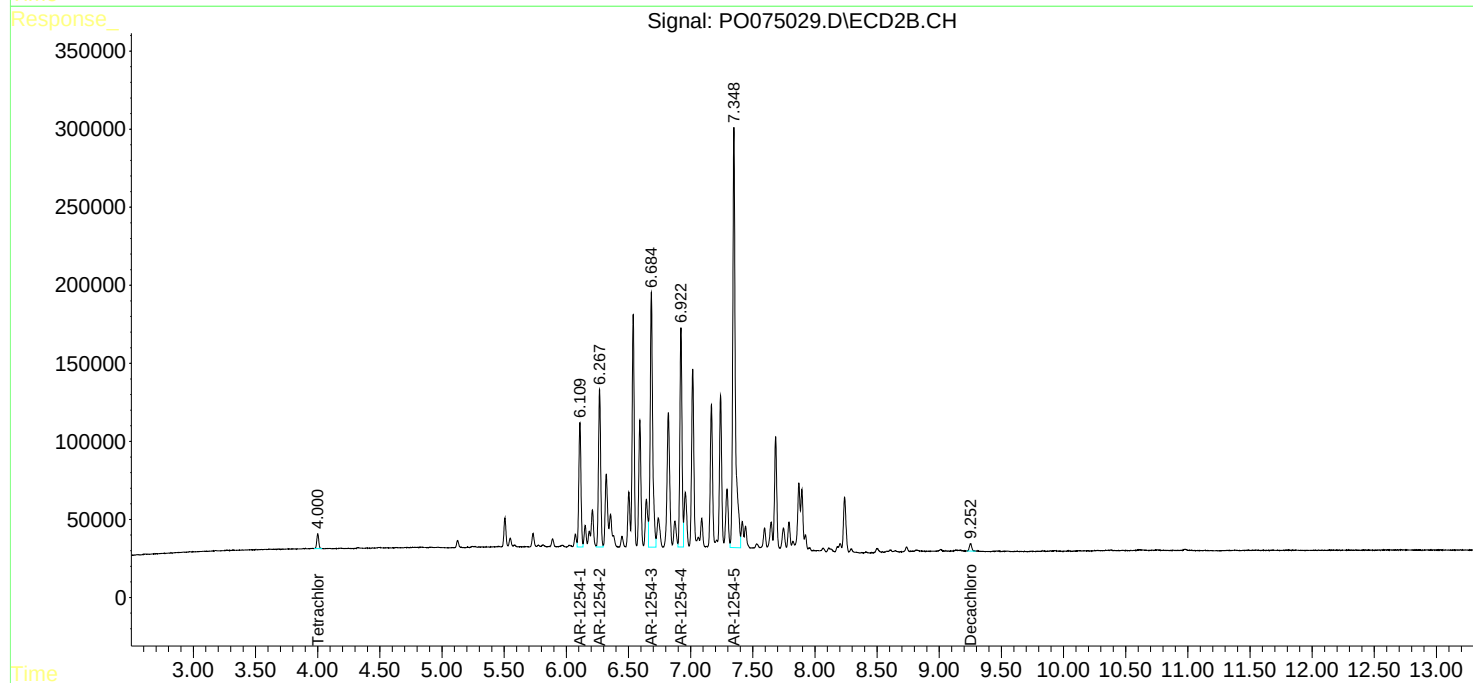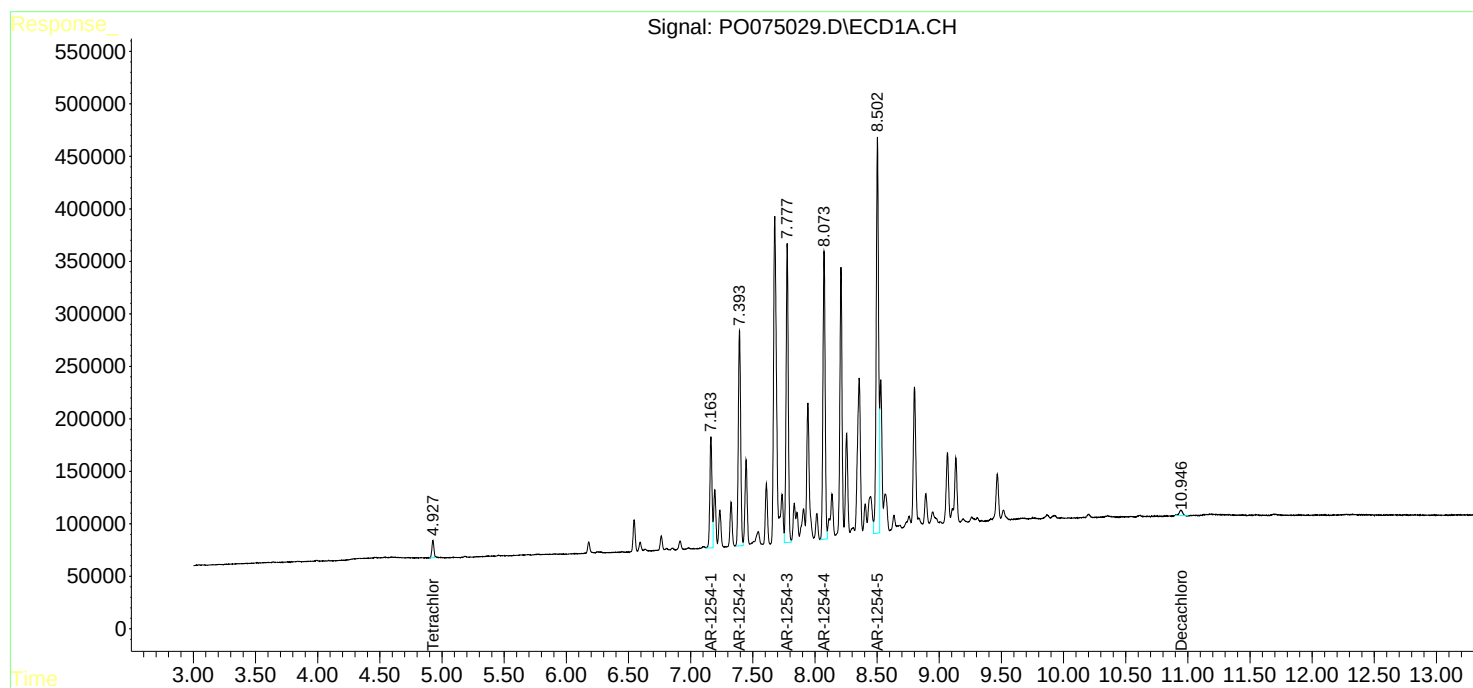

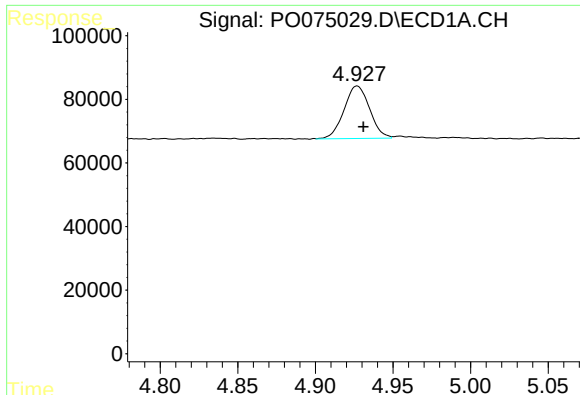


#1 Tetrachloro-m-xylene

R.T.: 4.927 min
 Delta R.T.: -0.004 min
 Response: 190149
 Conc: 1.80 ng/ml m

Instrument :
 ECD_O
 ClientSampleId :
 S1-03-DDL


Manual Integrations
 APPROVED

Ankita
 1/22/2021 12:11:39 PM

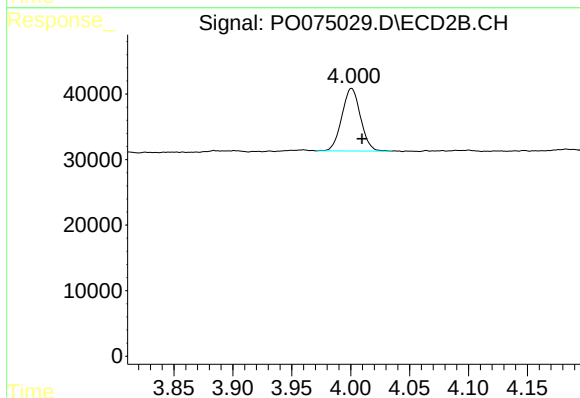


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
 Delta R.T.: -0.009 min
 Response: 105062
 Conc: 1.87 ng/ml

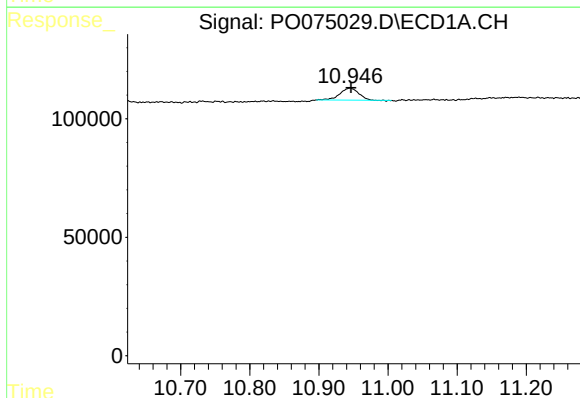


#2 Decachlorobiphenyl

R.T.: 10.945 min
 Delta R.T.: 0.000 min
 Response: 95844
 Conc: 0.94 ng/ml

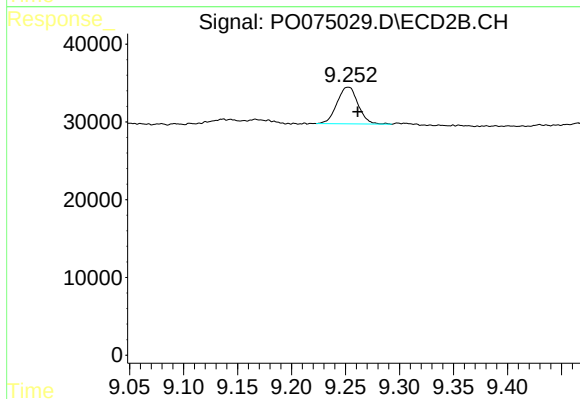

#2 Decachlorobiphenyl

R.T.: 9.252 min
 Delta R.T.: -0.009 min
 Response: 64126
 Conc: 1.17 ng/ml

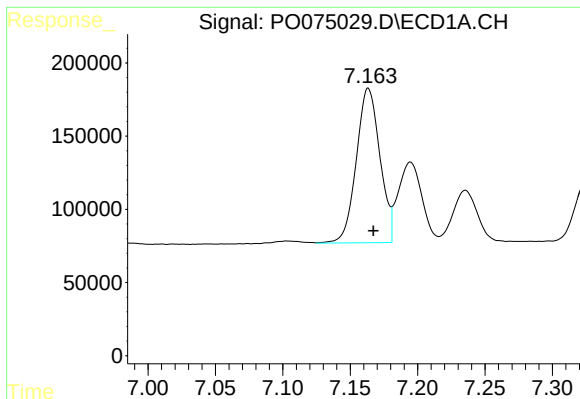


#26 AR-1254-1

R.T.: 7.163 min
Delta R.T.: -0.004 min
Response: 1288775
Conc: 293.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-03-DDL


Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:39 PM

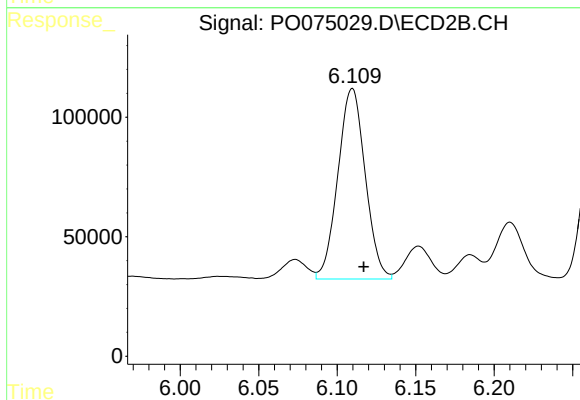


#26 AR-1254-1

R.T.: 6.110 min
Delta R.T.: -0.007 min
Response: 965327
Conc: 267.26 ng/ml

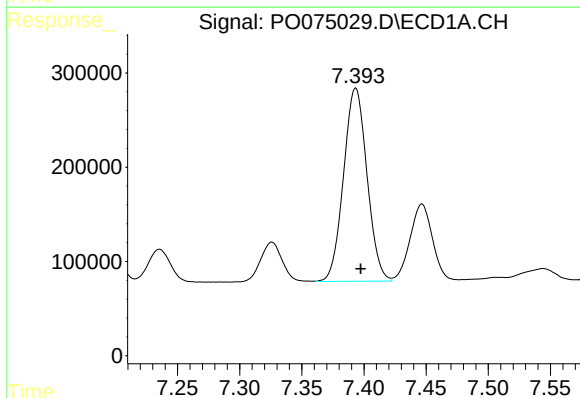


#27 AR-1254-2

R.T.: 7.393 min
Delta R.T.: -0.004 min
Response: 2692391
Conc: 395.31 ng/ml

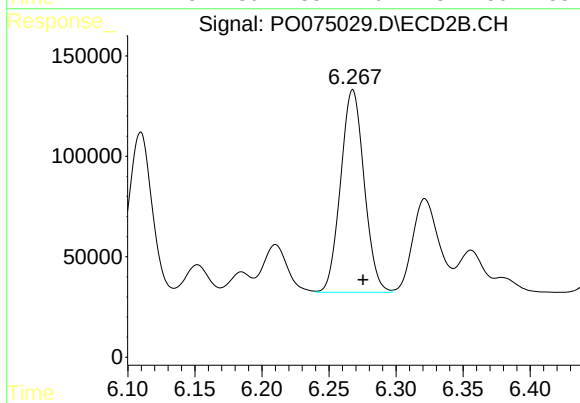

#27 AR-1254-2

R.T.: 6.268 min
Delta R.T.: -0.008 min
Response: 1230278
Conc: 394.76 ng/ml

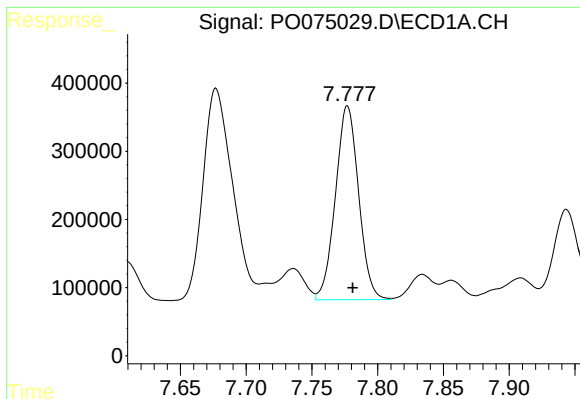


#28 AR-1254-3

R.T.: 7.777 min
Delta R.T.: -0.004 min
Response: 3492820
Conc: 497.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-03-DDL


Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:39 PM

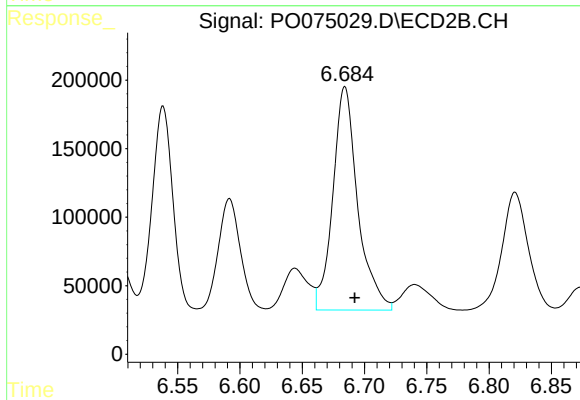


#28 AR-1254-3

R.T.: 6.684 min
Delta R.T.: -0.008 min
Response: 2267121
Conc: 462.31 ng/ml

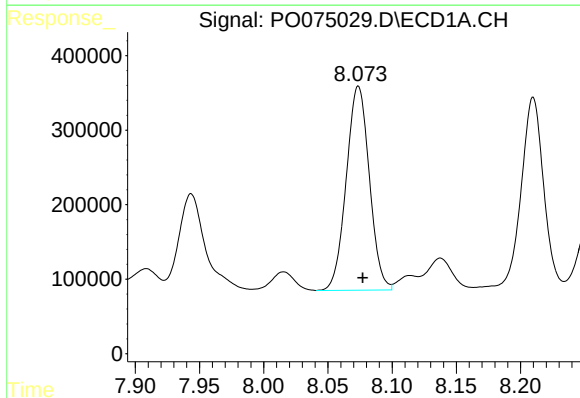


#29 AR-1254-4

R.T.: 8.074 min
Delta R.T.: -0.003 min
Response: 3423520
Conc: 564.50 ng/ml

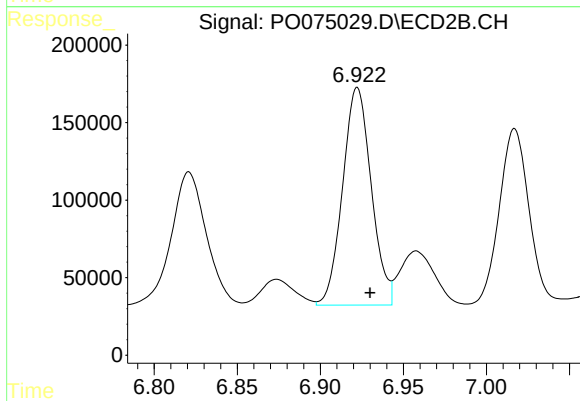

#29 AR-1254-4

R.T.: 6.922 min
Delta R.T.: -0.008 min
Response: 1686187
Conc: 486.24 ng/ml

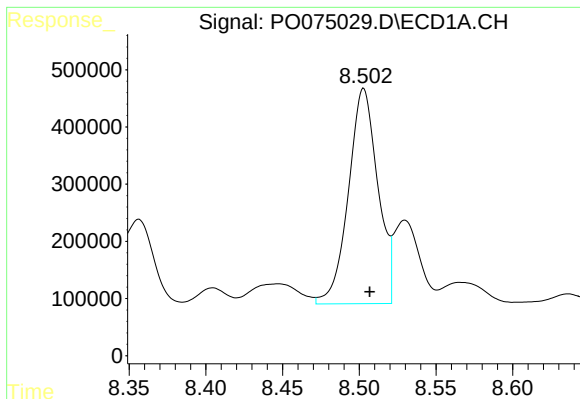


#30 AR-1254-5

R.T.: 8.503 min
Delta R.T.: -0.004 min
Response: 5035828
Conc: 866.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-03-DDL

Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:39 PM

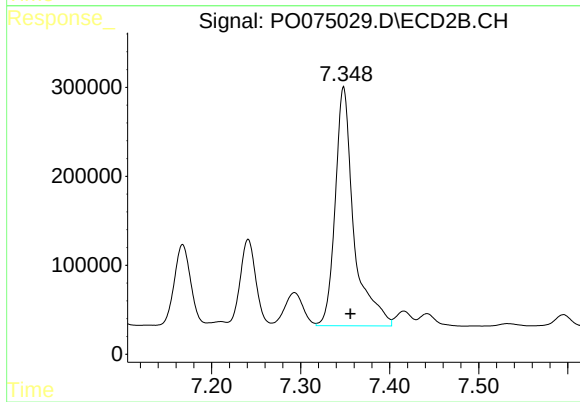

#30 AR-1254-5

R.T.: 7.348 min
Delta R.T.: -0.008 min
Response: 3903503
Conc: 862.47 ng/ml