

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012121\
 Data File : P0075031.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jan 2021 11:10
 Operator : AJ/MA
 Sample : M1084-17DL 2X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S1-05-DDL

Manual Integrations
 APPROVED

Ankita
 1/22/2021 12:11:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 14:29:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.927	4.000	1037531	540872	9.833	9.615
2) SA Decachlor...	10.945	9.253	585075	335134	5.765	6.104m
Target Compounds						
26) L6 AR-1254-1	7.163	6.109	1808196	1349948	411.127	373.739
27) L6 AR-1254-2	7.393	6.269	4071888	1933707	597.860	620.467
28) L6 AR-1254-3	7.777	6.685	5529118	3548075	788.261	723.518
29) L6 AR-1254-4	8.073	6.923	5926507	2850702	977.218	822.054
30) L6 AR-1254-5	8.503	7.349	9349759	9687867	1609.547	2140.520 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012121\
Data File : PO075031.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jan 2021 11:10
Operator : AJ/MA
Sample : M1084-17DL 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S1-05-DDL


Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 14:29:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

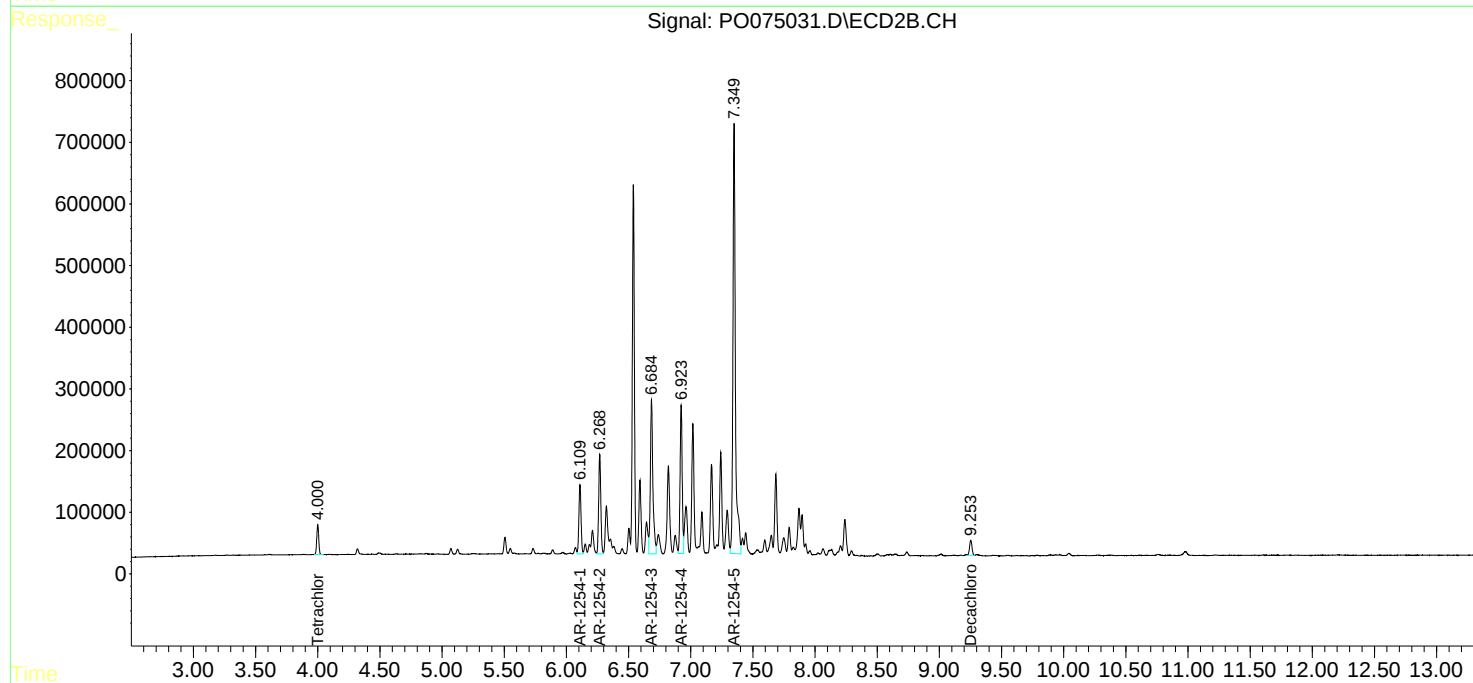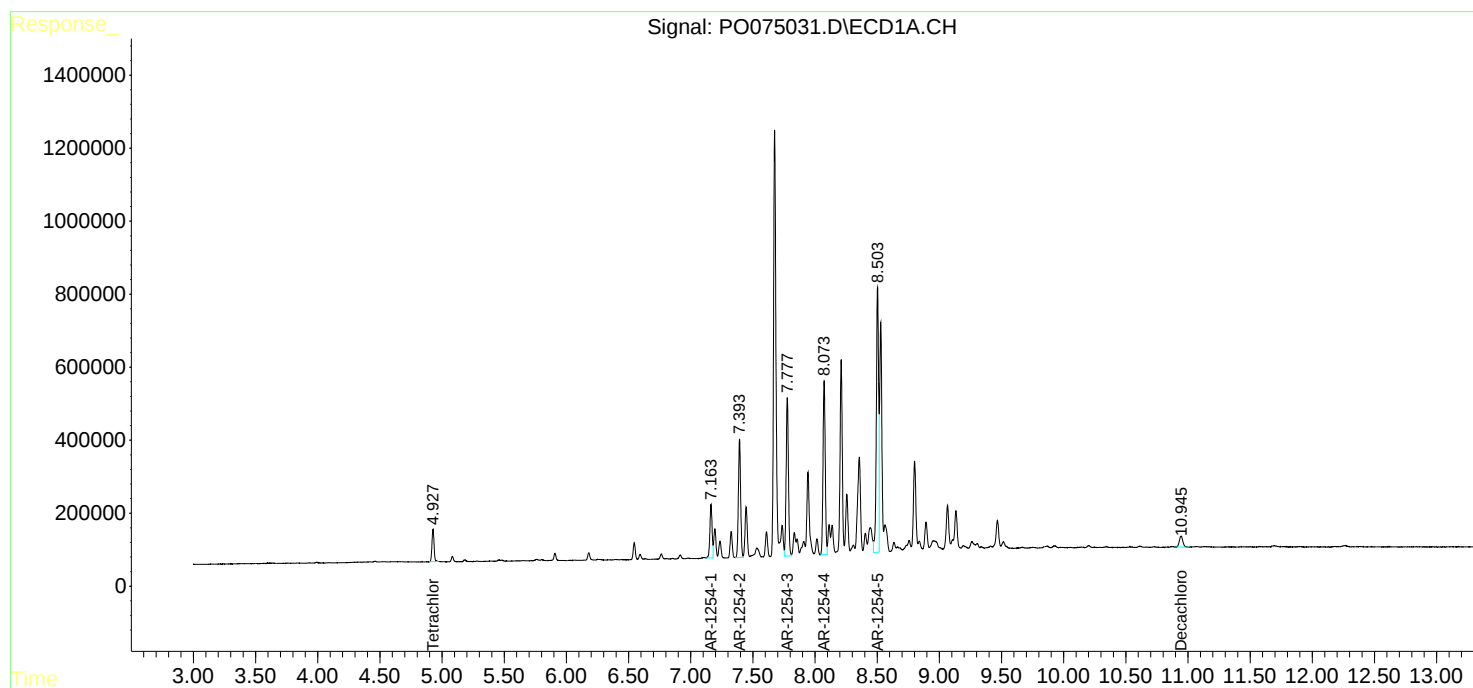

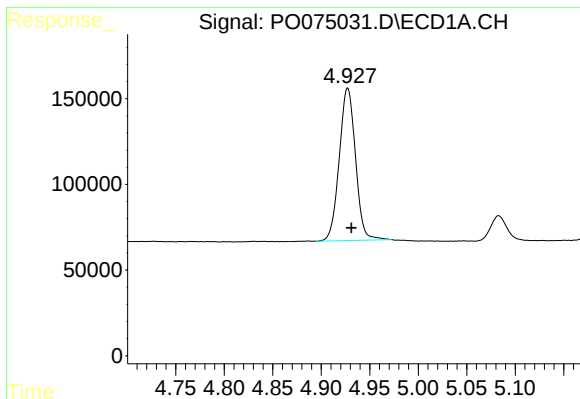


#1 Tetrachloro-m-xylene

R.T.: 4.927 min
Delta R.T.: -0.004 min
Response: 1037531
Conc: 9.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-05-DDL


Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:41 PM

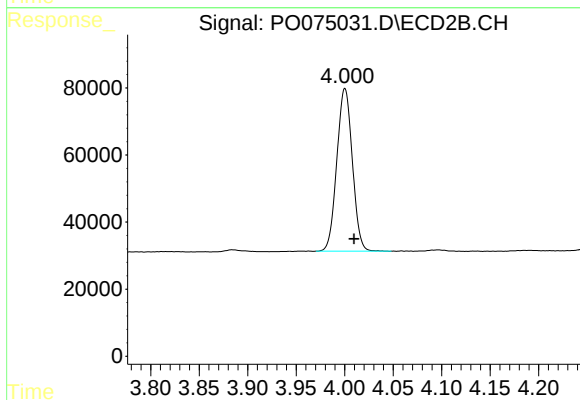


#1 Tetrachloro-m-xylene

R.T.: 4.000 min
Delta R.T.: -0.009 min
Response: 540872
Conc: 9.62 ng/ml

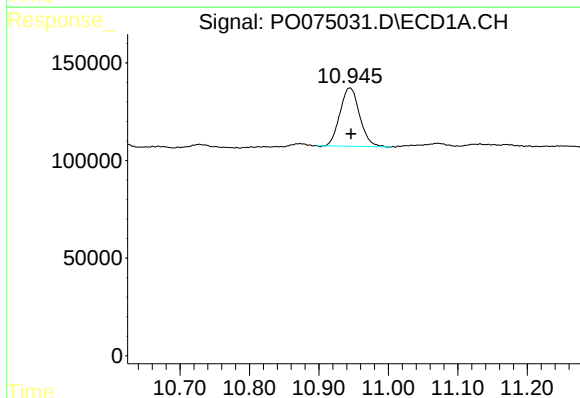


#2 Decachlorobiphenyl

R.T.: 10.945 min
Delta R.T.: -0.002 min
Response: 585075
Conc: 5.76 ng/ml

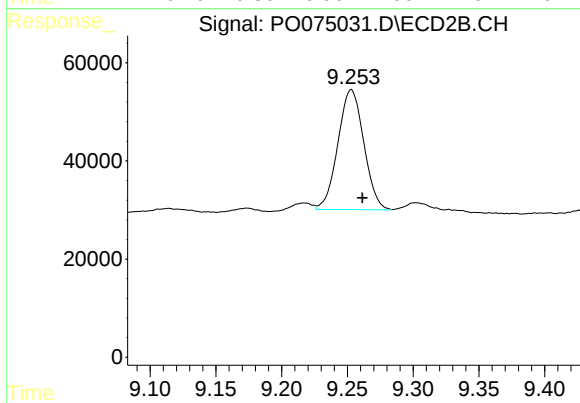

#2 Decachlorobiphenyl

R.T.: 9.253 min
Delta R.T.: -0.009 min
Response: 335134
Conc: 6.10 ng/ml m

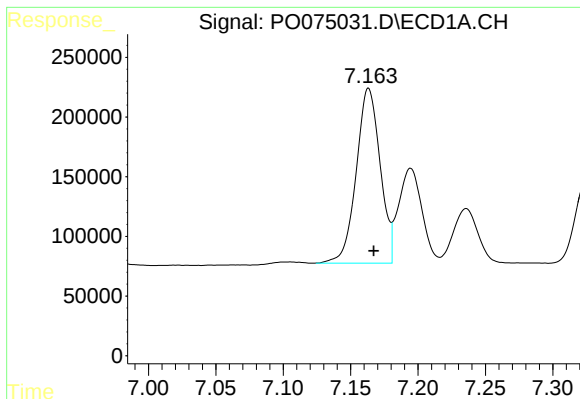


#26 AR-1254-1

R.T.: 7.163 min
Delta R.T.: -0.004 min
Response: 1808196
Conc: 411.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-05-DDL


Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:41 PM

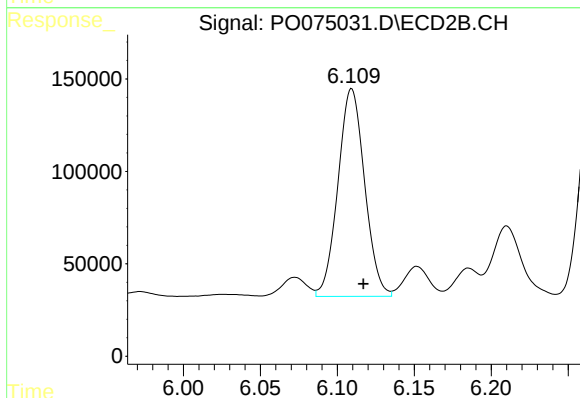


#26 AR-1254-1

R.T.: 6.109 min
Delta R.T.: -0.008 min
Response: 1349948
Conc: 373.74 ng/ml

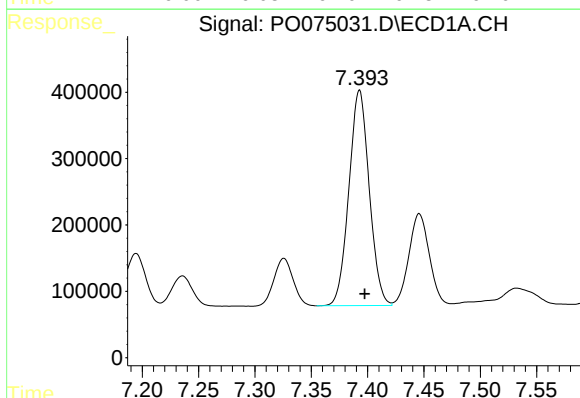


#27 AR-1254-2

R.T.: 7.393 min
Delta R.T.: -0.005 min
Response: 4071888
Conc: 597.86 ng/ml

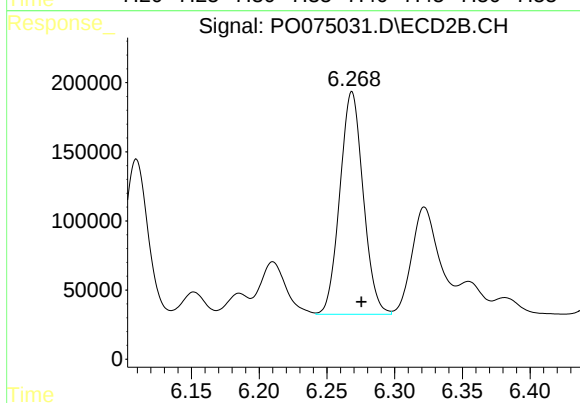

#27 AR-1254-2

R.T.: 6.269 min
Delta R.T.: -0.007 min
Response: 1933707
Conc: 620.47 ng/ml

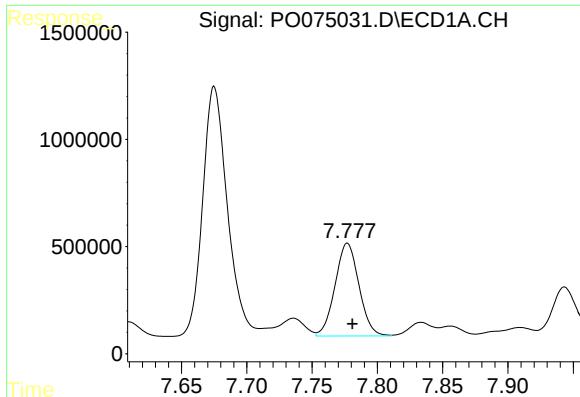


#28 AR-1254-3

R.T.: 7.777 min
Delta R.T.: -0.004 min
Response: 5529118
Conc: 788.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-05-DDL


Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:41 PM

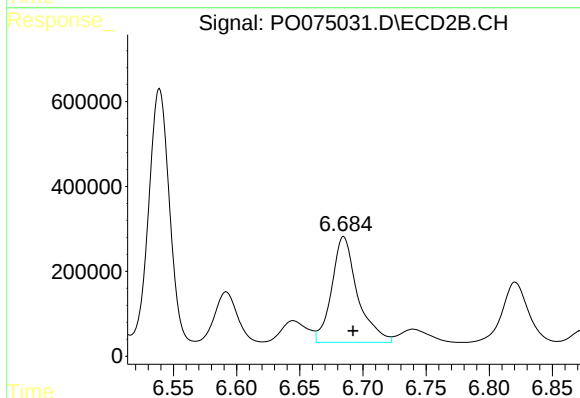


#28 AR-1254-3

R.T.: 6.685 min
Delta R.T.: -0.008 min
Response: 3548075
Conc: 723.52 ng/ml

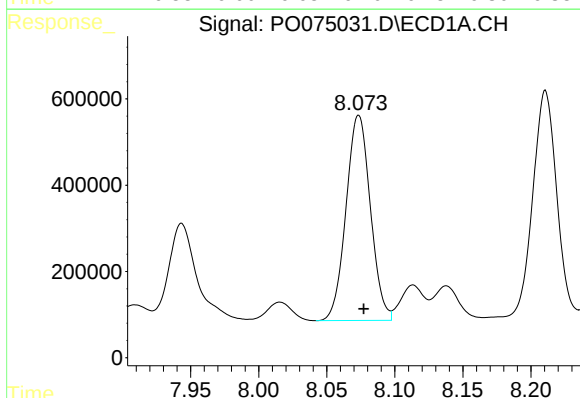


#29 AR-1254-4

R.T.: 8.073 min
Delta R.T.: -0.004 min
Response: 5926507
Conc: 977.22 ng/ml

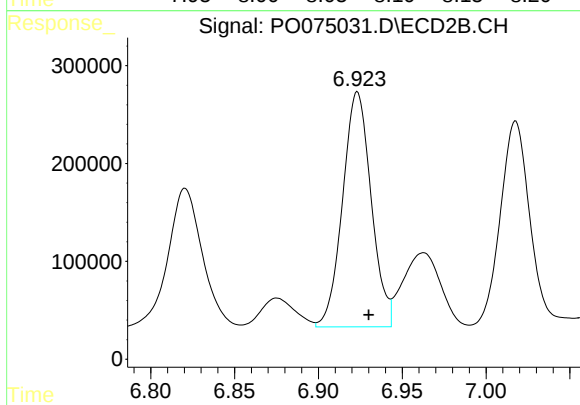

#29 AR-1254-4

R.T.: 6.923 min
Delta R.T.: -0.007 min
Response: 2850702
Conc: 822.05 ng/ml

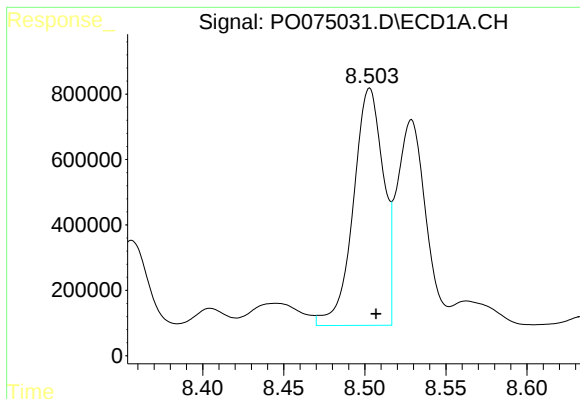


#30 AR-1254-5

R.T.: 8.503 min
Delta R.T.: -0.004 min
Response: 9349759
Conc: 1609.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-05-DDL

Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:41 PM

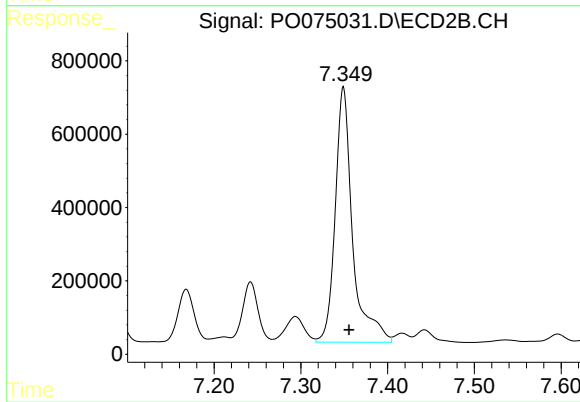

#30 AR-1254-5

R.T.: 7.349 min
Delta R.T.: -0.007 min
Response: 9687867
Conc: 2140.52 ng/ml