

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012121\
 Data File : P0075032.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jan 2021 11:27
 Operator : AJ/MA
 Sample : M1085-07DL 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S2-02-DDL

Manual Integrations
 APPROVED

Ankita
 1/22/2021 12:11:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 14:29:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.927	4.001	1153961	603945	10.936m	10.736
2) SA Decachlor...	10.945	9.250	704889	514758	6.945	9.376m#
Target Compounds						
26) L6 AR-1254-1	7.163	6.109	2035623	1348715	462.837	373.398
27) L6 AR-1254-2	7.393	6.268	4115628	1731349	604.282	555.536
28) L6 AR-1254-3	7.777	6.684	5173985	3263589	737.631	665.506
29) L6 AR-1254-4	8.074	6.923	4830313	2280041	796.467	657.493
30) L6 AR-1254-5	8.504	7.348	7932976	7274448	1365.650	1607.279

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012121\
Data File : PO075032.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jan 2021 11:27
Operator : AJ/MA
Sample : M1085-07DL 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S2-02-DDL


Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 14:29:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

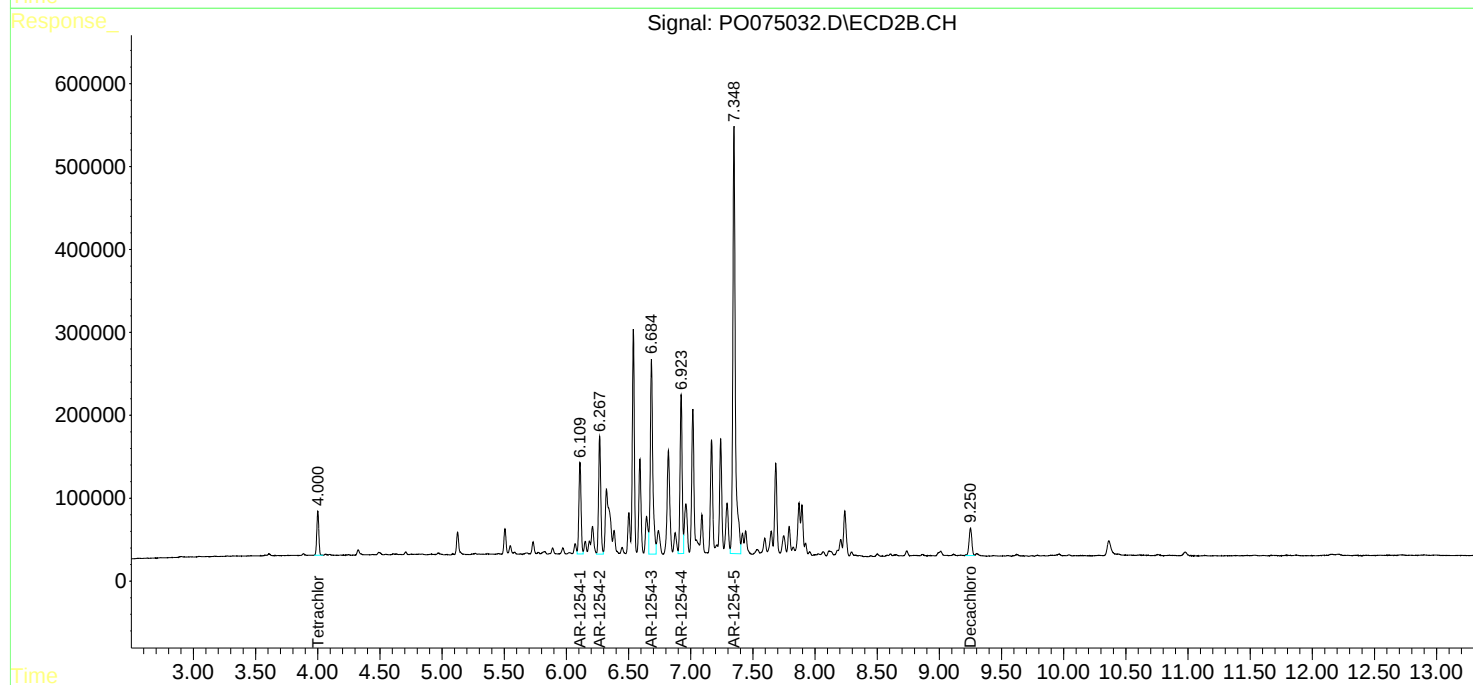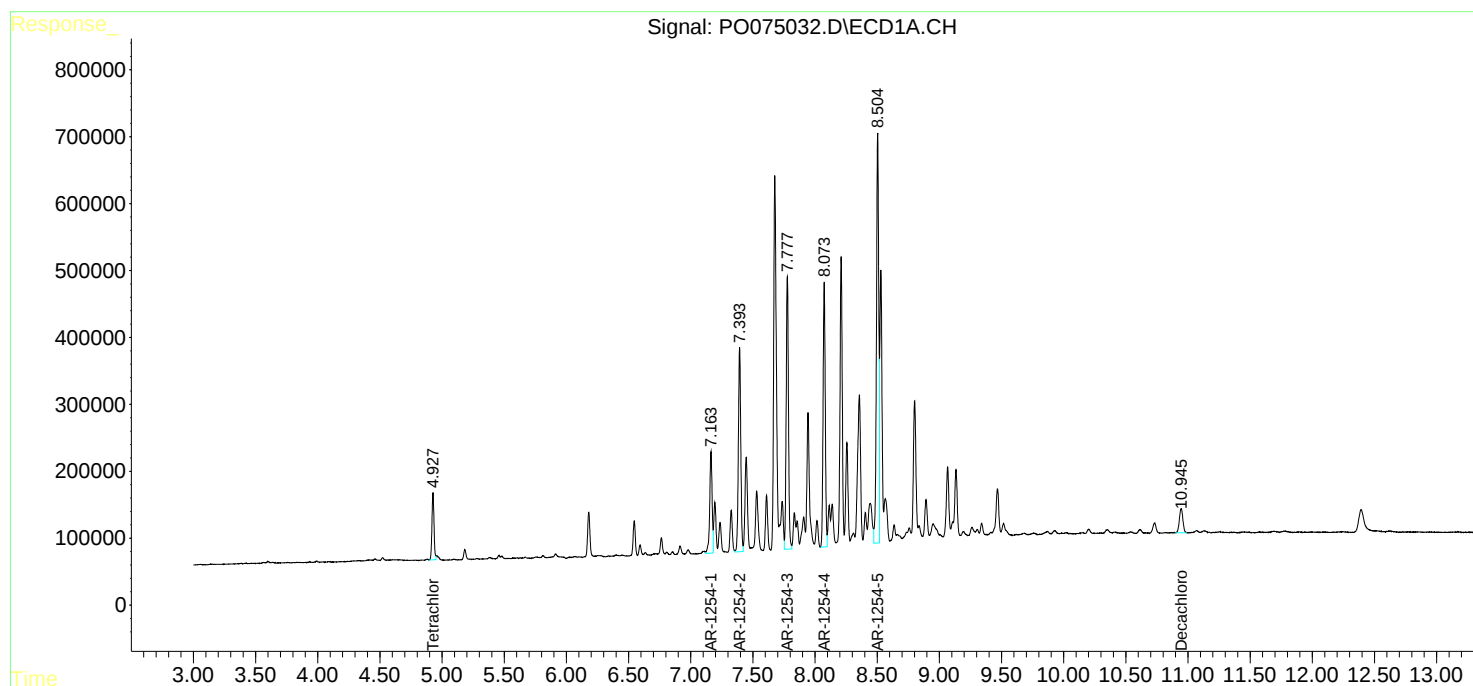

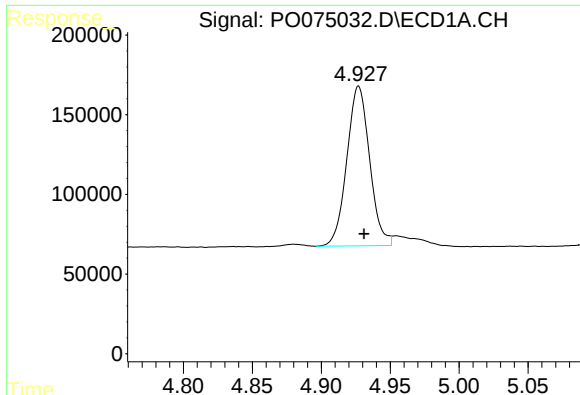


#1 Tetrachloro-m-xylene

R.T.: 4.927 min
Delta R.T.: -0.004 min
Response: 1153961
Conc: 10.94 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S2-02-DDL


Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:43 PM

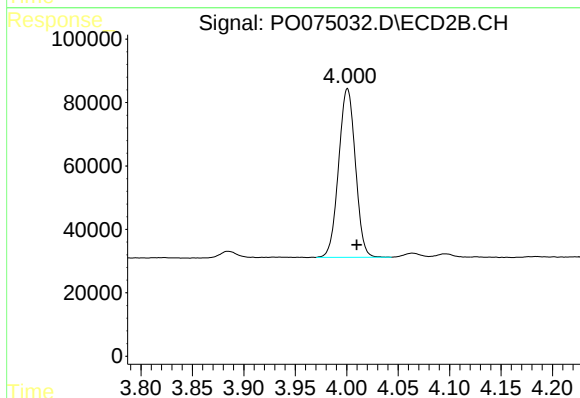


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: -0.009 min
Response: 603945
Conc: 10.74 ng/ml

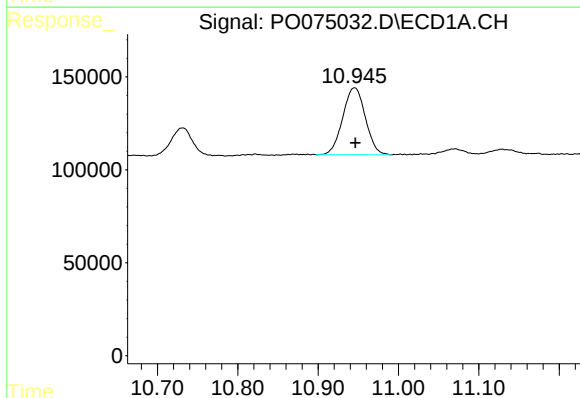


#2 Decachlorobiphenyl

R.T.: 10.945 min
Delta R.T.: -0.001 min
Response: 704889
Conc: 6.95 ng/ml

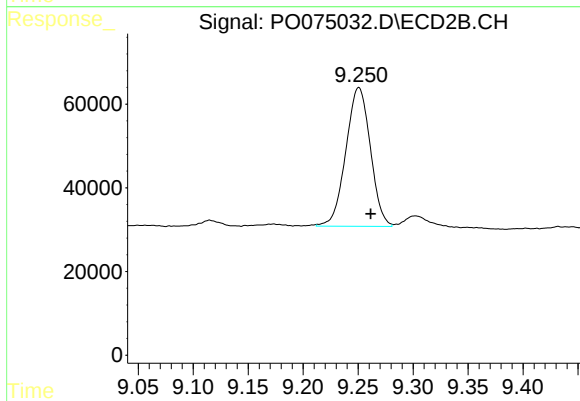

#2 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.011 min
Response: 514758
Conc: 9.38 ng/ml m

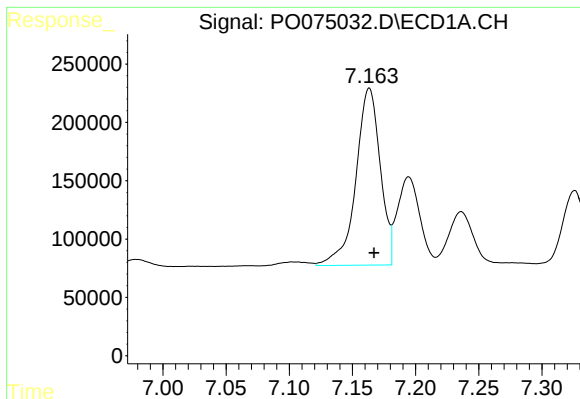


#26 AR-1254-1

R.T.: 7.163 min
Delta R.T.: -0.004 min
Response: 2035623
Conc: 462.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-02-DDL


Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:43 PM

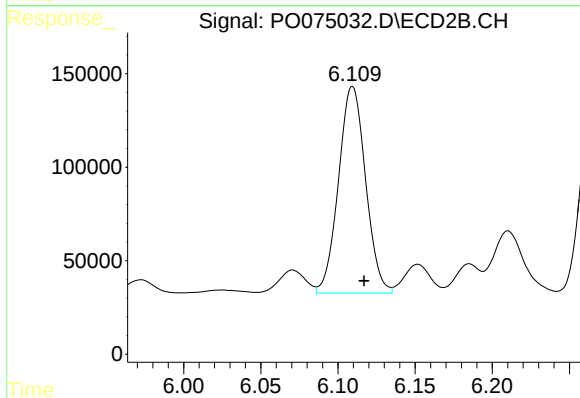


#26 AR-1254-1

R.T.: 6.109 min
Delta R.T.: -0.007 min
Response: 1348715
Conc: 373.40 ng/ml

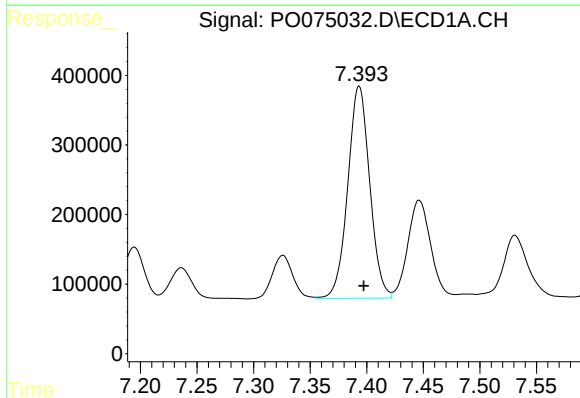


#27 AR-1254-2

R.T.: 7.393 min
Delta R.T.: -0.004 min
Response: 4115628
Conc: 604.28 ng/ml

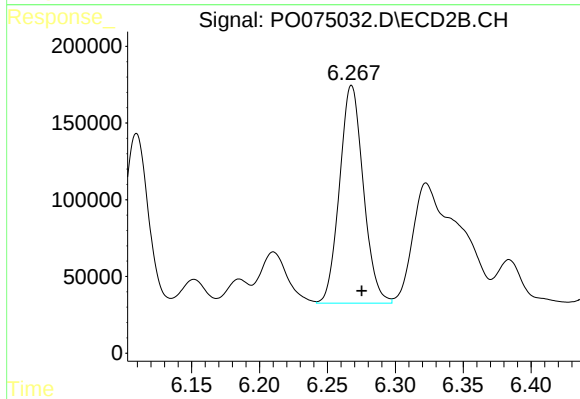

#27 AR-1254-2

R.T.: 6.268 min
Delta R.T.: -0.008 min
Response: 1731349
Conc: 555.54 ng/ml

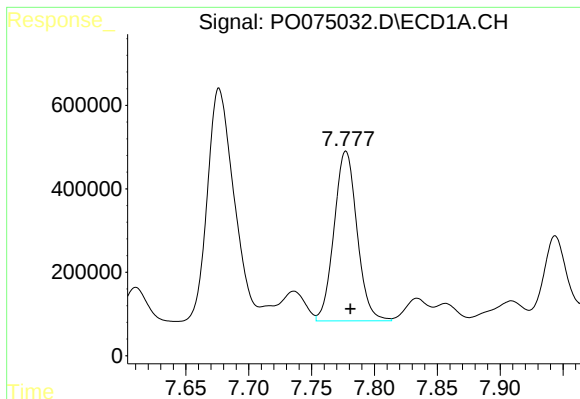


#28 AR-1254-3

R.T.: 7.777 min
Delta R.T.: -0.004 min
Response: 5173985
Conc: 737.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-02-DDL


Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:43 PM

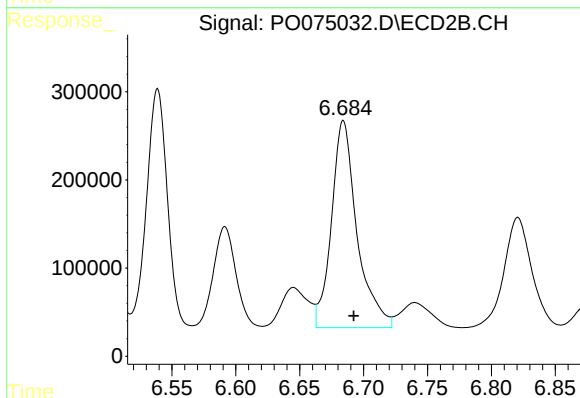


#28 AR-1254-3

R.T.: 6.684 min
Delta R.T.: -0.008 min
Response: 3263589
Conc: 665.51 ng/ml

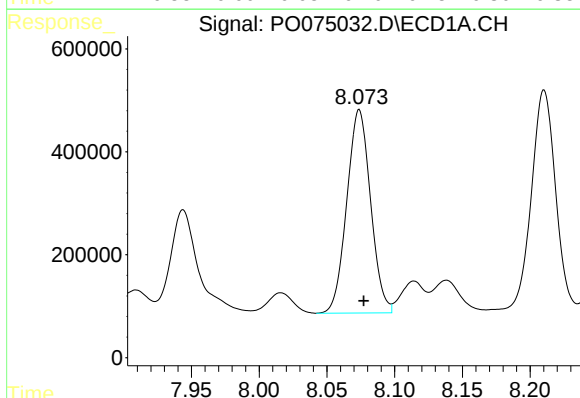


#29 AR-1254-4

R.T.: 8.074 min
Delta R.T.: -0.003 min
Response: 4830313
Conc: 796.47 ng/ml

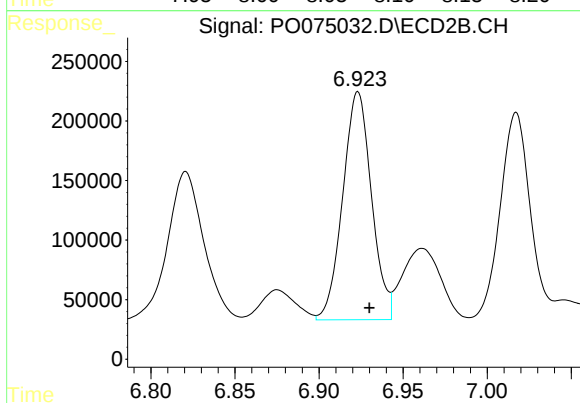

#29 AR-1254-4

R.T.: 6.923 min
Delta R.T.: -0.007 min
Response: 2280041
Conc: 657.49 ng/ml

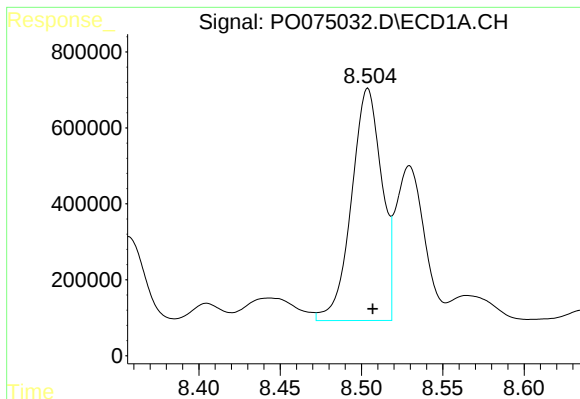


#30 AR-1254-5

R.T.: 8.504 min
Delta R.T.: -0.003 min
Response: 7932976
Conc: 1365.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-02-DDL

Manual Integrations
APPROVED

Ankita
1/22/2021 12:11:43 PM

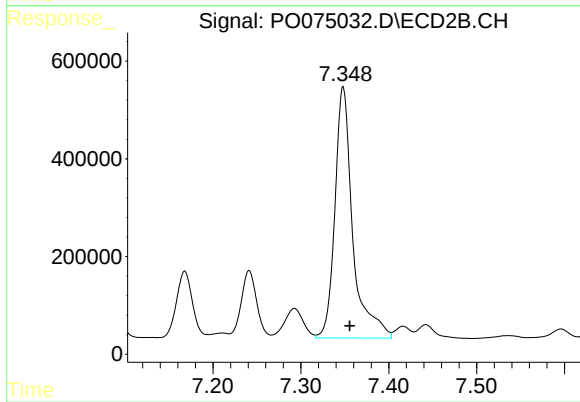

#30 AR-1254-5

R.T.: 7.348 min
Delta R.T.: -0.008 min
Response: 7274448
Conc: 1607.28 ng/ml