

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012122\
 Data File : PP043165.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jan 2022 11:14
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 23:17:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.873	4.040	458409	504907	19.374	20.216
2) SA Decachlor...	10.794	9.366	392914	412670	26.878	21.155
Target Compounds						
30) L6 AR-1254-5	8.435f	0.000	5599	0	5.976	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012122\
Data File : PP043165.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jan 2022 11:14
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 23:17:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

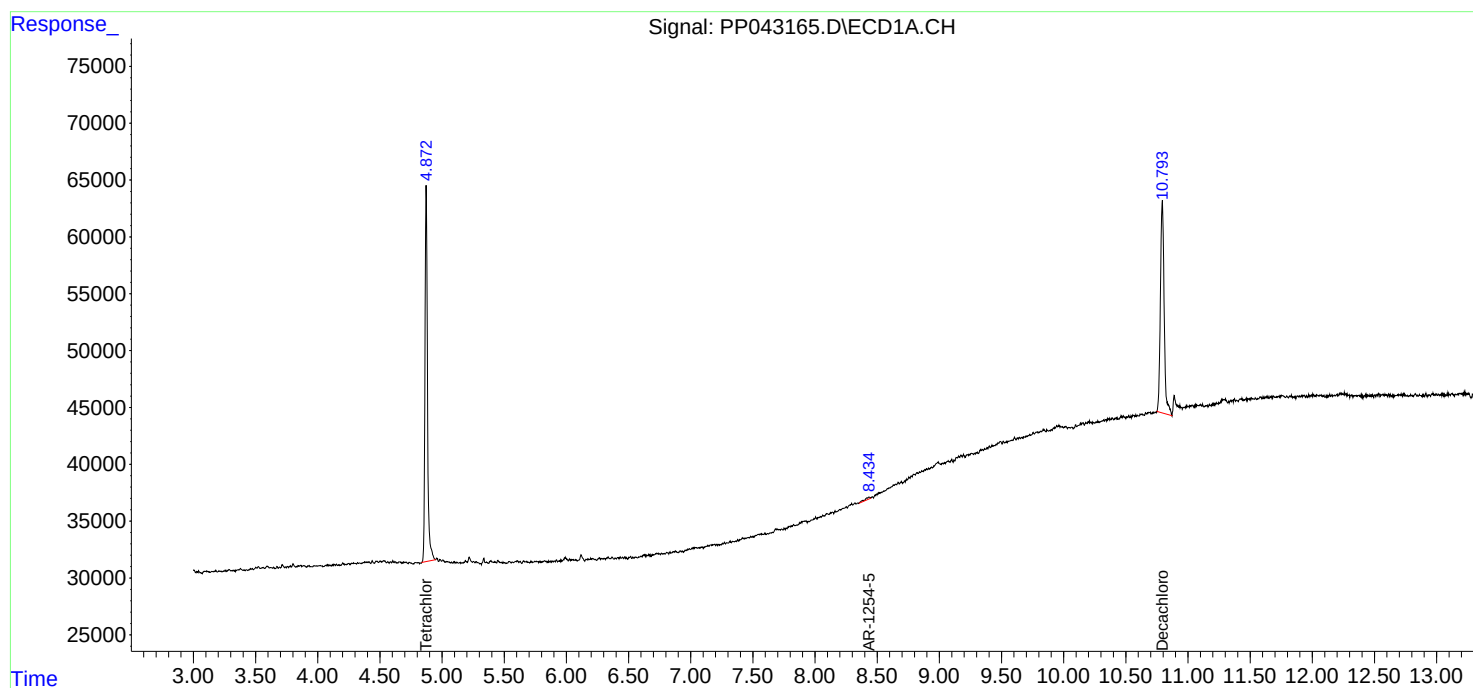


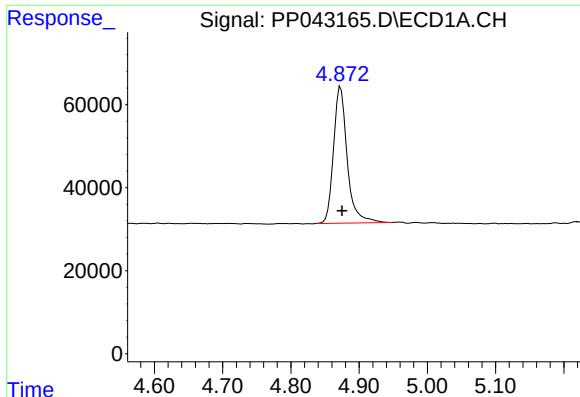

#1 Tetrachloro-m-xylene


R.T.: 4.873 min
Delta R.T.: -0.002 min
Response: 458409
Conc: 19.37 ng/ml

Instrument :
ECD_O
ClientSampleId :

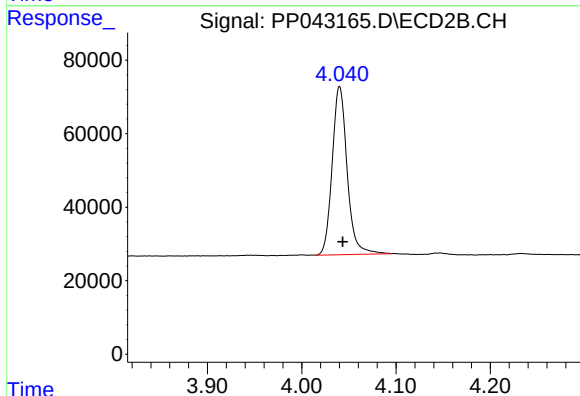


#1 Tetrachloro-m-xylene

R.T.: 4.040 min
Delta R.T.: -0.003 min
Response: 504907
Conc: 20.22 ng/ml

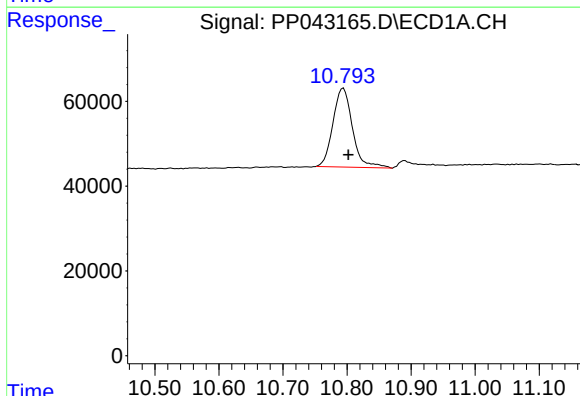


#2 Decachlorobiphenyl

R.T.: 10.794 min
Delta R.T.: -0.008 min
Response: 392914
Conc: 26.88 ng/ml

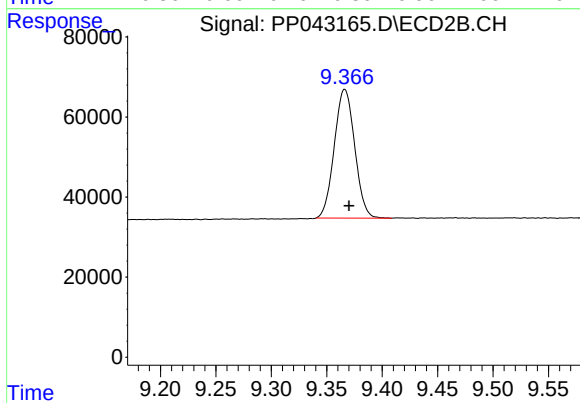

#2 Decachlorobiphenyl


R.T.: 9.366 min
Delta R.T.: -0.004 min
Response: 412670
Conc: 21.16 ng/ml

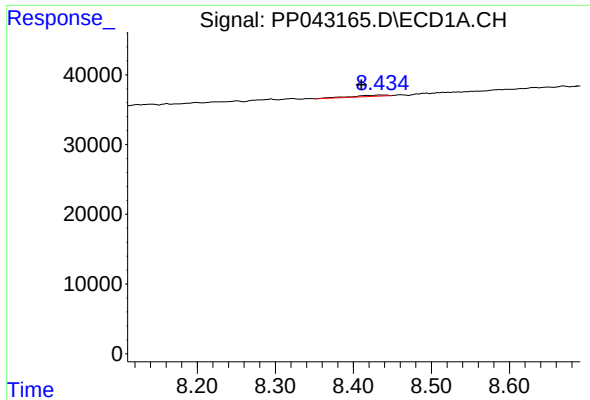

#30 AR-1254-5

R.T.: 8.435 min
Delta R.T.: 0.025 min
Response: 5599
Conc: 5.98 ng/ml

Instrument :
ECD_O
ClientSampleId :

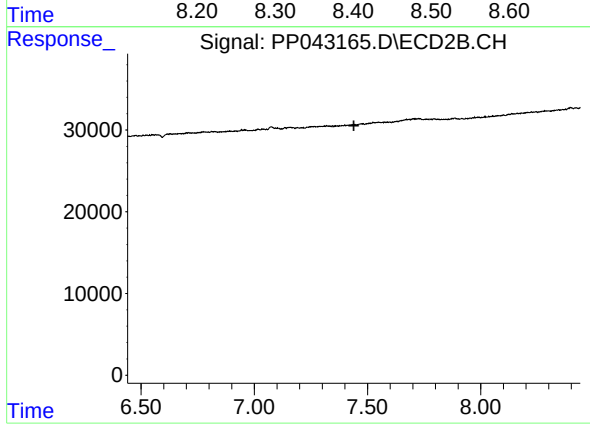

#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.