

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012122\
 Data File : PP043168.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Jan 2022 13:17
 Operator : AJ\MA
 Sample : PB142171BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 23:18:45 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 13 19:45:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.870	4.039	427425	480605	18.064	19.243
2)	SA Decachlor...	10.788	9.363	336785	386256	23.038	19.801
Target Compounds							
8)	L2 AR-1221-1	5.103	0.000	21861	0	82.119	N.D. #
9)	L2 AR-1221-2	5.218	0.000	14710	0	72.786	N.D. #
30)	L6 AR-1254-5	8.415	0.000	3900	0	4.163	N.D. #
31)	L7 AR-1260-1	7.889f	0.000	107	0	0.112	N.D. #
32)	L7 AR-1260-2	8.151f	0.000	9487	0	9.186	N.D. #
35)	L7 AR-1260-5	9.040	0.000	2901	0	1.763	N.D. #
37)	L8 AR-1262-2	9.040	0.000	2901	0	1.676	N.D. #
38)	L8 AR-1262-3	0.000	8.291	0	7711	N.D.	6.912 #
41)	L9 AR-1268-1	0.000	8.291	0	7711	N.D.	2.502 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012122\
Data File : PP043168.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Jan 2022 13:17
Operator : AJ\MA
Sample : PB142171BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 23:18:45 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 13 19:45:07 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

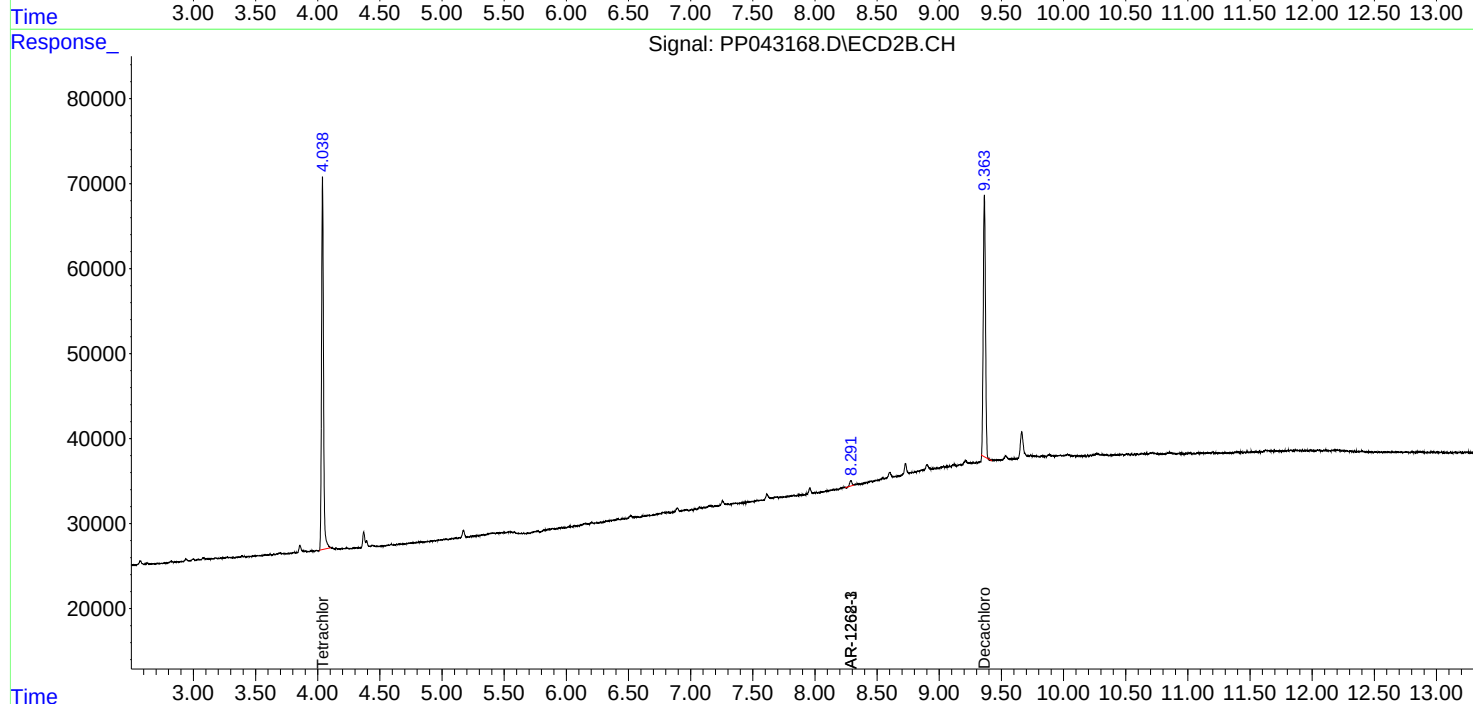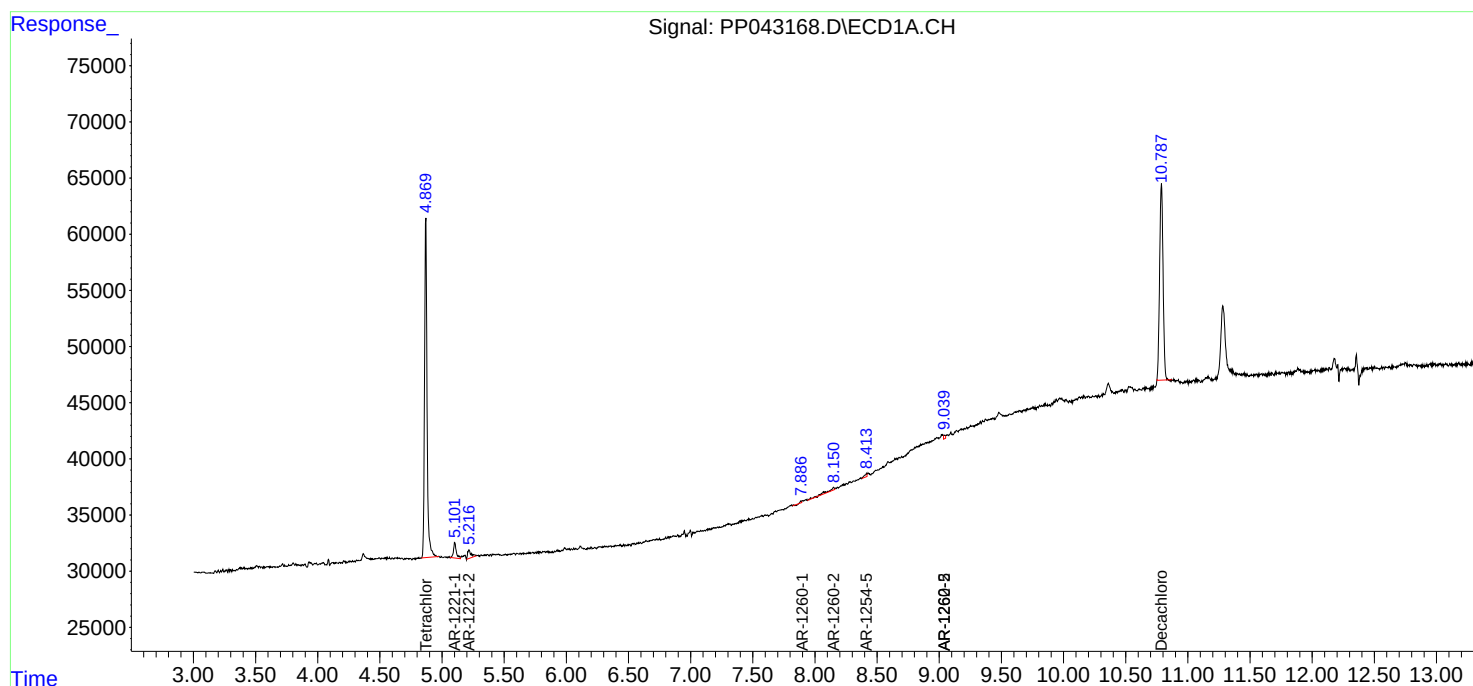


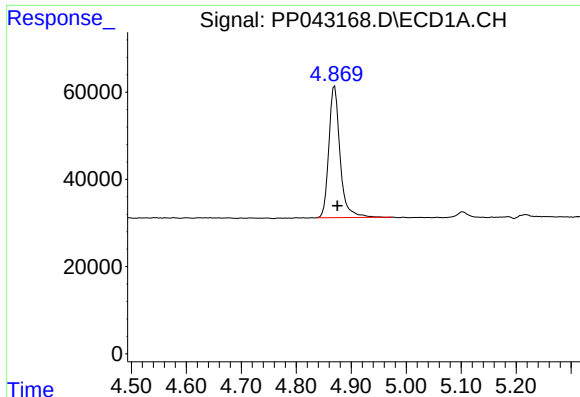

#1 Tetrachloro-m-xylene


R.T.: 4.870 min
Delta R.T.: -0.005 min
Response: 427425
Conc: 18.06 ng/ml

Instrument :
ECD_O
ClientSampleId :

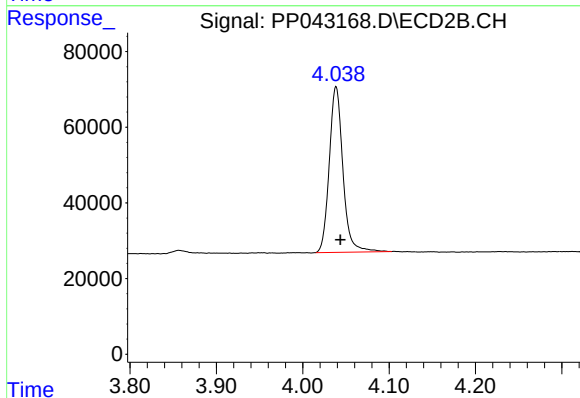


#1 Tetrachloro-m-xylene

R.T.: 4.039 min
Delta R.T.: -0.005 min
Response: 480605
Conc: 19.24 ng/ml

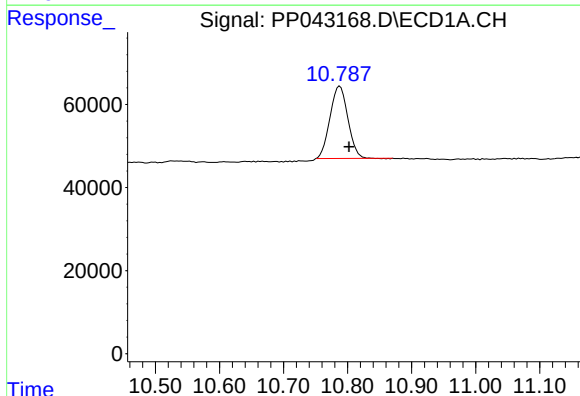


#2 Decachlorobiphenyl

R.T.: 10.788 min
Delta R.T.: -0.014 min
Response: 336785
Conc: 23.04 ng/ml

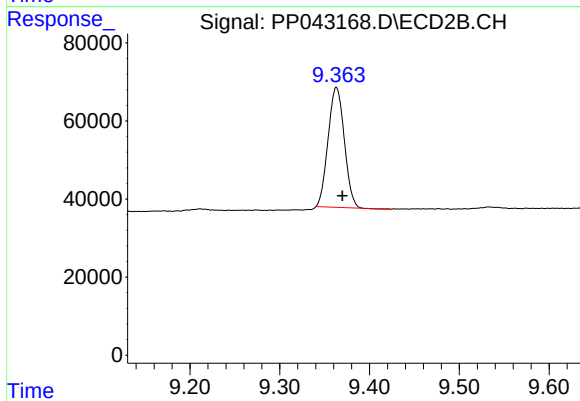

#2 Decachlorobiphenyl


R.T.: 9.363 min
Delta R.T.: -0.007 min
Response: 386256
Conc: 19.80 ng/ml

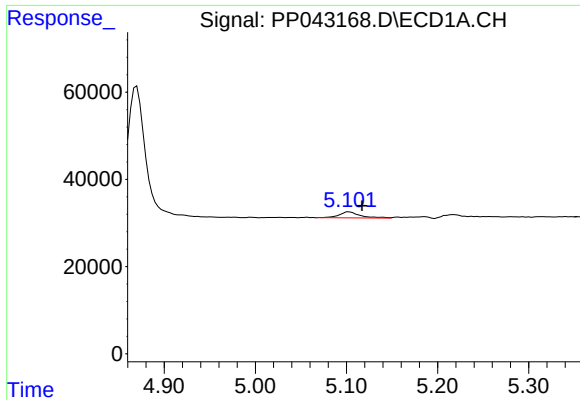

#8 AR-1221-1


R.T.: 5.103 min
Delta R.T.: -0.014 min
Response: 21861
Conc: 82.12 ng/ml

Instrument :
ECD_O
ClientSampleId :

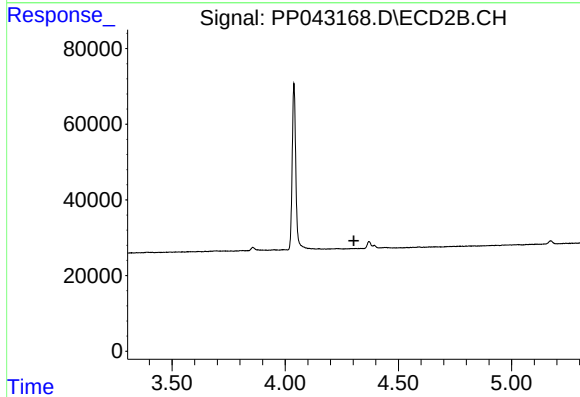


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.303 min
Response: 0
Conc: N.D.

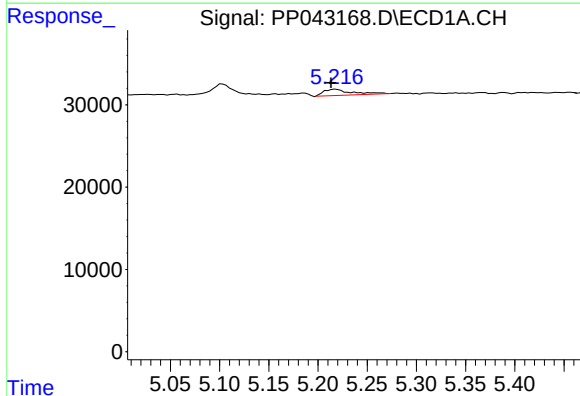


#9 AR-1221-2

R.T.: 5.218 min
Delta R.T.: 0.005 min
Response: 14710
Conc: 72.79 ng/ml

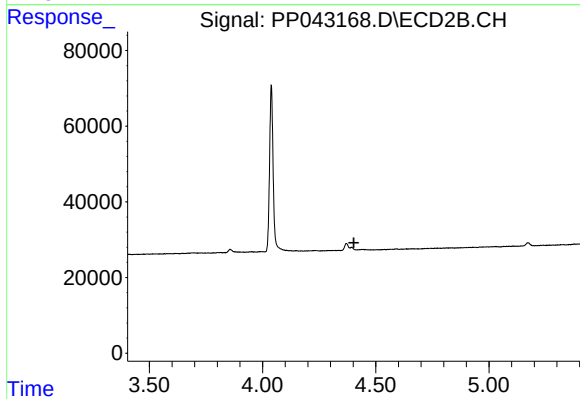

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.403 min
Response: 0
Conc: N.D.

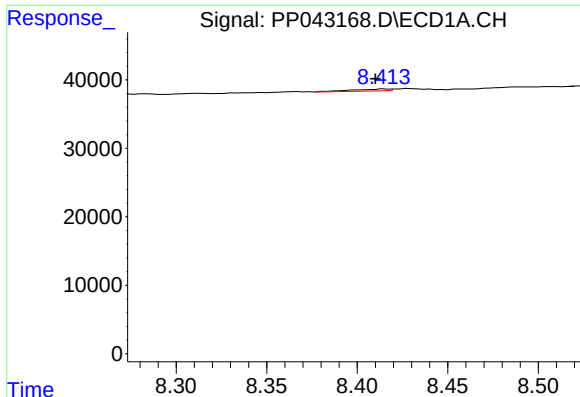

#30 AR-1254-5


R.T.: 8.415 min
Delta R.T.: 0.005 min
Response: 3900
Conc: 4.16 ng/ml

Instrument :
ECD_O
ClientSampleId :

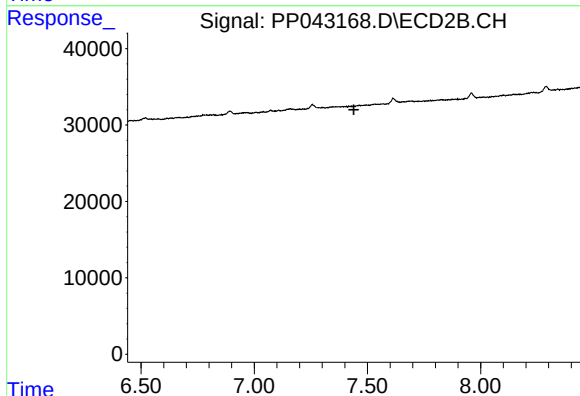


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.440 min
Response: 0
Conc: N.D.

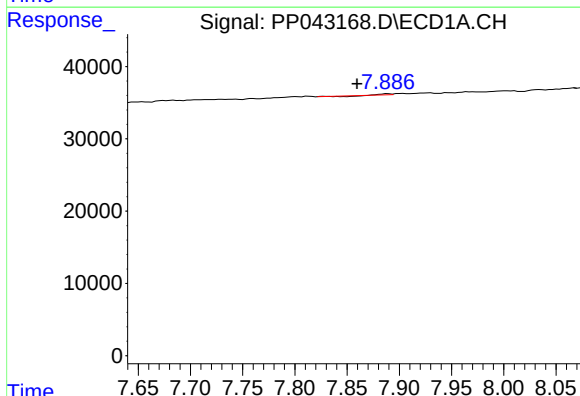


#31 AR-1260-1

R.T.: 7.889 min
Delta R.T.: 0.029 min
Response: 107
Conc: 0.11 ng/ml

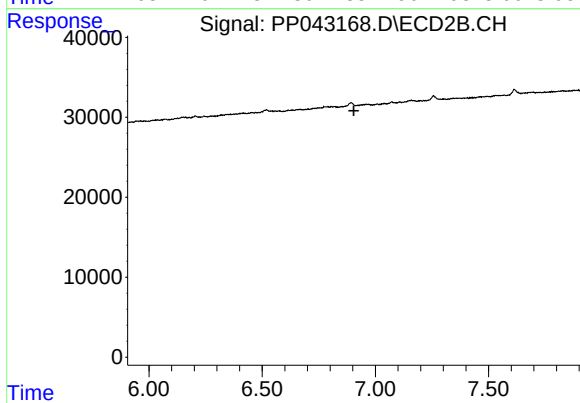

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.905 min
Response: 0
Conc: N.D.

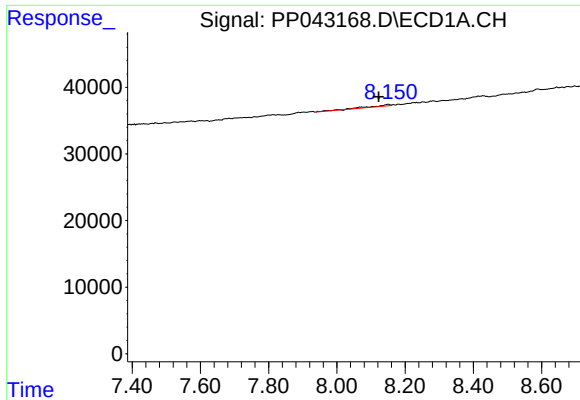

#32 AR-1260-2


R.T.: 8.151 min
Delta R.T.: 0.028 min
Response: 9487
Conc: 9.19 ng/ml

Instrument :
ECD_O
ClientSampleId :

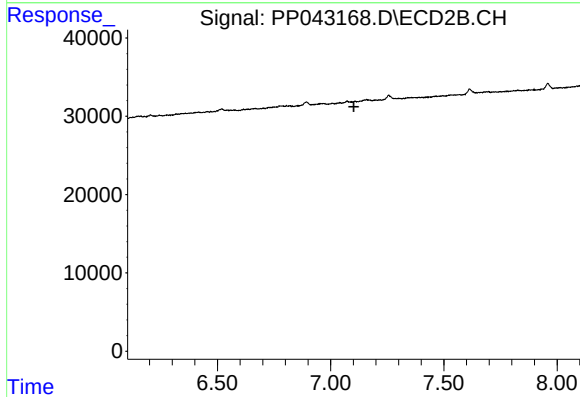


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.102 min
Response: 0
Conc: N.D.

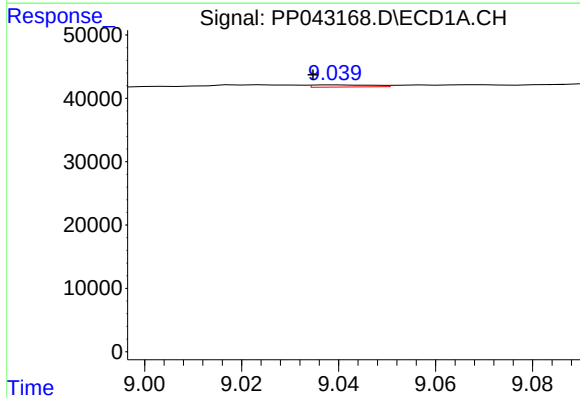


#35 AR-1260-5

R.T.: 9.040 min
Delta R.T.: 0.005 min
Response: 2901
Conc: 1.76 ng/ml

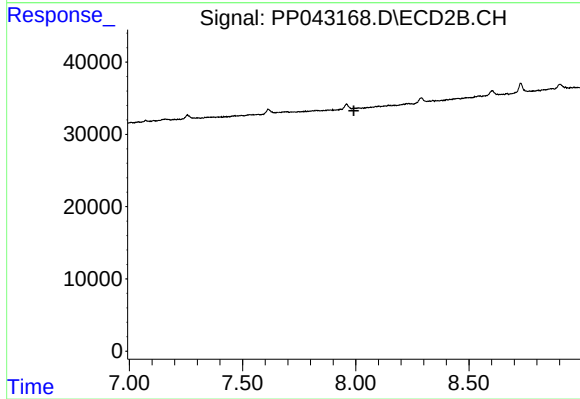

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.992 min
Response: 0
Conc: N.D.

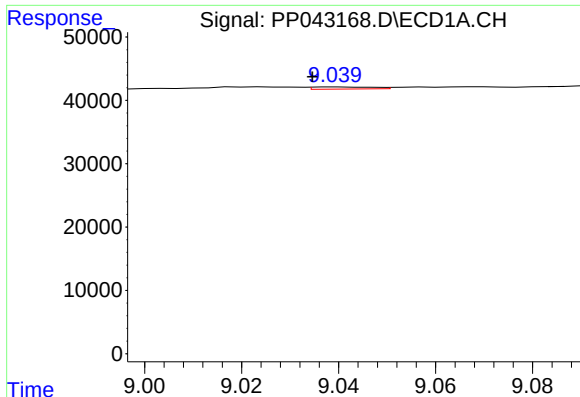

#37 AR-1262-2


R.T.: 9.040 min
Delta R.T.: 0.005 min
Response: 2901
Conc: 1.68 ng/ml

Instrument :
ECD_O
ClientSampleId :

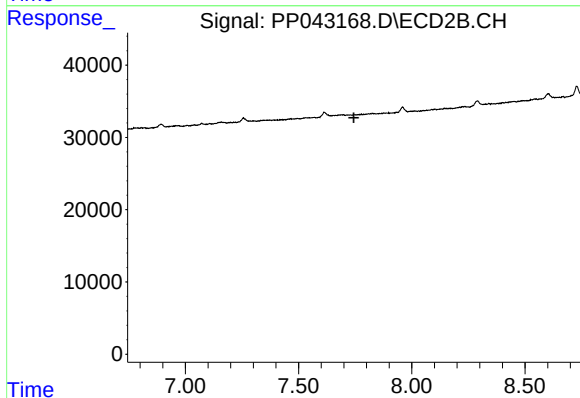


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.744 min
Response: 0
Conc: N.D.

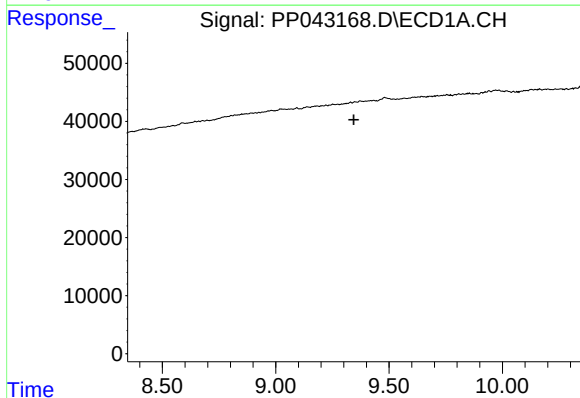


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.344 min
Response: 0
Conc: N.D.

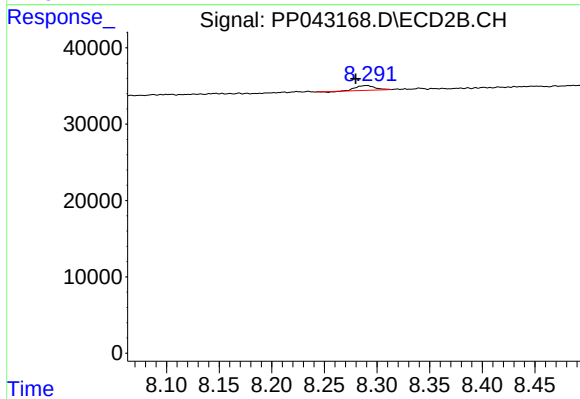

#38 AR-1262-3


R.T.: 8.291 min
Delta R.T.: 0.011 min
Response: 7711
Conc: 6.91 ng/ml

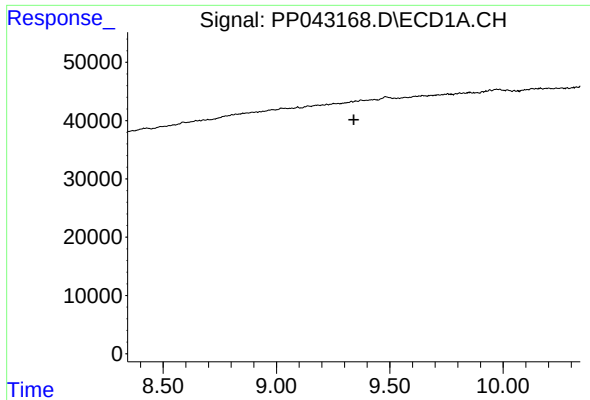

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.341 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

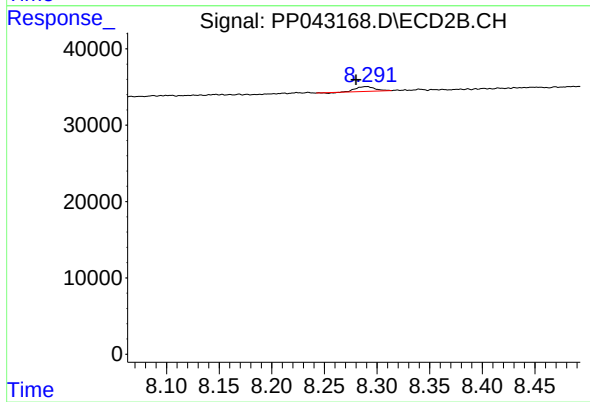

#41 AR-1268-1

R.T.: 8.291 min
Delta R.T.: 0.011 min
Response: 7711
Conc: 2.50 ng/ml