

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012220\
 Data File : P0065788.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2020 18:06
 Operator : DD\AJ
 Sample : PB126209BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 01:11:24 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.161	3.437	398792	499731	21.839	22.718
2)	SA Decachlor...	9.659	8.335	716312	862558	21.141	20.799
Target Compounds							
3)	L1 AR-1016-1	5.246	0.000	22550	0	25.856	N.D. #
9)	L2 AR-1221-2	4.462	0.000	5837	0	37.388	N.D. #
16)	L4 AR-1242-1	5.246	0.000	22550	0	38.734	N.D. #
24)	L5 AR-1248-4	6.151	0.000	8360	0	8.825	N.D. #
26)	L6 AR-1254-1	6.151	0.000	8360	0	9.854	N.D. #
28)	L6 AR-1254-3	6.739	0.000	6854	0	4.422	N.D. #
30)	L6 AR-1254-5	7.429	0.000	4933	0	3.513	N.D. #
45)	L9 AR-1268-5	9.362	8.107	9110	9599	0.822	0.668



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012220\
Data File : P0065788.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2020 18:06
Operator : DD\AJ
Sample : PB126209BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 01:11:24 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

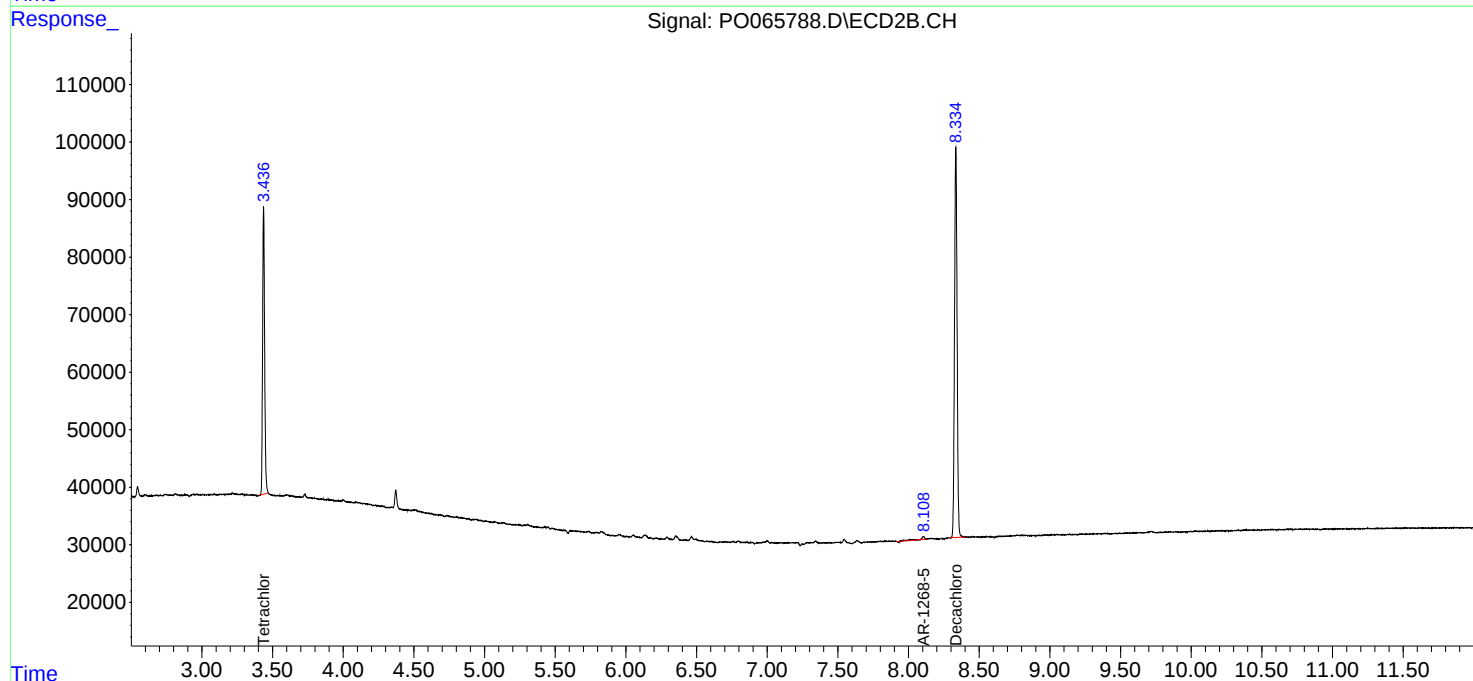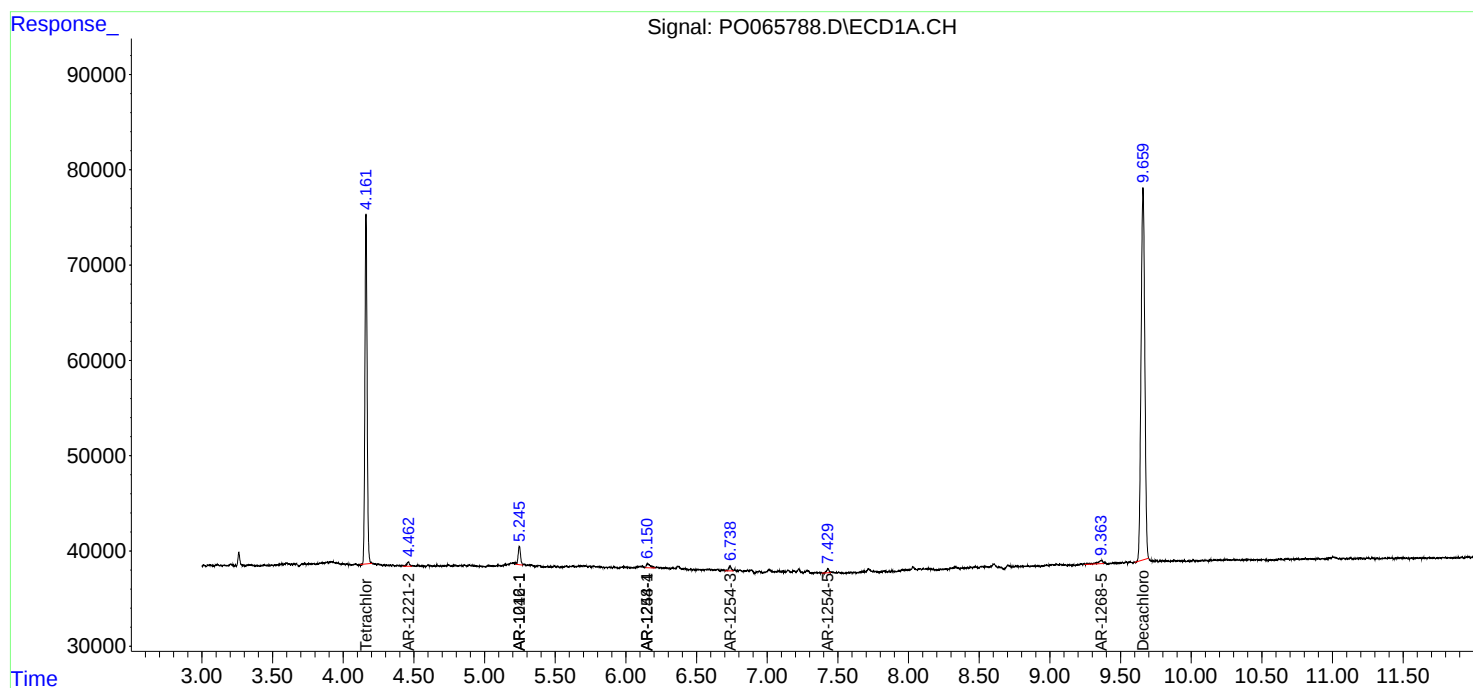


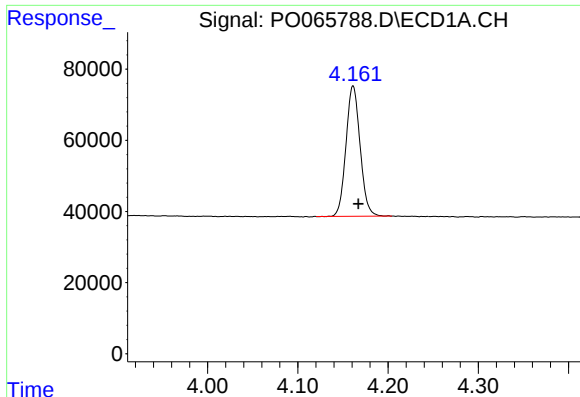

#1 Tetrachloro-m-xylene


R.T.: 4.161 min
Delta R.T.: -0.006 min
Response: 398792
Conc: 21.84 ng/ml

Instrument :
ECD_O
ClientSampleId :

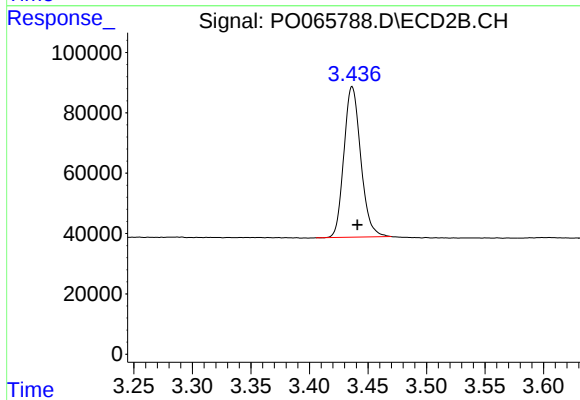


#1 Tetrachloro-m-xylene

R.T.: 3.437 min
Delta R.T.: -0.005 min
Response: 499731
Conc: 22.72 ng/ml

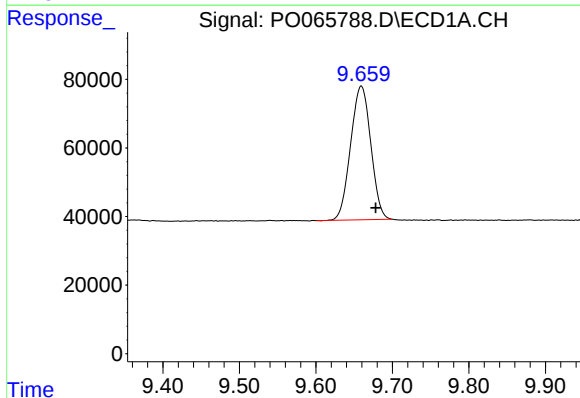


#2 Decachlorobiphenyl

R.T.: 9.659 min
Delta R.T.: -0.019 min
Response: 716312
Conc: 21.14 ng/ml

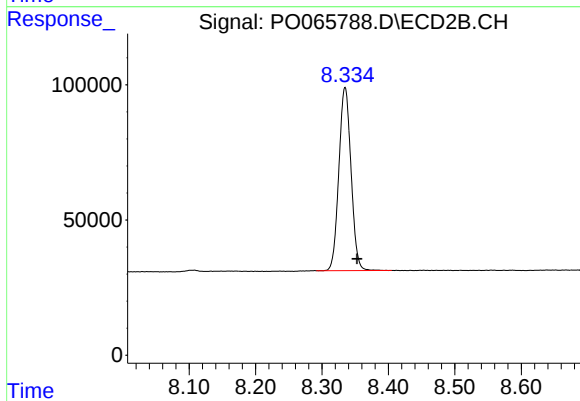

#2 Decachlorobiphenyl


R.T.: 8.335 min
Delta R.T.: -0.018 min
Response: 862558
Conc: 20.80 ng/ml

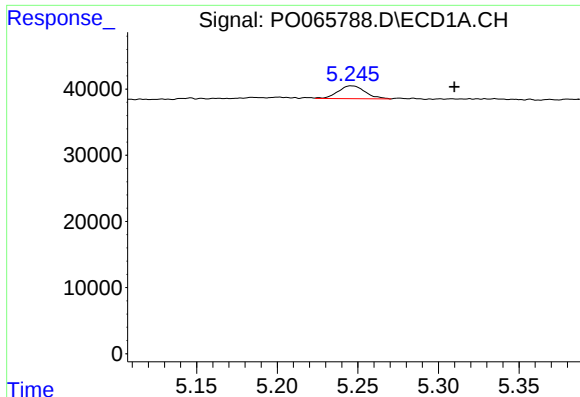

#3 AR-1016-1


R.T.: 5.246 min
Delta R.T.: -0.064 min
Response: 22550
Conc: 25.86 ng/ml

Instrument :
ECD_O
ClientSampleId :

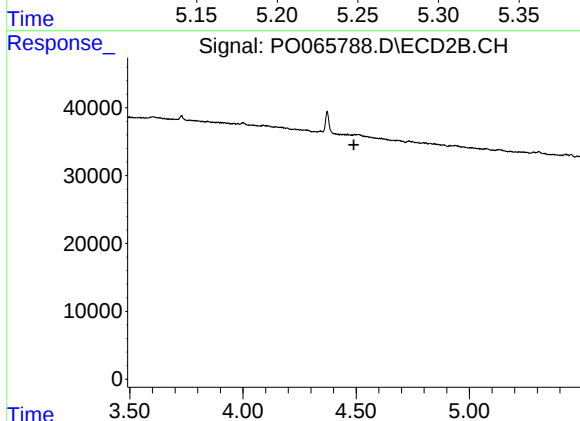


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

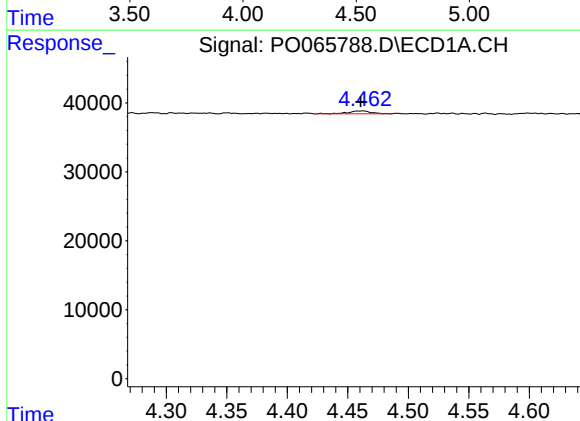


#9 AR-1221-2

R.T.: 4.462 min
Delta R.T.: 0.002 min
Response: 5837
Conc: 37.39 ng/ml

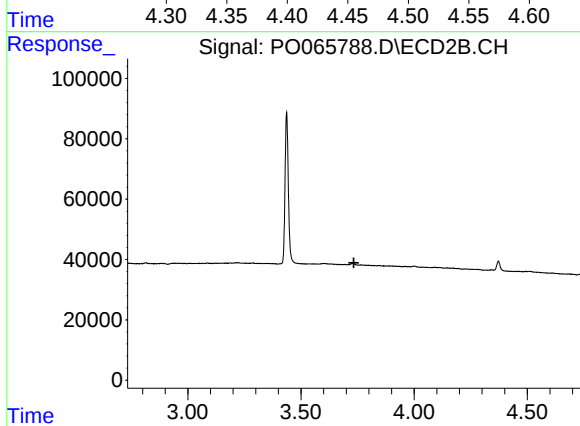

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 3.734 min
Response: 0
Conc: N.D.

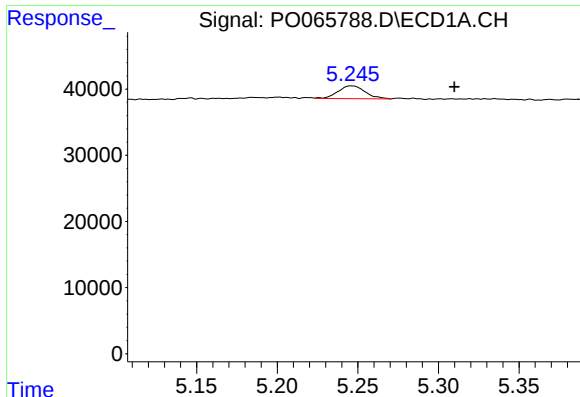

#16 AR-1242-1


R.T.: 5.246 min
Delta R.T.: -0.064 min
Response: 22550
Conc: 38.73 ng/ml

Instrument :
ECD_O
ClientSampleId :

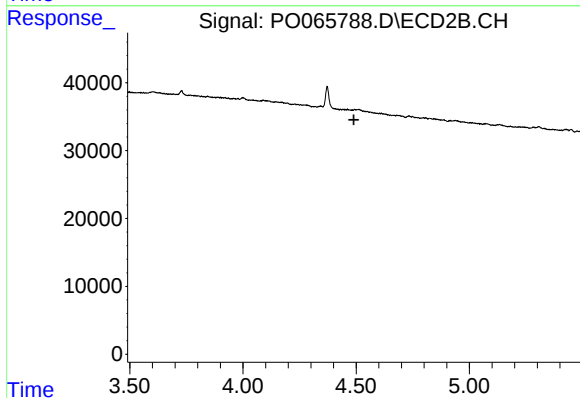


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

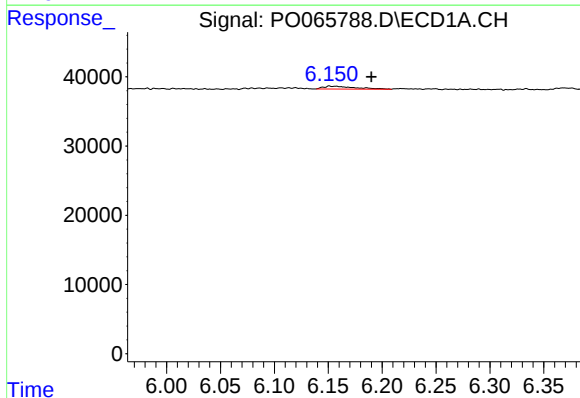


#24 AR-1248-4

R.T.: 6.151 min
Delta R.T.: -0.039 min
Response: 8360
Conc: 8.82 ng/ml

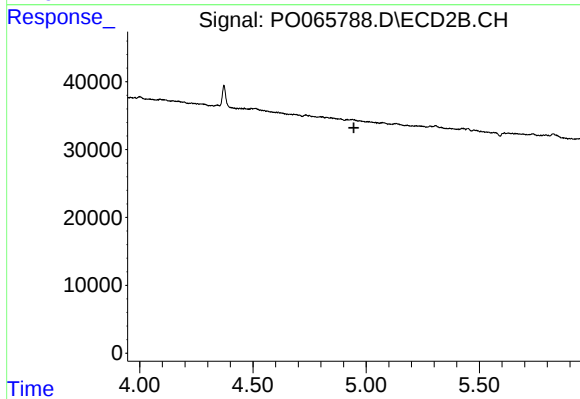

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 4.946 min
Response: 0
Conc: N.D.

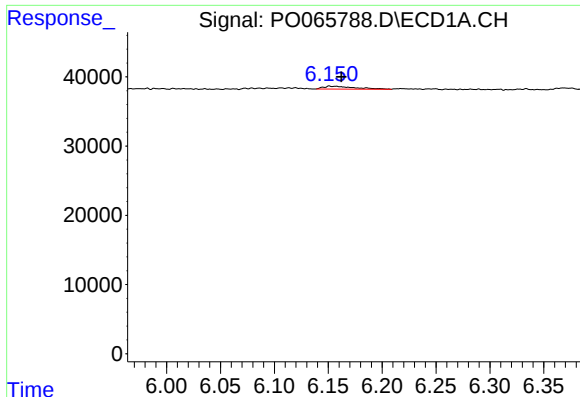

#26 AR-1254-1


R.T.: 6.151 min
Delta R.T.: -0.011 min
Response: 8360
Conc: 9.85 ng/ml

Instrument :
ECD_O
ClientSampleId :

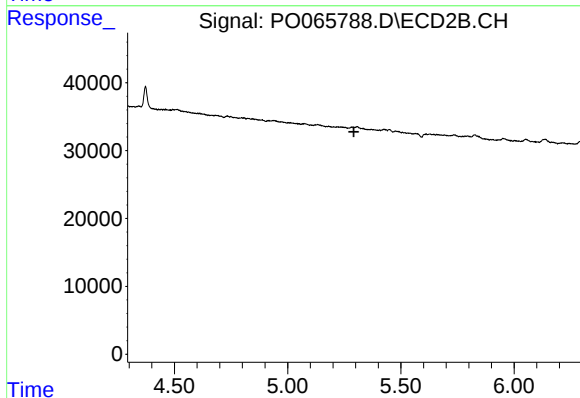


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.292 min
Response: 0
Conc: N.D.

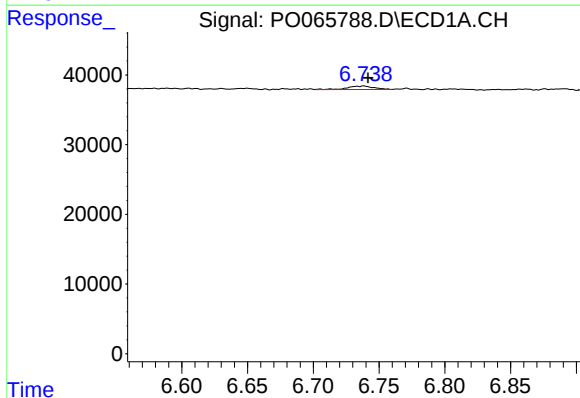


#28 AR-1254-3

R.T.: 6.739 min
Delta R.T.: -0.003 min
Response: 6854
Conc: 4.42 ng/ml

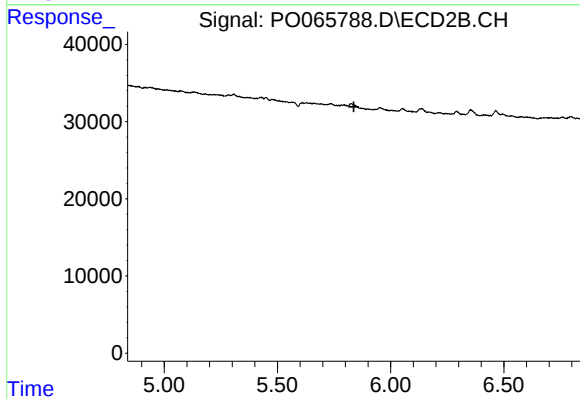

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 5.837 min
Response: 0
Conc: N.D.

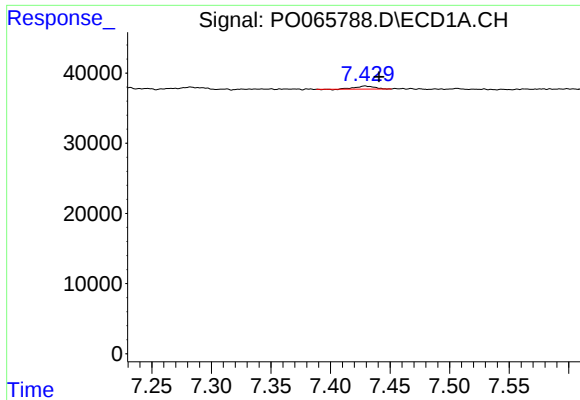

#30 AR-1254-5


R.T.: 7.429 min
Delta R.T.: -0.012 min
Response: 4933
Conc: 3.51 ng/ml

Instrument :
ECD_O
ClientSampleId :

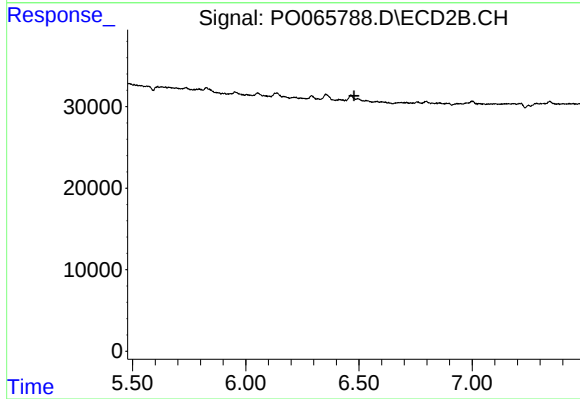


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.478 min
Response: 0
Conc: N.D.

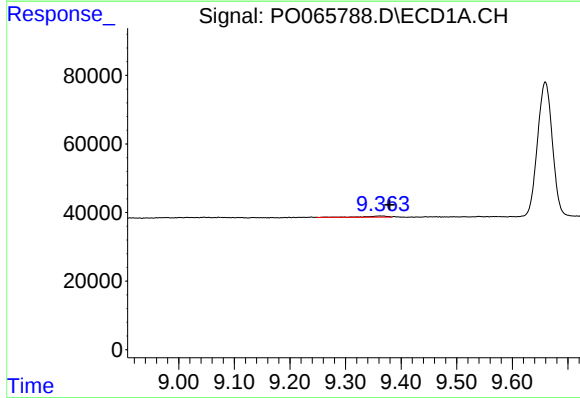

#45 AR-1268-5

R.T.: 9.362 min
Delta R.T.: -0.018 min
Response: 9110
Conc: 0.82 ng/ml

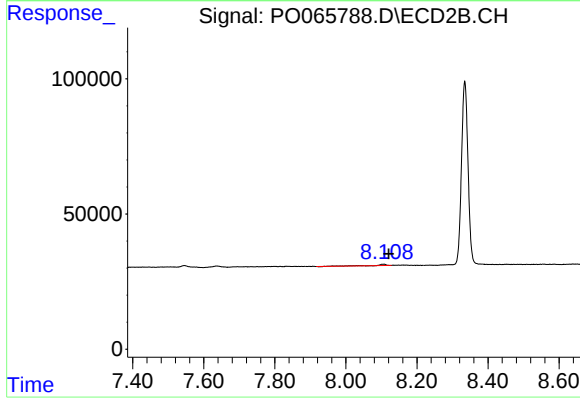

#45 AR-1268-5

R.T.: 8.107 min
Delta R.T.: -0.013 min
Response: 9599
Conc: 0.67 ng/ml