

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012220\
 Data File : P0065803.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2020 23:41
 Operator : DD\AJ
 Sample : L1161-09
 Misc : AR1242 MDL 25 PPB
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT1-2020

Manual Integrations
 APPROVED

Ankita
 1/23/2020 4:15:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 03:20:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.161	3.436	299830	374460	16.420	17.023
2)	SA Decachlor...	9.657	8.334	562198	680577	16.593	16.411
Target Compounds							
16)	L4 AR-1242-1	5.312	4.495	16838	18674	28.922	27.398
17)	L4 AR-1242-2	5.332	4.513	23891	25514	27.940	26.624
18)	L4 AR-1242-3	5.393	4.684	13995	15793	26.689	30.812
19)	L4 AR-1242-4	5.489	4.767	11621	12679	27.431m	24.258
20)	L4 AR-1242-5	6.217	5.281	15681	21729	28.797	29.896m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012220\
Data File : PO065803.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2020 23:41
Operator : DD\AJ
Sample : L1161-09
Misc : AR1242 MDL 25 PPB
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 03:20:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

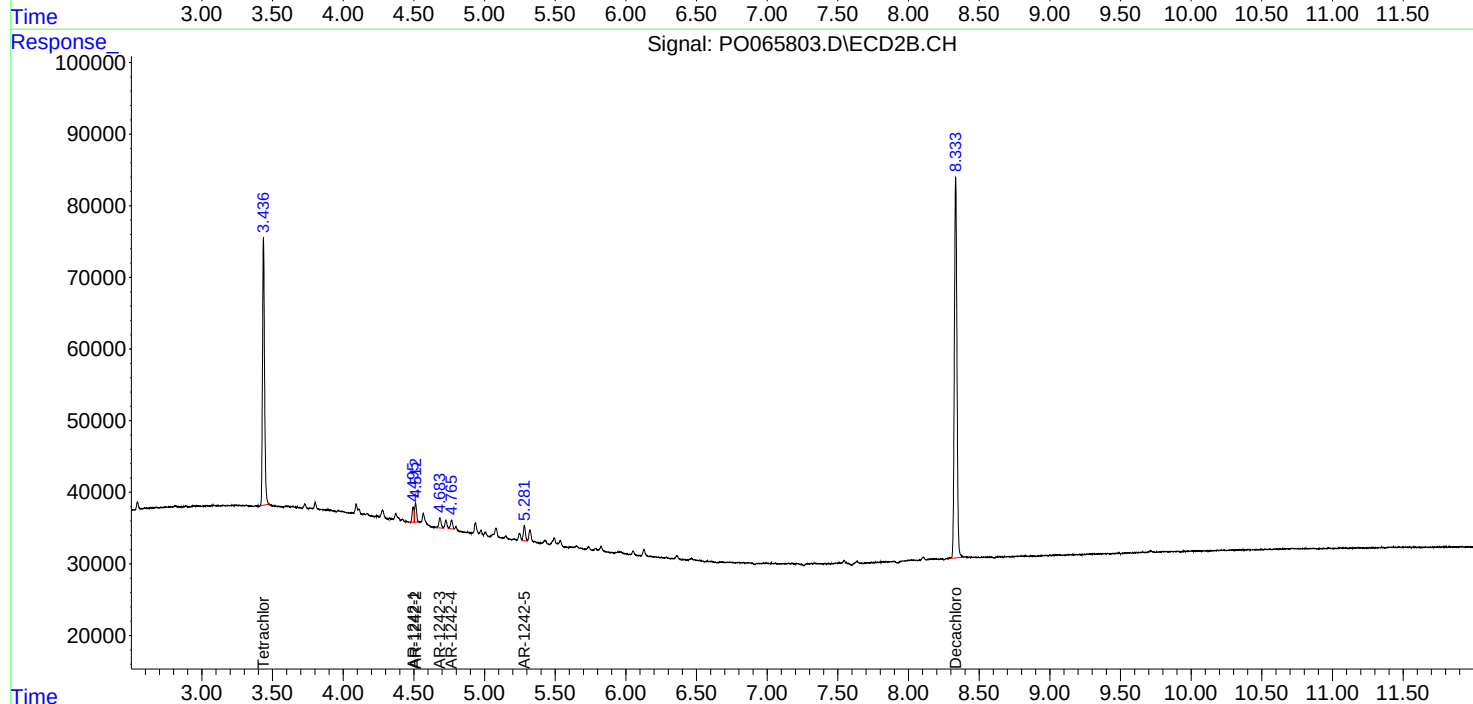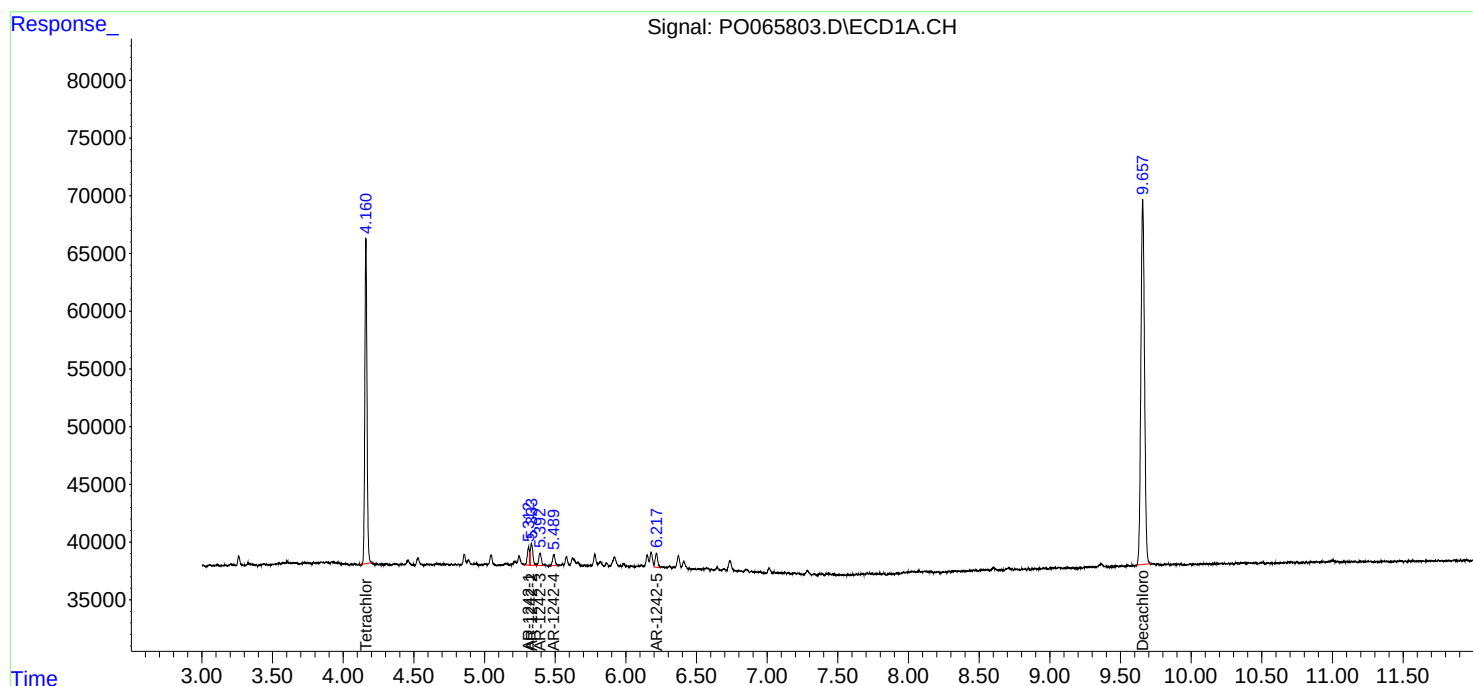

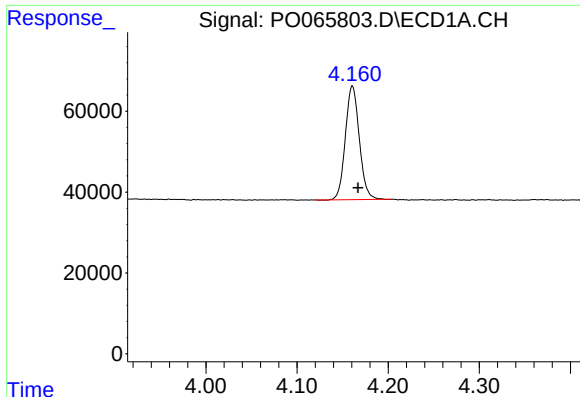


#1 Tetrachloro-m-xylene

R.T.: 4.161 min
Delta R.T.: -0.006 min
Response: 299830
Conc: 16.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:09 PM

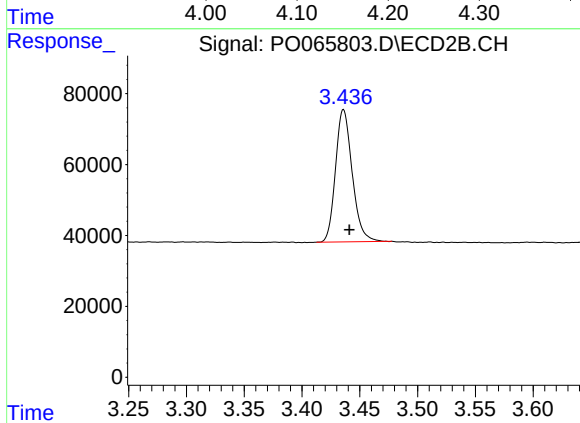


#1 Tetrachloro-m-xylene

R.T.: 3.436 min
Delta R.T.: -0.005 min
Response: 374460
Conc: 17.02 ng/ml

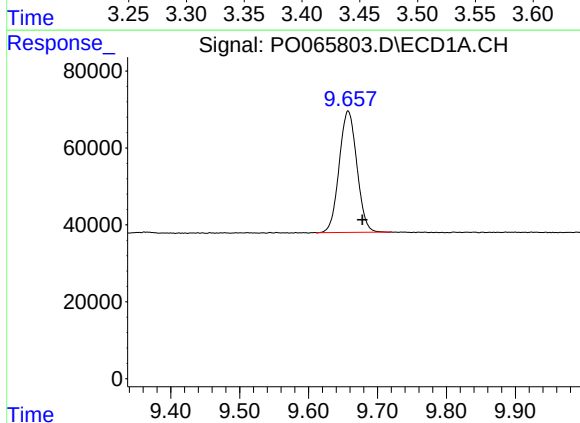


#2 Decachlorobiphenyl

R.T.: 9.657 min
Delta R.T.: -0.021 min
Response: 562198
Conc: 16.59 ng/ml

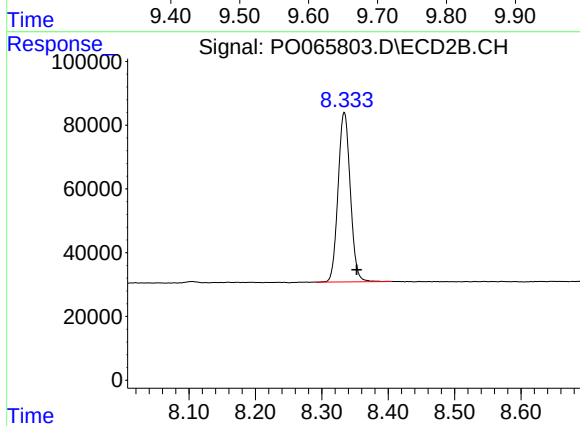

#2 Decachlorobiphenyl

R.T.: 8.334 min
Delta R.T.: -0.019 min
Response: 680577
Conc: 16.41 ng/ml

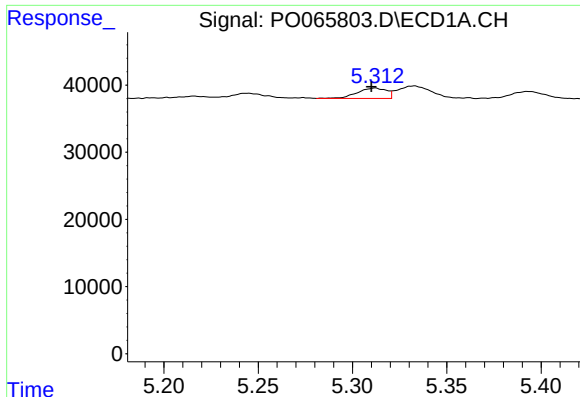


#16 AR-1242-1

R.T.: 5.312 min
Delta R.T.: 0.002 min
Response: 16838
Conc: 28.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:09 PM

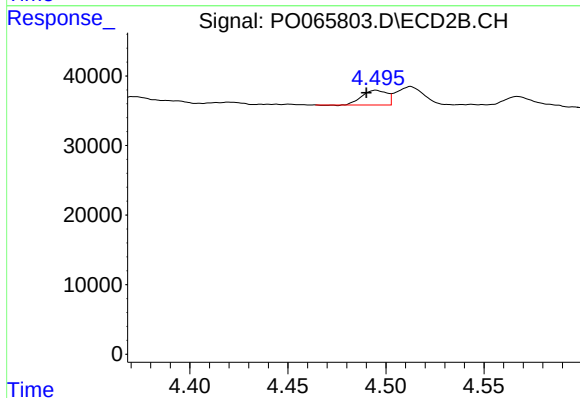


#16 AR-1242-1

R.T.: 4.495 min
Delta R.T.: 0.005 min
Response: 18674
Conc: 27.40 ng/ml

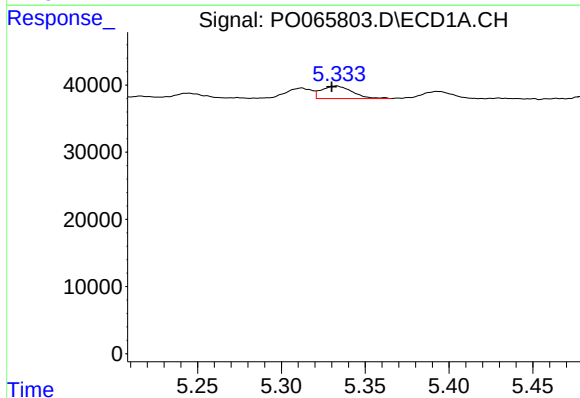


#17 AR-1242-2

R.T.: 5.332 min
Delta R.T.: 0.002 min
Response: 23891
Conc: 27.94 ng/ml

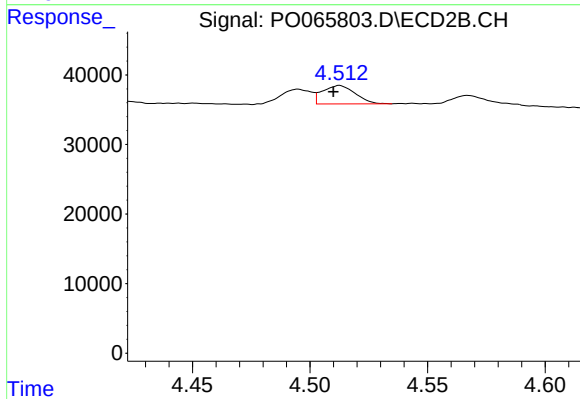

#17 AR-1242-2

R.T.: 4.513 min
Delta R.T.: 0.003 min
Response: 25514
Conc: 26.62 ng/ml

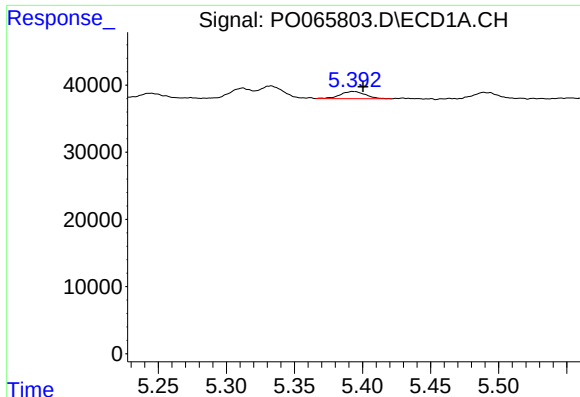


#18 AR-1242-3

R.T.: 5.393 min
Delta R.T.: -0.007 min
Response: 13995
Conc: 26.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:09 PM

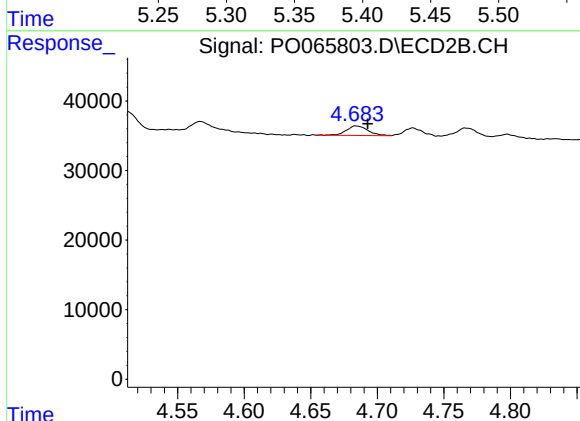


#18 AR-1242-3

R.T.: 4.684 min
Delta R.T.: -0.009 min
Response: 15793
Conc: 30.81 ng/ml

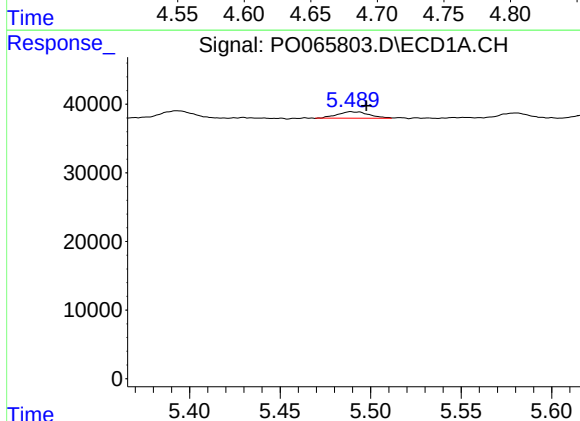


#19 AR-1242-4

R.T.: 5.489 min
Delta R.T.: -0.009 min
Response: 11621
Conc: 27.43 ng/ml m

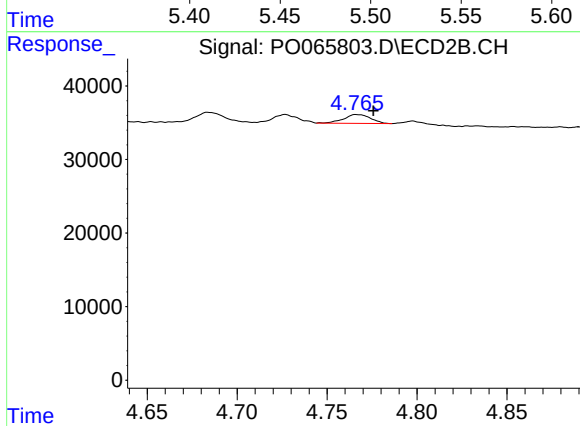

#19 AR-1242-4

R.T.: 4.767 min
Delta R.T.: -0.009 min
Response: 12679
Conc: 24.26 ng/ml

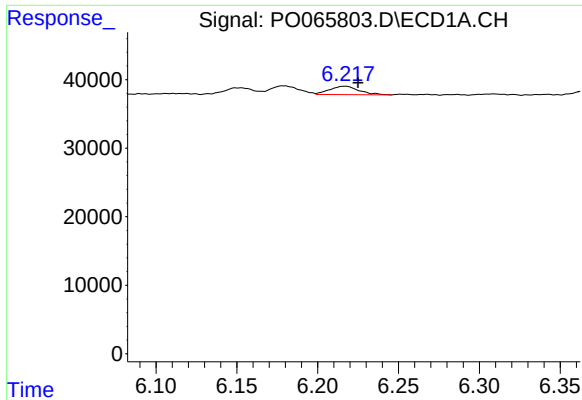


#20 AR-1242-5

R.T.: 6.217 min
Delta R.T.: -0.008 min
Response: 15681
Conc: 28.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020

Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:09 PM

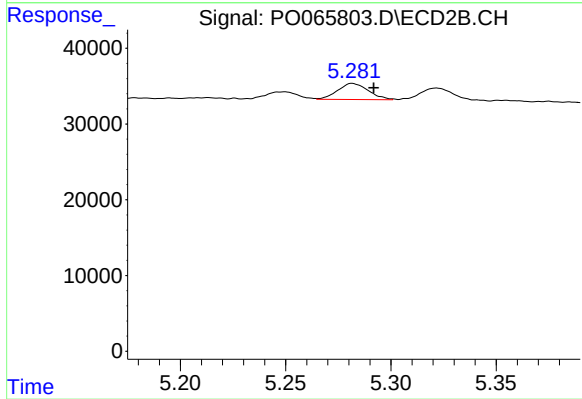

#20 AR-1242-5

R.T.: 5.281 min
Delta R.T.: -0.011 min
Response: 21729
Conc: 29.90 ng/ml m