

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012220\
 Data File : P0065804.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2020 23:57
 Operator : DD\AJ
 Sample : L1161-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT1-2020

Manual Integrations
 APPROVED

Ankita
 1/23/2020 4:15:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 03:23:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.161	3.436	416235	519875	22.794	23.633
2)	SA Decachlor...	9.658	8.335	784644	947114	23.158	22.838
Target Compounds							
21)	L5 AR-1248-1	5.310	4.494	14668	21752	31.523	39.238m
22)	L5 AR-1248-2	5.580	4.727	24882	26958	37.709	35.136
23)	L5 AR-1248-3	5.780	4.768	26144	24031	34.697	30.543
24)	L5 AR-1248-4	6.180	4.936	37555	40033	39.646	41.766
25)	L5 AR-1248-5	6.217	5.322	34249	34733	37.442	34.311

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012220\
Data File : PO065804.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2020 23:57
Operator : DD\AJ
Sample : L1161-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 03:23:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

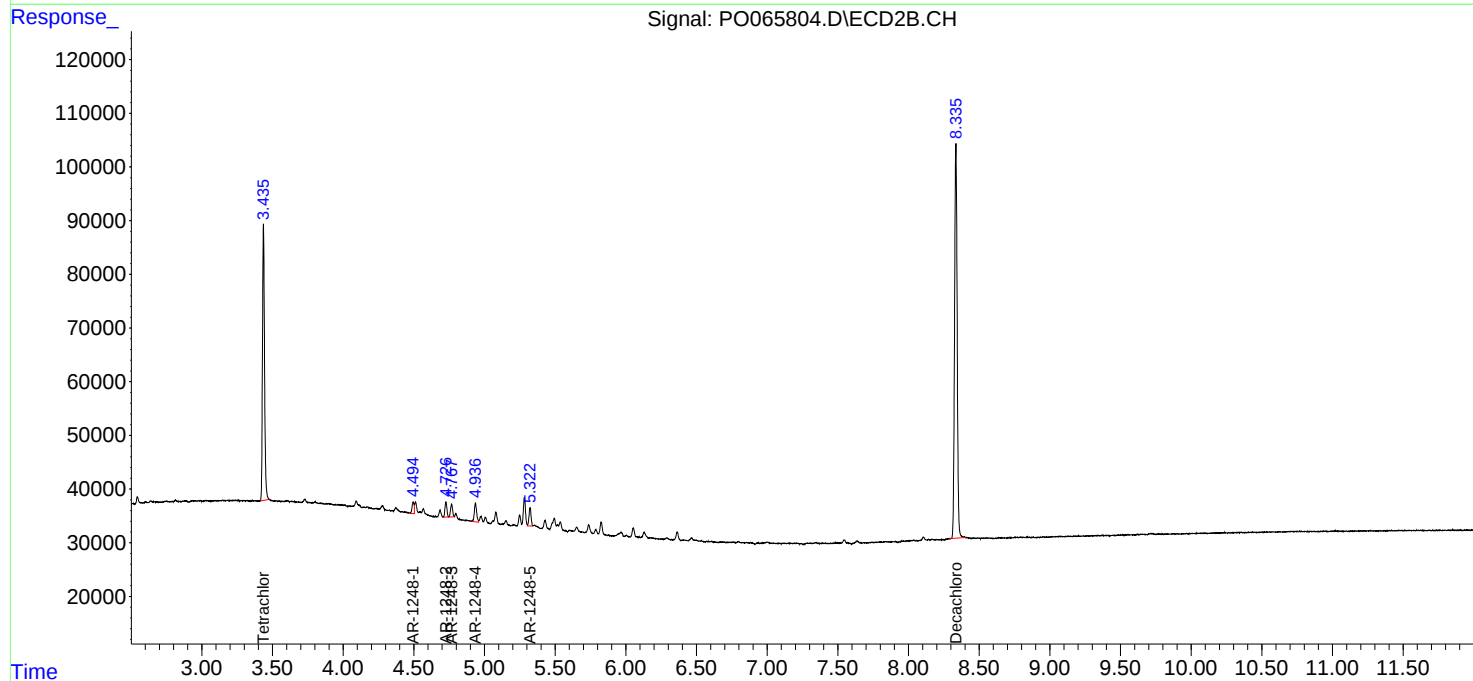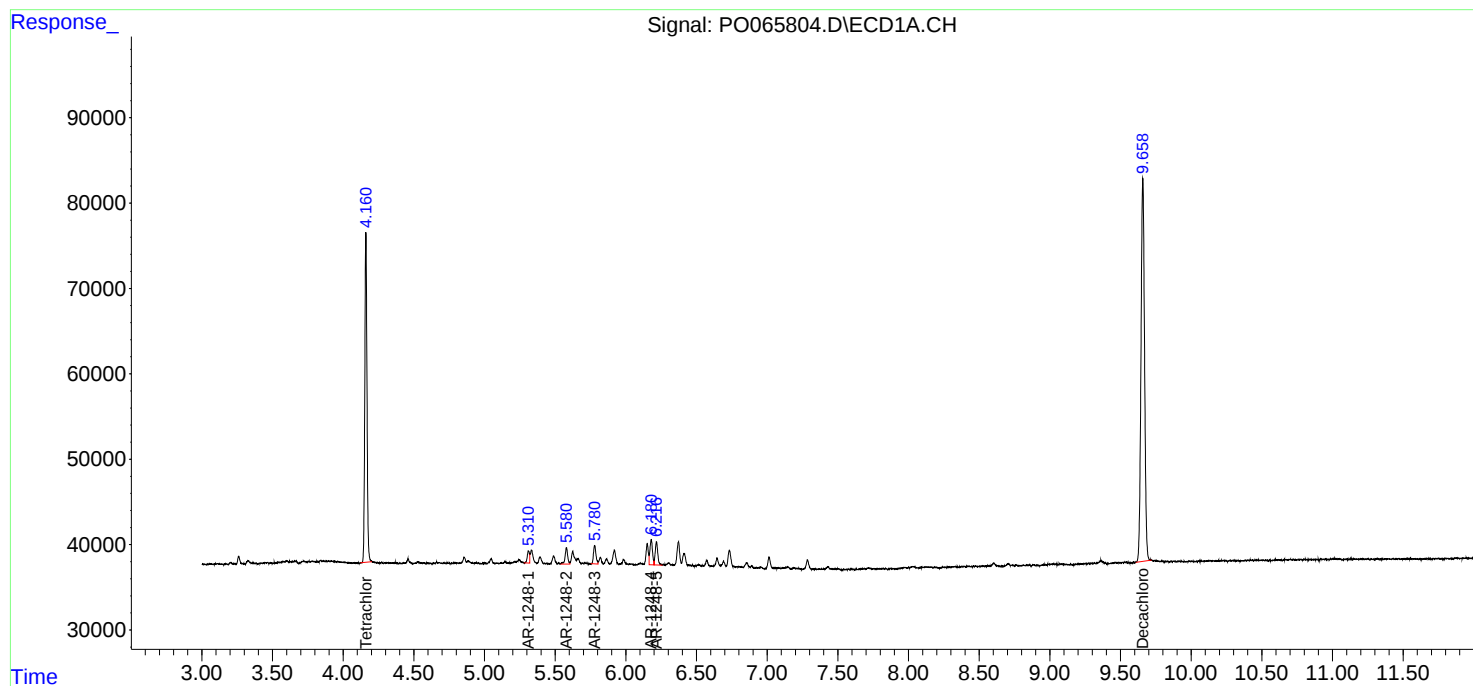

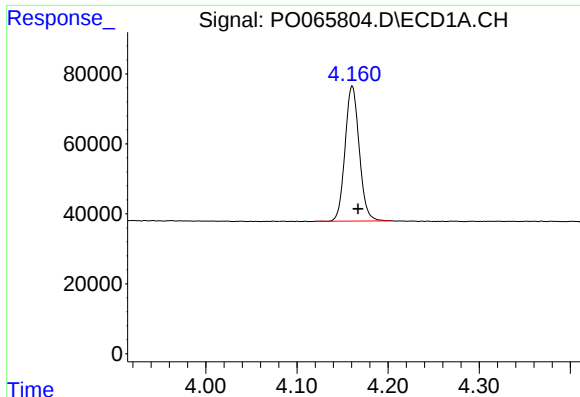


#1 Tetrachloro-m-xylene

R.T.: 4.161 min
Delta R.T.: -0.006 min
Response: 416235
Conc: 22.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:10 PM

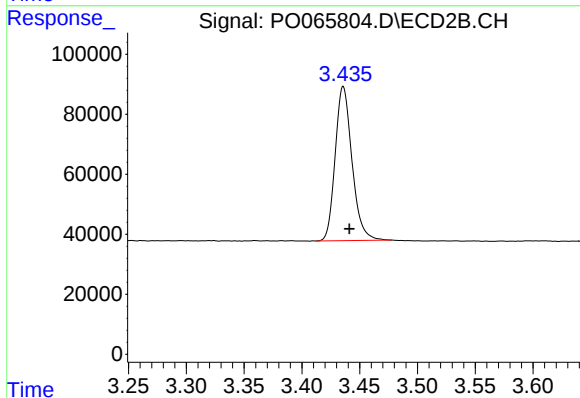


#1 Tetrachloro-m-xylene

R.T.: 3.436 min
Delta R.T.: -0.005 min
Response: 519875
Conc: 23.63 ng/ml

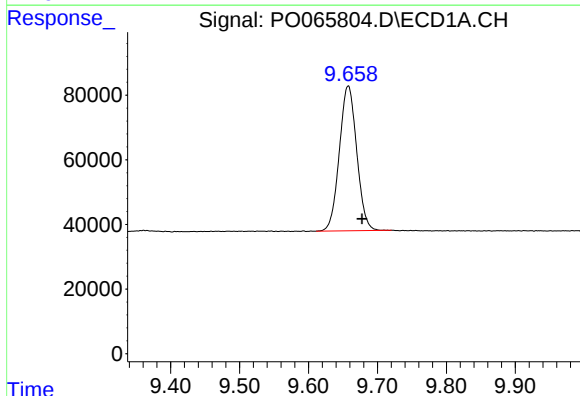


#2 Decachlorobiphenyl

R.T.: 9.658 min
Delta R.T.: -0.020 min
Response: 784644
Conc: 23.16 ng/ml

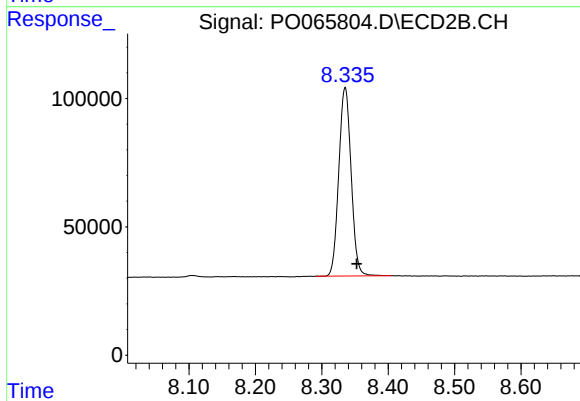

#2 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: -0.017 min
Response: 947114
Conc: 22.84 ng/ml

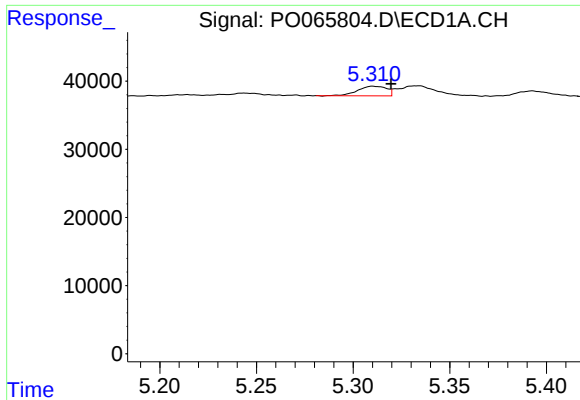


#21 AR-1248-1

R.T.: 5.310 min
Delta R.T.: -0.009 min
Response: 14668
Conc: 31.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:10 PM

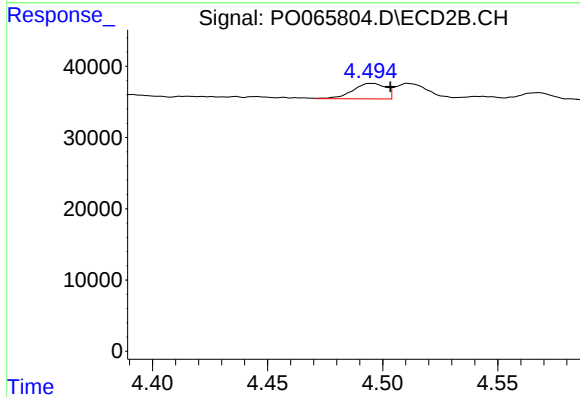


#21 AR-1248-1

R.T.: 4.494 min
Delta R.T.: -0.010 min
Response: 21752
Conc: 39.24 ng/ml m

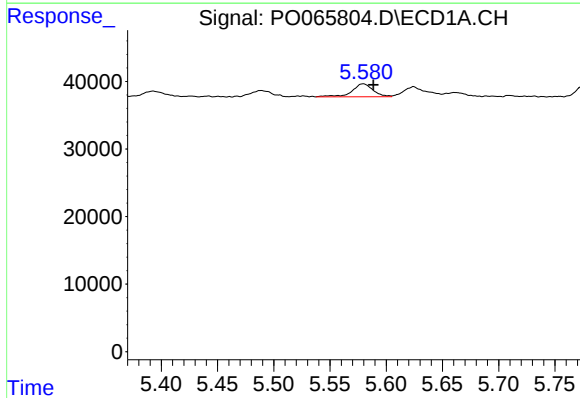


#22 AR-1248-2

R.T.: 5.580 min
Delta R.T.: -0.009 min
Response: 24882
Conc: 37.71 ng/ml

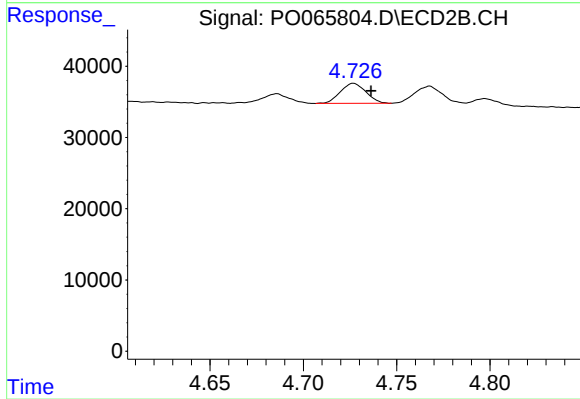

#22 AR-1248-2

R.T.: 4.727 min
Delta R.T.: -0.009 min
Response: 26958
Conc: 35.14 ng/ml

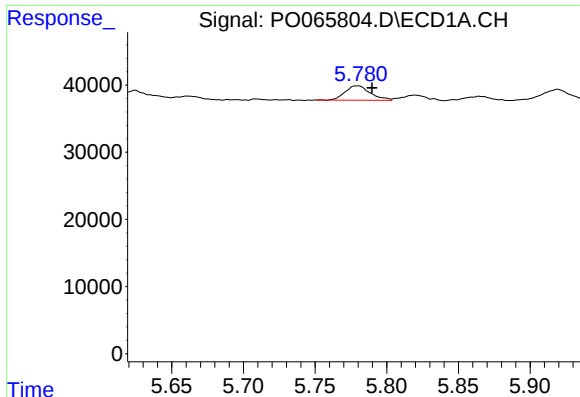


#23 AR-1248-3

R.T.: 5.780 min
Delta R.T.: -0.010 min
Response: 26144
Conc: 34.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:10 PM

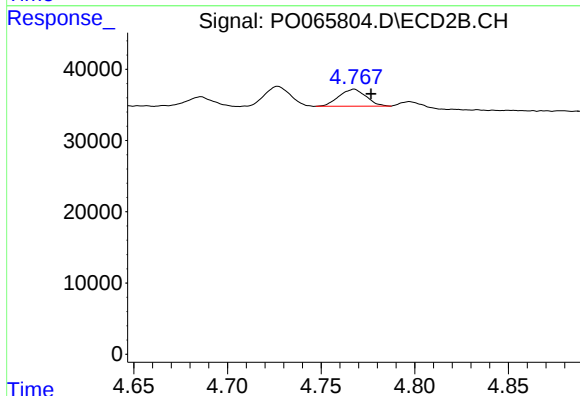


#23 AR-1248-3

R.T.: 4.768 min
Delta R.T.: -0.009 min
Response: 24031
Conc: 30.54 ng/ml

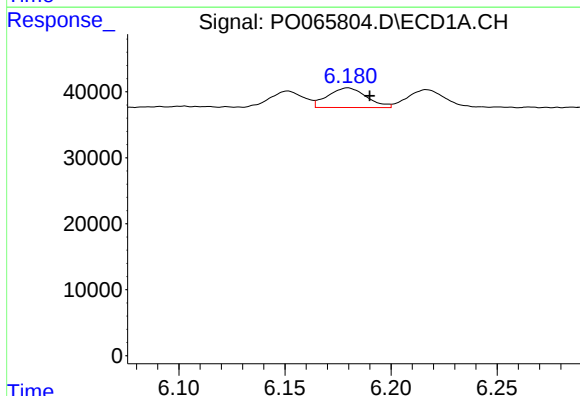


#24 AR-1248-4

R.T.: 6.180 min
Delta R.T.: -0.010 min
Response: 37555
Conc: 39.65 ng/ml

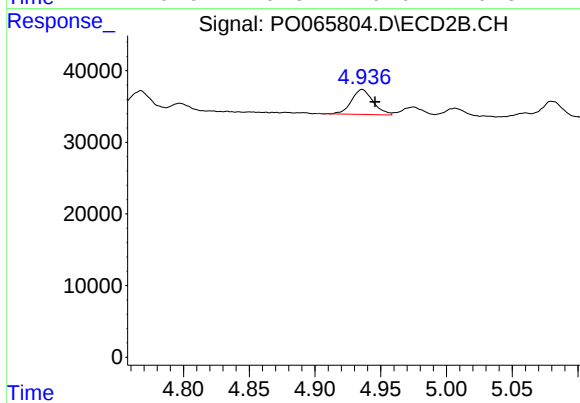

#24 AR-1248-4

R.T.: 4.936 min
Delta R.T.: -0.010 min
Response: 40033
Conc: 41.77 ng/ml

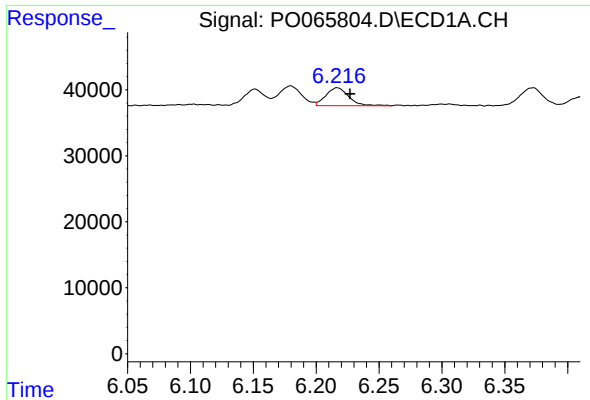


#25 AR-1248-5

R.T.: 6.217 min
Delta R.T.: -0.010 min
Response: 34249
Conc: 37.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020

Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:10 PM

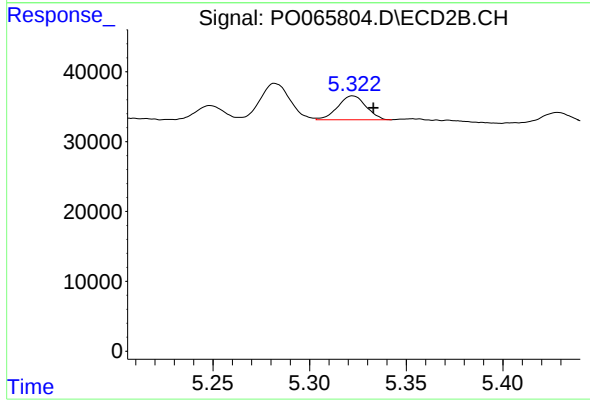

#25 AR-1248-5

R.T.: 5.322 min
Delta R.T.: -0.011 min
Response: 34733
Conc: 34.31 ng/ml