

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0012220\
 Data File : P0065805.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jan 2020 00:14
 Operator : DD\AJ
 Sample : L1161-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MDL-WATER-03-QT1-2020

Manual Integrations
 APPROVED

Ankita
 1/23/2020 4:15:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 03:25:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.161	3.436	290227	362482	15.894	16.478
2)	SA Decachlor...	9.658	8.333	523627	633191	15.454	15.269
Target Compounds							
26)	L6 AR-1254-1	6.152	5.282	27161	43391	32.017	29.951
27)	L6 AR-1254-2	6.369	5.427	44830	41494	32.622	31.370m
28)	L6 AR-1254-3	6.731	5.825	49781	65571	32.119m	29.097
29)	L6 AR-1254-4	7.015	6.052	39142	39863	30.707	26.442
30)	L6 AR-1254-5	7.430	6.465	36378	62951	25.904	28.281

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012220\
Data File : P0065805.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jan 2020 00:14
Operator : DD\AJ
Sample : L1161-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 03:25:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

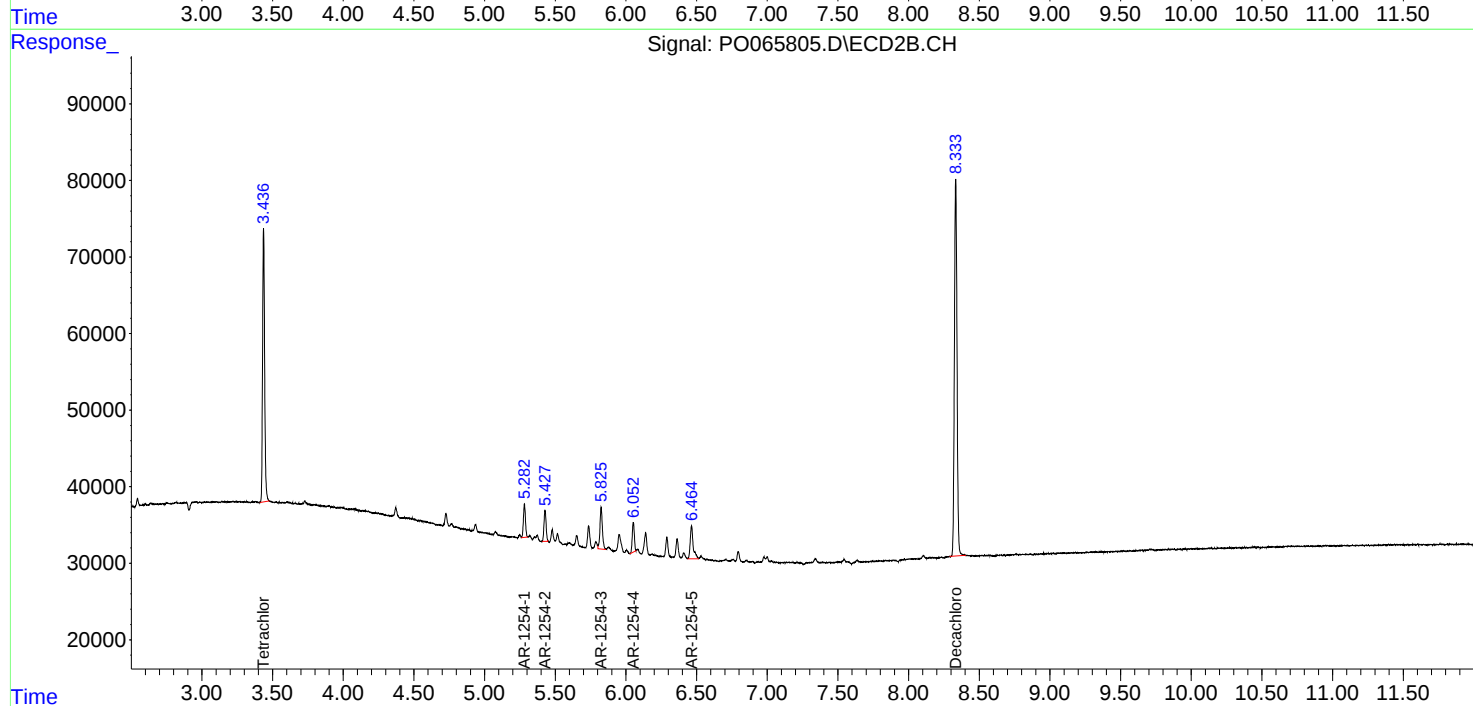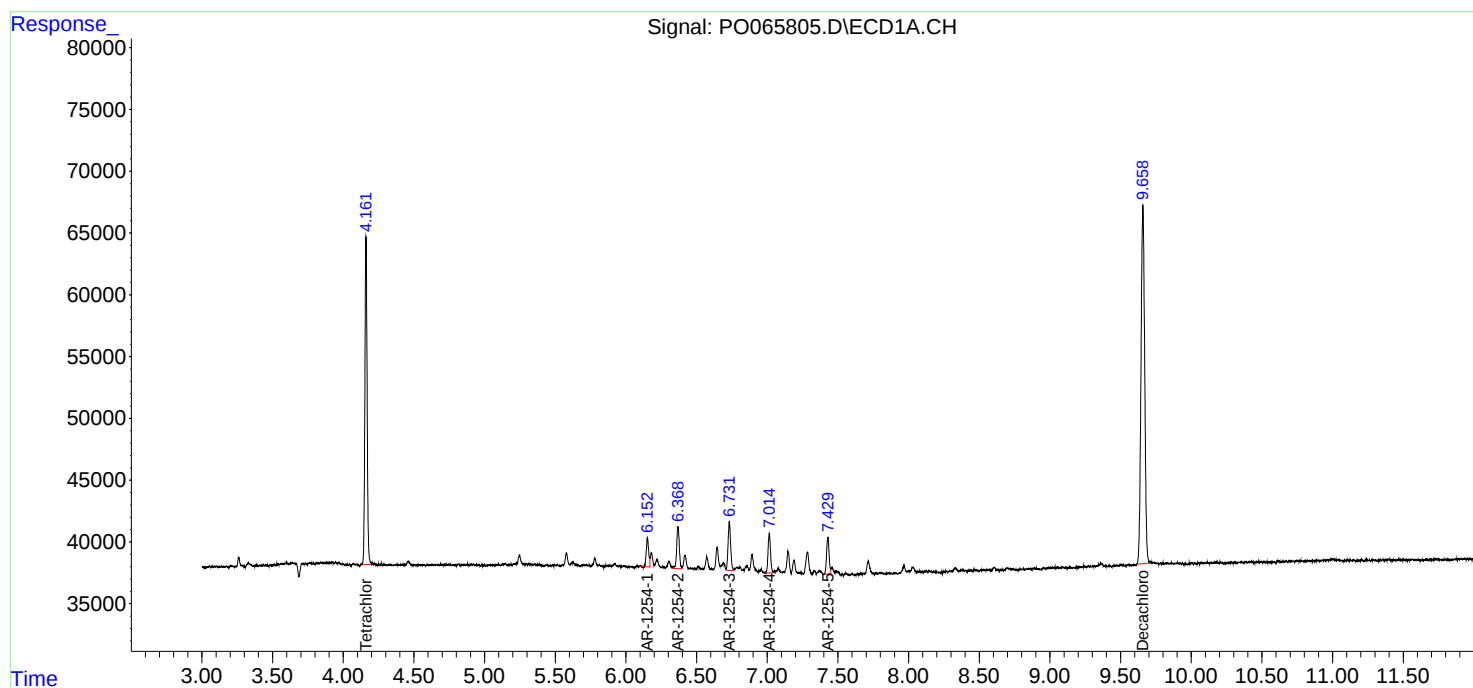

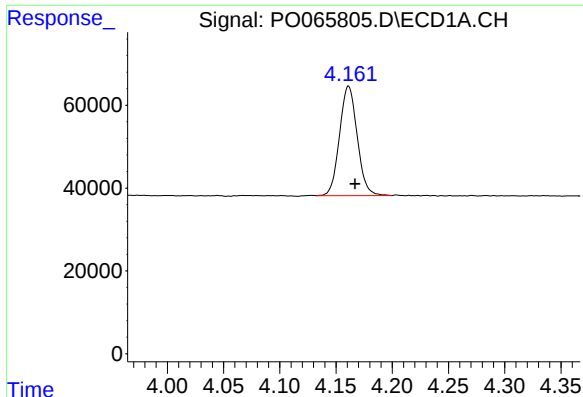


#1 Tetrachloro-m-xylene

R.T.: 4.161 min
Delta R.T.: -0.006 min
Response: 290227
Conc: 15.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:12 PM

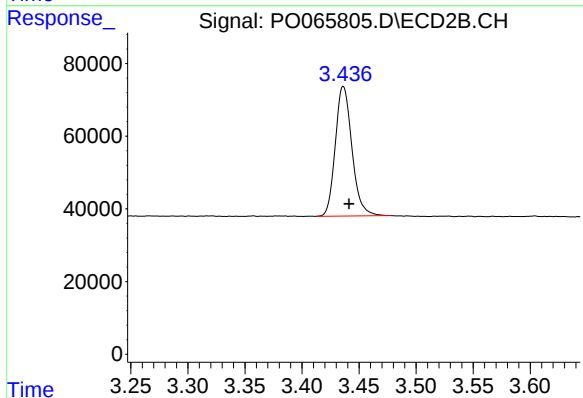


#1 Tetrachloro-m-xylene

R.T.: 3.436 min
Delta R.T.: -0.005 min
Response: 362482
Conc: 16.48 ng/ml

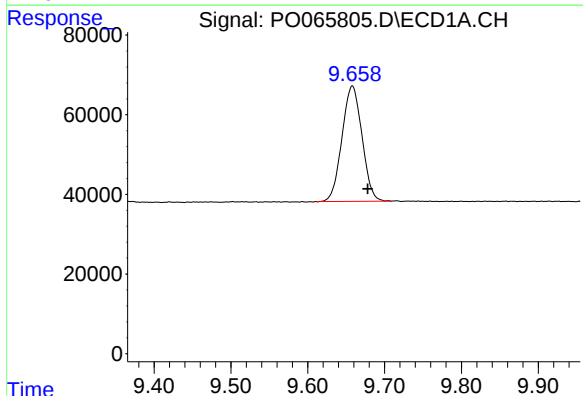


#2 Decachlorobiphenyl

R.T.: 9.658 min
Delta R.T.: -0.020 min
Response: 523627
Conc: 15.45 ng/ml

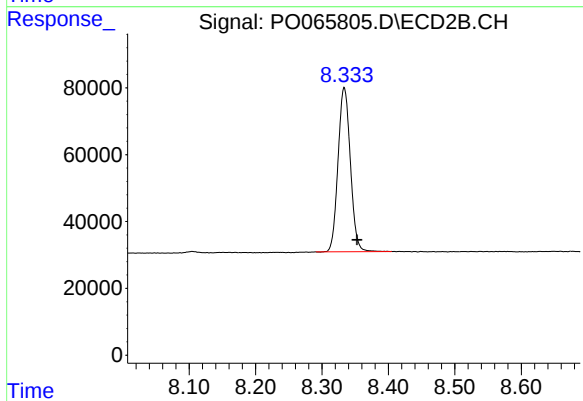

#2 Decachlorobiphenyl

R.T.: 8.333 min
Delta R.T.: -0.019 min
Response: 633191
Conc: 15.27 ng/ml

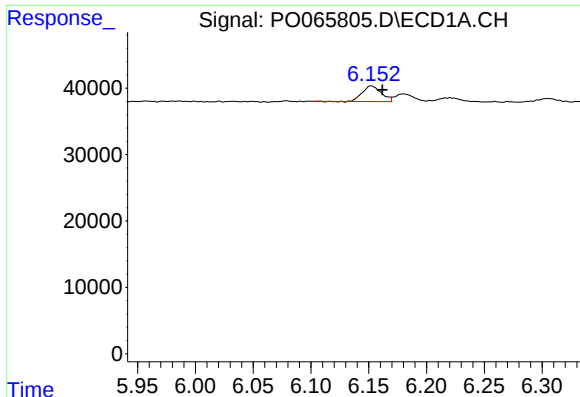


#26 AR-1254-1

R.T.: 6.152 min
Delta R.T.: -0.010 min
Response: 27161
Conc: 32.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:12 PM

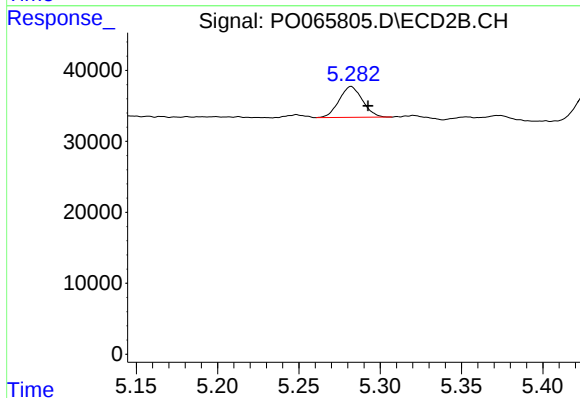


#26 AR-1254-1

R.T.: 5.282 min
Delta R.T.: -0.010 min
Response: 43391
Conc: 29.95 ng/ml

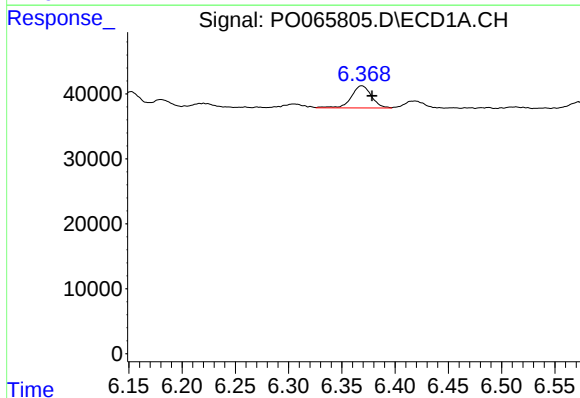


#27 AR-1254-2

R.T.: 6.369 min
Delta R.T.: -0.010 min
Response: 44830
Conc: 32.62 ng/ml

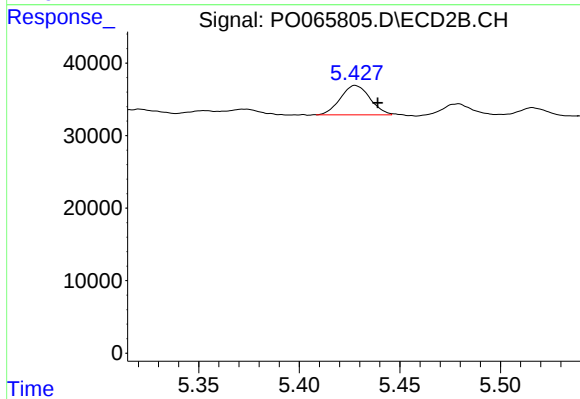

#27 AR-1254-2

R.T.: 5.427 min
Delta R.T.: -0.012 min
Response: 41494
Conc: 31.37 ng/ml m

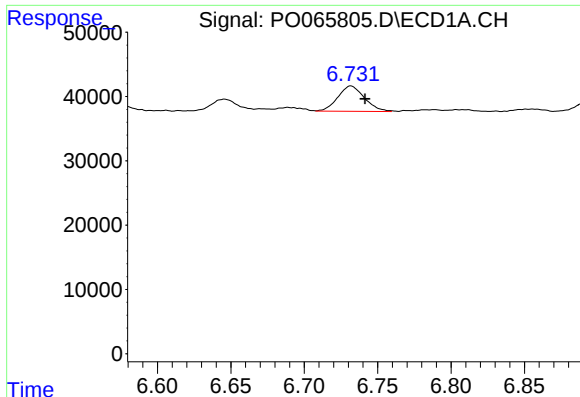


#28 AR-1254-3

R.T.: 6.731 min
Delta R.T.: -0.010 min
Response: 49781
Conc: 32.12 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:12 PM

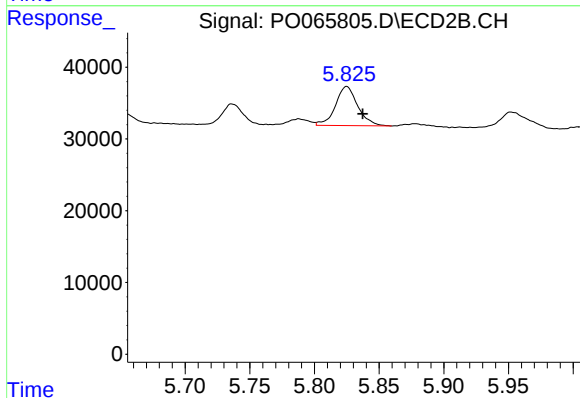


#28 AR-1254-3

R.T.: 5.825 min
Delta R.T.: -0.012 min
Response: 65571
Conc: 29.10 ng/ml

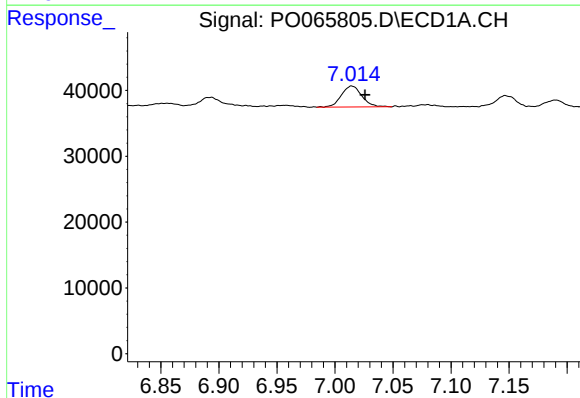


#29 AR-1254-4

R.T.: 7.015 min
Delta R.T.: -0.011 min
Response: 39142
Conc: 30.71 ng/ml

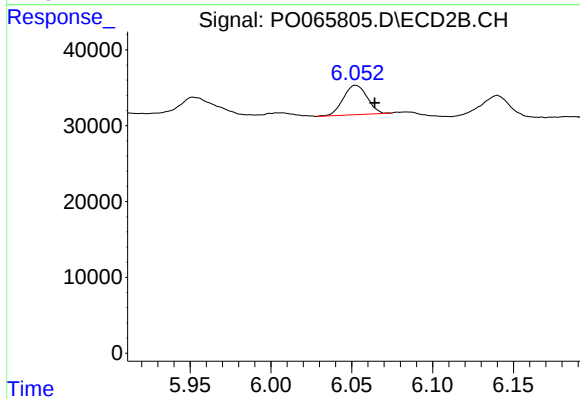

#29 AR-1254-4

R.T.: 6.052 min
Delta R.T.: -0.012 min
Response: 39863
Conc: 26.44 ng/ml

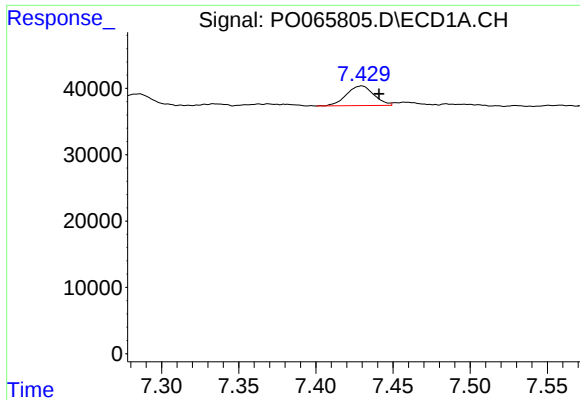


#30 AR-1254-5

R.T.: 7.430 min
Delta R.T.: -0.011 min
Response: 36378
Conc: 25.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020

Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:12 PM

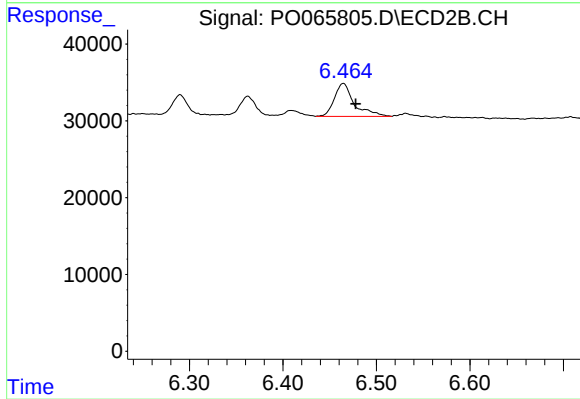

#30 AR-1254-5

R.T.: 6.465 min
Delta R.T.: -0.013 min
Response: 62951
Conc: 28.28 ng/ml