

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0012220\
 Data File : P0065835.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jan 2020 11:57
 Operator : DD\AJ
 Sample : L1213-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 TP-2

Manual Integrations
 APPROVED

Ankita
 1/23/2020 4:15:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 12:11:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.149	3.427	578031	682047	31.655m	31.006m
2) SA Decachlor...	9.643	8.324	581100	642699	17.150	15.498
Target Compounds						
31) L7 AR-1260-1	6.881	5.944	37839	60428	27.435m	32.097
32) L7 AR-1260-2	7.133	6.130	123831	120047	70.578m	49.412 #
33) L7 AR-1260-3	7.493	6.281	36719	63404	25.979	29.292
34) L7 AR-1260-4	7.713	6.747	50670	32608	29.019	16.253m#
35) L7 AR-1260-5	8.022	6.991	64362	74339	19.192	15.017

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012220\
Data File : P0065835.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jan 2020 11:57
Operator : DD\AJ
Sample : L1213-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TP-2


Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 12:11:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

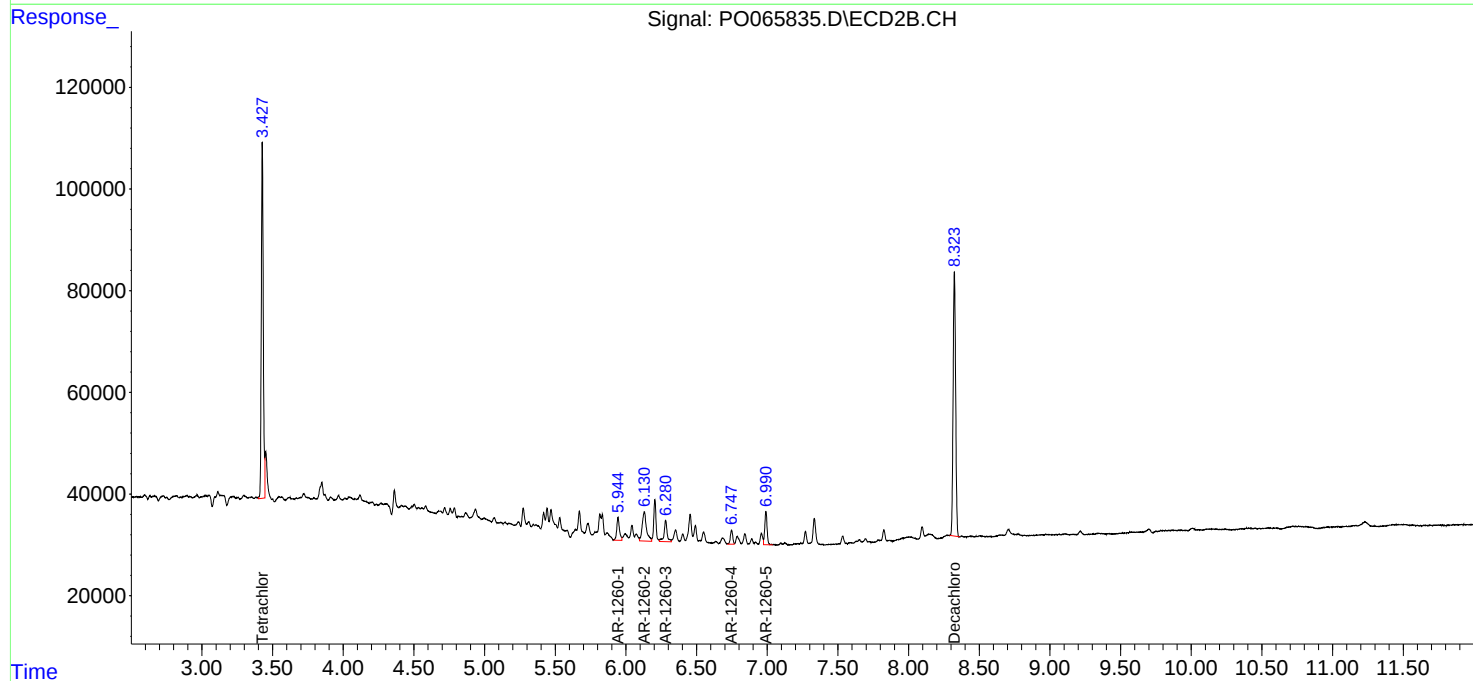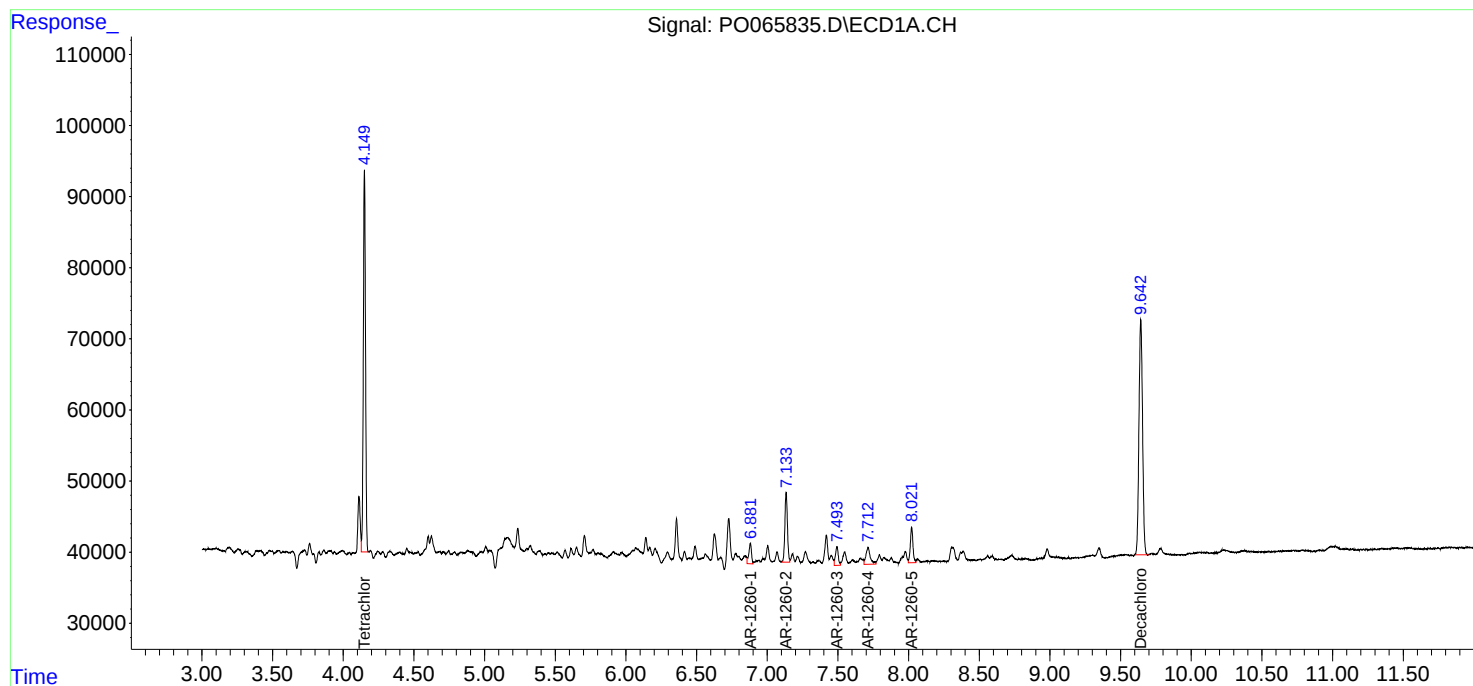

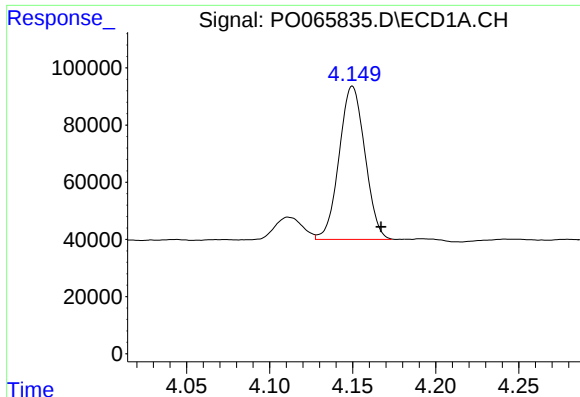


#1 Tetrachloro-m-xylene

R.T.: 4.149 min
Delta R.T.: -0.018 min
Response: 578031
Conc: 31.65 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:51 PM

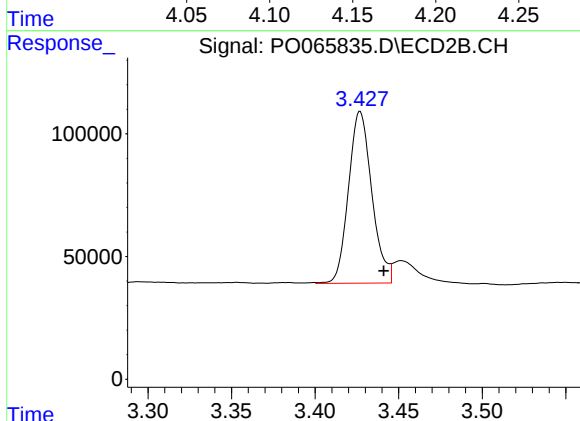


#1 Tetrachloro-m-xylene

R.T.: 3.427 min
Delta R.T.: -0.015 min
Response: 682047
Conc: 31.01 ng/ml m

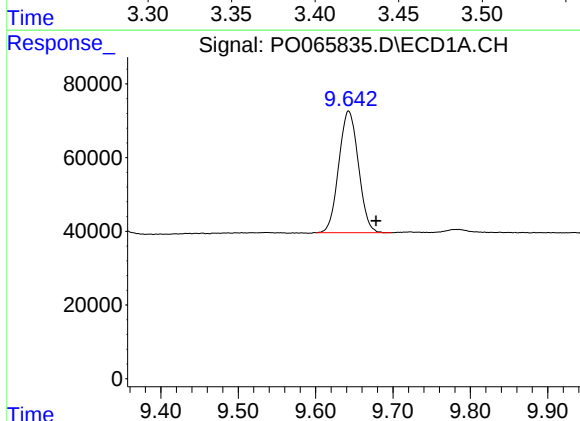


#2 Decachlorobiphenyl

R.T.: 9.643 min
Delta R.T.: -0.035 min
Response: 581100
Conc: 17.15 ng/ml

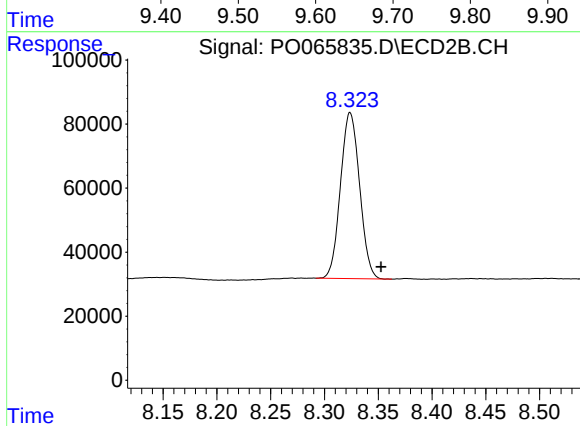

#2 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.029 min
Response: 642699
Conc: 15.50 ng/ml

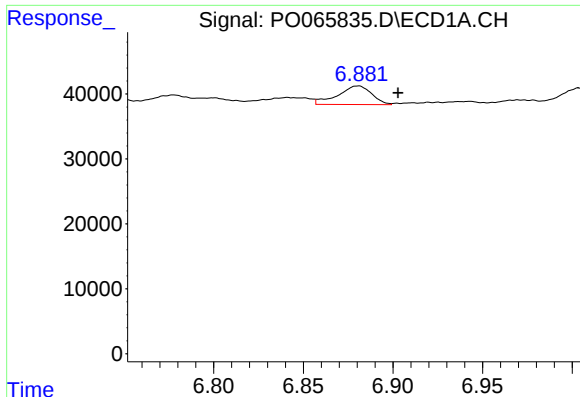


#31 AR-1260-1

R.T.: 6.881 min
Delta R.T.: -0.022 min
Response: 37839
Conc: 27.43 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:51 PM

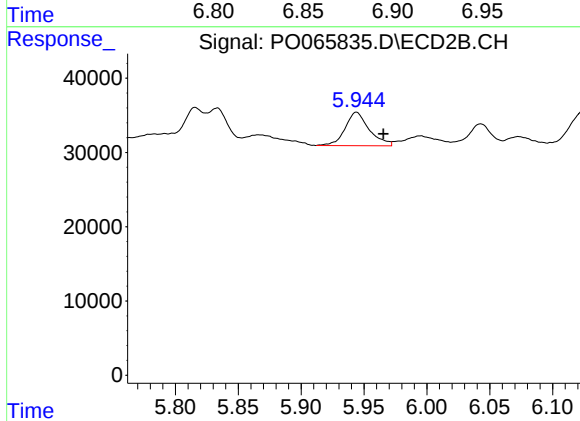


#31 AR-1260-1

R.T.: 5.944 min
Delta R.T.: -0.021 min
Response: 60428
Conc: 32.10 ng/ml

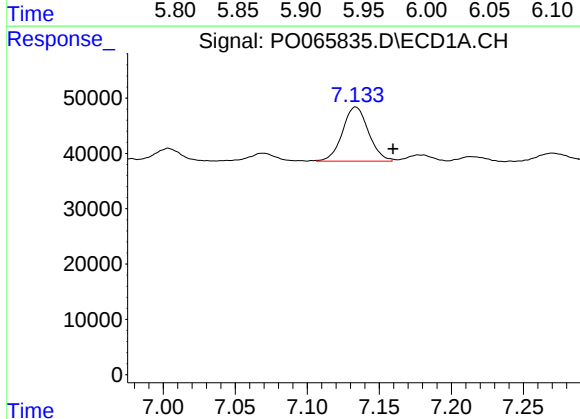


#32 AR-1260-2

R.T.: 7.133 min
Delta R.T.: -0.026 min
Response: 123831
Conc: 70.58 ng/ml m

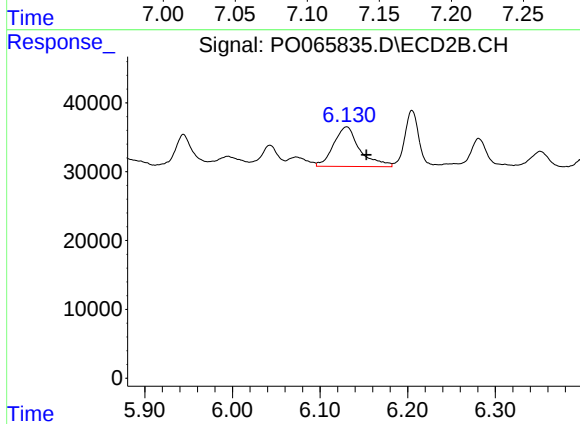

#32 AR-1260-2

R.T.: 6.130 min
Delta R.T.: -0.023 min
Response: 120047
Conc: 49.41 ng/ml

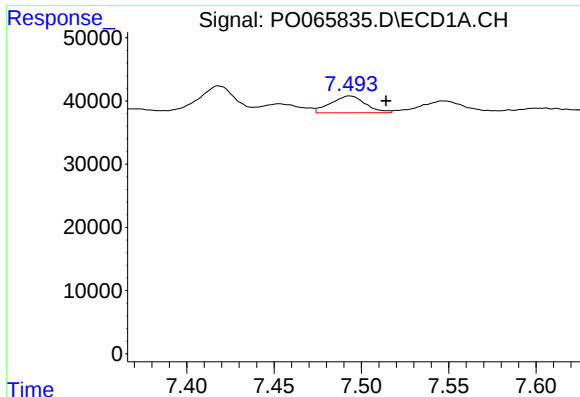


#33 AR-1260-3

R.T.: 7.493 min
Delta R.T.: -0.021 min
Response: 36719
Conc: 25.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2


Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:51 PM

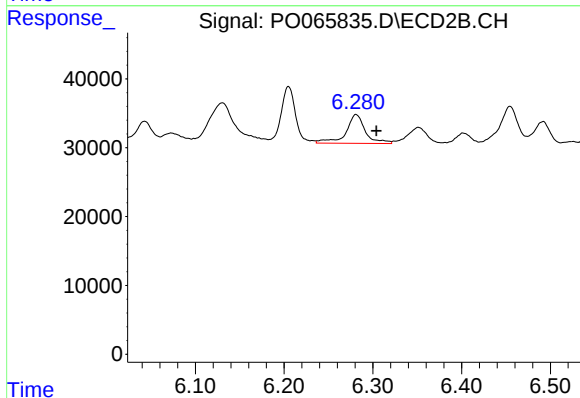


#33 AR-1260-3

R.T.: 6.281 min
Delta R.T.: -0.023 min
Response: 63404
Conc: 29.29 ng/ml

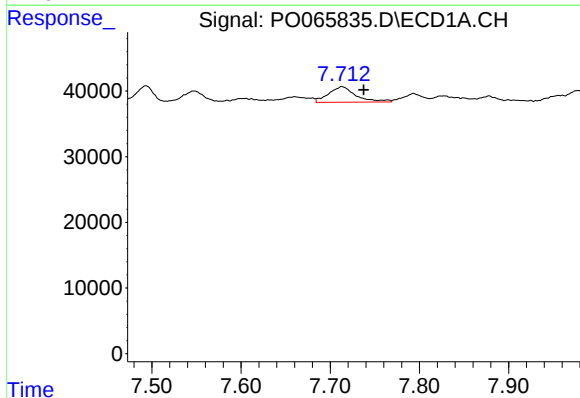


#34 AR-1260-4

R.T.: 7.713 min
Delta R.T.: -0.024 min
Response: 50670
Conc: 29.02 ng/ml

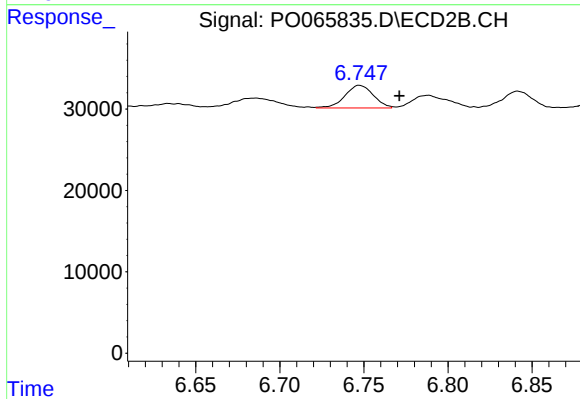

#34 AR-1260-4

R.T.: 6.747 min
Delta R.T.: -0.024 min
Response: 32608
Conc: 16.25 ng/ml m

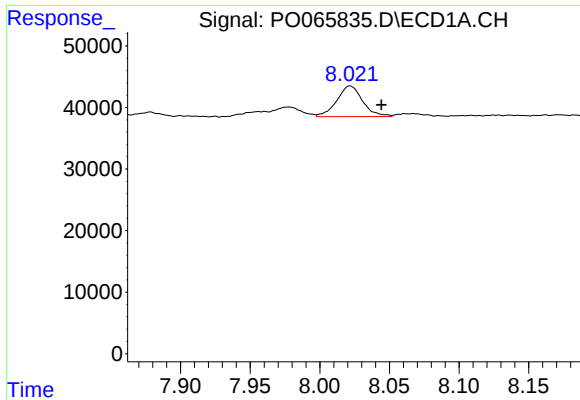


#35 AR-1260-5

R.T.: 8.022 min
Delta R.T.: -0.022 min
Response: 64362
Conc: 19.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2

Manual Integrations
APPROVED

Ankita
1/23/2020 4:15:51 PM

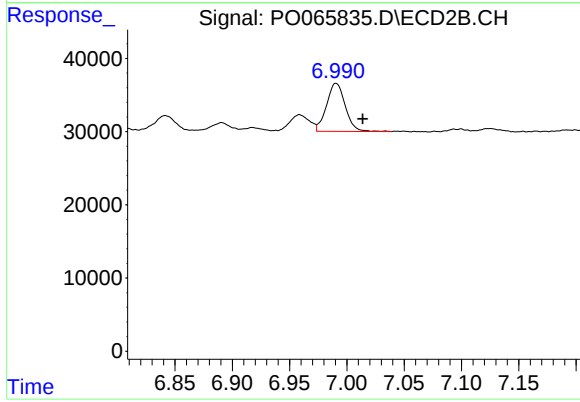

#35 AR-1260-5

R.T.: 6.991 min
Delta R.T.: -0.023 min
Response: 74339
Conc: 15.02 ng/ml