

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0012220\
 Data File : P0065841.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jan 2020 13:36
 Operator : DD\AJ
 Sample : L1219-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ST-CONCRETE

Manual Integrations
 APPROVED

Ankita
 1/23/2020 4:16:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 13:51:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.150	3.428	628973	829042	34.445m	37.688
2) SA Decachlor...	9.643	8.325	802357	882766	23.681	21.287
Target Compounds						
31) L7 AR-1260-1	6.882	5.944	56343	92331	40.851m	49.043
32) L7 AR-1260-2	7.137	6.131	83047	103447	47.333m	42.580
33) L7 AR-1260-3	7.493	6.281	37668	73923	26.651	34.152 #
34) L7 AR-1260-4	7.713	6.748	54883	38536	31.432m	19.208m#
35) L7 AR-1260-5	8.022	6.991	82470	94152	24.591	19.019

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012220\
Data File : P0065841.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jan 2020 13:36
Operator : DD\AJ
Sample : L1219-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ST-CONCRETE


Manual Integrations
APPROVED

Ankita
1/23/2020 4:16:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 13:51:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

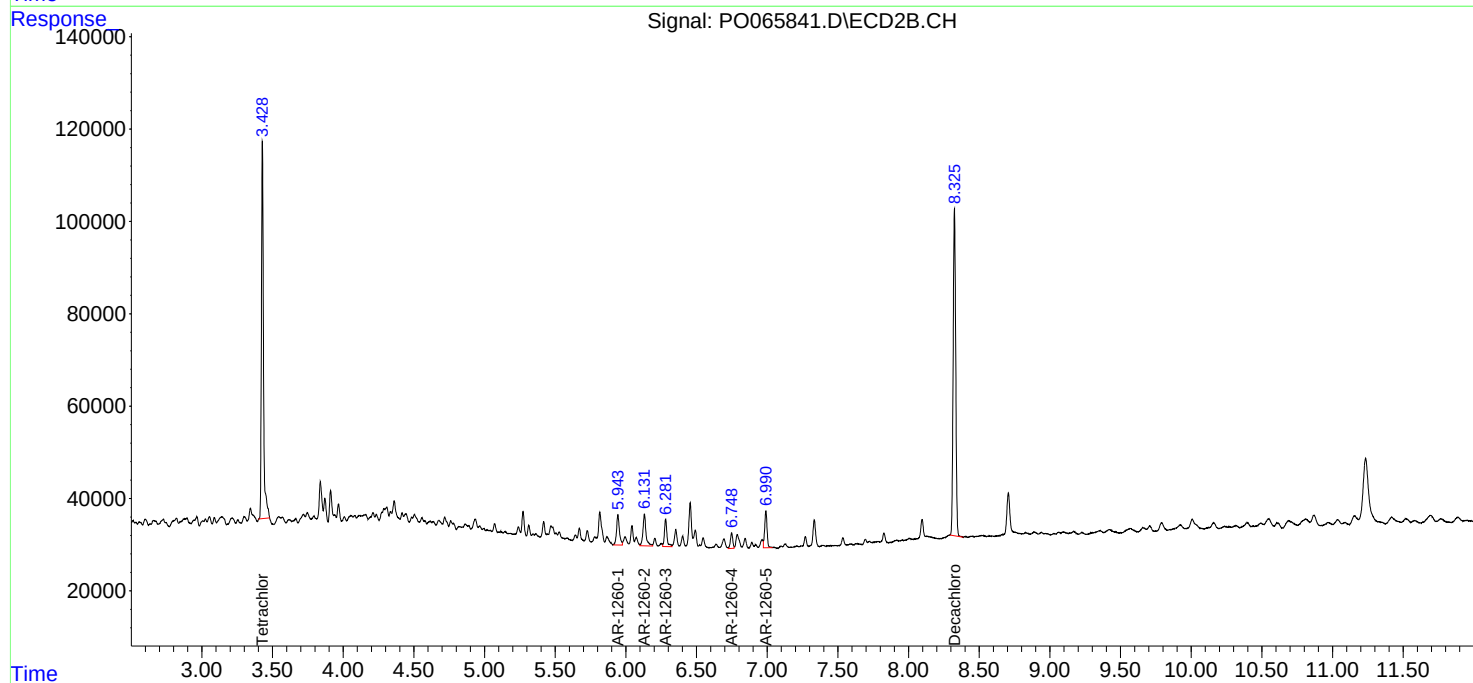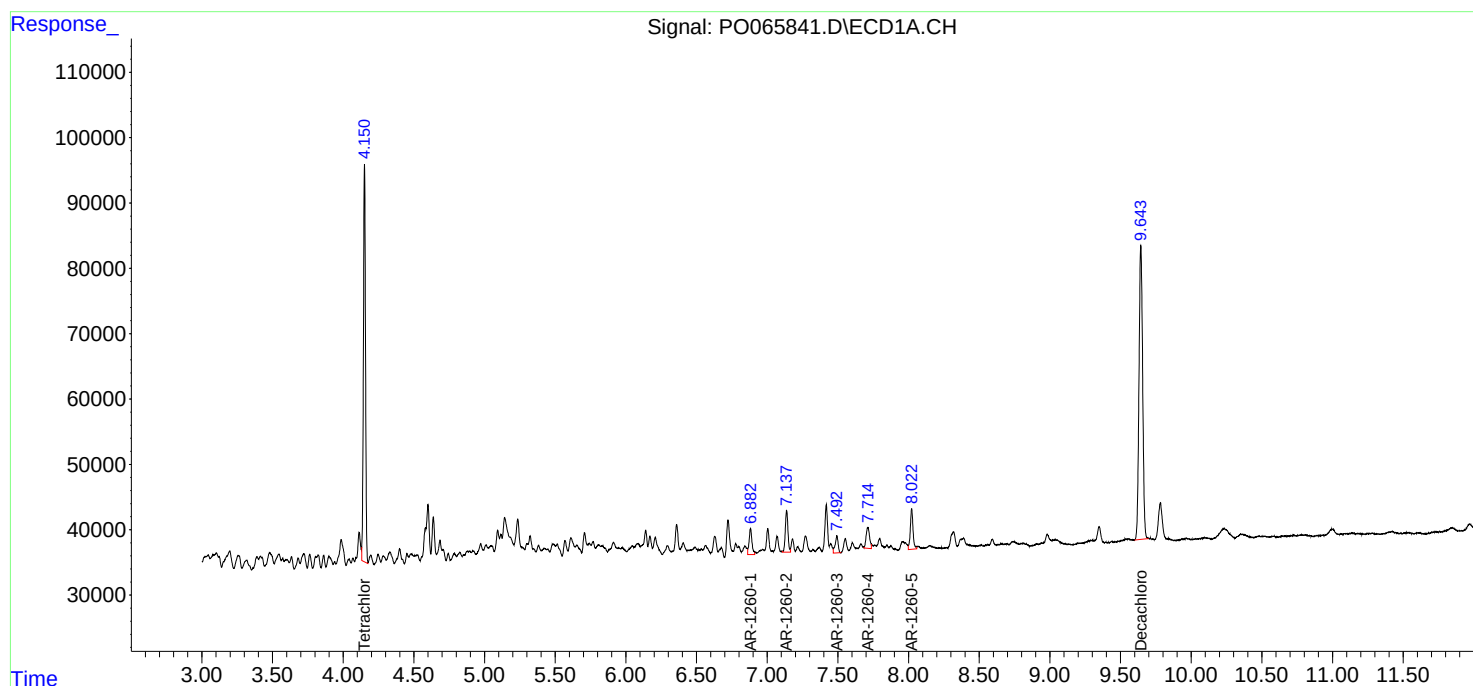

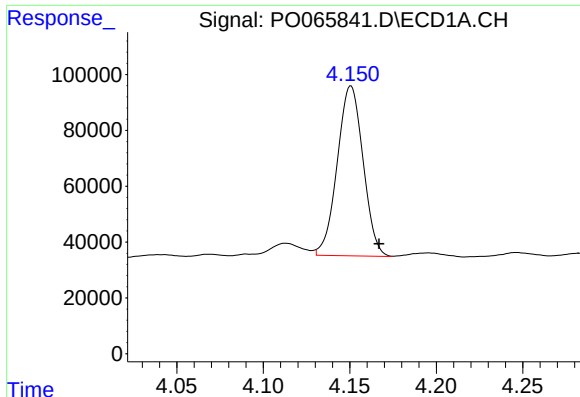


#1 Tetrachloro-m-xylene

R.T.: 4.150 min
Delta R.T.: -0.017 min
Response: 628973
Conc: 34.44 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ST-CONCRETE


Manual Integrations
APPROVED

Ankita
1/23/2020 4:16:15 PM

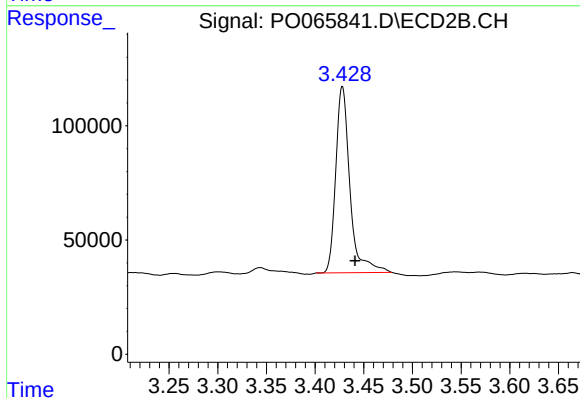


#1 Tetrachloro-m-xylene

R.T.: 3.428 min
Delta R.T.: -0.013 min
Response: 829042
Conc: 37.69 ng/ml

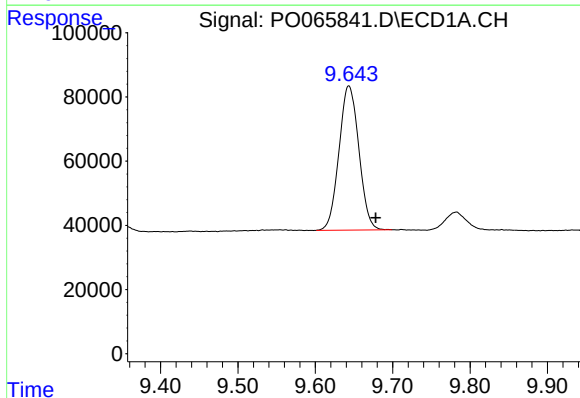


#2 Decachlorobiphenyl

R.T.: 9.643 min
Delta R.T.: -0.035 min
Response: 802357
Conc: 23.68 ng/ml

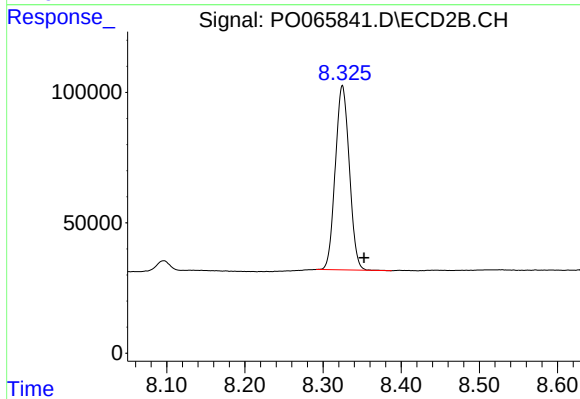

#2 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.028 min
Response: 882766
Conc: 21.29 ng/ml

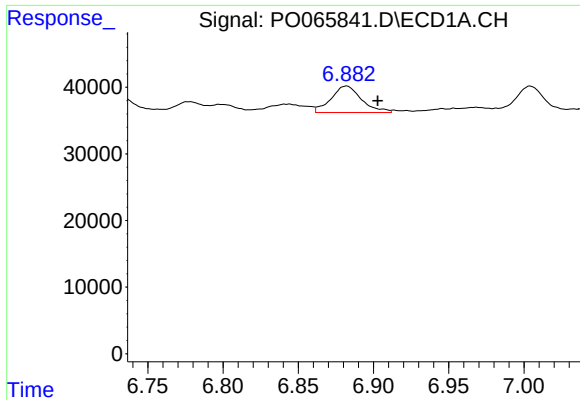


#31 AR-1260-1

R.T.: 6.882 min
Delta R.T.: -0.021 min
Response: 56343
Conc: 40.85 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ST-CONCRETE


Manual Integrations
APPROVED

Ankita
1/23/2020 4:16:15 PM

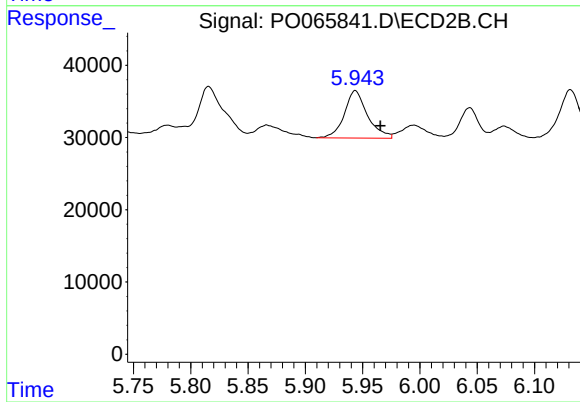


#31 AR-1260-1

R.T.: 5.944 min
Delta R.T.: -0.022 min
Response: 92331
Conc: 49.04 ng/ml

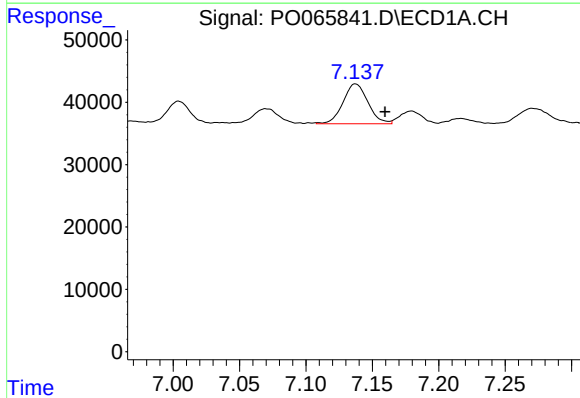


#32 AR-1260-2

R.T.: 7.137 min
Delta R.T.: -0.023 min
Response: 83047
Conc: 47.33 ng/ml m

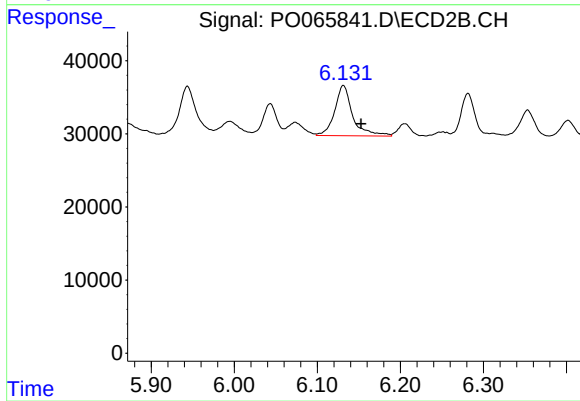

#32 AR-1260-2

R.T.: 6.131 min
Delta R.T.: -0.022 min
Response: 103447
Conc: 42.58 ng/ml

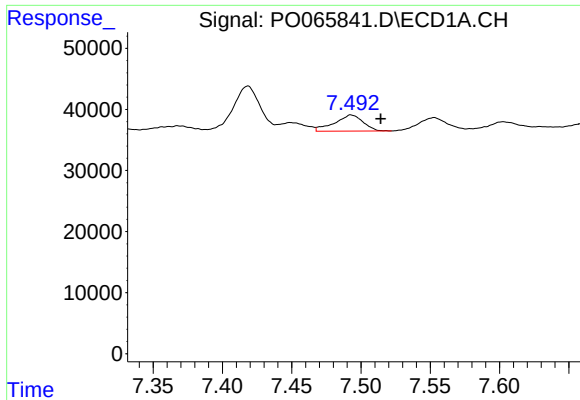


#33 AR-1260-3

R.T.: 7.493 min
Delta R.T.: -0.021 min
Response: 37668
Conc: 26.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
ST-CONCRETE


Manual Integrations
APPROVED

Ankita
1/23/2020 4:16:15 PM

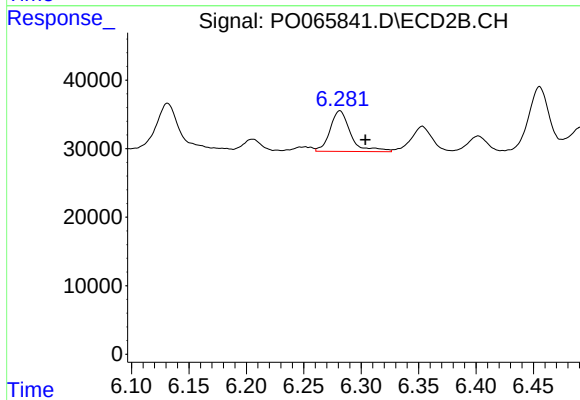


#33 AR-1260-3

R.T.: 6.281 min
Delta R.T.: -0.022 min
Response: 73923
Conc: 34.15 ng/ml

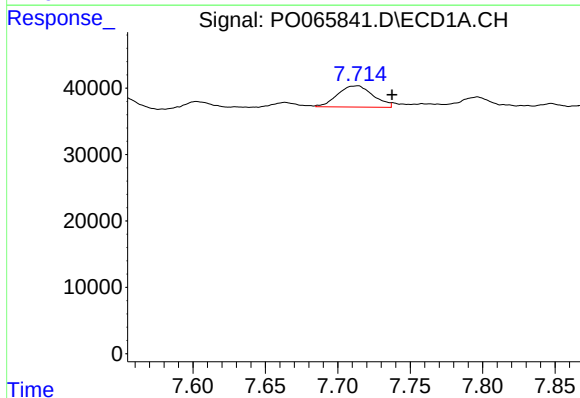


#34 AR-1260-4

R.T.: 7.713 min
Delta R.T.: -0.024 min
Response: 54883
Conc: 31.43 ng/ml m

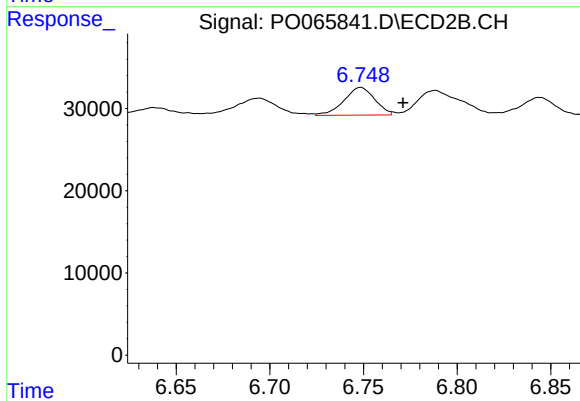

#34 AR-1260-4

R.T.: 6.748 min
Delta R.T.: -0.023 min
Response: 38536
Conc: 19.21 ng/ml m

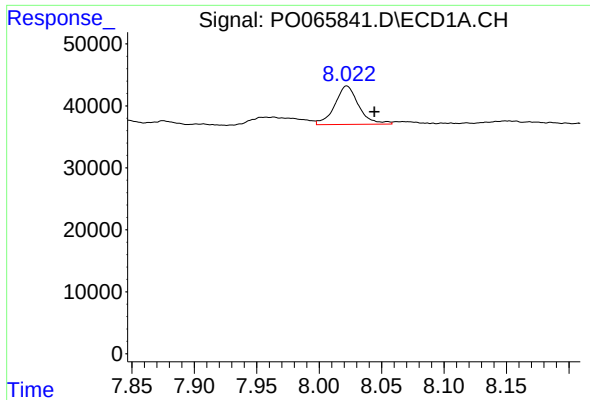


#35 AR-1260-5

R.T.: 8.022 min
Delta R.T.: -0.022 min
Response: 82470
Conc: 24.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
ST-CONCRETE

Manual Integrations
APPROVED

Ankita
1/23/2020 4:16:15 PM

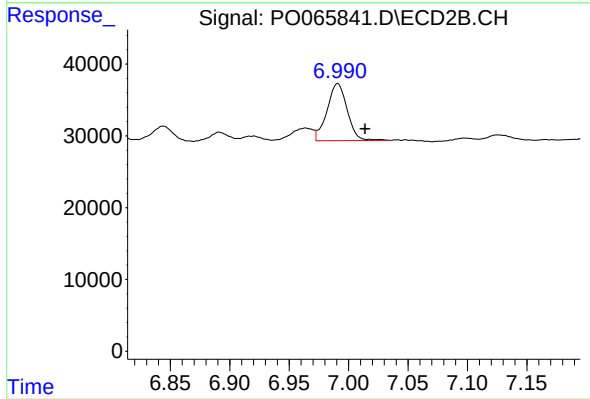

#35 AR-1260-5

R.T.: 6.991 min
Delta R.T.: -0.023 min
Response: 94152
Conc: 19.02 ng/ml