

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012220\
 Data File : P0065842.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jan 2020 13:53
 Operator : DD\AJ
 Sample : L1219-01RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ST-CONCRETERE

Manual Integrations
 APPROVED

Ankita
 1/23/2020 4:16:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 14:07:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.151	3.429	626378	820483	34.303m	37.299
2) SA Decachlor...	9.644	8.326	825927	908055	24.376	21.897
Target Compounds						
31) L7 AR-1260-1	6.881	5.945	51933	103158	37.654m	54.794 #
32) L7 AR-1260-2	7.137	6.132	81676	103100	46.552m	42.437m
33) L7 AR-1260-3	7.494	6.281	46520	65498	32.913	30.260m
34) L7 AR-1260-4	7.711	6.749	47168	41859	27.014m	20.864m
35) L7 AR-1260-5	8.022	6.992	76732	97754	22.880m	19.746

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012220\
Data File : P0065842.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jan 2020 13:53
Operator : DD\AJ
Sample : L1219-01RE
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ST-CONCRETERE


Manual Integrations
APPROVED

Ankita
1/23/2020 4:16:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 14:07:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

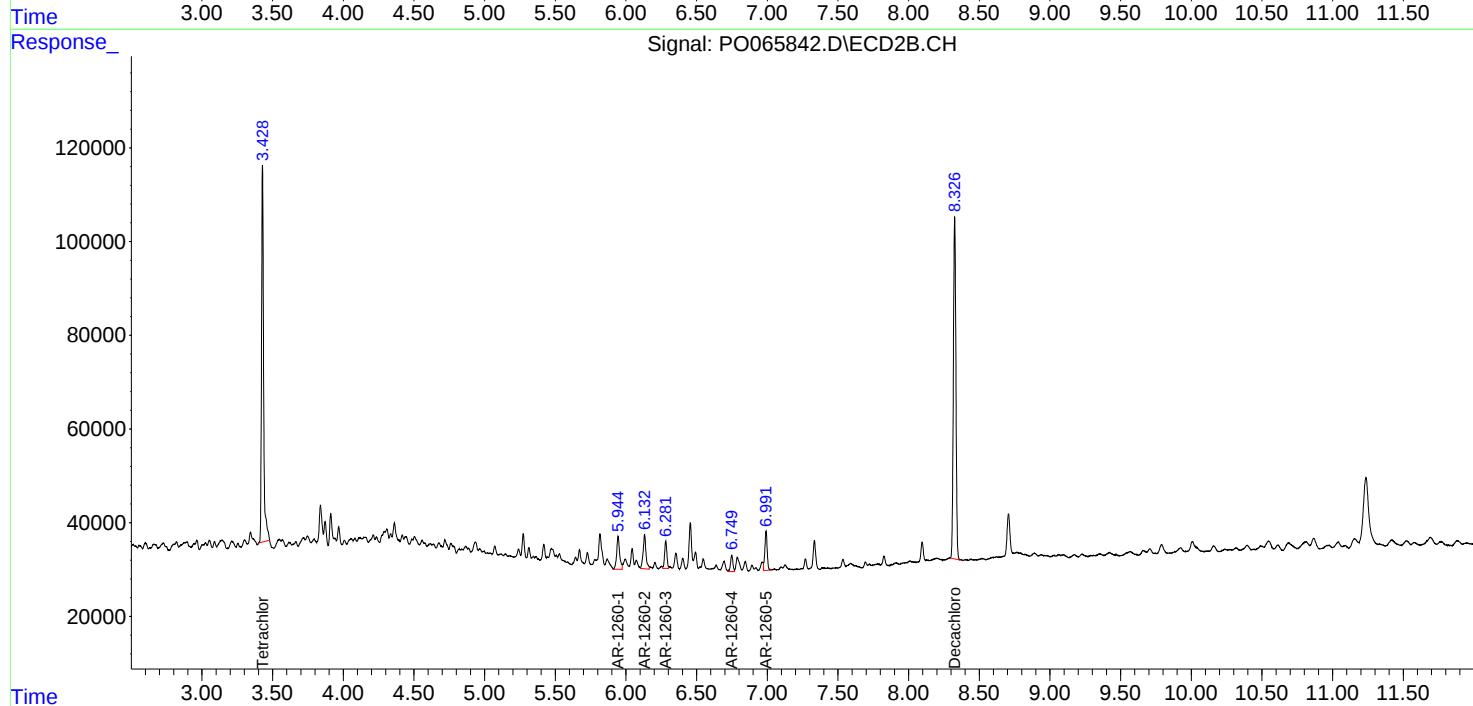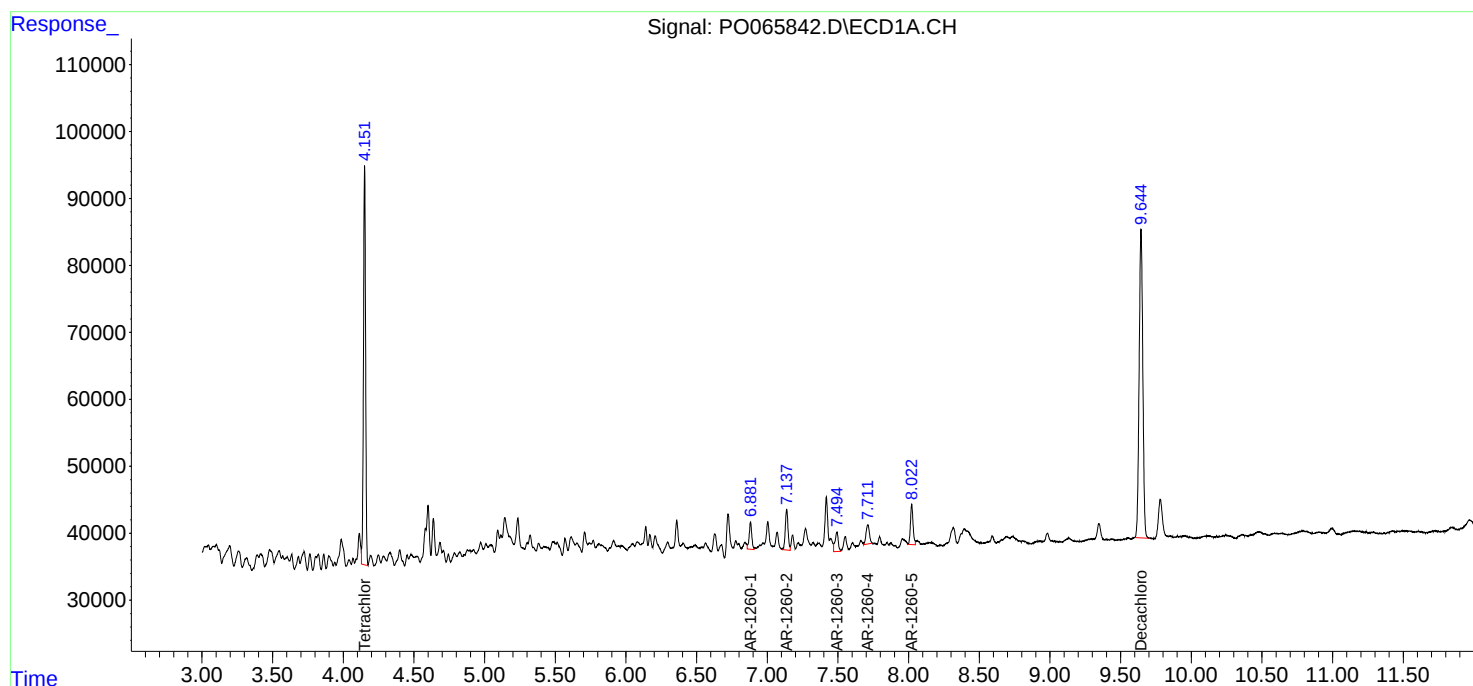

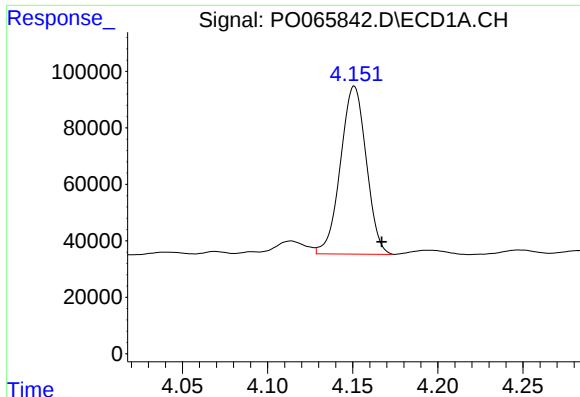


#1 Tetrachloro-m-xylene

R.T.: 4.151 min
Delta R.T.: -0.016 min
Response: 626378
Conc: 34.30 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ST-CONCRETERE


Manual Integrations
APPROVED

Ankita
1/23/2020 4:16:16 PM

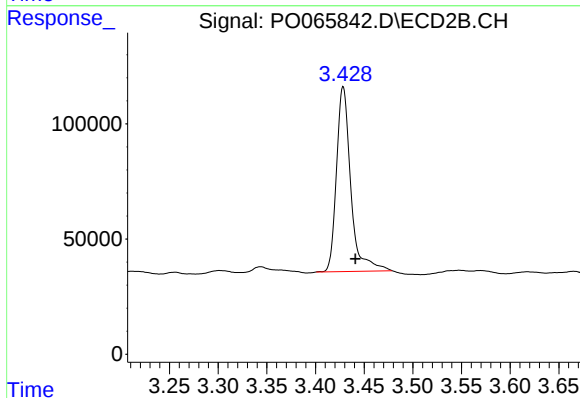


#1 Tetrachloro-m-xylene

R.T.: 3.429 min
Delta R.T.: -0.013 min
Response: 820483
Conc: 37.30 ng/ml

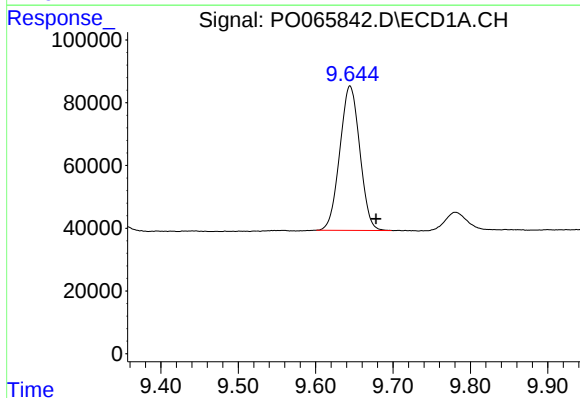


#2 Decachlorobiphenyl

R.T.: 9.644 min
Delta R.T.: -0.034 min
Response: 825927
Conc: 24.38 ng/ml

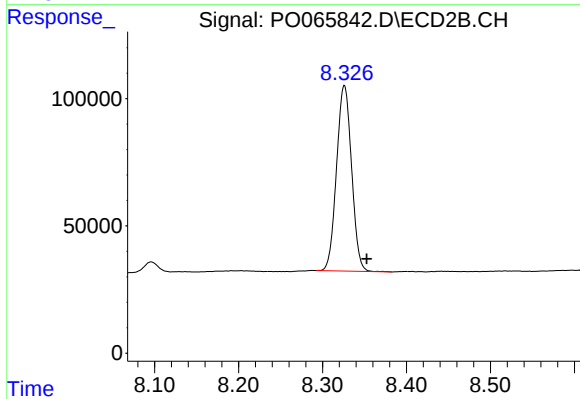

#2 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: -0.027 min
Response: 908055
Conc: 21.90 ng/ml

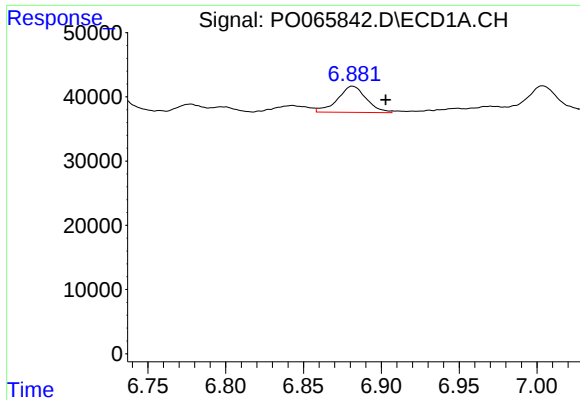


#31 AR-1260-1

R.T.: 6.881 min
Delta R.T.: -0.022 min
Response: 51933
Conc: 37.65 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ST-CONCRETERE


Manual Integrations
APPROVED

Ankita
1/23/2020 4:16:16 PM

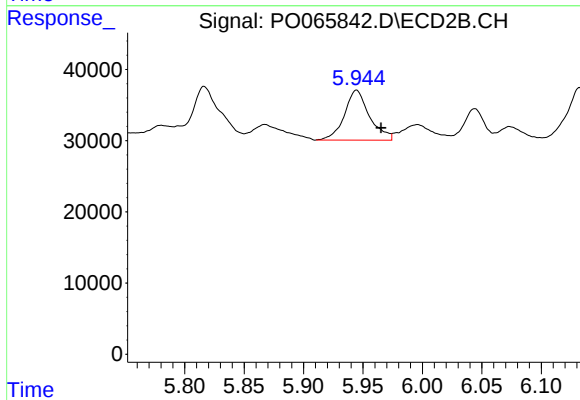


#31 AR-1260-1

R.T.: 5.945 min
Delta R.T.: -0.021 min
Response: 103158
Conc: 54.79 ng/ml

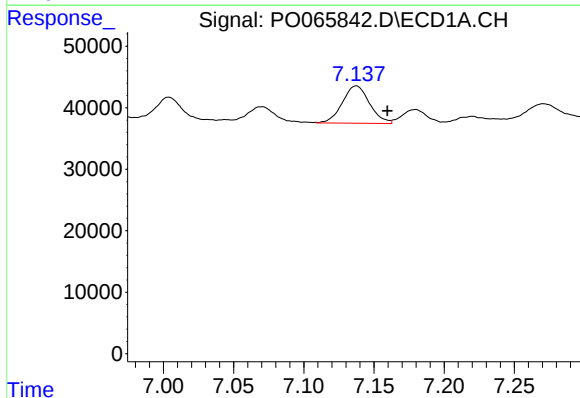


#32 AR-1260-2

R.T.: 7.137 min
Delta R.T.: -0.022 min
Response: 81676
Conc: 46.55 ng/ml m

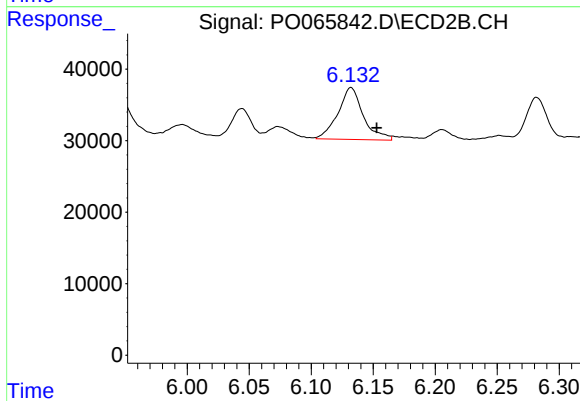

#32 AR-1260-2

R.T.: 6.132 min
Delta R.T.: -0.021 min
Response: 103100
Conc: 42.44 ng/ml m

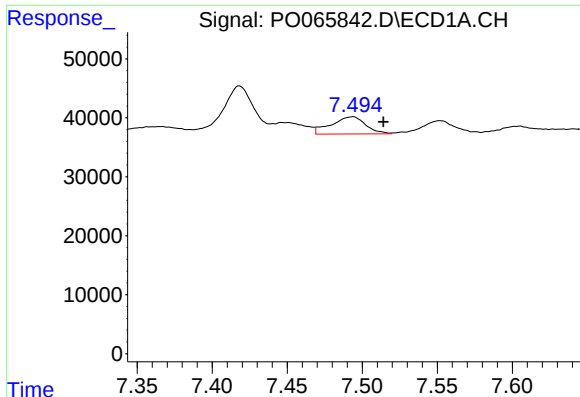


#33 AR-1260-3

R.T.: 7.494 min
Delta R.T.: -0.021 min
Response: 46520
Conc: 32.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
ST-CONCRETERE


Manual Integrations
APPROVED

Ankita
1/23/2020 4:16:16 PM

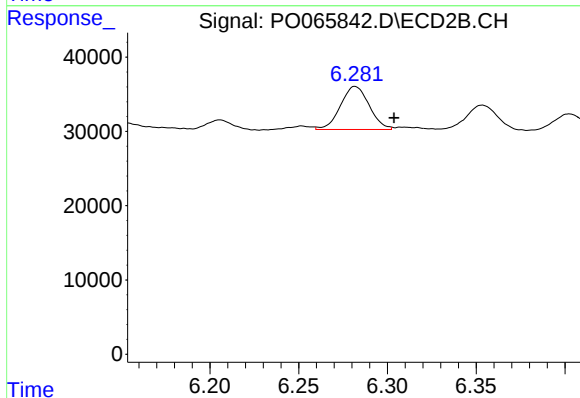


#33 AR-1260-3

R.T.: 6.281 min
Delta R.T.: -0.023 min
Response: 65498
Conc: 30.26 ng/ml m

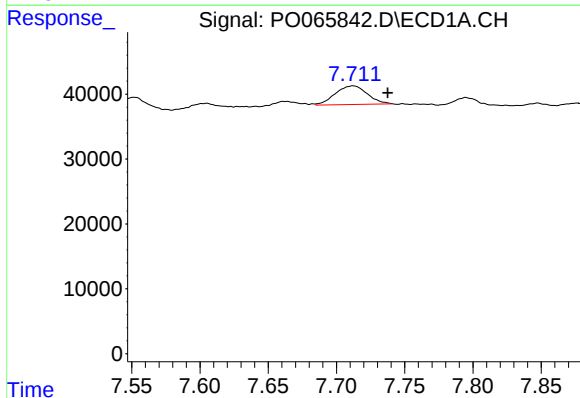


#34 AR-1260-4

R.T.: 7.711 min
Delta R.T.: -0.026 min
Response: 47168
Conc: 27.01 ng/ml m

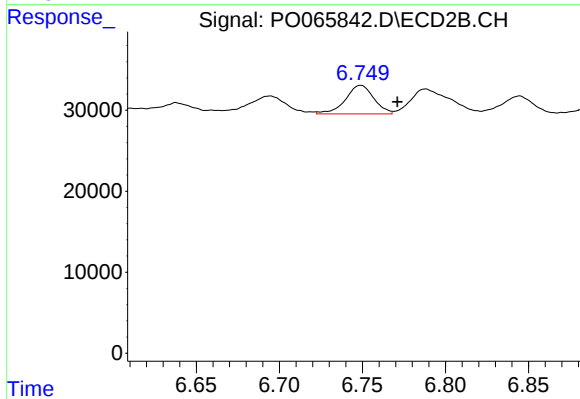

#34 AR-1260-4

R.T.: 6.749 min
Delta R.T.: -0.022 min
Response: 41859
Conc: 20.86 ng/ml m

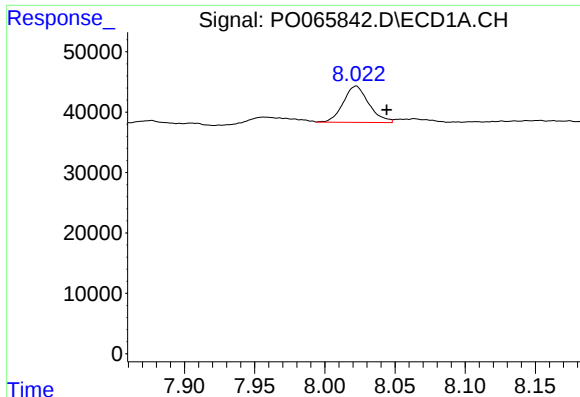


#35 AR-1260-5

R.T.: 8.022 min
Delta R.T.: -0.022 min
Response: 76732
Conc: 22.88 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ST-CONCRETERE

Manual Integrations
APPROVED

Ankita
1/23/2020 4:16:16 PM

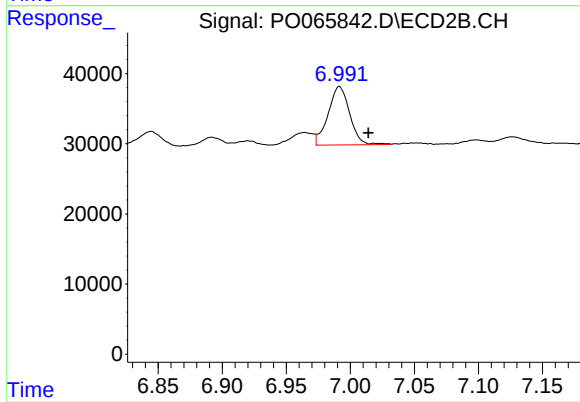

#35 AR-1260-5

R.T.: 6.992 min
Delta R.T.: -0.022 min
Response: 97754
Conc: 19.75 ng/ml