

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012221\
 Data File : P0075068.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2021 10:05
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 16:50:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.938	4.002	2231689	1136468	21.150	20.203
2) SA Decachlor...	10.958	9.255	2077125	1054810	20.466	19.212
Target Compounds						
45) L9 AR-1268-5	0.000	9.012	0	28271	N.D.	1.194 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012221\
Data File : P0075068.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2021 10:05
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 16:50:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

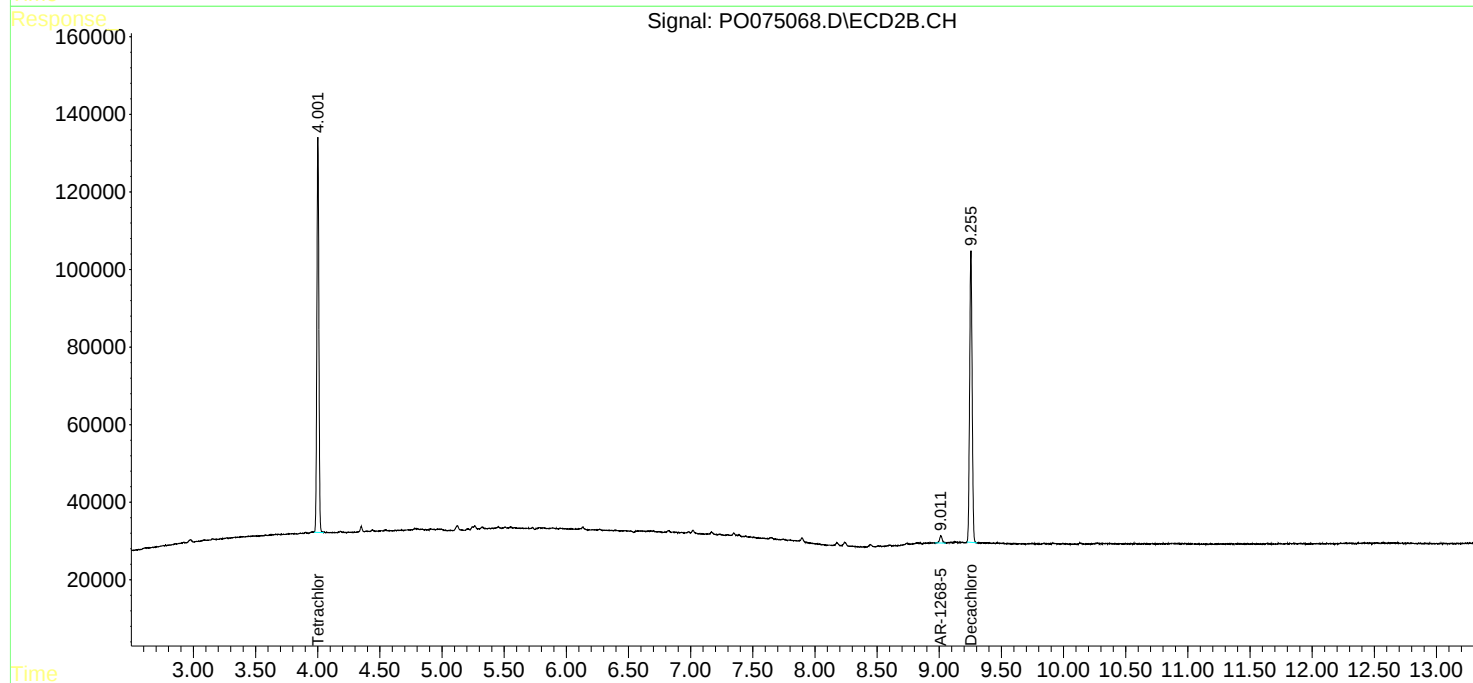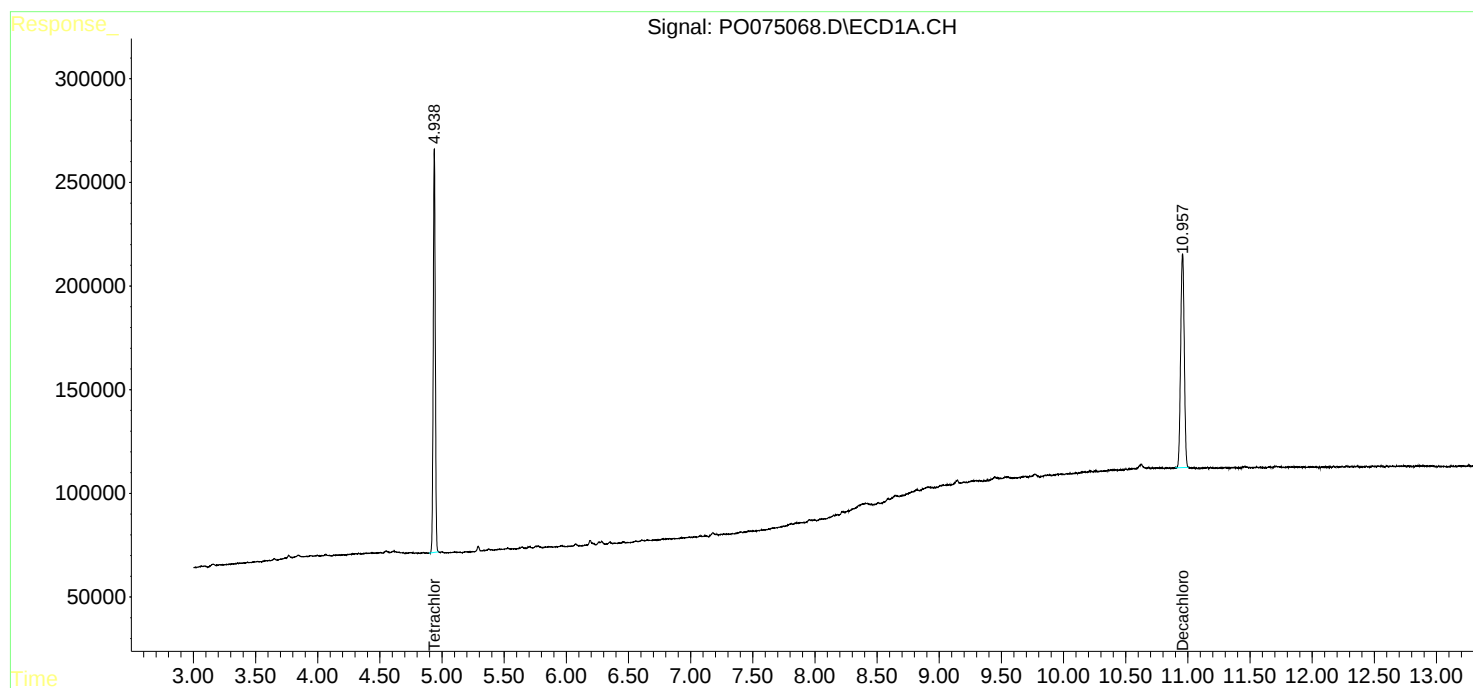


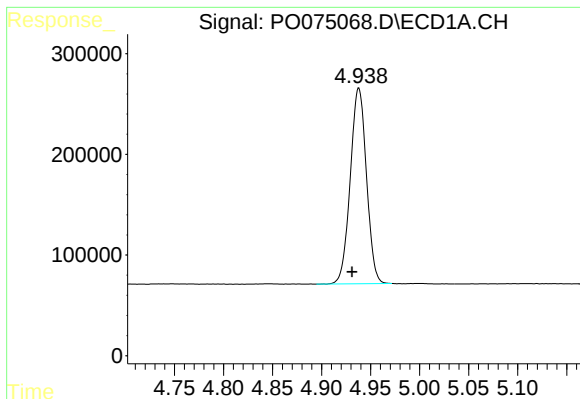

#1 Tetrachloro-m-xylene


R.T.: 4.938 min
Delta R.T.: 0.007 min
Response: 2231689
Conc: 21.15 ng/ml

Instrument :
ECD_O
ClientSampleId :

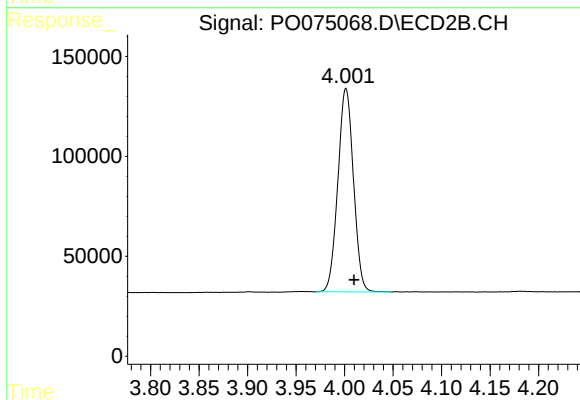


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.008 min
Response: 1136468
Conc: 20.20 ng/ml

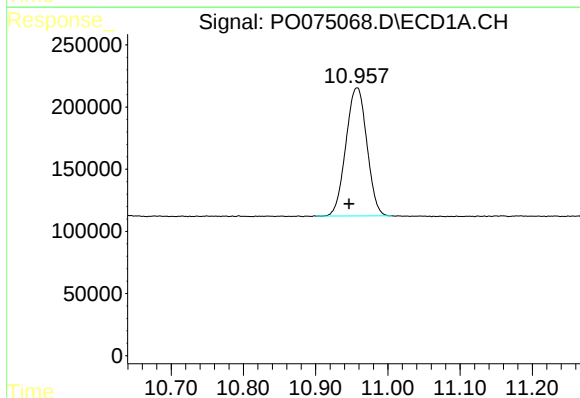


#2 Decachlorobiphenyl

R.T.: 10.958 min
Delta R.T.: 0.011 min
Response: 2077125
Conc: 20.47 ng/ml

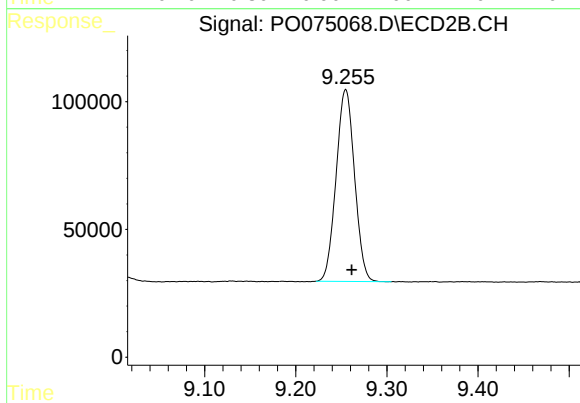

#2 Decachlorobiphenyl


R.T.: 9.255 min
Delta R.T.: -0.007 min
Response: 1054810
Conc: 19.21 ng/ml

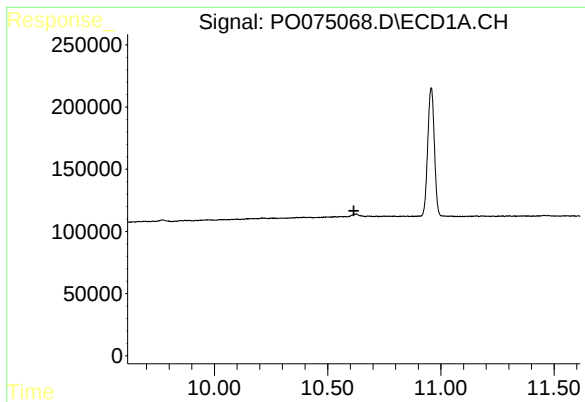

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.616 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

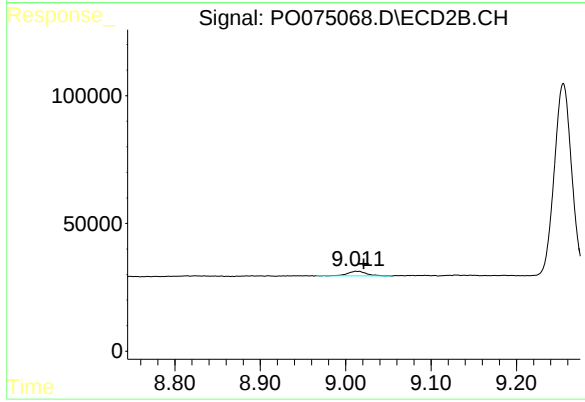

#45 AR-1268-5

R.T.: 9.012 min
Delta R.T.: -0.009 min
Response: 28271
Conc: 1.19 ng/ml