

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012221\
 Data File : P0075119.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Jan 2021 1:16
 Operator : AJ/MA
 Sample : M1189-12
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 05:30:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.930	4.004	1832011	953391	17.362	16.949
2)	SA Decachlor...	10.947	9.253	1123618	573163	11.071	10.439
Target Compounds							
8)	L2 AR-1221-1	5.182	0.000	79632	0	64.831	N.D. #
9)	L2 AR-1221-2	5.284	0.000	37605	0	41.736	N.D. #
34)	L7 AR-1260-4	8.809	0.000	14409	0	2.634	N.D. #
35)	L7 AR-1260-5	9.138	0.000	104015	0	8.325	N.D. #
37)	L8 AR-1262-2	9.138	0.000	104015	0	6.794	N.D. #
38)	L8 AR-1262-3	0.000	8.165f	0	45283	N.D.	11.452 #
41)	L9 AR-1268-1	0.000	8.165f	0	45283	N.D.	4.045 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012221\
Data File : P0075119.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Jan 2021 1:16
Operator : AJ/MA
Sample : M1189-12
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 05:30:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

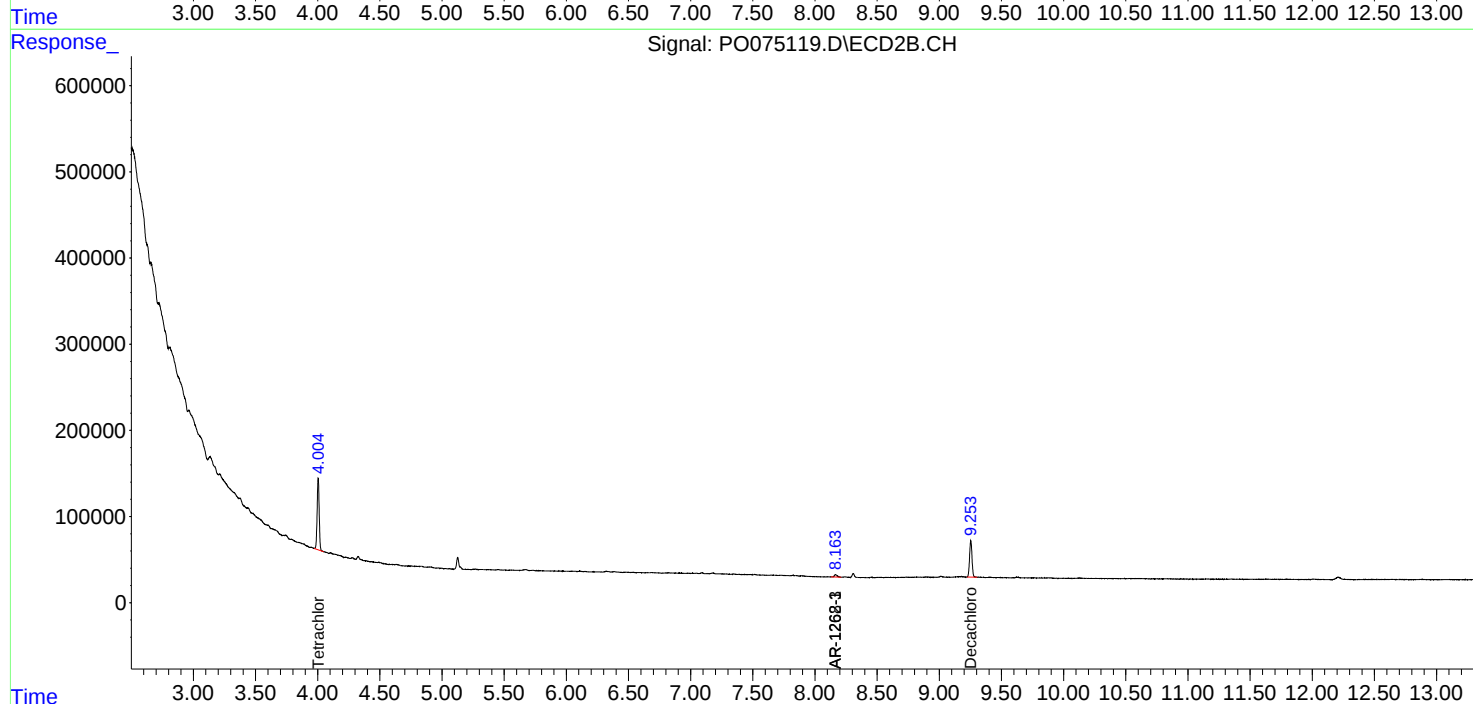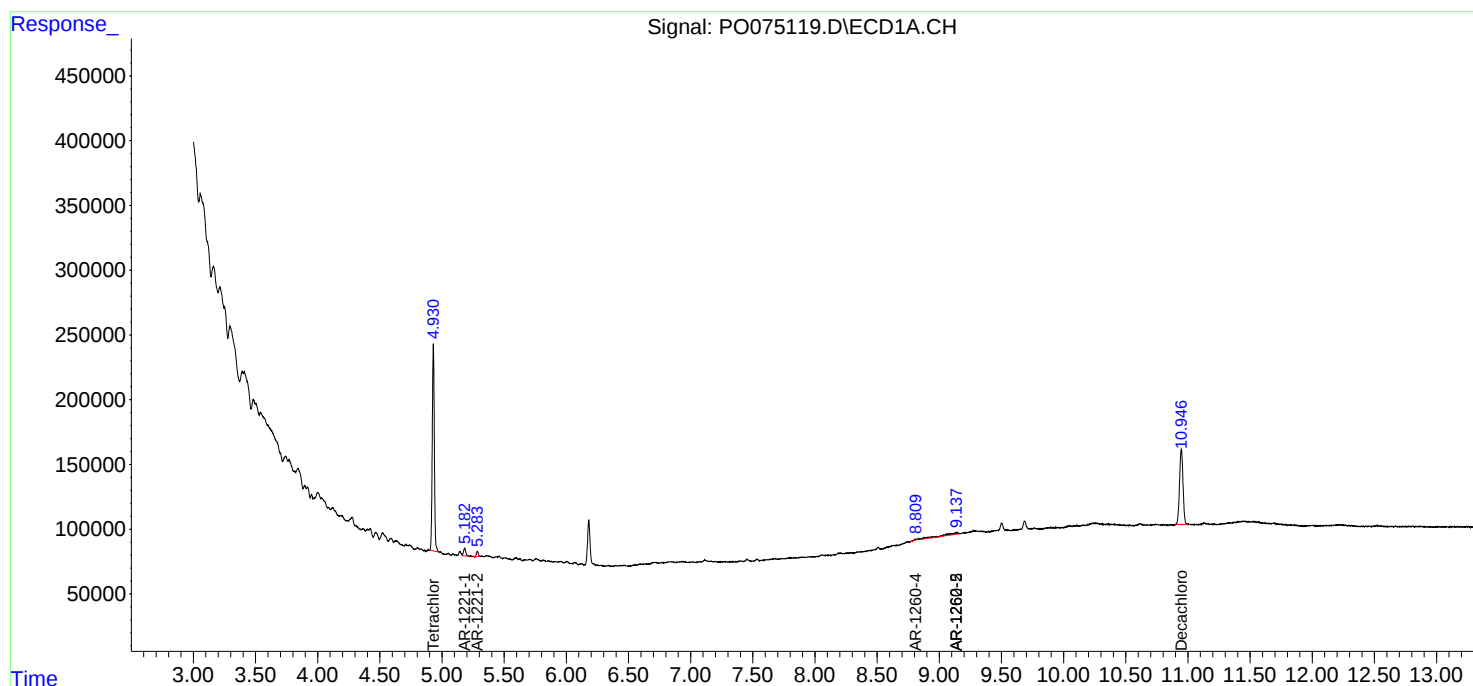


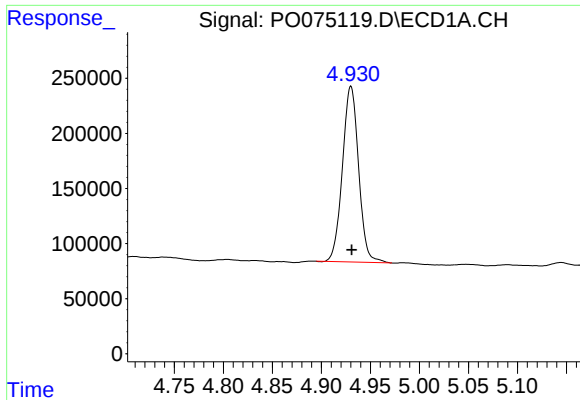

#1 Tetrachloro-m-xylene


R.T.: 4.930 min
Delta R.T.: 0.000 min
Response: 1832011
Conc: 17.36 ng/ml

Instrument :
ECD_O
ClientSampleId :

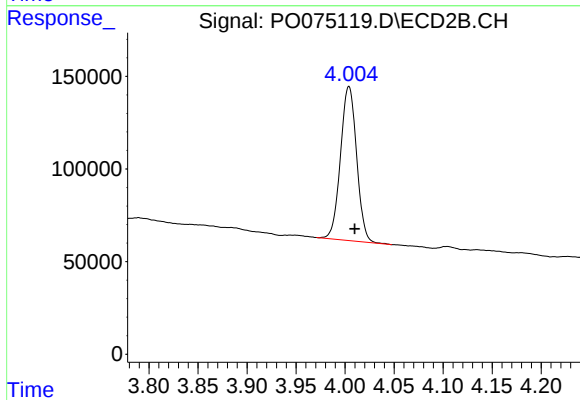


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.006 min
Response: 953391
Conc: 16.95 ng/ml

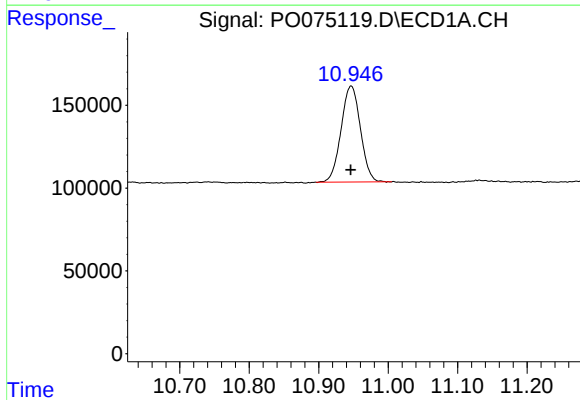


#2 Decachlorobiphenyl

R.T.: 10.947 min
Delta R.T.: 0.000 min
Response: 1123618
Conc: 11.07 ng/ml

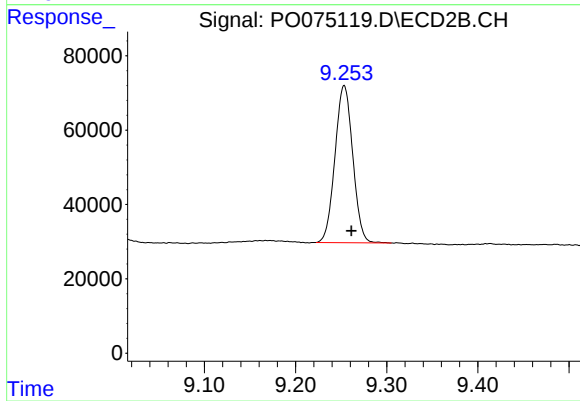

#2 Decachlorobiphenyl


R.T.: 9.253 min
Delta R.T.: -0.008 min
Response: 573163
Conc: 10.44 ng/ml

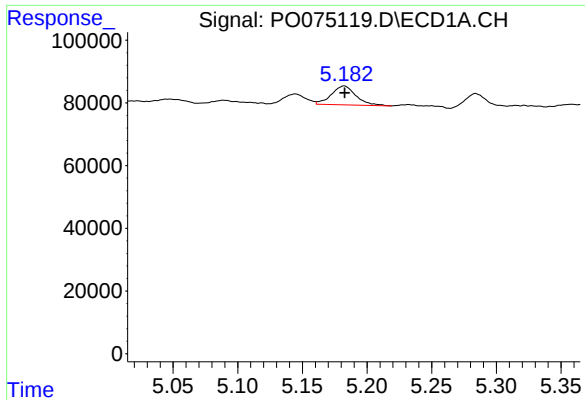

#8 AR-1221-1


R.T.: 5.182 min
Delta R.T.: 0.000 min
Response: 79632
Conc: 64.83 ng/ml

Instrument :
ECD_O
ClientSampleId :

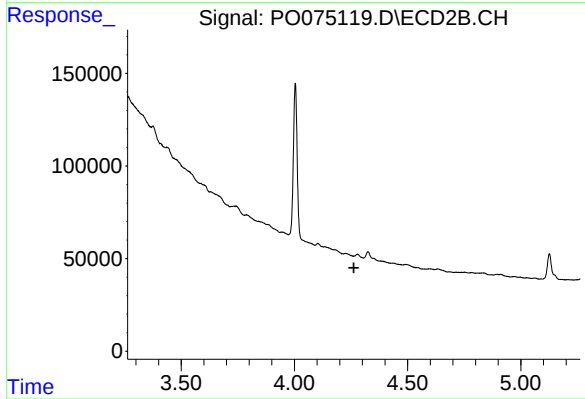


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.263 min
Response: 0
Conc: N.D.

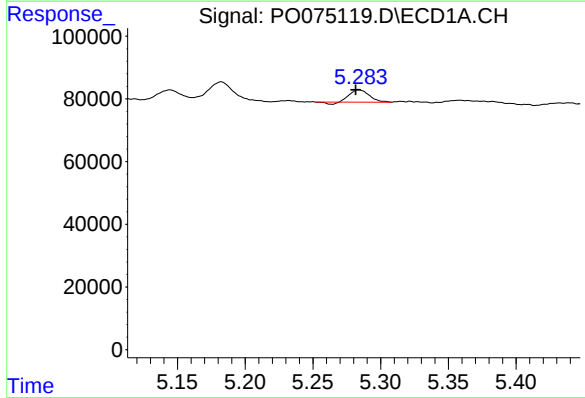


#9 AR-1221-2

R.T.: 5.284 min
Delta R.T.: 0.002 min
Response: 37605
Conc: 41.74 ng/ml

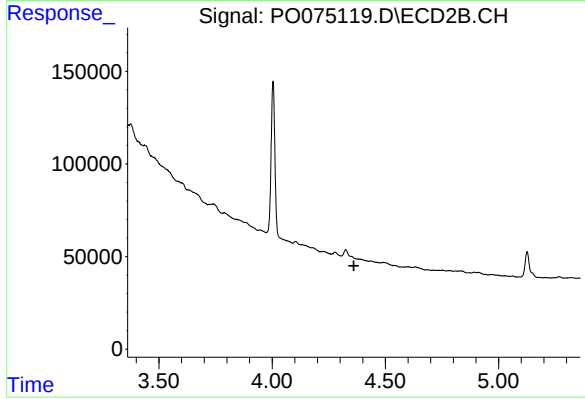

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.361 min
Response: 0
Conc: N.D.

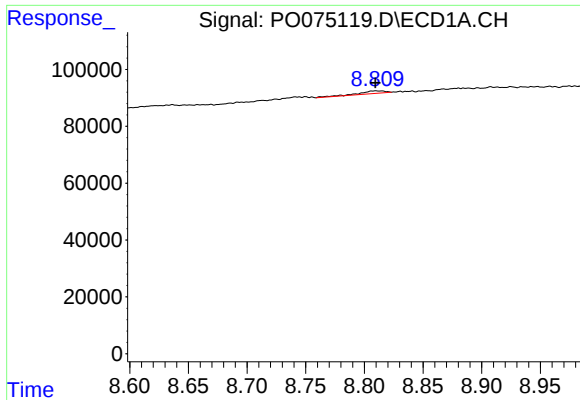

#34 AR-1260-4


R.T.: 8.809 min
Delta R.T.: 0.000 min
Response: 14409
Conc: 2.63 ng/ml

Instrument :
ECD_O
ClientSampleId :

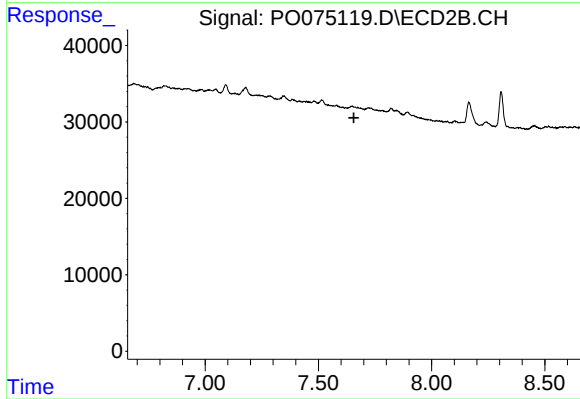


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.657 min
Response: 0
Conc: N.D.

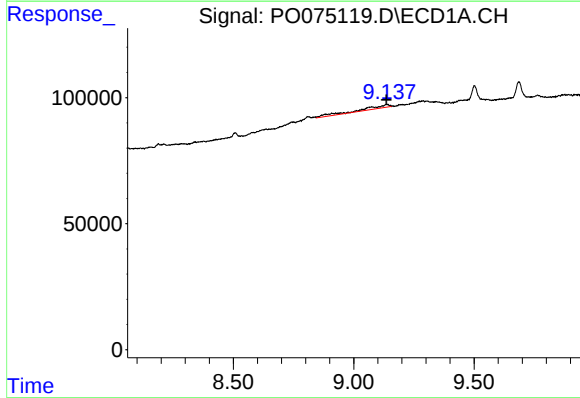


#35 AR-1260-5

R.T.: 9.138 min
Delta R.T.: 0.002 min
Response: 104015
Conc: 8.32 ng/ml

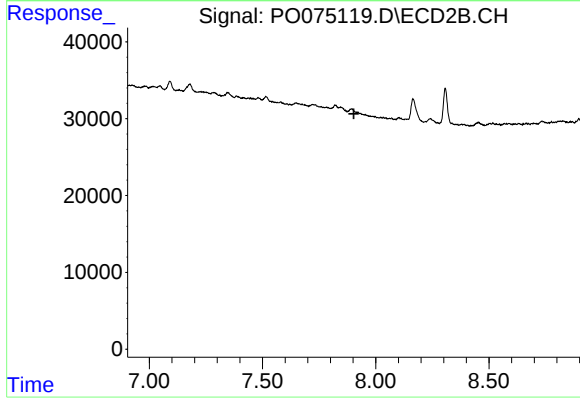

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.903 min
Response: 0
Conc: N.D.

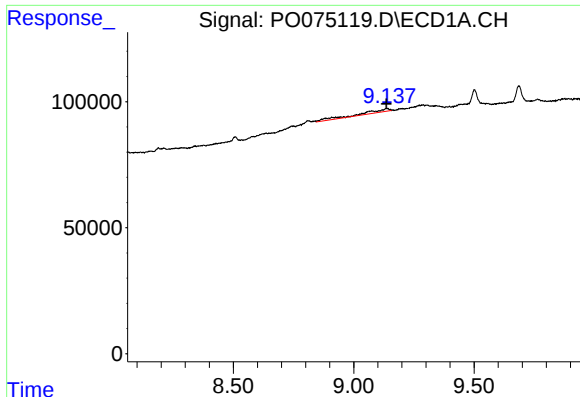

#37 AR-1262-2


R.T.: 9.138 min
Delta R.T.: 0.001 min
Response: 104015
Conc: 6.79 ng/ml

Instrument :
ECD_O
ClientSampleId :

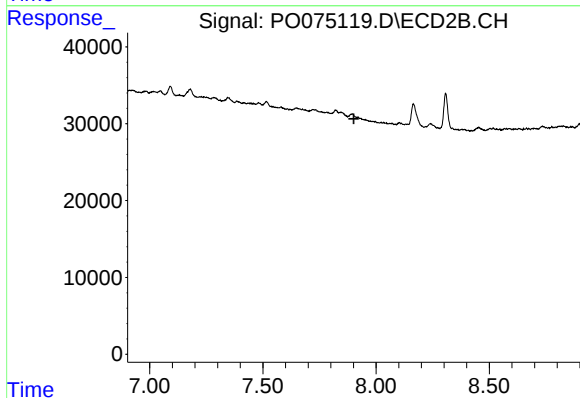


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.902 min
Response: 0
Conc: N.D.

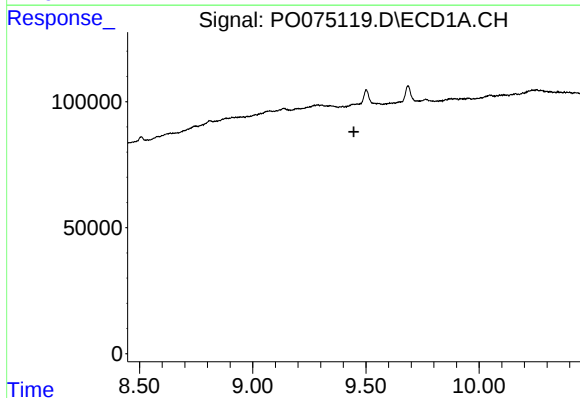


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.447 min
Response: 0
Conc: N.D.

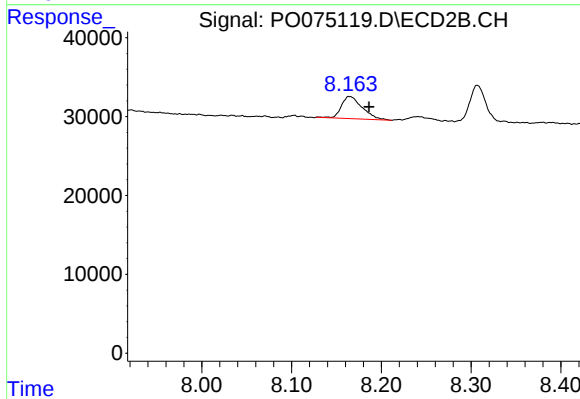

#38 AR-1262-3


R.T.: 8.165 min
Delta R.T.: -0.022 min
Response: 45283
Conc: 11.45 ng/ml

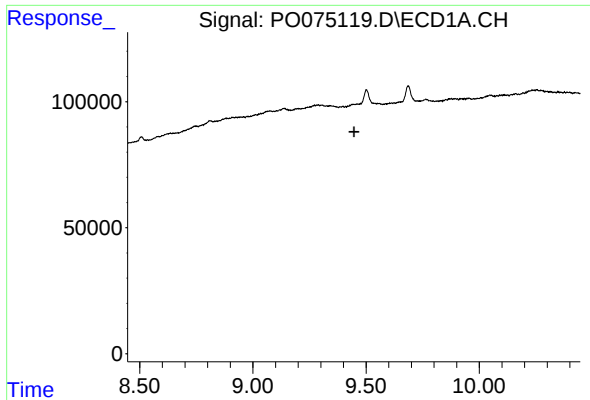

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.446 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

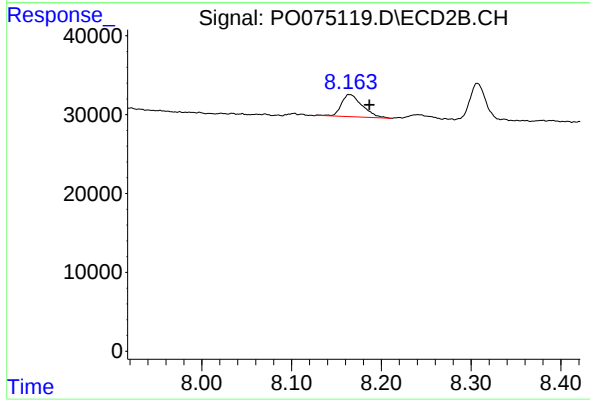

#41 AR-1268-1

R.T.: 8.165 min
Delta R.T.: -0.022 min
Response: 45283
Conc: 4.05 ng/ml