

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012221\
 Data File : P0075082.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2021 14:07
 Operator : AJ/MA
 Sample : M1191-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0041-043-COMP-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 22 16:56:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.935	4.001	2318620	1169029	21.974	20.782
2) SA Decachlor...	10.952	9.254	1786050	890911	17.598	16.227

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012221\
Data File : P0075082.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2021 14:07
Operator : AJ/MA
Sample : M1191-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
0041-043-COMP-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 22 16:56:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

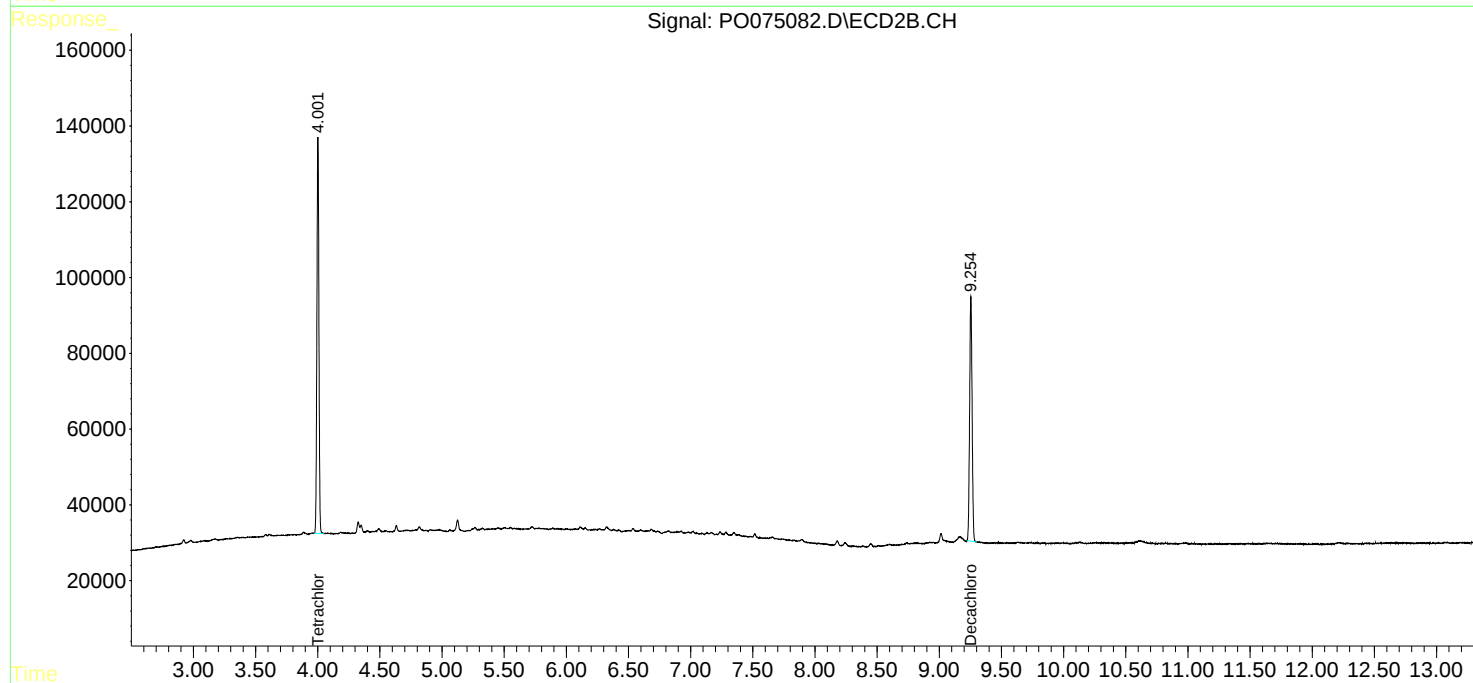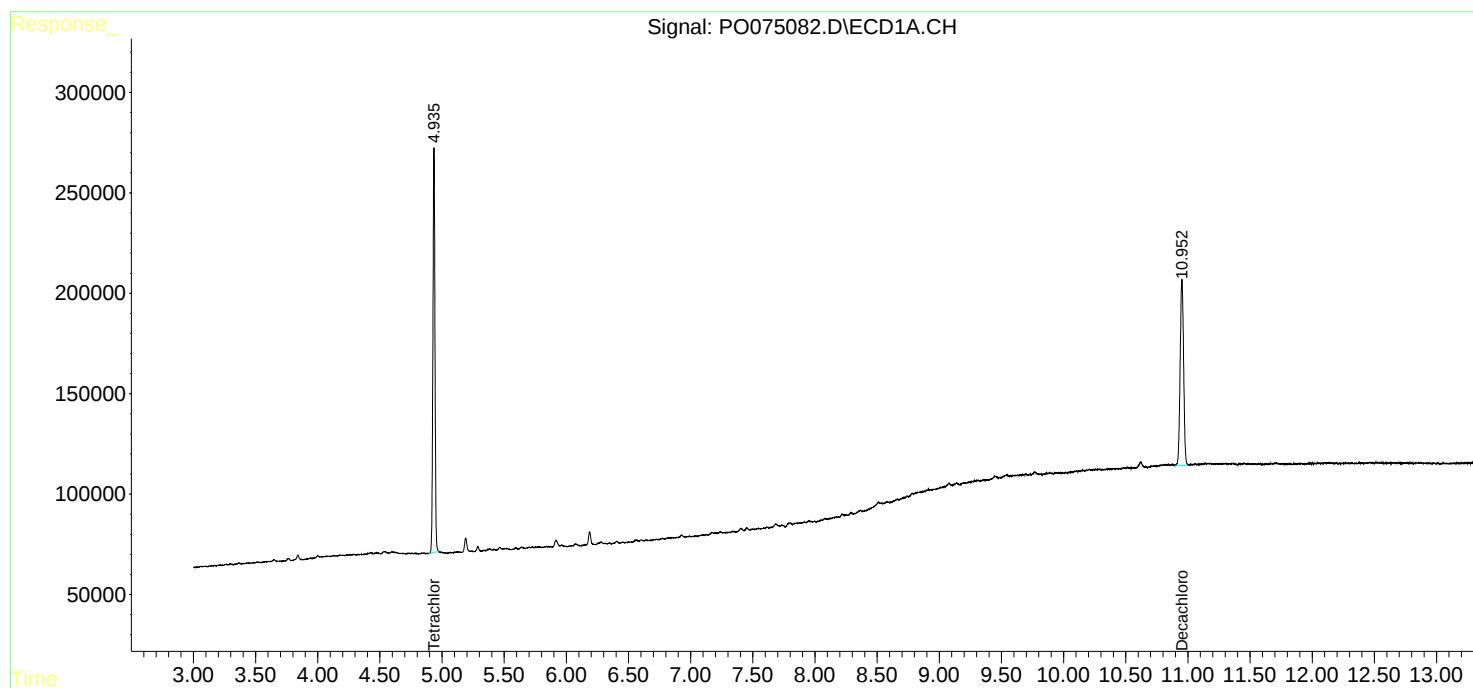


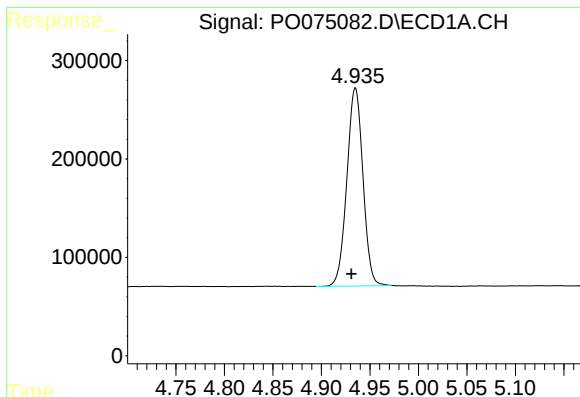

#1 Tetrachloro-m-xylene


R.T.: 4.935 min
Delta R.T.: 0.004 min
Response: 2318620
Conc: 21.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
0041-043-COMP-C

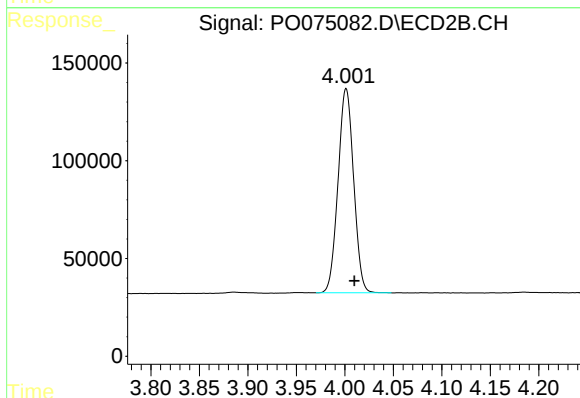


#1 Tetrachloro-m-xylene

R.T.: 4.001 min
Delta R.T.: -0.008 min
Response: 1169029
Conc: 20.78 ng/ml

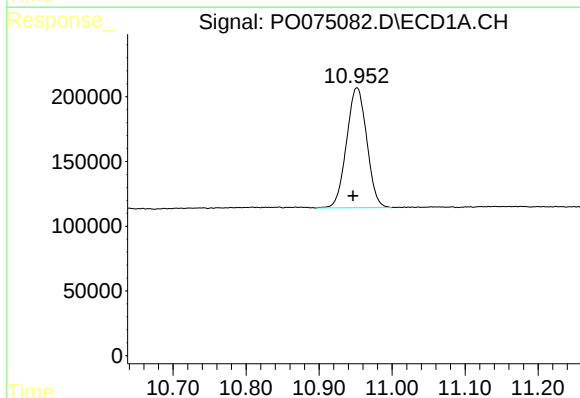

#2 Decachlorobiphenyl

R.T.: 10.952 min
Delta R.T.: 0.006 min
Response: 1786050
Conc: 17.60 ng/ml

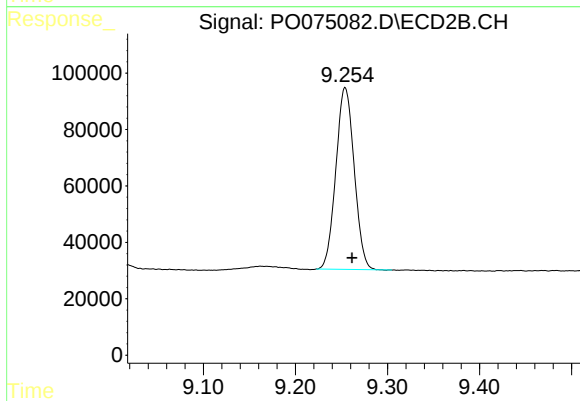

#2 Decachlorobiphenyl

R.T.: 9.254 min
Delta R.T.: -0.007 min
Response: 890911
Conc: 16.23 ng/ml