

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012221\
 Data File : P0075091.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2021 16:42
 Operator : AJ/MA
 Sample : M1207-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-SF-03-010-B

Manual Integrations
 APPROVED

Ankita
 1/25/2021 10:48:35 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 05:24:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.928	4.002	1540914	963265	14.603m	17.124
2) SA Decachlor...	10.948	9.254	1579889	745023	15.567	13.569
Target Compounds						
26) L6 AR-1254-1	7.175	6.112	752396	582439	171.071m	161.251
27) L6 AR-1254-2	7.400	6.268	989338	259618	145.261	83.303 #
28) L6 AR-1254-3	7.780	6.685	706933	394229	100.784	80.390
29) L6 AR-1254-4	8.074	6.924	528467	220566	87.139	63.604 #
30) L6 AR-1254-5	8.504	7.348	623199	481384	107.283	106.361

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012221\
Data File : PO075091.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2021 16:42
Operator : AJ/MA
Sample : M1207-03
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
FK-SF-03-010-B


Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:35 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 05:24:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

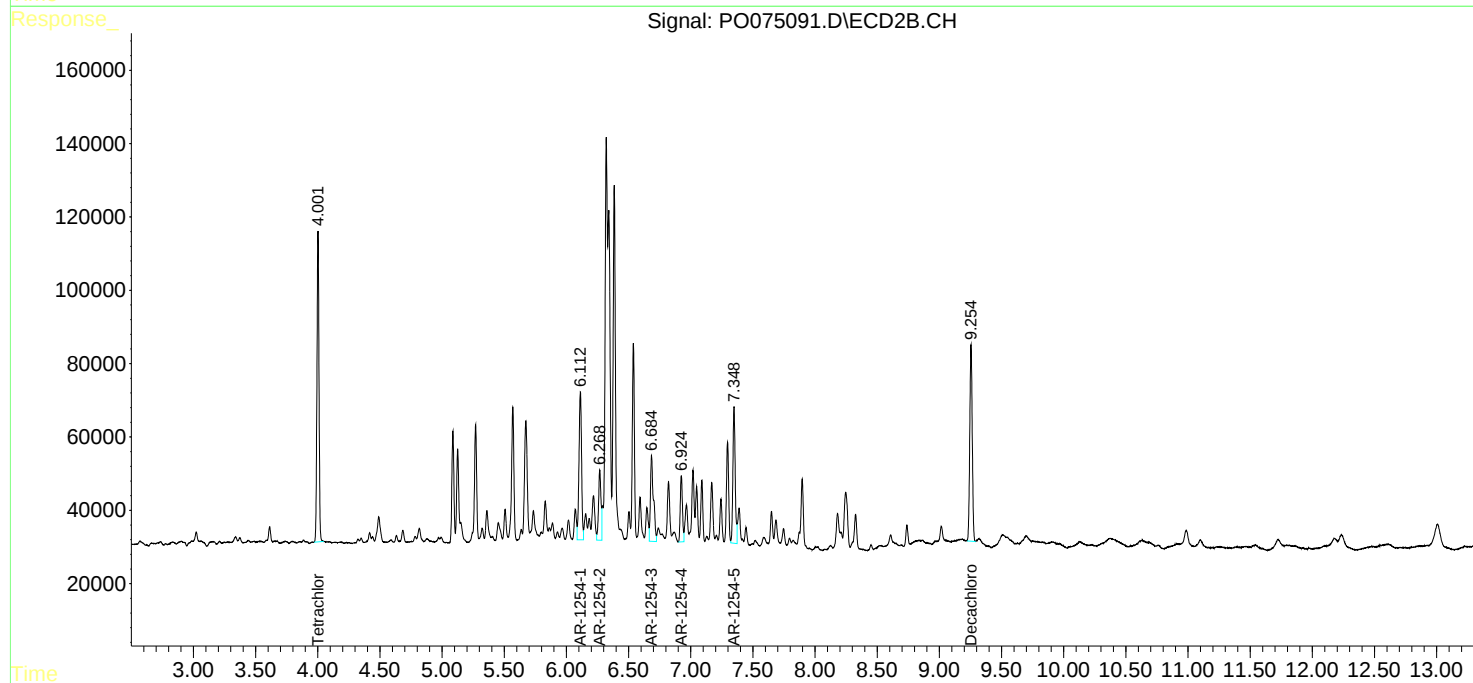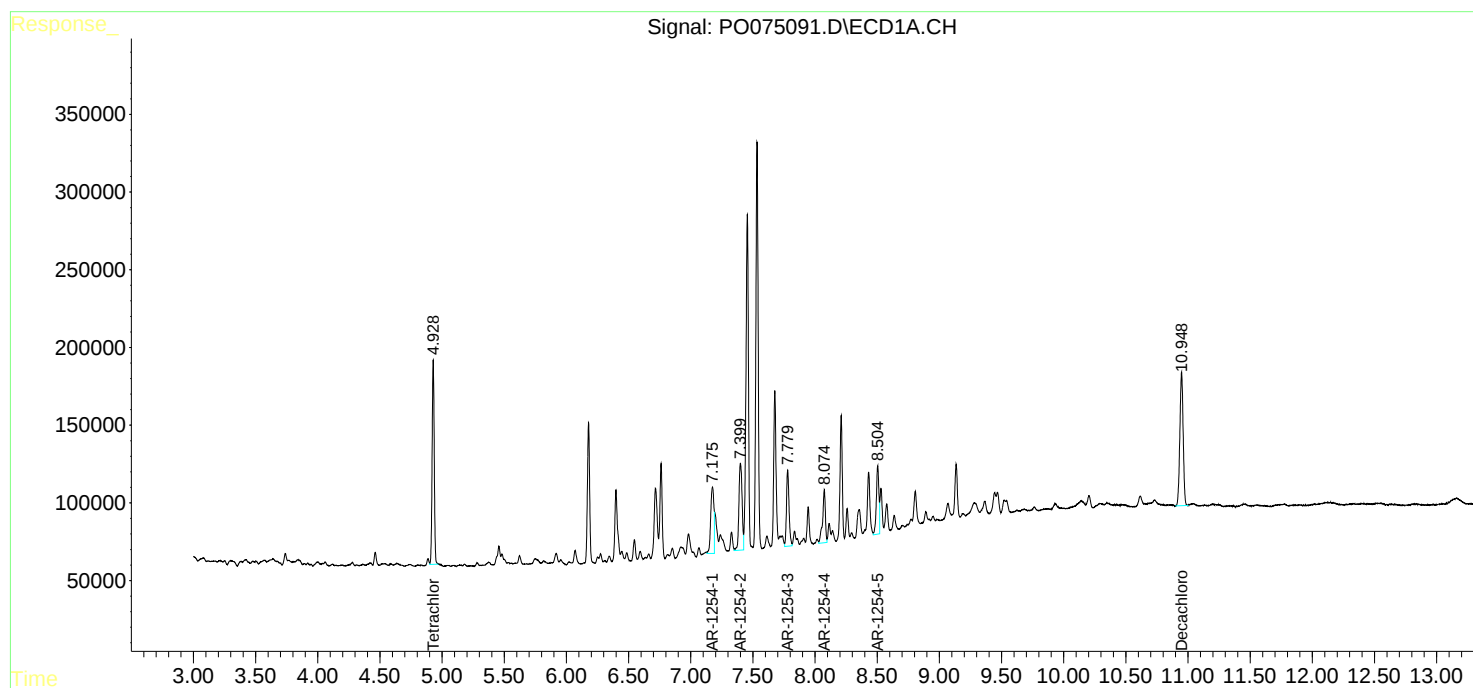

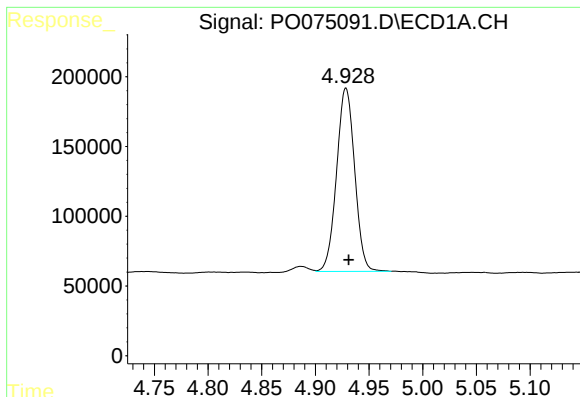


#1 Tetrachloro-m-xylene

R.T.: 4.928 min
Delta R.T.: -0.003 min
Response: 1540914
Conc: 14.60 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-010-B


Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:35 AM

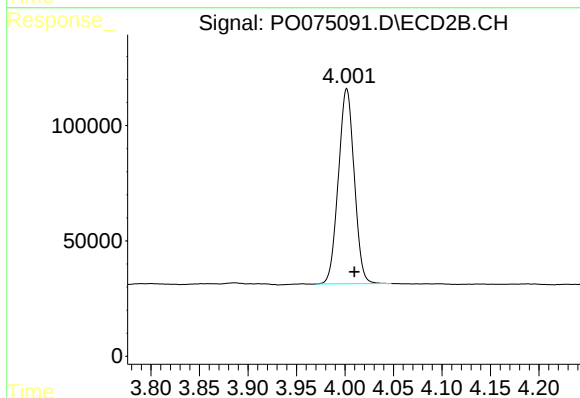


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.008 min
Response: 963265
Conc: 17.12 ng/ml

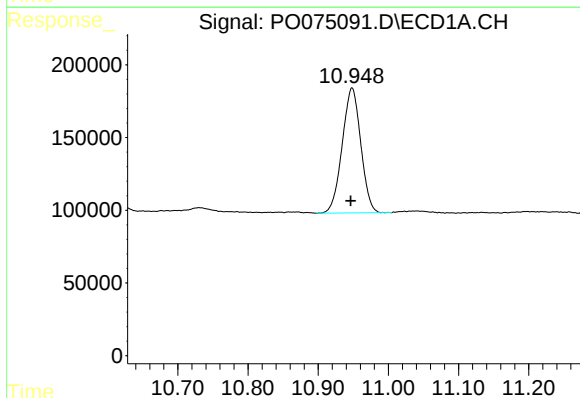


#2 Decachlorobiphenyl

R.T.: 10.948 min
Delta R.T.: 0.002 min
Response: 1579889
Conc: 15.57 ng/ml

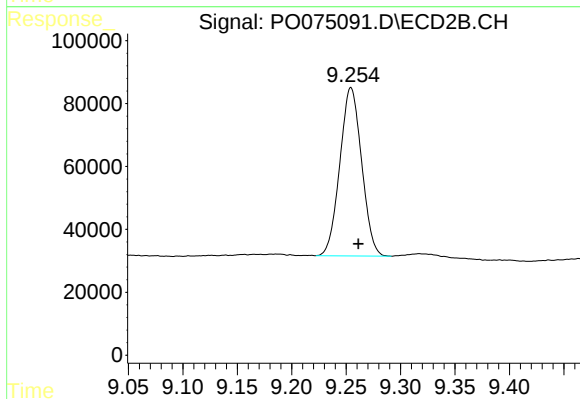

#2 Decachlorobiphenyl

R.T.: 9.254 min
Delta R.T.: -0.007 min
Response: 745023
Conc: 13.57 ng/ml

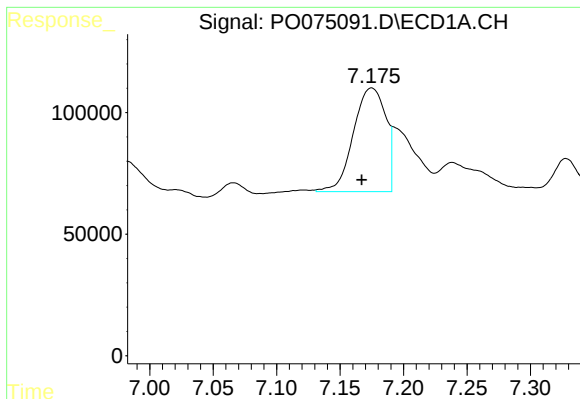


#26 AR-1254-1

R.T.: 7.175 min
Delta R.T.: 0.007 min
Response: 752396
Conc: 171.07 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-010-B


Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:35 AM

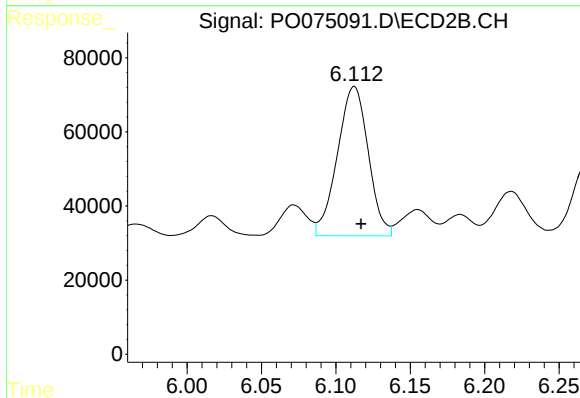


#26 AR-1254-1

R.T.: 6.112 min
Delta R.T.: -0.005 min
Response: 582439
Conc: 161.25 ng/ml

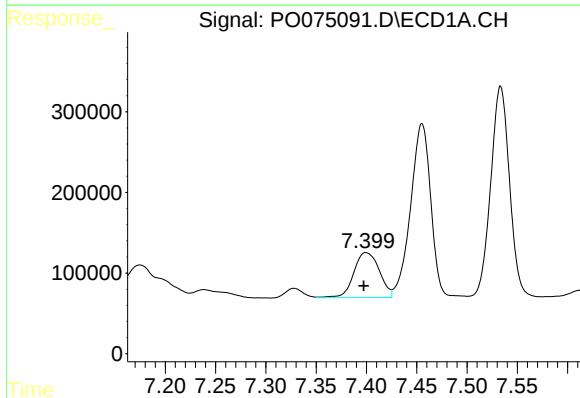


#27 AR-1254-2

R.T.: 7.400 min
Delta R.T.: 0.002 min
Response: 989338
Conc: 145.26 ng/ml

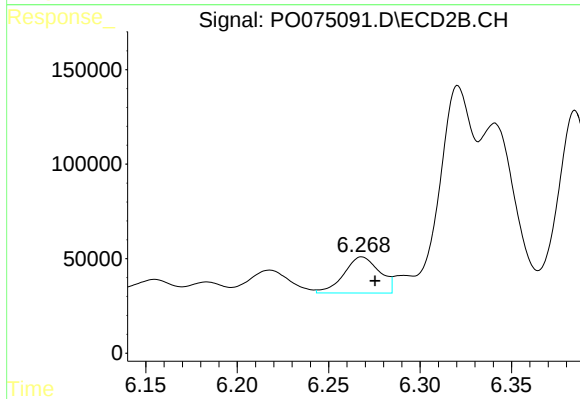

#27 AR-1254-2

R.T.: 6.268 min
Delta R.T.: -0.007 min
Response: 259618
Conc: 83.30 ng/ml

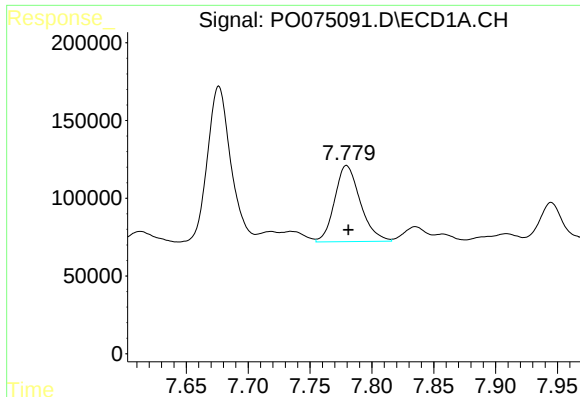


#28 AR-1254-3

R.T.: 7.780 min
Delta R.T.: -0.001 min
Response: 706933
Conc: 100.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-010-B


Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:35 AM

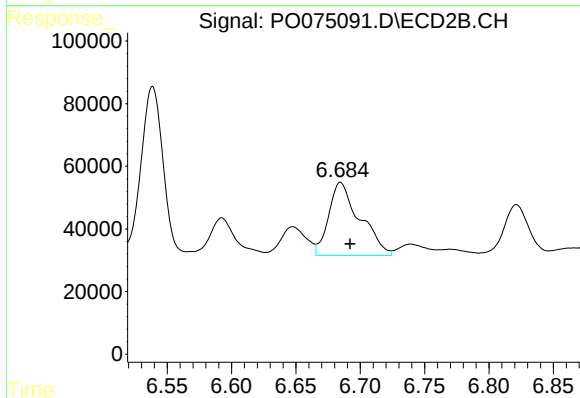


#28 AR-1254-3

R.T.: 6.685 min
Delta R.T.: -0.008 min
Response: 394229
Conc: 80.39 ng/ml

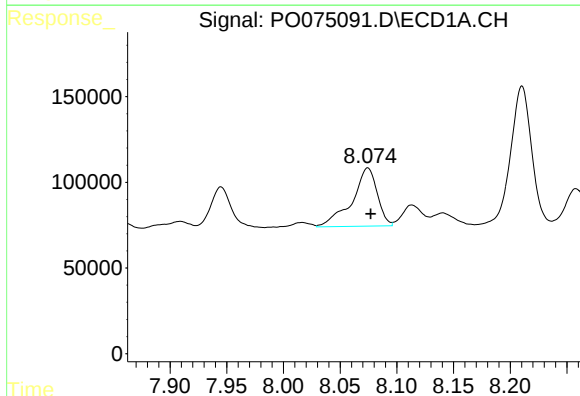


#29 AR-1254-4

R.T.: 8.074 min
Delta R.T.: -0.003 min
Response: 528467
Conc: 87.14 ng/ml

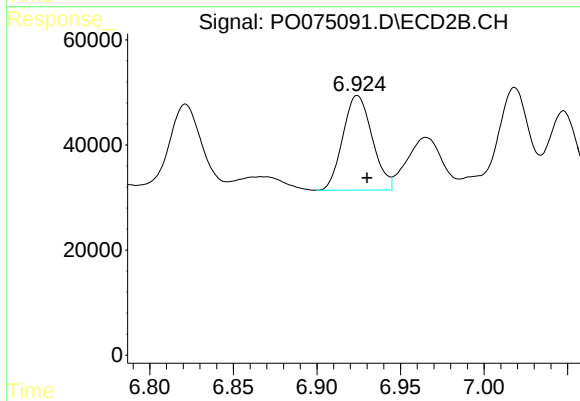

#29 AR-1254-4

R.T.: 6.924 min
Delta R.T.: -0.006 min
Response: 220566
Conc: 63.60 ng/ml

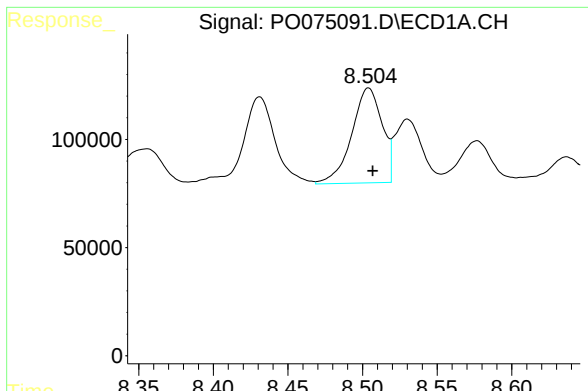


#30 AR-1254-5

R.T.: 8.504 min
Delta R.T.: -0.003 min
Response: 623199
Conc: 107.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-010-B

Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:35 AM

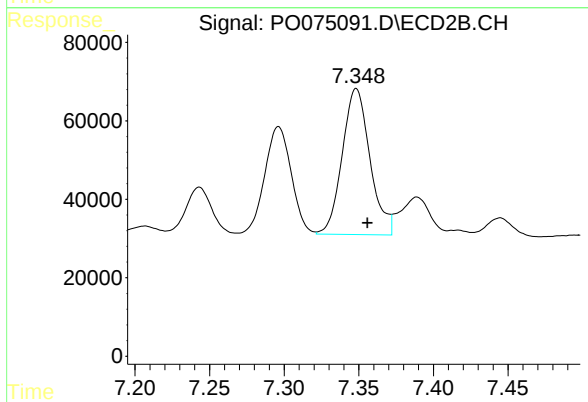

#30 AR-1254-5

R.T.: 7.348 min
Delta R.T.: -0.008 min
Response: 481384
Conc: 106.36 ng/ml