

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012221\
 Data File : P0075092.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2021 16:59
 Operator : AJ/MA
 Sample : M1208-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-SF-03-011-A

Manual Integrations
 APPROVED

Ankita
 1/25/2021 10:48:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 05:24:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.928	4.002	1696214	1091740	16.075	19.408
2)	SA Decachlor...	10.946	9.254	1731516	802452	17.061	14.615
Target Compounds							
26)	L6 AR-1254-1	7.175	6.113	790498	587044	179.735m	162.526
27)	L6 AR-1254-2	7.401	6.267	1001871	185177	147.101	59.418 #
28)	L6 AR-1254-3	7.780	6.685	668639	353416	95.325	72.068
29)	L6 AR-1254-4	8.072	6.924	393987	189069	64.964m	54.521
30)	L6 AR-1254-5	8.503	7.348	565368	585863	97.327	129.445 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012221\
Data File : PO075092.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2021 16:59
Operator : AJ/MA
Sample : M1208-01
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
FK-SF-03-011-A


Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 05:24:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

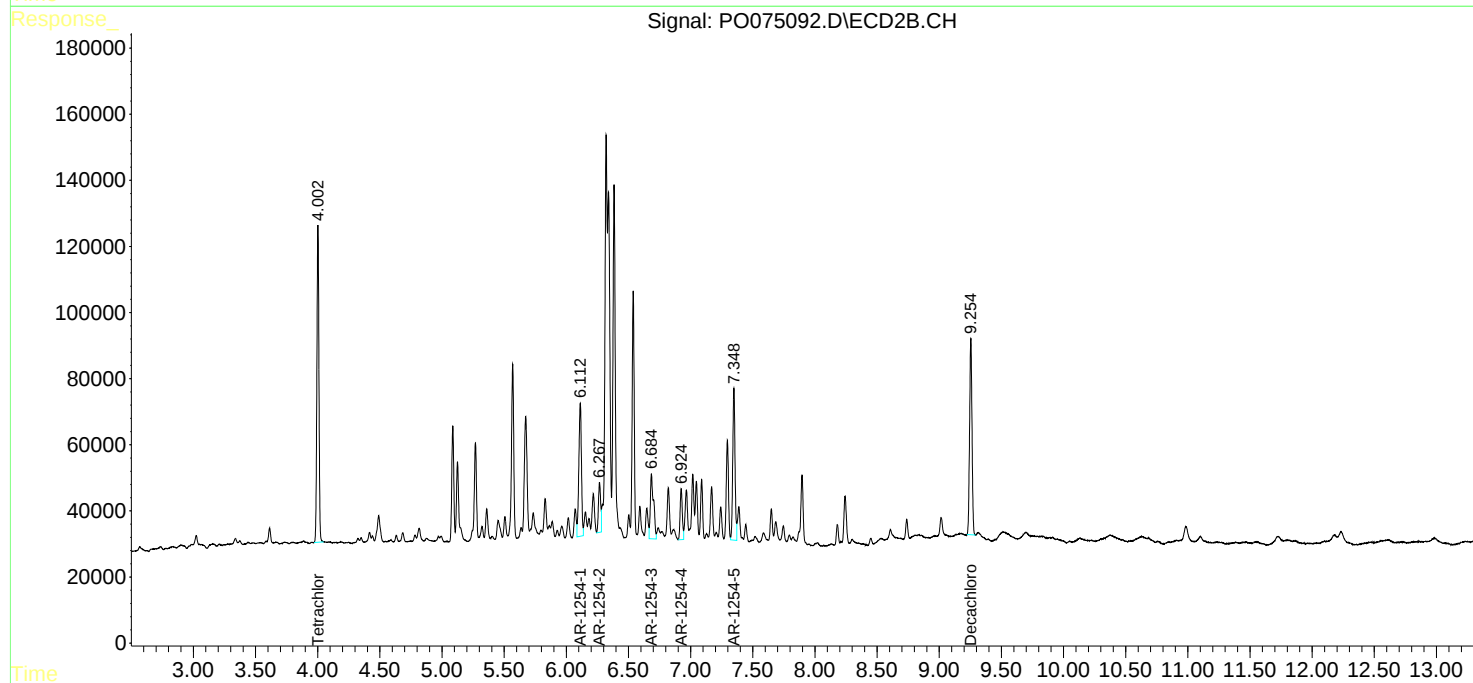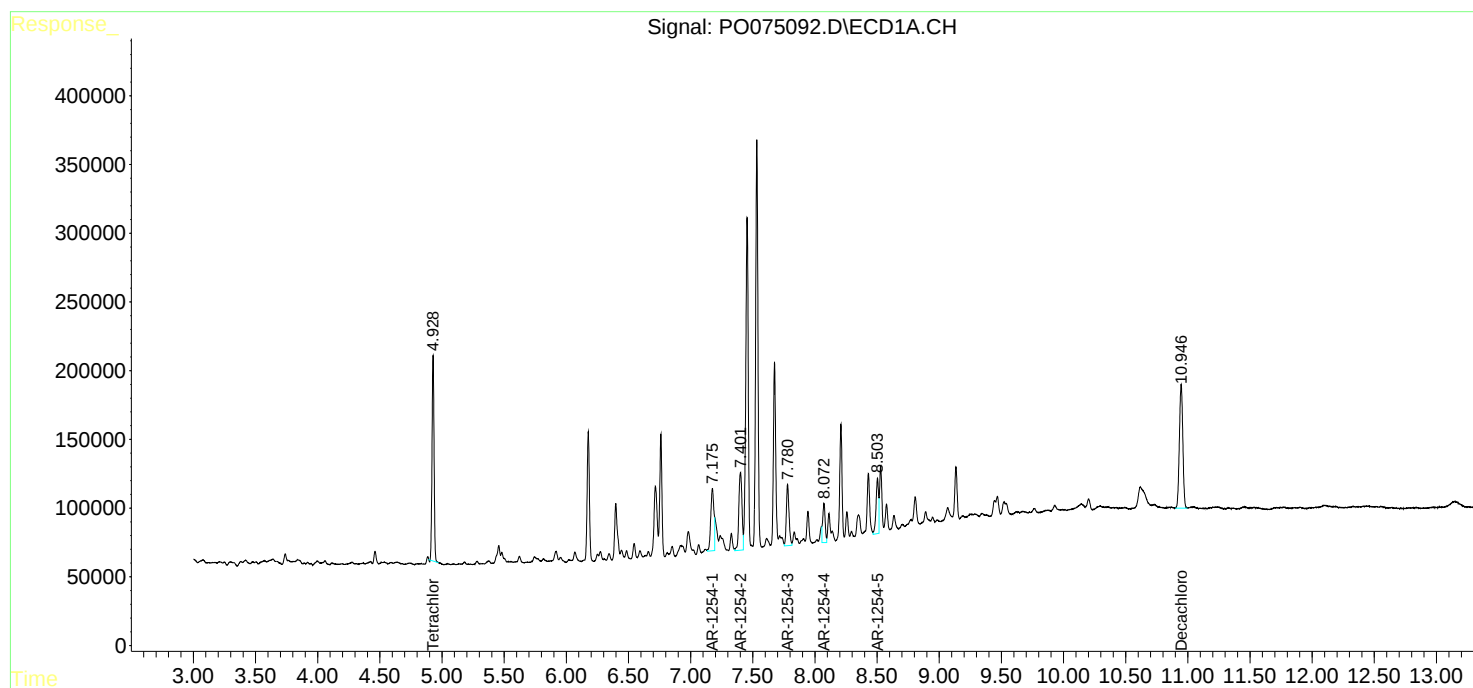

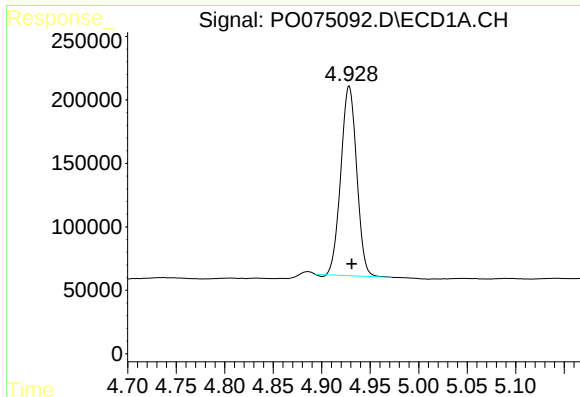


#1 Tetrachloro-m-xylene

R.T.: 4.928 min
Delta R.T.: -0.003 min
Response: 1696214
Conc: 16.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-011-A


Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:37 AM

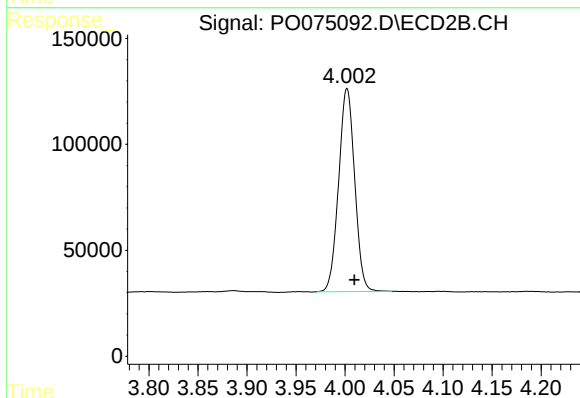


#1 Tetrachloro-m-xylene

R.T.: 4.002 min
Delta R.T.: -0.008 min
Response: 1091740
Conc: 19.41 ng/ml

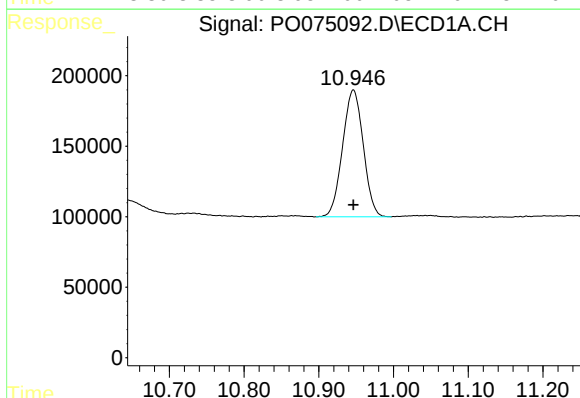


#2 Decachlorobiphenyl

R.T.: 10.946 min
Delta R.T.: 0.000 min
Response: 1731516
Conc: 17.06 ng/ml

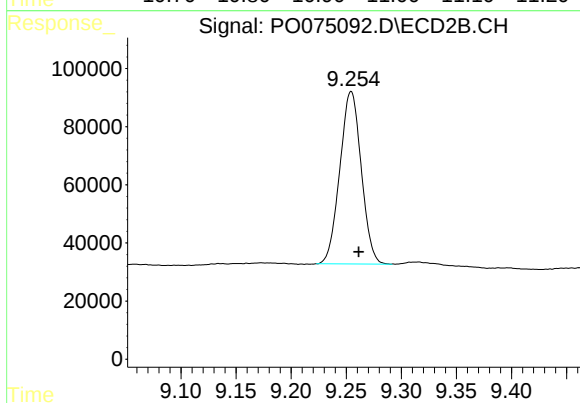

#2 Decachlorobiphenyl

R.T.: 9.254 min
Delta R.T.: -0.007 min
Response: 802452
Conc: 14.62 ng/ml

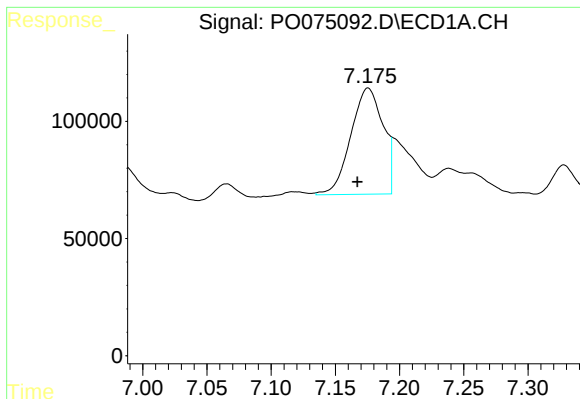


#26 AR-1254-1

R.T.: 7.175 min
Delta R.T.: 0.008 min
Response: 790498
Conc: 179.73 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-011-A


Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:37 AM

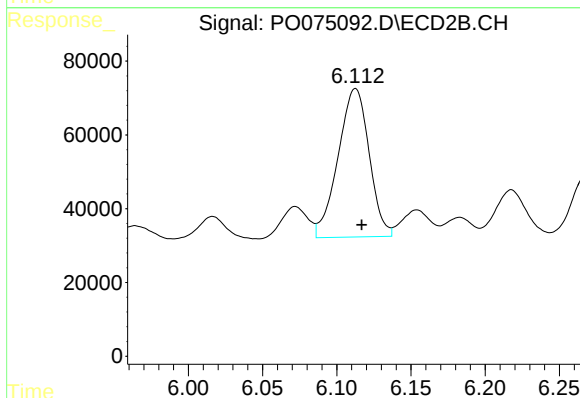


#26 AR-1254-1

R.T.: 6.113 min
Delta R.T.: -0.004 min
Response: 587044
Conc: 162.53 ng/ml

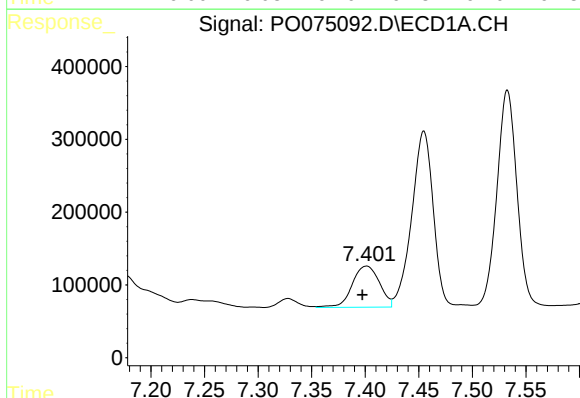


#27 AR-1254-2

R.T.: 7.401 min
Delta R.T.: 0.004 min
Response: 1001871
Conc: 147.10 ng/ml

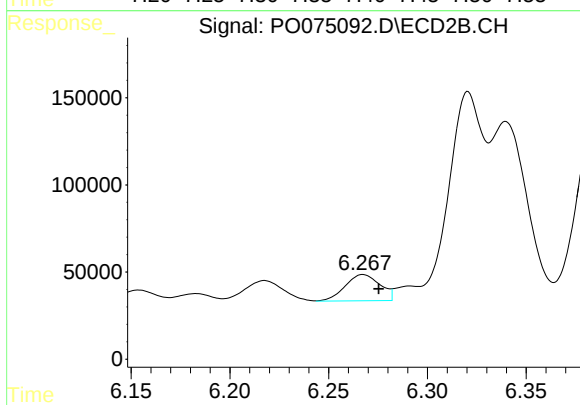

#27 AR-1254-2

R.T.: 6.267 min
Delta R.T.: -0.008 min
Response: 185177
Conc: 59.42 ng/ml

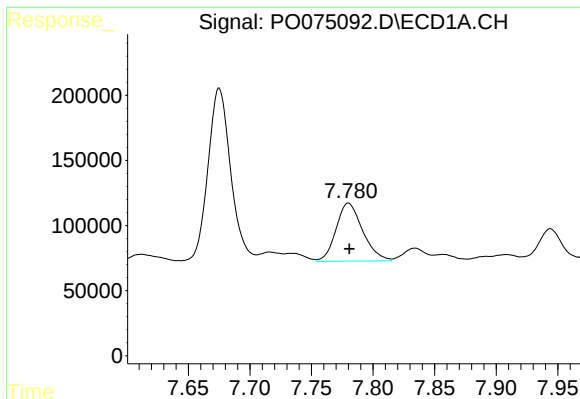


#28 AR-1254-3

R.T.: 7.780 min
Delta R.T.: 0.000 min
Response: 668639
Conc: 95.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-011-A


Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:37 AM

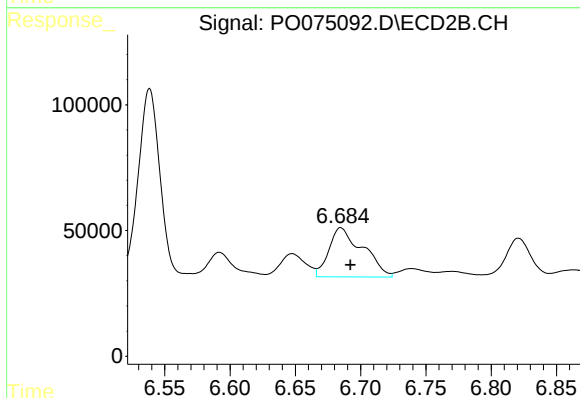


#28 AR-1254-3

R.T.: 6.685 min
Delta R.T.: -0.007 min
Response: 353416
Conc: 72.07 ng/ml

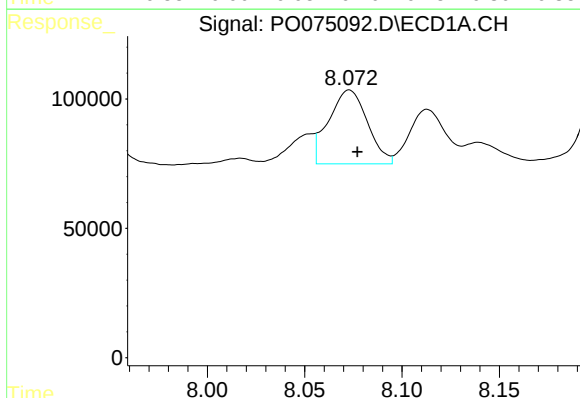


#29 AR-1254-4

R.T.: 8.072 min
Delta R.T.: -0.005 min
Response: 393987
Conc: 64.96 ng/ml m

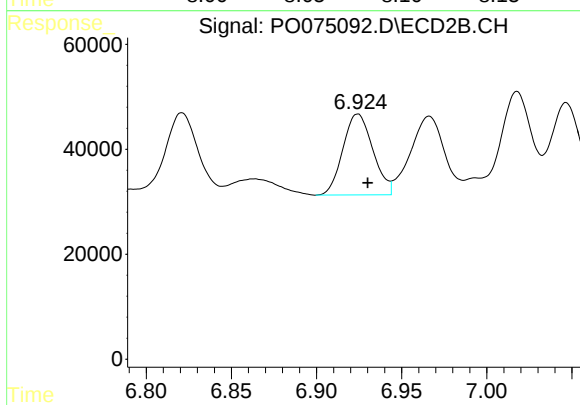

#29 AR-1254-4

R.T.: 6.924 min
Delta R.T.: -0.006 min
Response: 189069
Conc: 54.52 ng/ml

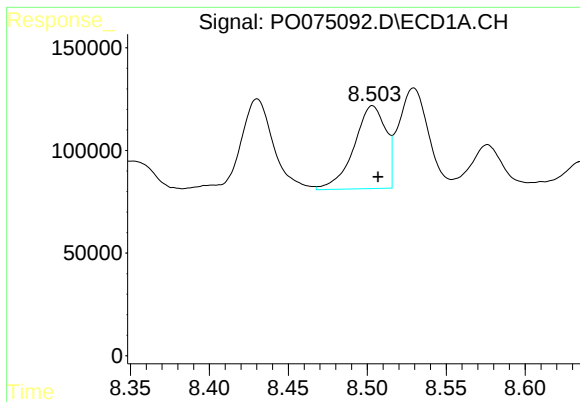


#30 AR-1254-5

R.T.: 8.503 min
Delta R.T.: -0.004 min
Response: 565368
Conc: 97.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-011-A

Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:37 AM

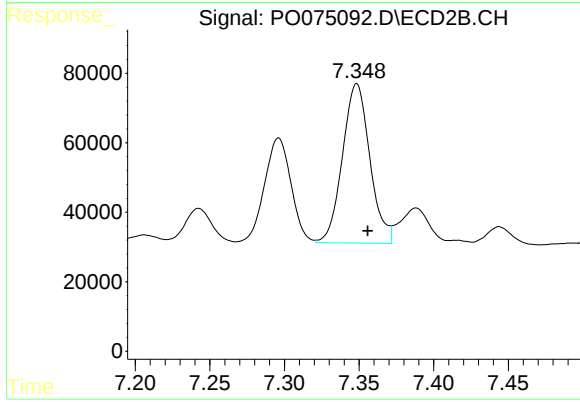

#30 AR-1254-5

R.T.: 7.348 min
Delta R.T.: -0.007 min
Response: 585863
Conc: 129.45 ng/ml