

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012221\
 Data File : P0075093.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2021 17:16
 Operator : AJ/MA
 Sample : M1208-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-SF-03-011-B

Manual Integrations
 APPROVED

Ankita
 1/25/2021 10:48:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 05:24:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.930	4.003	1640937	1041902	15.551	18.522
2) SA Decachlor...	10.948	9.255	1661863	779480	16.374	14.197
Target Compounds						
26) L6 AR-1254-1	7.177	6.114	768859	586296	174.815m	162.319
27) L6 AR-1254-2	7.402	6.269	993290	199164	145.841	63.905 #
28) L6 AR-1254-3	7.782	6.685	610444	199483	87.028	40.678 #
29) L6 AR-1254-4	8.075	6.926	304382	147586	50.189m	42.559
30) L6 AR-1254-5	8.505	7.350	430907	425907	74.180	94.104 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012221\
Data File : PO075093.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2021 17:16
Operator : AJ/MA
Sample : M1208-03
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
FK-SF-03-011-B


Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:39 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 05:24:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

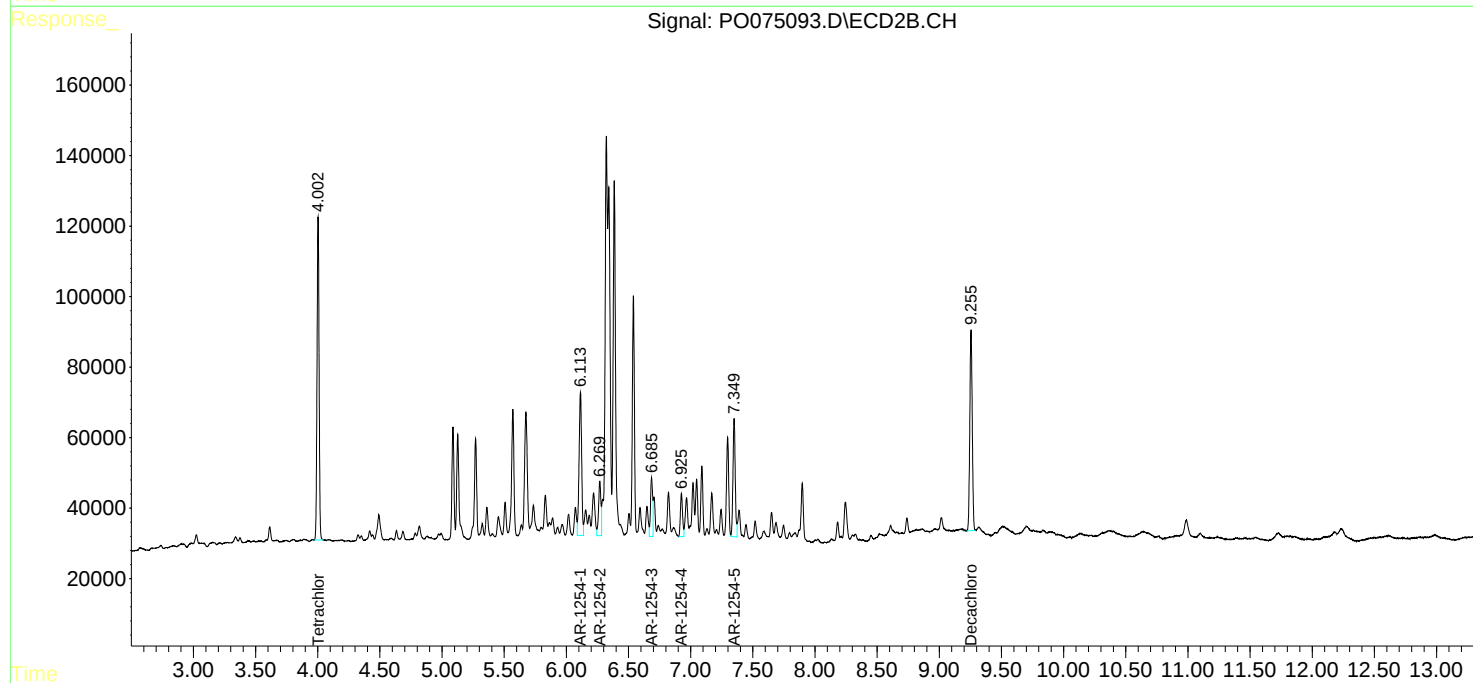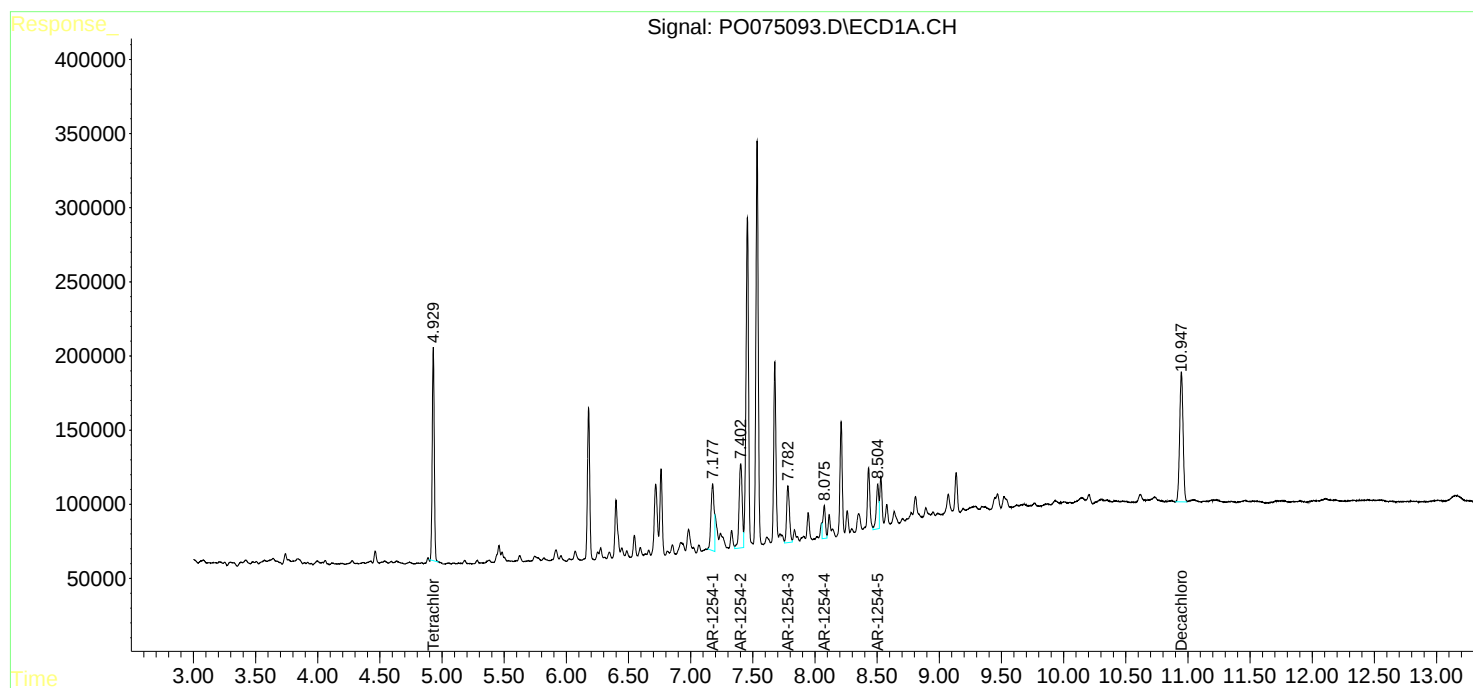

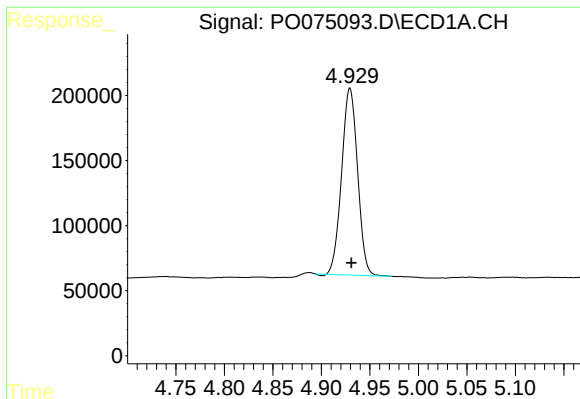


#1 Tetrachloro-m-xylene

R.T.: 4.930 min
Delta R.T.: -0.001 min
Response: 1640937
Conc: 15.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-011-B


Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:39 AM

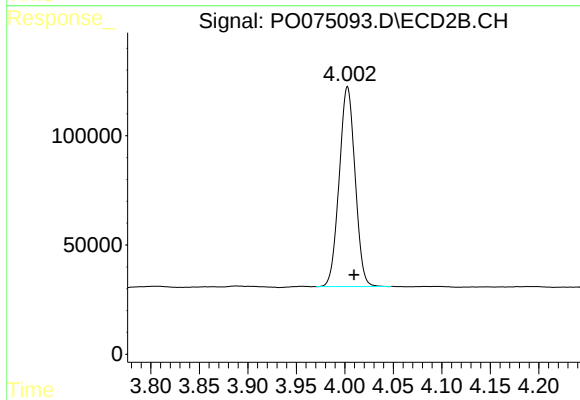


#1 Tetrachloro-m-xylene

R.T.: 4.003 min
Delta R.T.: -0.007 min
Response: 1041902
Conc: 18.52 ng/ml

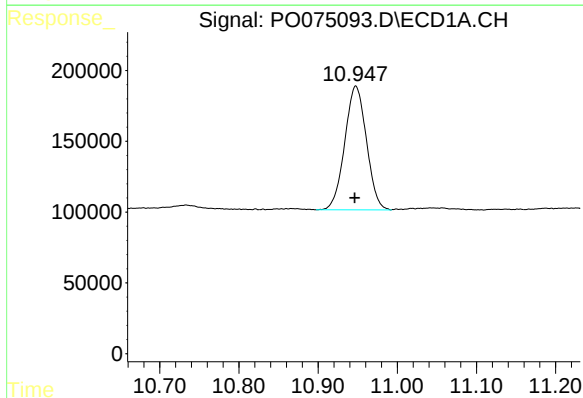


#2 Decachlorobiphenyl

R.T.: 10.948 min
Delta R.T.: 0.001 min
Response: 1661863
Conc: 16.37 ng/ml

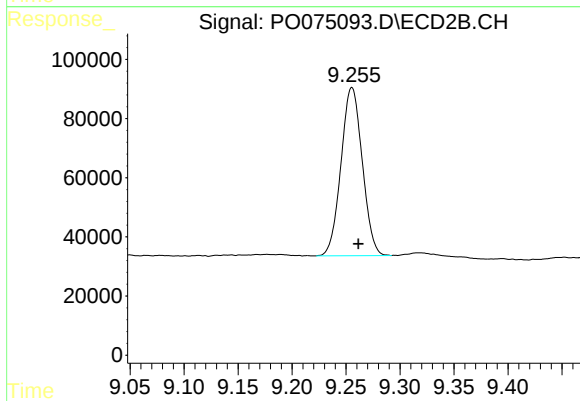

#2 Decachlorobiphenyl

R.T.: 9.255 min
Delta R.T.: -0.006 min
Response: 779480
Conc: 14.20 ng/ml

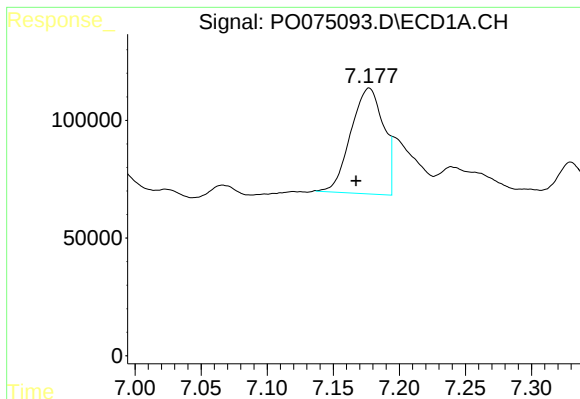


#26 AR-1254-1

R.T.: 7.177 min
Delta R.T.: 0.010 min
Response: 768859
Conc: 174.81 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-011-B


Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:39 AM

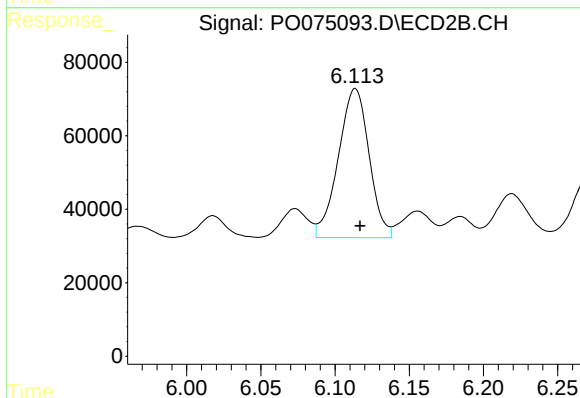


#26 AR-1254-1

R.T.: 6.114 min
Delta R.T.: -0.003 min
Response: 586296
Conc: 162.32 ng/ml

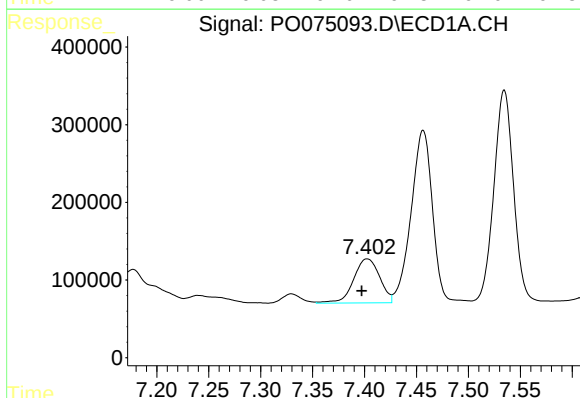


#27 AR-1254-2

R.T.: 7.402 min
Delta R.T.: 0.005 min
Response: 993290
Conc: 145.84 ng/ml

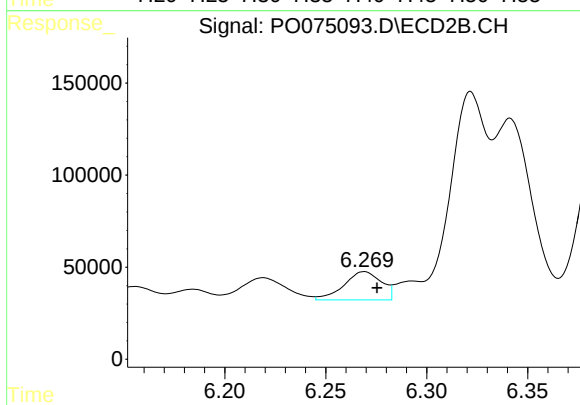

#27 AR-1254-2

R.T.: 6.269 min
Delta R.T.: -0.006 min
Response: 199164
Conc: 63.91 ng/ml

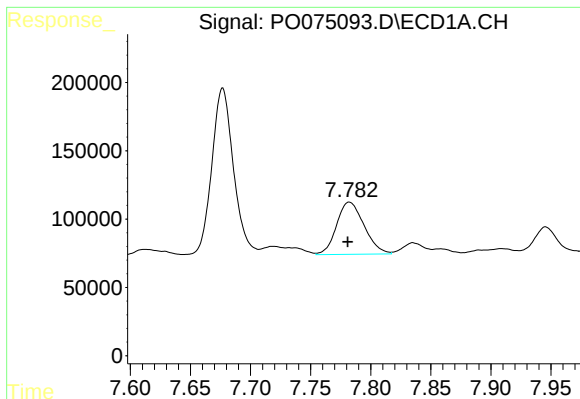


#28 AR-1254-3

R.T.: 7.782 min
Delta R.T.: 0.001 min
Response: 610444
Conc: 87.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-011-B


Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:39 AM

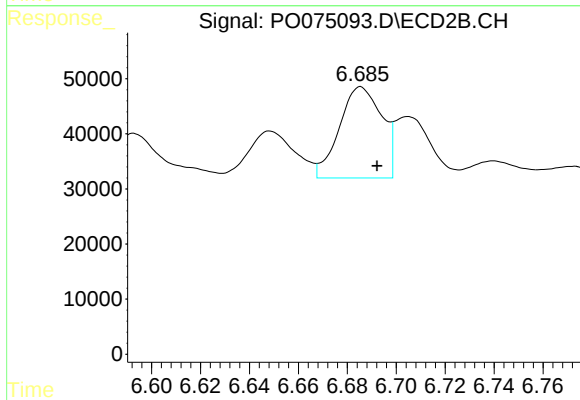


#28 AR-1254-3

R.T.: 6.685 min
Delta R.T.: -0.007 min
Response: 199483
Conc: 40.68 ng/ml

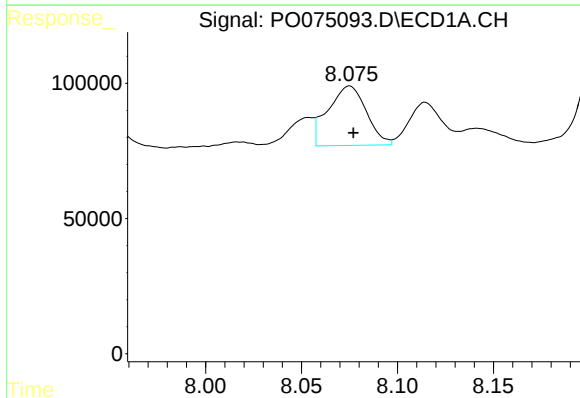


#29 AR-1254-4

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 304382
Conc: 50.19 ng/ml m

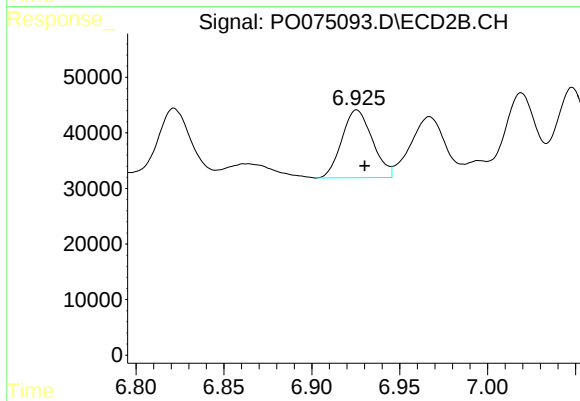

#29 AR-1254-4

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 147586
Conc: 42.56 ng/ml

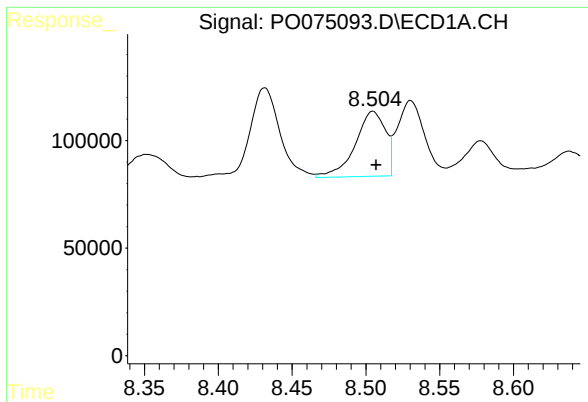


#30 AR-1254-5

R.T.: 8.505 min
Delta R.T.: -0.002 min
Response: 430907
Conc: 74.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-03-011-B

Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:39 AM

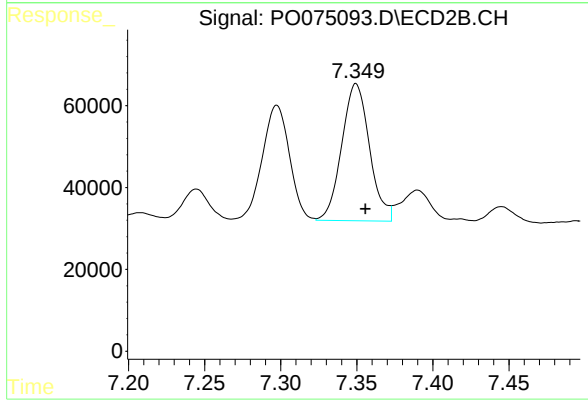

#30 AR-1254-5

R.T.: 7.350 min
Delta R.T.: -0.006 min
Response: 425907
Conc: 94.10 ng/ml