

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012221\
 Data File : P0075112.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Jan 2021 23:16
 Operator : AJ/MA
 Sample : M1187-01 10X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K77029M-END-1

Manual Integrations
 APPROVED

Ankita
 1/25/2021 10:48:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 23 05:29:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.932	4.004	108126	84344	1.025	1.499 #
2) SA Decachlor...	10.946	9.254	230010	79575	2.266	1.449m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012221\
Data File : P0075112.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Jan 2021 23:16
Operator : AJ/MA
Sample : M1187-01 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
K77029M-END-1


Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 23 05:29:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

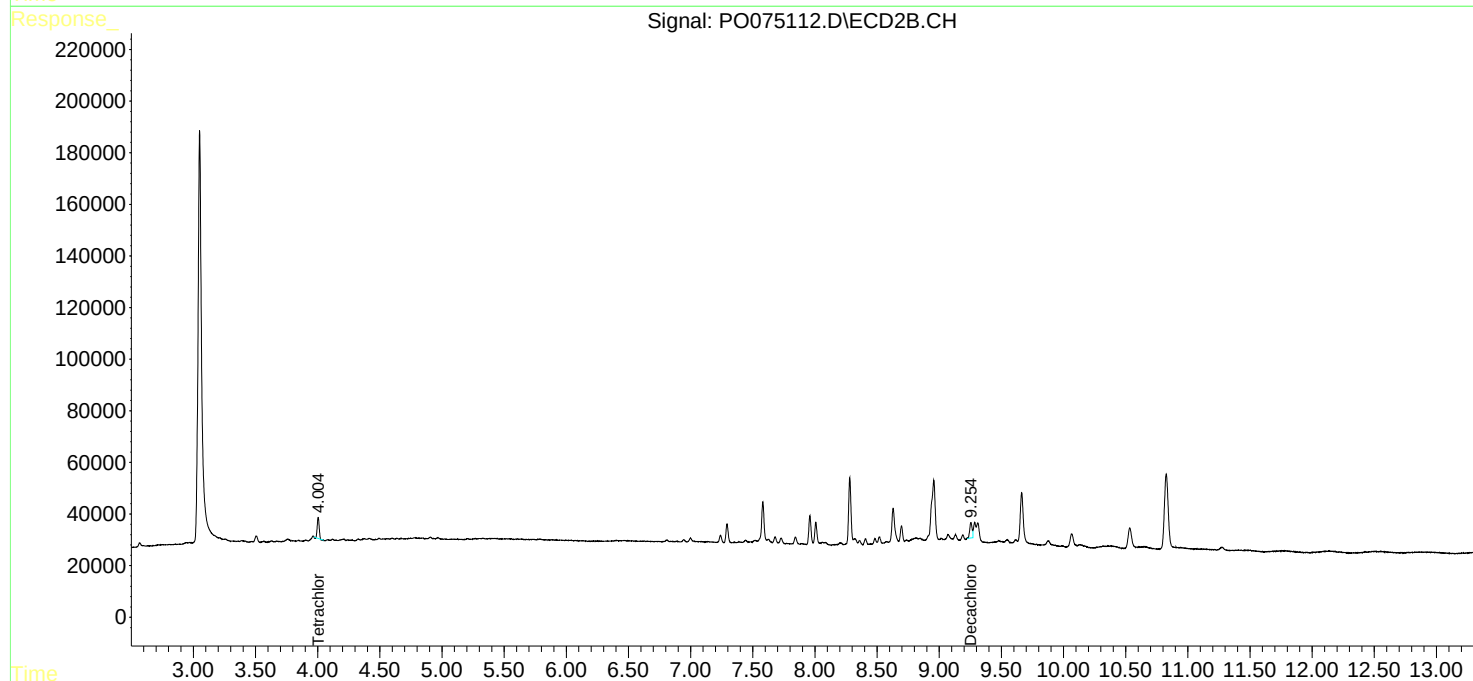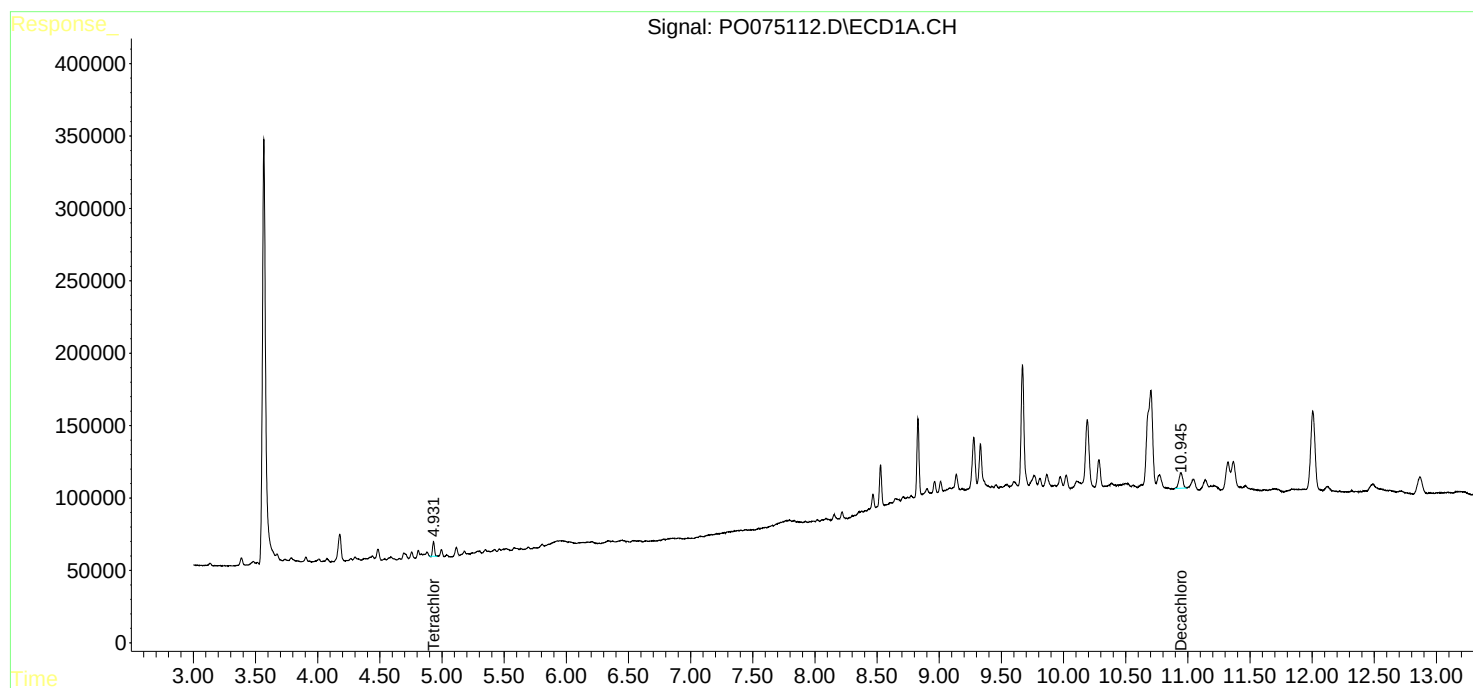

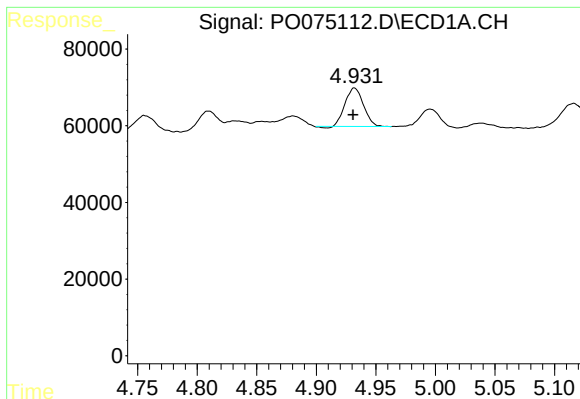


#1 Tetrachloro-m-xylene

R.T.: 4.932 min
Delta R.T.: 0.001 min
Response: 108126
Conc: 1.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
K77029M-END-1


Manual Integrations
APPROVED

Ankita
1/25/2021 10:48:56 AM

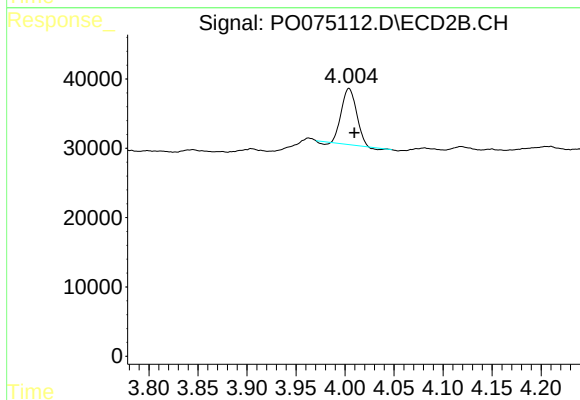


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.006 min
Response: 84344
Conc: 1.50 ng/ml

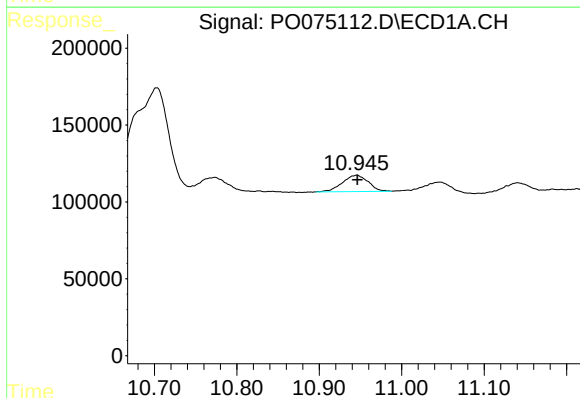

#2 Decachlorobiphenyl

R.T.: 10.946 min
Delta R.T.: 0.000 min
Response: 230010
Conc: 2.27 ng/ml

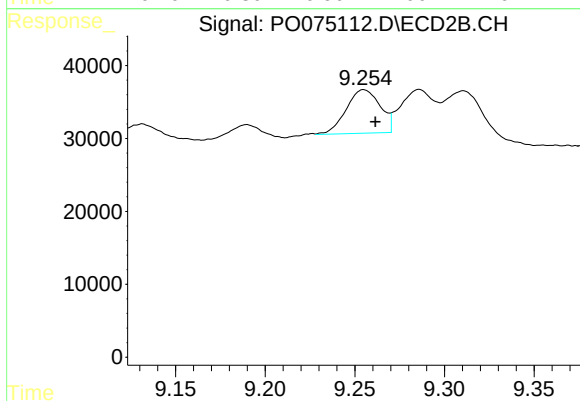

#2 Decachlorobiphenyl

R.T.: 9.254 min
Delta R.T.: -0.007 min
Response: 79575
Conc: 1.45 ng/ml m