

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012320\
 Data File : P0065870.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jan 2020 00:20
 Operator : DD\AJ
 Sample : L1161-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT1-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 04:03:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.154	3.431	290466	334632	12.527	12.598
2) SA Decachlor...	9.648	8.329	554772	661702	13.327	13.616
Target Compounds						
32) L7 AR-1260-2	0.000	6.123	0	23854	N.D.	7.528 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012320\
Data File : PO065870.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jan 2020 00:20
Operator : DD\AJ
Sample : L1161-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 04:03:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

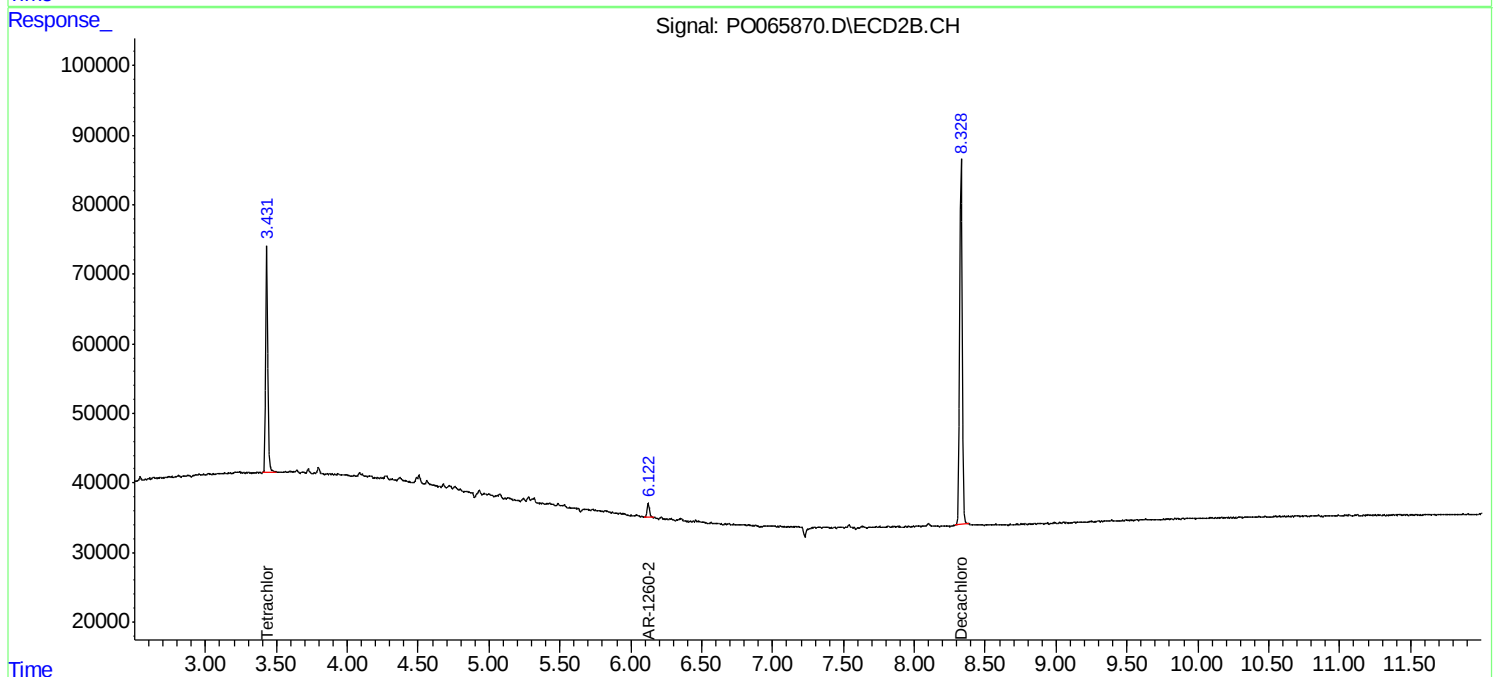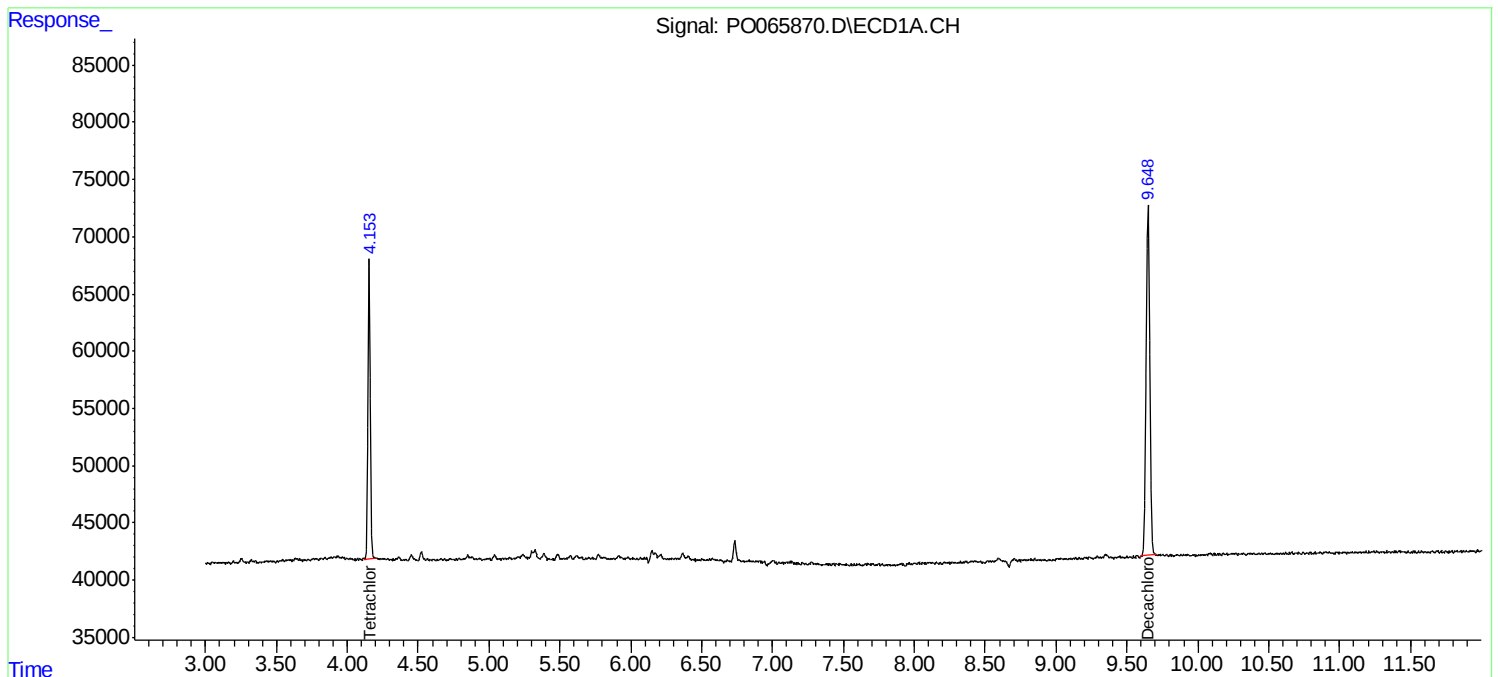


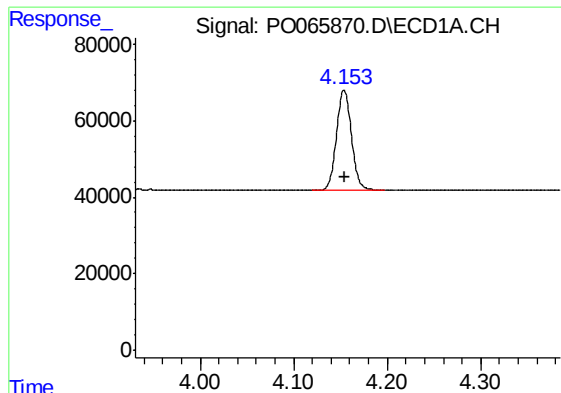

#1 Tetrachloro-m-xylene


R.T.: 4.154 min
Delta R.T.: -0.001 min
Response: 290466
Conc: 12.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020

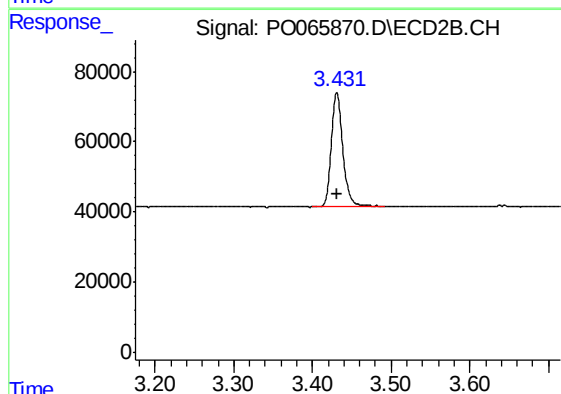


#1 Tetrachloro-m-xylene

R.T.: 3.431 min
Delta R.T.: 0.000 min
Response: 334632
Conc: 12.60 ng/ml

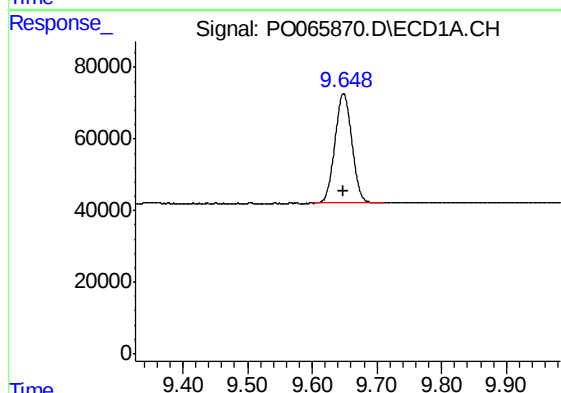


#2 Decachlorobiphenyl

R.T.: 9.648 min
Delta R.T.: 0.000 min
Response: 554772
Conc: 13.33 ng/ml

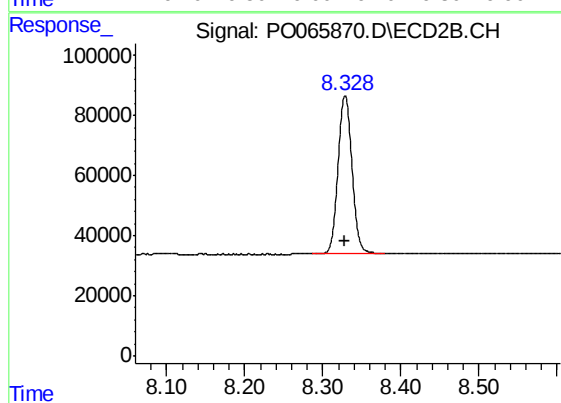

#2 Decachlorobiphenyl


R.T.: 8.329 min
Delta R.T.: 0.000 min
Response: 661702
Conc: 13.62 ng/ml

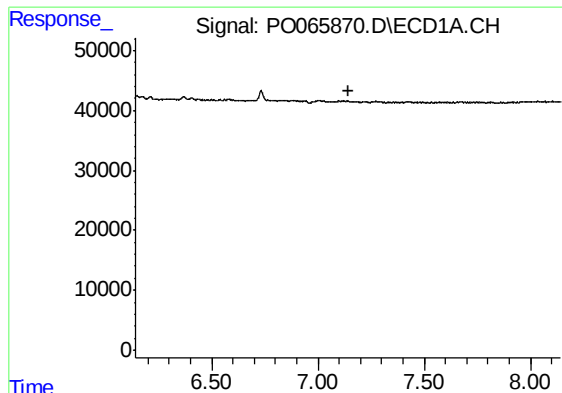

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.142 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020

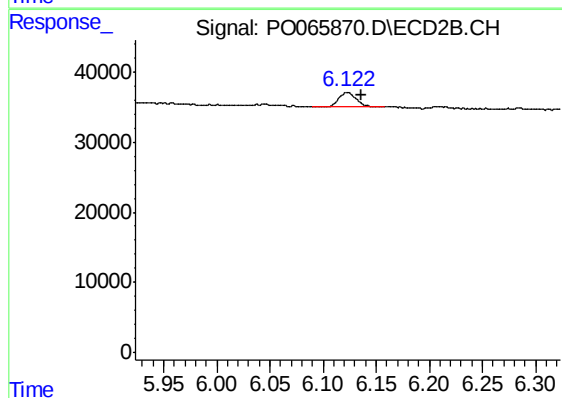

#32 AR-1260-2

R.T.: 6.123 min
Delta R.T.: -0.013 min
Response: 23854
Conc: 7.53 ng/ml