

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012320\
 Data File : P0065871.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jan 2020 00:36
 Operator : DD\AJ
 Sample : L1161-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT1-2020

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 04:04:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.154	3.431	250312	283936	10.795	10.690
2)	SA Decachlor...	9.649	8.329	499547	600102	12.000	12.349
Target Compounds							
7)	L1 AR-1016-5	0.000	4.930	0	22955	N.D.	21.291 #
15)	L3 AR-1232-5	0.000	4.930	0	22955	N.D.	57.607 #
20)	L4 AR-1242-5	0.000	5.277	0	25353	N.D.	22.902 #
24)	L5 AR-1248-4	0.000	4.930	0	22955	N.D.	17.989 #
25)	L5 AR-1248-5	0.000	5.277	0	25353	N.D.	18.165 #
26)	L6 AR-1254-1	0.000	5.277	0	25353	N.D.	11.339 #
32)	L7 AR-1260-2	0.000	6.124	0	22055	N.D.	6.960 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012320\
Data File : PO065871.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jan 2020 00:36
Operator : DD\AJ
Sample : L1161-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 04:04:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

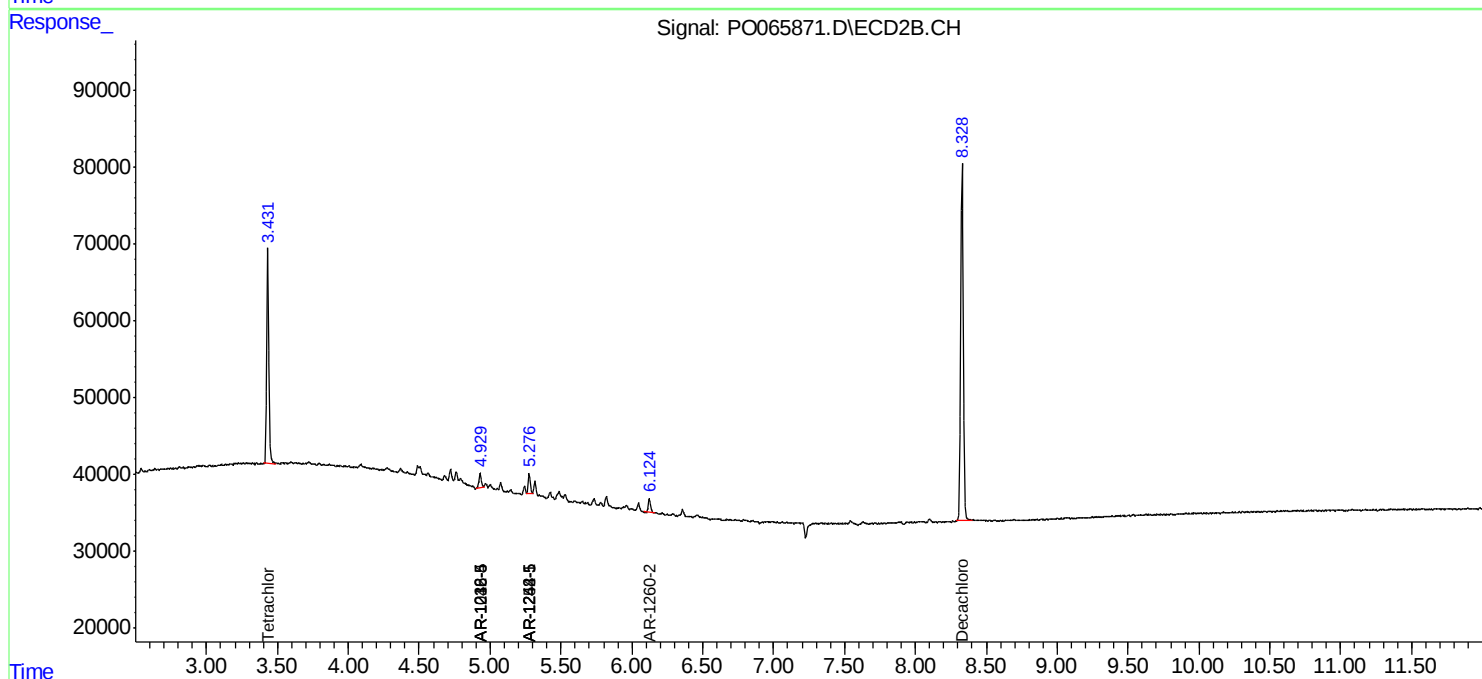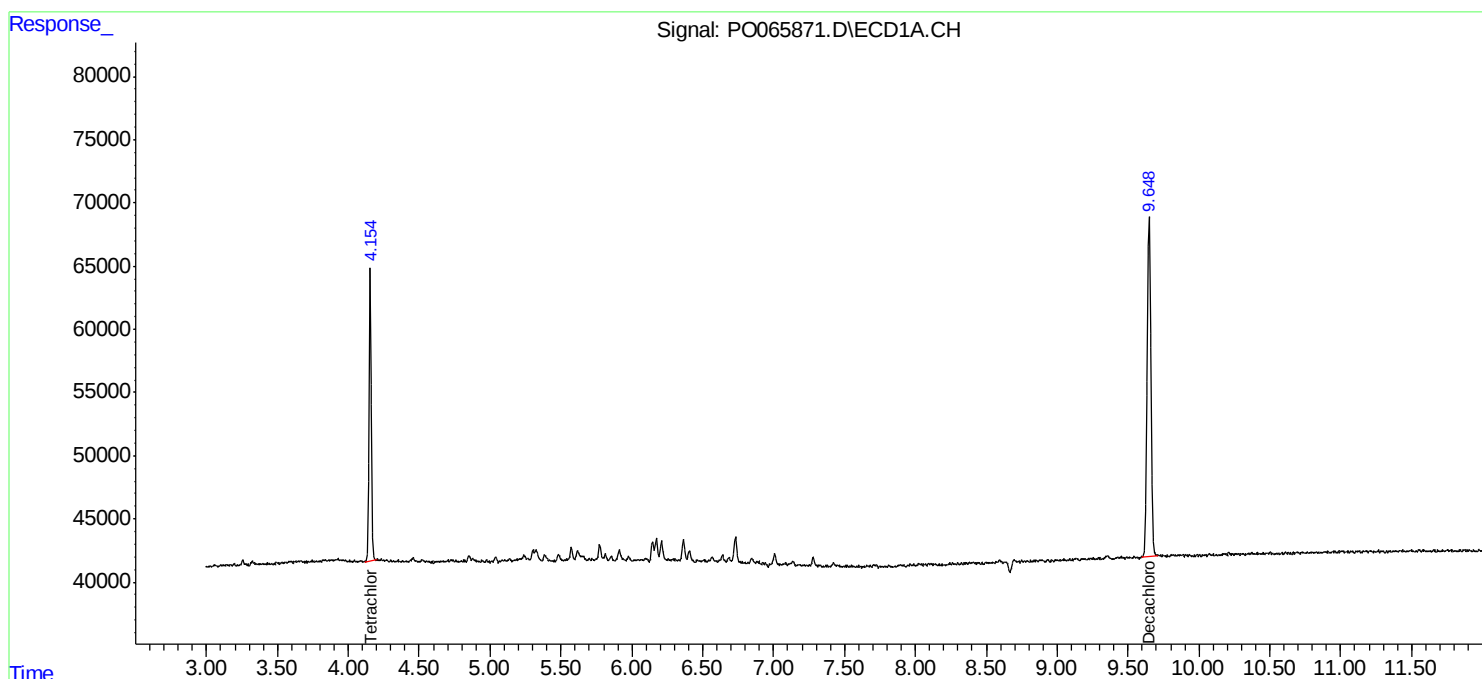


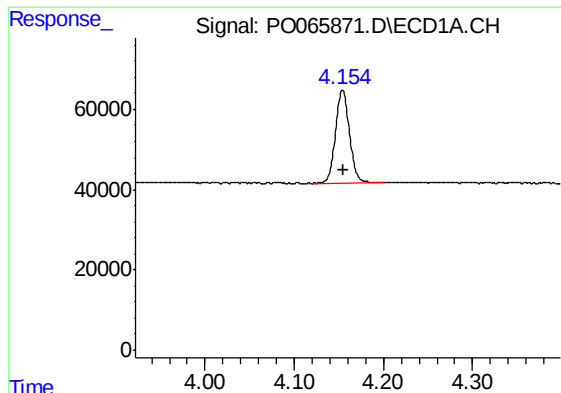

#1 Tetrachloro-m-xylene


R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 250312
Conc: 10.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020

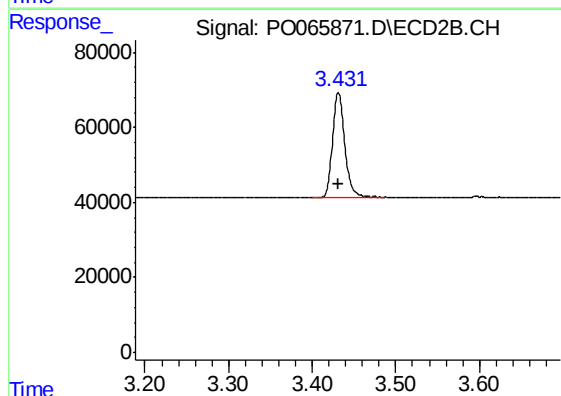


#1 Tetrachloro-m-xylene

R.T.: 3.431 min
Delta R.T.: 0.000 min
Response: 283936
Conc: 10.69 ng/ml

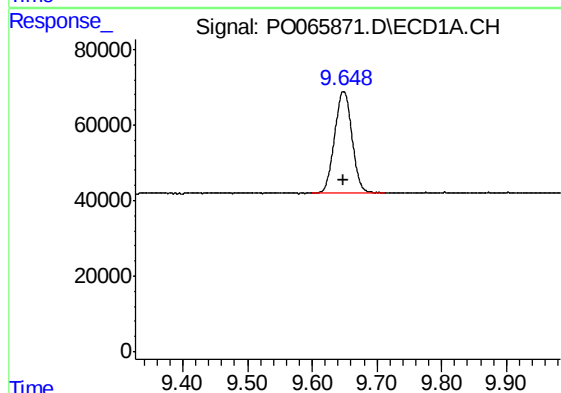


#2 Decachlorobiphenyl

R.T.: 9.649 min
Delta R.T.: 0.000 min
Response: 499547
Conc: 12.00 ng/ml

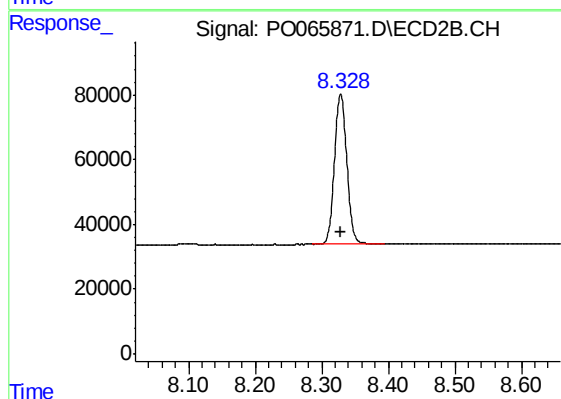

#2 Decachlorobiphenyl


R.T.: 8.329 min
Delta R.T.: 0.000 min
Response: 600102
Conc: 12.35 ng/ml

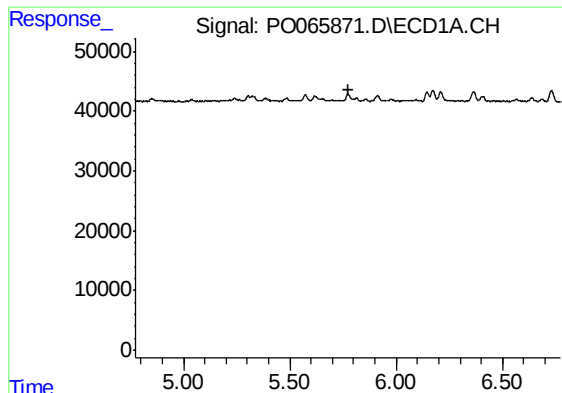

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 5.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020

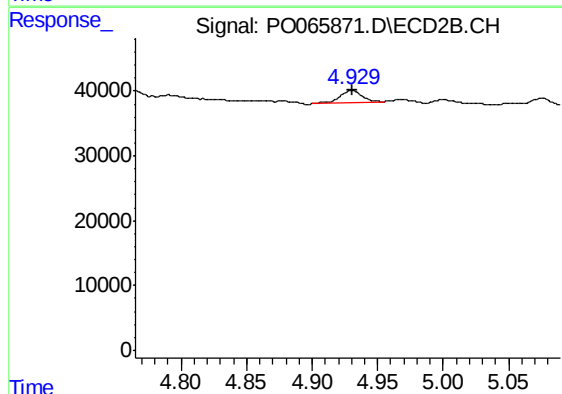


#7 AR-1016-5

R.T.: 4.930 min
Delta R.T.: 0.000 min
Response: 22955
Conc: 21.29 ng/ml

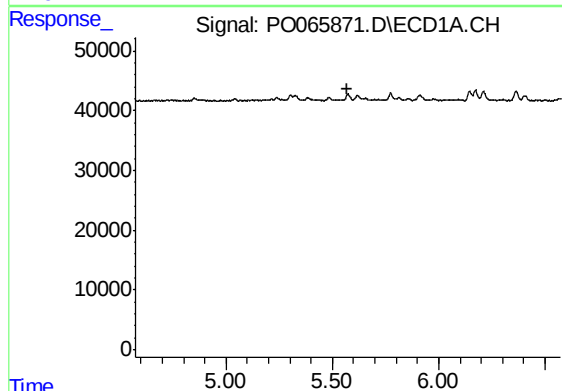


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.573 min
Response: 0
Conc: N.D.

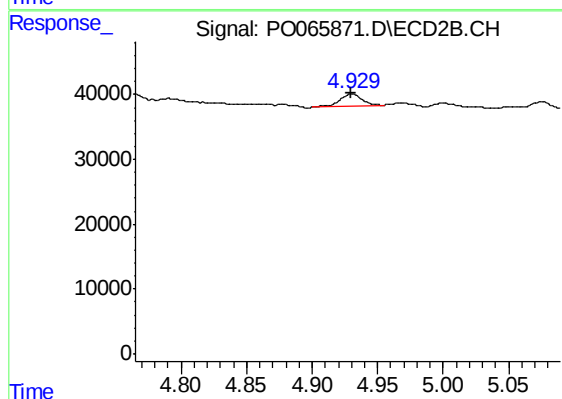

#15 AR-1232-5


R.T.: 4.930 min
Delta R.T.: 0.000 min
Response: 22955
Conc: 57.61 ng/ml

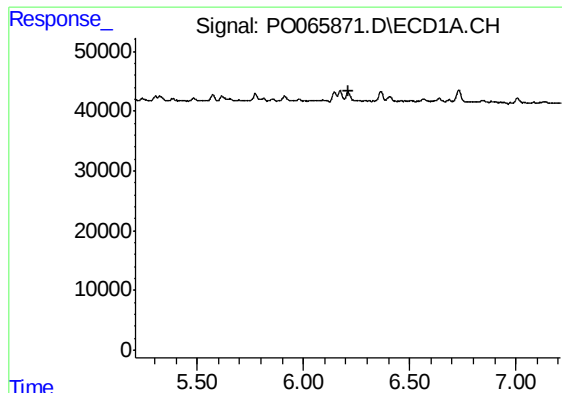

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020

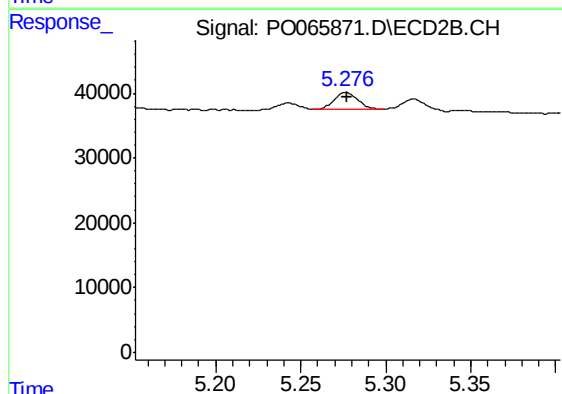


#20 AR-1242-5

R.T.: 5.277 min
Delta R.T.: 0.000 min
Response: 25353
Conc: 22.90 ng/ml

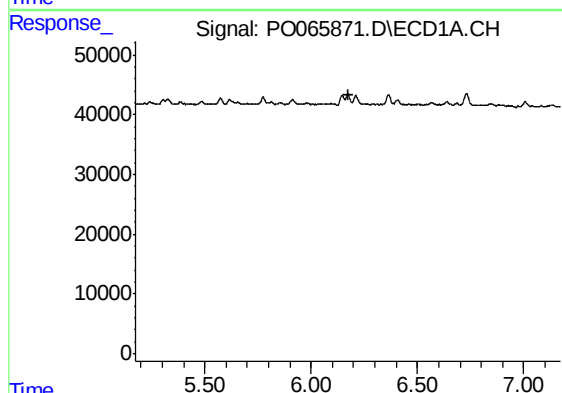


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.173 min
Response: 0
Conc: N.D.

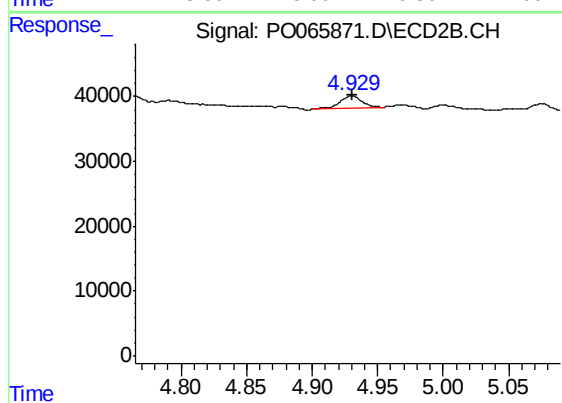

#24 AR-1248-4


R.T.: 4.930 min
Delta R.T.: 0.000 min
Response: 22955
Conc: 17.99 ng/ml

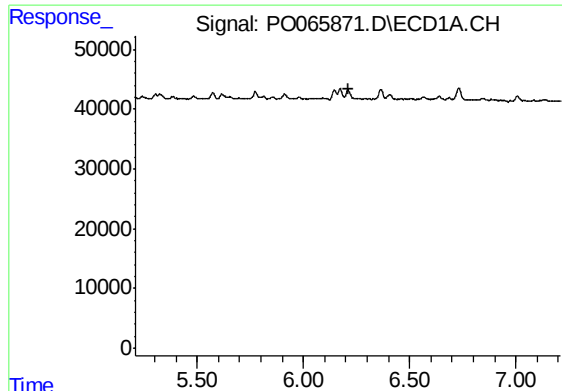

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.210 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020

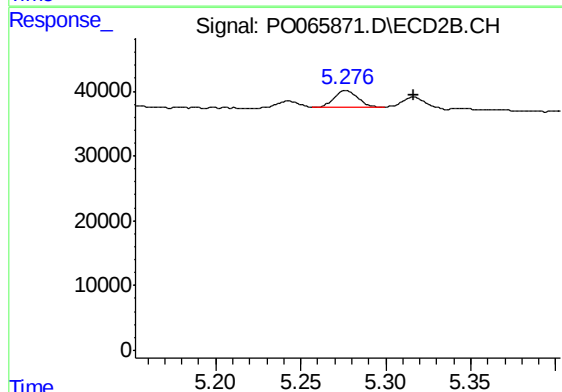


#25 AR-1248-5

R.T.: 5.277 min
Delta R.T.: -0.040 min
Response: 25353
Conc: 18.17 ng/ml

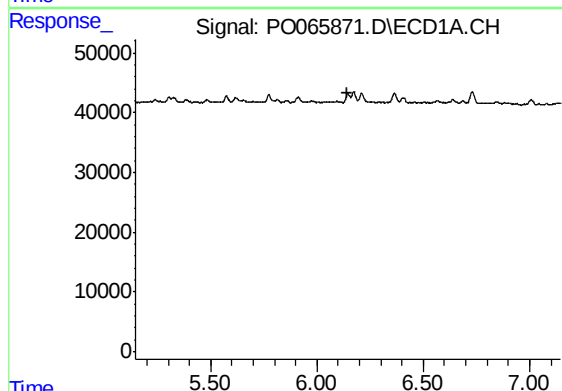


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.146 min
Response: 0
Conc: N.D.

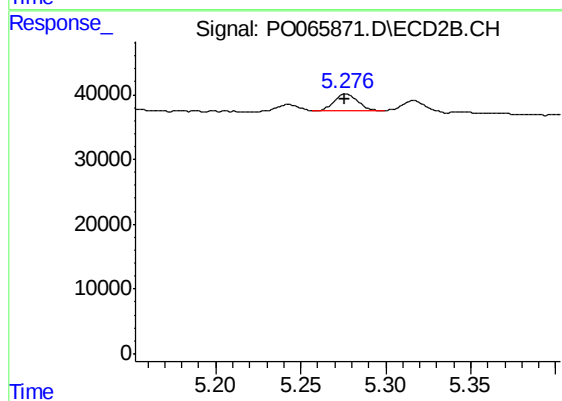

#26 AR-1254-1


R.T.: 5.277 min
Delta R.T.: 0.000 min
Response: 25353
Conc: 11.34 ng/ml

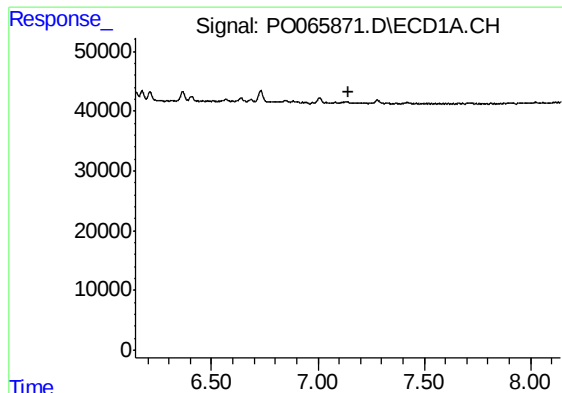

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.142 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020

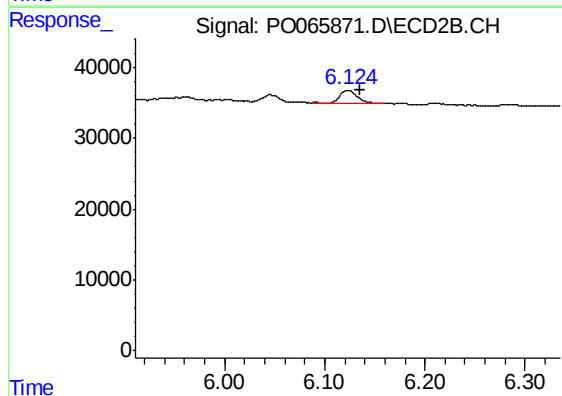

#32 AR-1260-2

R.T.: 6.124 min
Delta R.T.: -0.012 min
Response: 22055
Conc: 6.96 ng/ml