

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012320\
 Data File : P0065870.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jan 2020 00:20
 Operator : DD\AJ
 Sample : L1161-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT1-2020

Manual Integrations
 APPROVED

mohammad
 1/24/2020 1:52:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 04:39:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.154	3.431	290765	336969	12.540	12.686
2)	SA Decachlor...	9.648	8.329	556852	667096	13.377	13.727
Target Compounds							
11)	L3 AR-1232-1	4.524	3.796	9469	10831	17.436	17.016
12)	L3 AR-1232-2	5.041	4.507	5535	12469	19.164	16.223
13)	L3 AR-1232-3	5.324	4.679	10000	6831	14.846	17.753m
14)	L3 AR-1232-4	5.481	4.760	5852	8012	17.415	22.753m#
15)	L3 AR-1232-5	5.575	4.930	5645	8085	22.758m	20.289m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012320\
Data File : PO065870.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jan 2020 00:20
Operator : DD\AJ
Sample : L1161-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

mohammad
1/24/2020 1:52:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 04:39:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

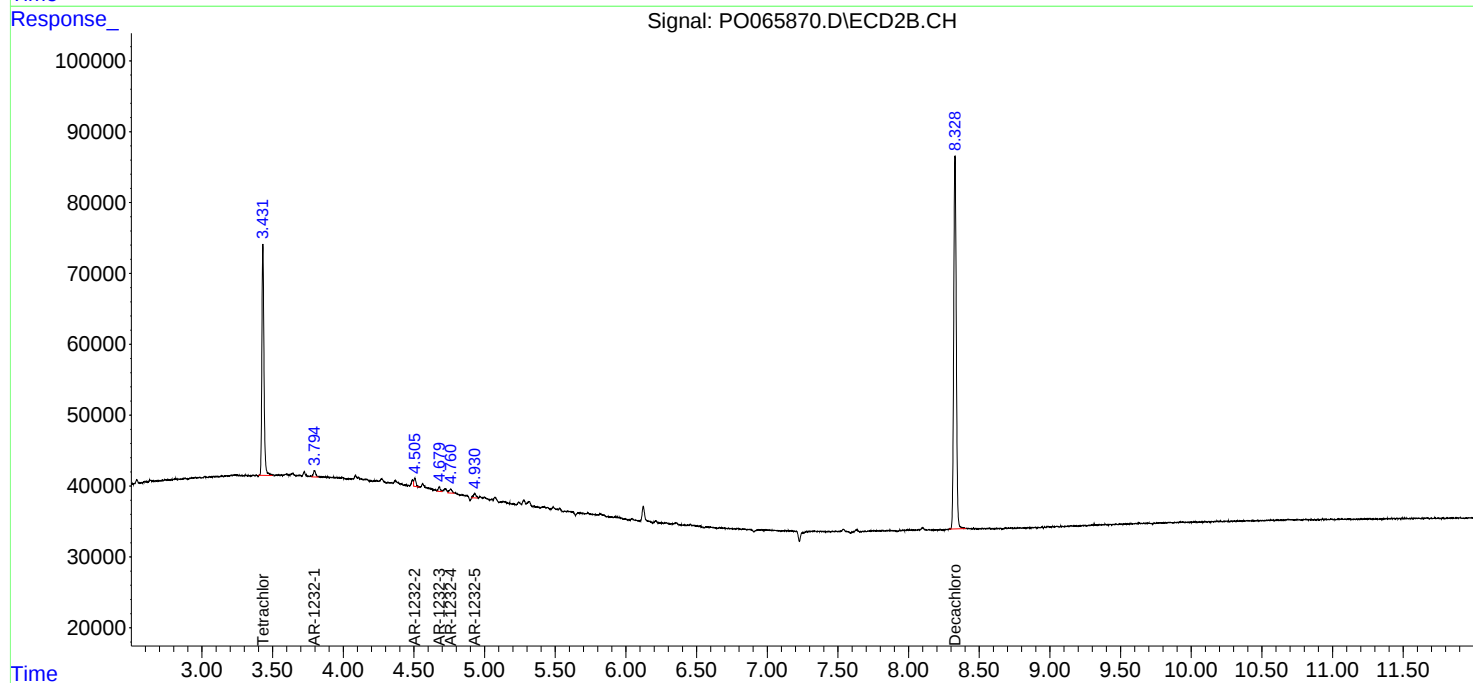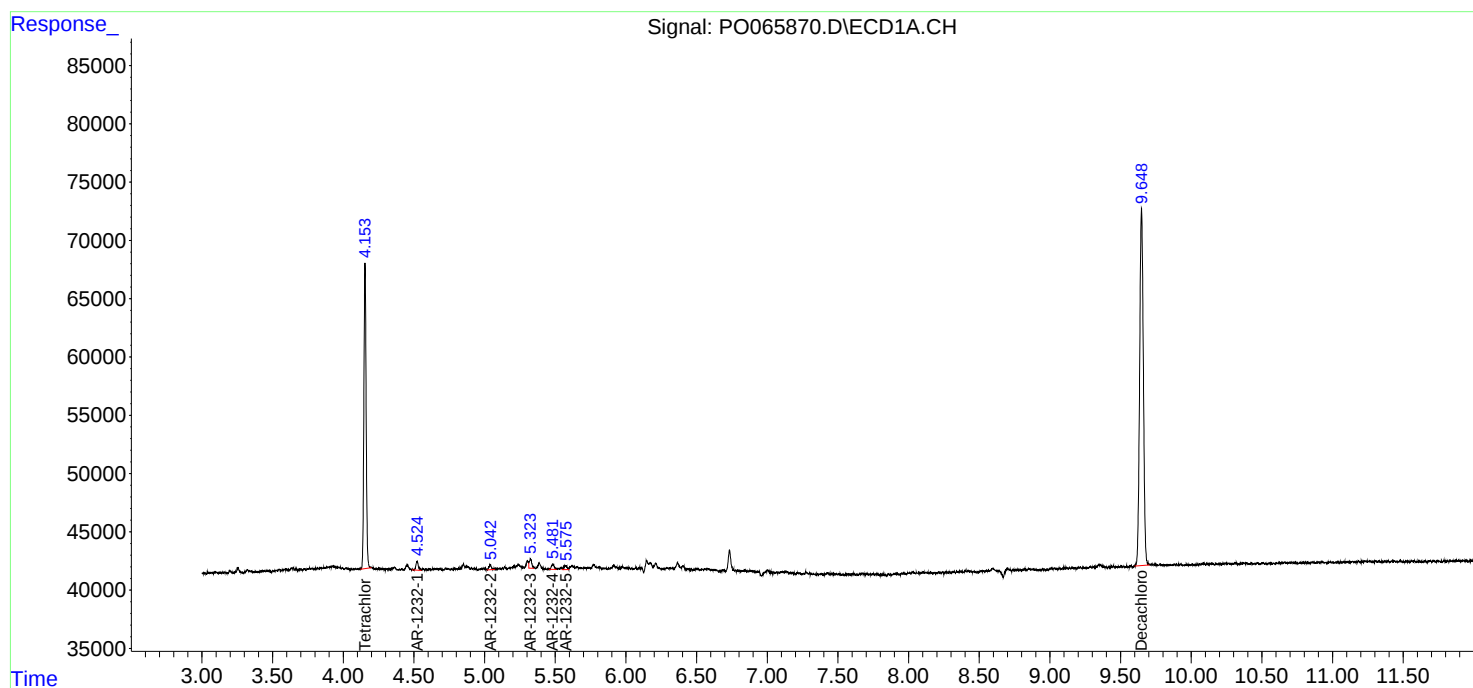

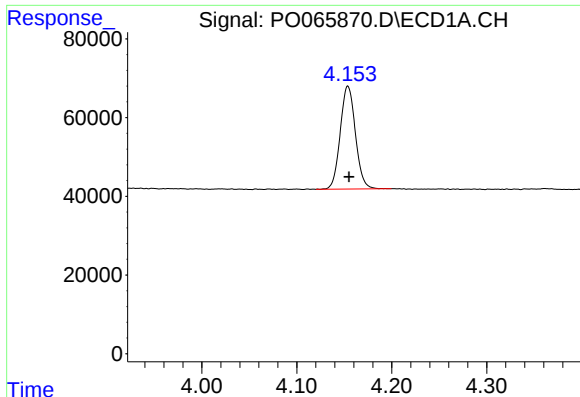


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: -0.001 min
Response: 290765
Conc: 12.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

mohammad
1/24/2020 1:52:41 PM

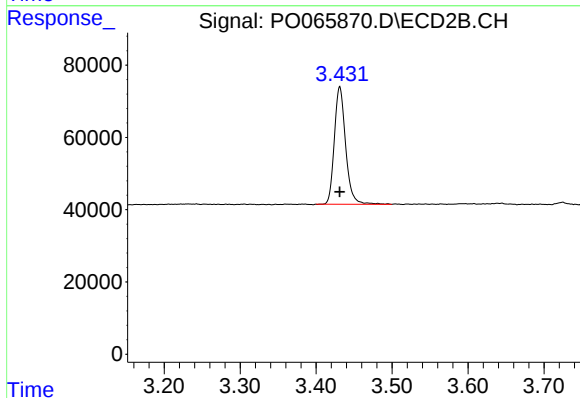


#1 Tetrachloro-m-xylene

R.T.: 3.431 min
Delta R.T.: 0.000 min
Response: 336969
Conc: 12.69 ng/ml

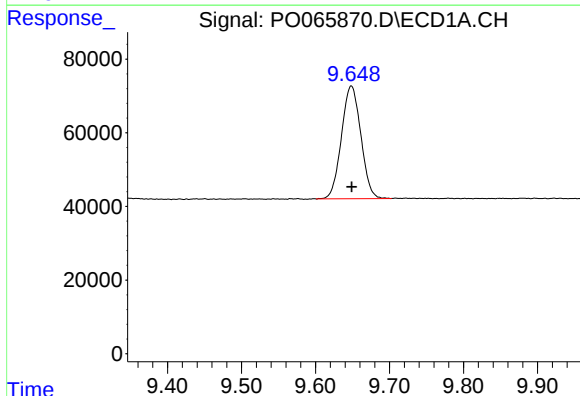


#2 Decachlorobiphenyl

R.T.: 9.648 min
Delta R.T.: 0.000 min
Response: 556852
Conc: 13.38 ng/ml

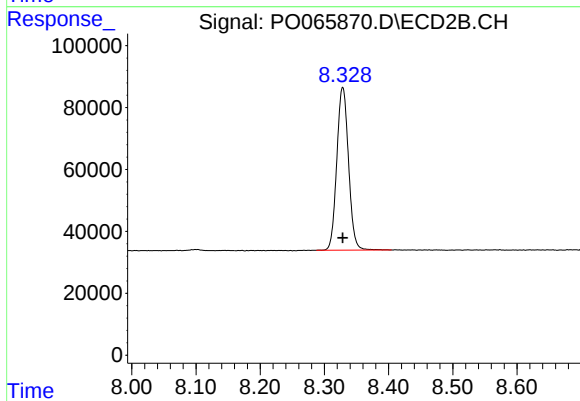

#2 Decachlorobiphenyl

R.T.: 8.329 min
Delta R.T.: 0.000 min
Response: 667096
Conc: 13.73 ng/ml

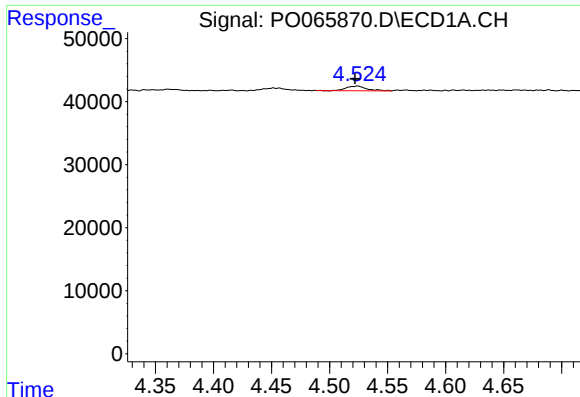


#11 AR-1232-1

R.T.: 4.524 min
Delta R.T.: 0.002 min
Response: 9469
Conc: 17.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

mohammad
1/24/2020 1:52:41 PM

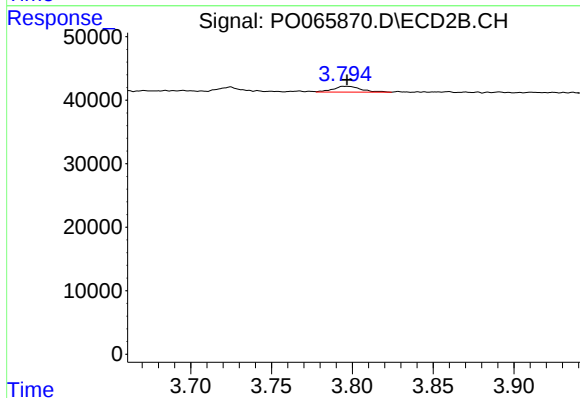


#11 AR-1232-1

R.T.: 3.796 min
Delta R.T.: 0.000 min
Response: 10831
Conc: 17.02 ng/ml

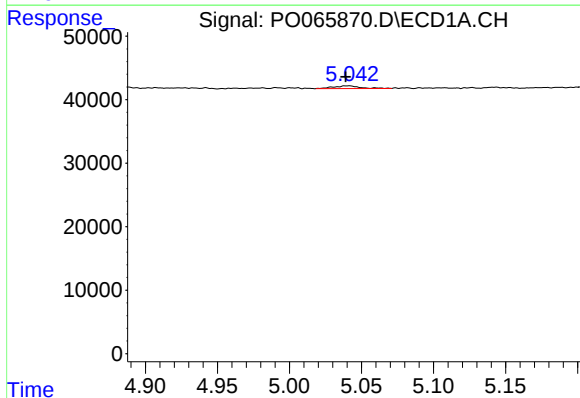


#12 AR-1232-2

R.T.: 5.041 min
Delta R.T.: 0.002 min
Response: 5535
Conc: 19.16 ng/ml

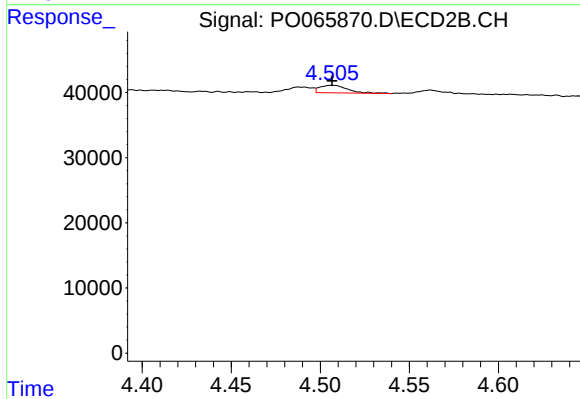

#12 AR-1232-2

R.T.: 4.507 min
Delta R.T.: 0.000 min
Response: 12469
Conc: 16.22 ng/ml

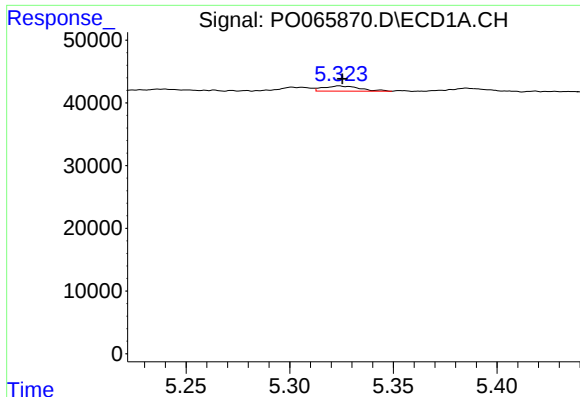


#13 AR-1232-3

R.T.: 5.324 min
Delta R.T.: -0.002 min
Response: 10000
Conc: 14.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

mohammad
1/24/2020 1:52:41 PM

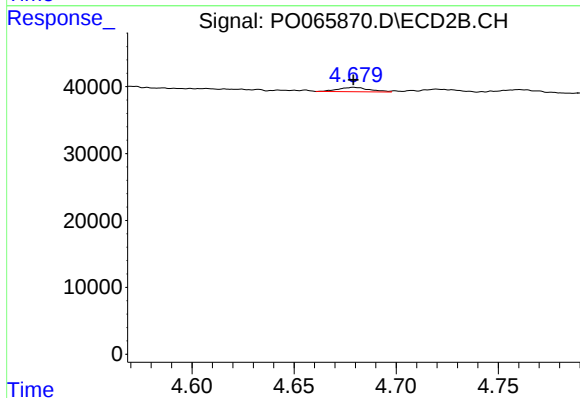


#13 AR-1232-3

R.T.: 4.679 min
Delta R.T.: 0.000 min
Response: 6831
Conc: 17.75 ng/ml m

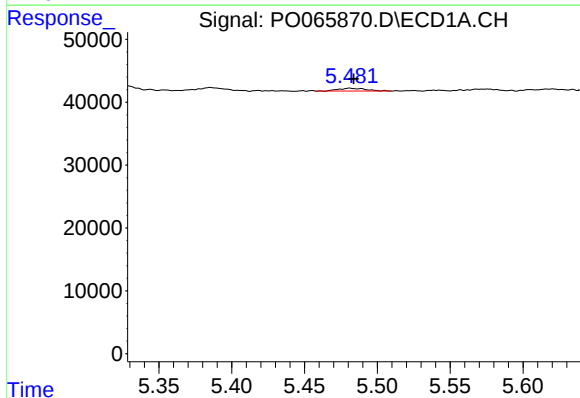


#14 AR-1232-4

R.T.: 5.481 min
Delta R.T.: -0.003 min
Response: 5852
Conc: 17.41 ng/ml

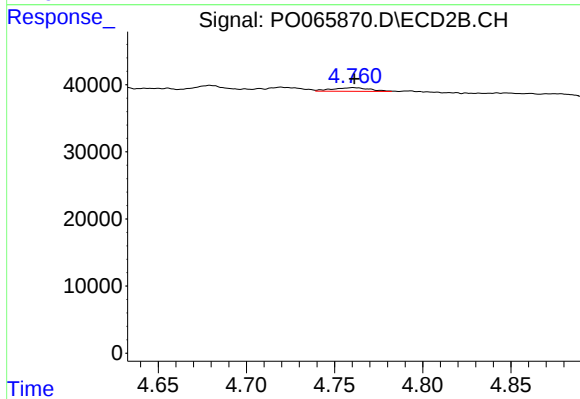

#14 AR-1232-4

R.T.: 4.760 min
Delta R.T.: -0.001 min
Response: 8012
Conc: 22.75 ng/ml m

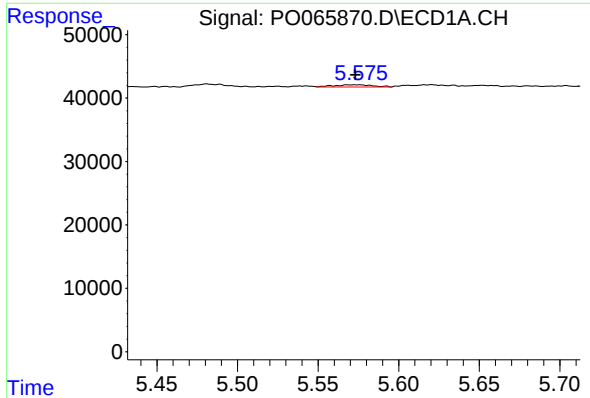


#15 AR-1232-5

R.T.: 5.575 min
Delta R.T.: 0.002 min
Response: 5645
Conc: 22.76 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020

Manual Integrations
APPROVED

mohammad
1/24/2020 1:52:41 PM

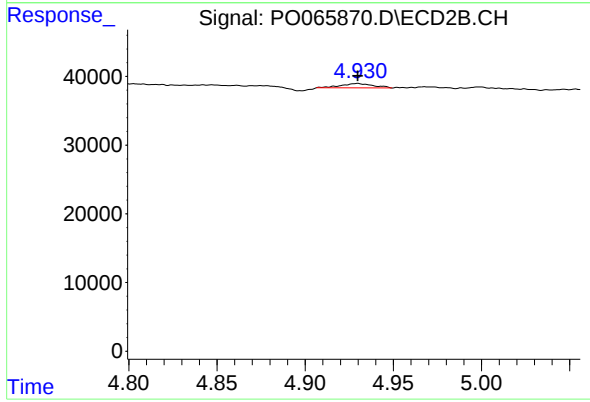

#15 AR-1232-5

R.T.: 4.930 min
Delta R.T.: 0.000 min
Response: 8085
Conc: 20.29 ng/ml m