

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0012320\
 Data File : P0065872.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jan 2020 00:53
 Operator : DD\AJ
 Sample : L1161-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MDL-WATER-03-QT1-2020

Manual Integrations
 APPROVED

mohammad
 1/24/2020 1:52:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 04:47:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.155	3.432	273225	312535	11.783	11.766
2)	SA Decachlor...	9.648	8.329	531378	637648	12.765	13.121
Target Compounds							
26)	L6 AR-1254-1	6.145	5.277	28529	35400	21.494m	15.832 #
27)	L6 AR-1254-2	6.362	5.423	43356	39178	19.903	19.074
28)	L6 AR-1254-3	6.727	5.820	66304	57527	27.266	16.964 #
29)	L6 AR-1254-4	7.007	6.047	41204	35098	19.661	15.323
30)	L6 AR-1254-5	7.422	6.460	33265	55482	15.504m	17.157

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012320\
Data File : PO065872.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jan 2020 00:53
Operator : DD\AJ
Sample : L1161-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

mohammad
1/24/2020 1:52:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 04:47:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

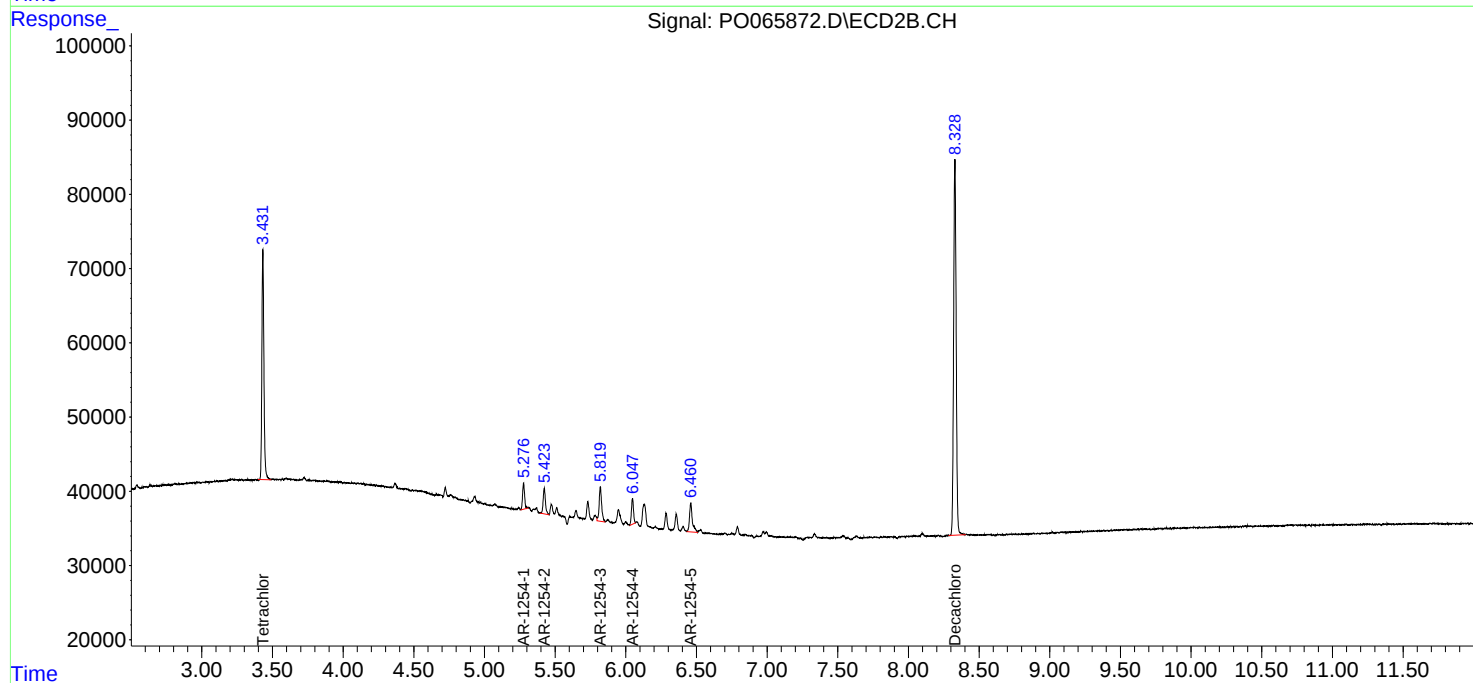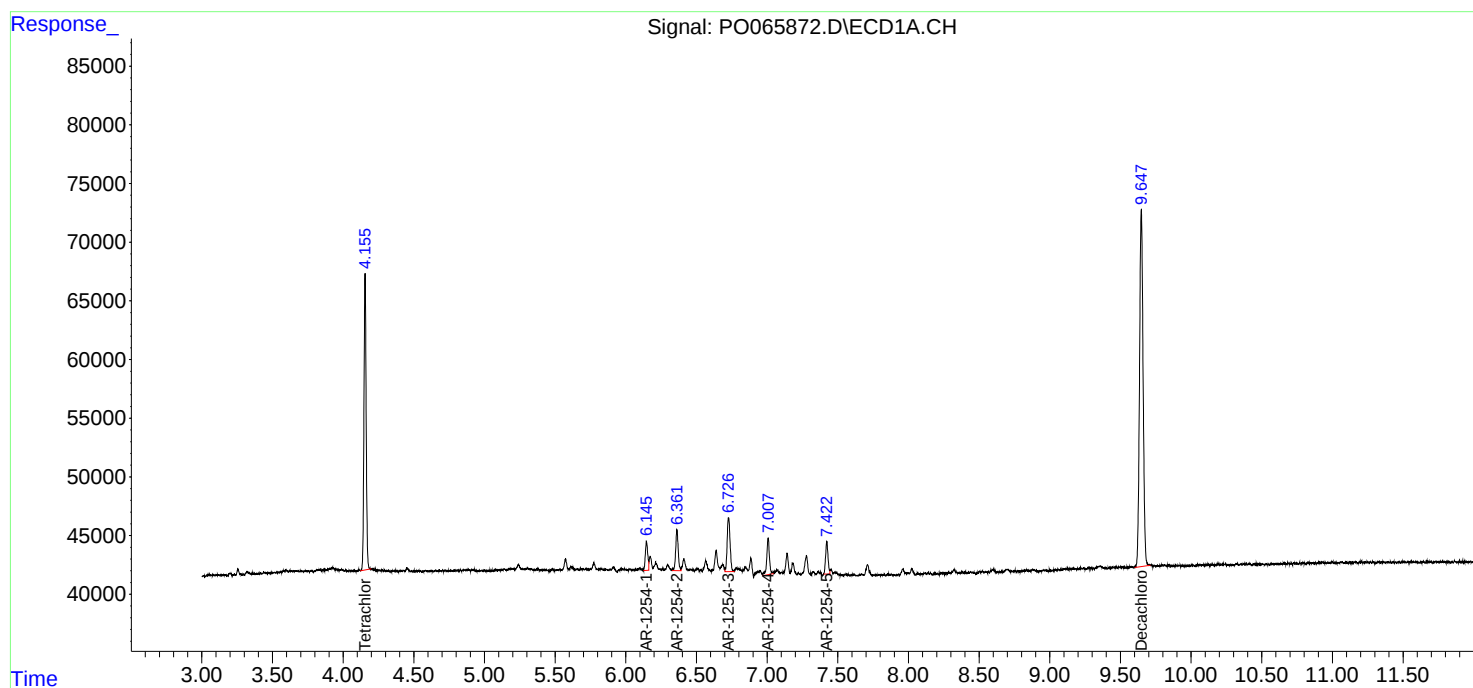

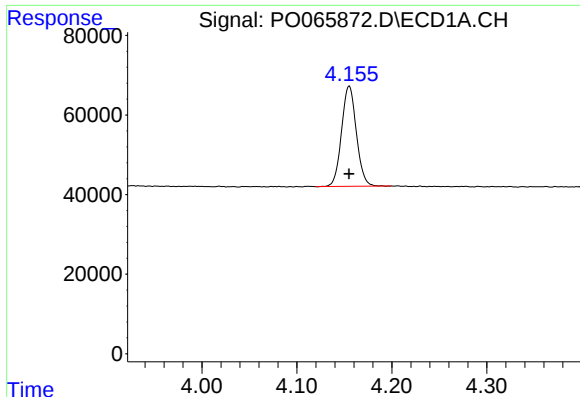


#1 Tetrachloro-m-xylene

R.T.: 4.155 min
Delta R.T.: 0.000 min
Response: 273225
Conc: 11.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

mohammad
1/24/2020 1:52:45 PM

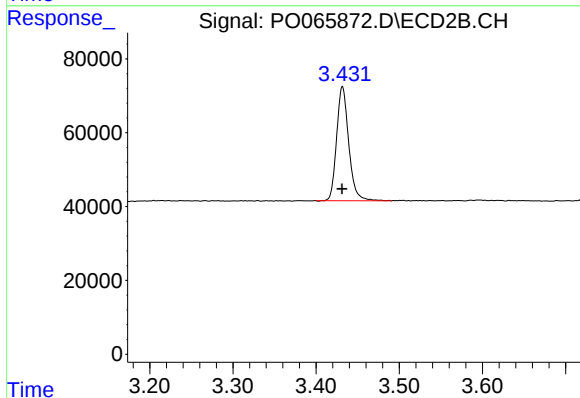


#1 Tetrachloro-m-xylene

R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 312535
Conc: 11.77 ng/ml

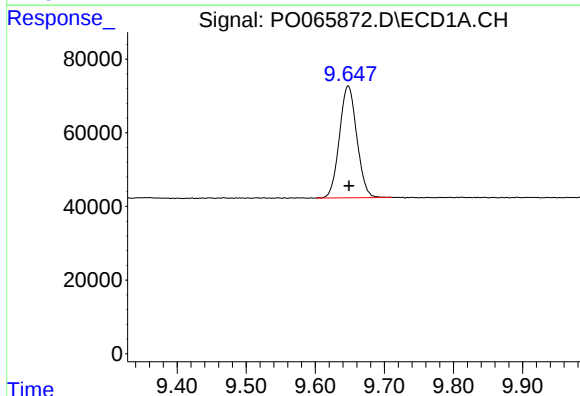


#2 Decachlorobiphenyl

R.T.: 9.648 min
Delta R.T.: -0.001 min
Response: 531378
Conc: 12.77 ng/ml

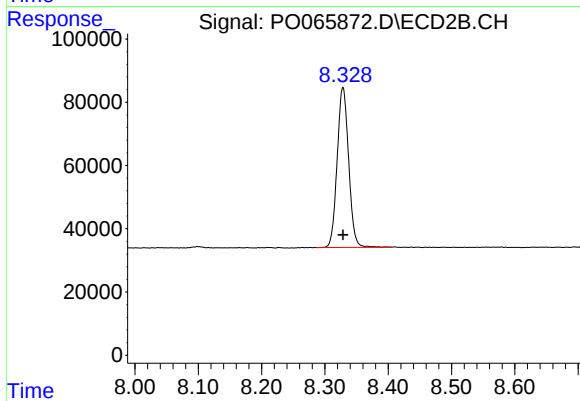

#2 Decachlorobiphenyl

R.T.: 8.329 min
Delta R.T.: 0.000 min
Response: 637648
Conc: 13.12 ng/ml

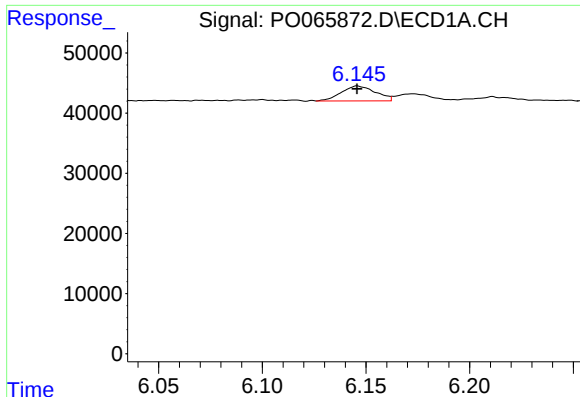


#26 AR-1254-1

R.T.: 6.145 min
Delta R.T.: 0.000 min
Response: 28529
Conc: 21.49 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

mohammad
1/24/2020 1:52:45 PM

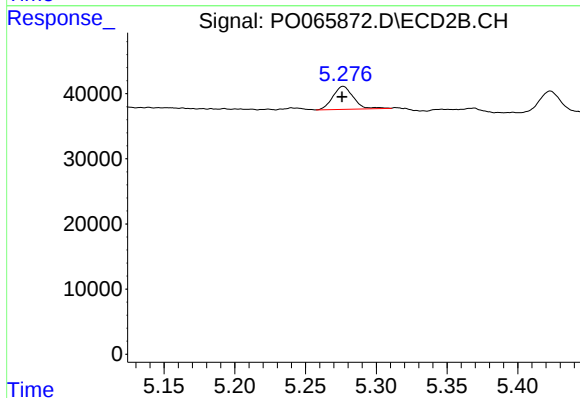


#26 AR-1254-1

R.T.: 5.277 min
Delta R.T.: 0.000 min
Response: 35400
Conc: 15.83 ng/ml

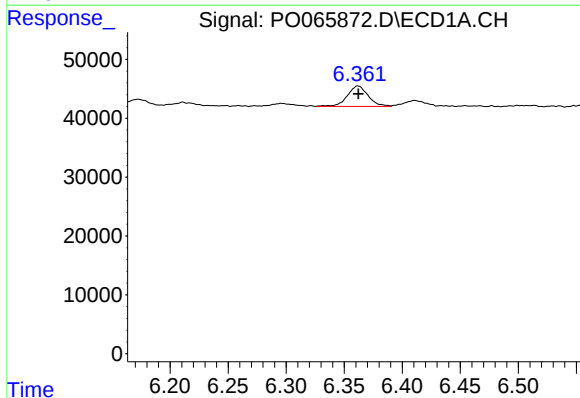


#27 AR-1254-2

R.T.: 6.362 min
Delta R.T.: 0.000 min
Response: 43356
Conc: 19.90 ng/ml

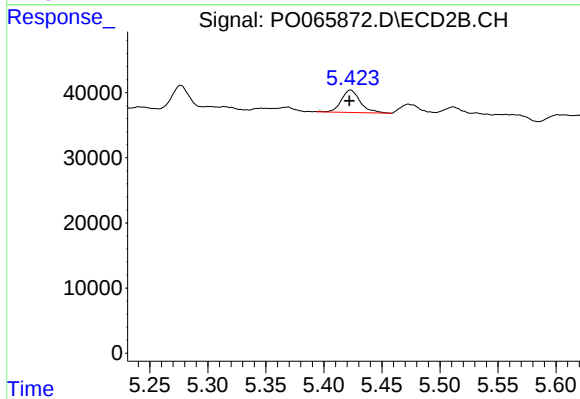

#27 AR-1254-2

R.T.: 5.423 min
Delta R.T.: 0.000 min
Response: 39178
Conc: 19.07 ng/ml

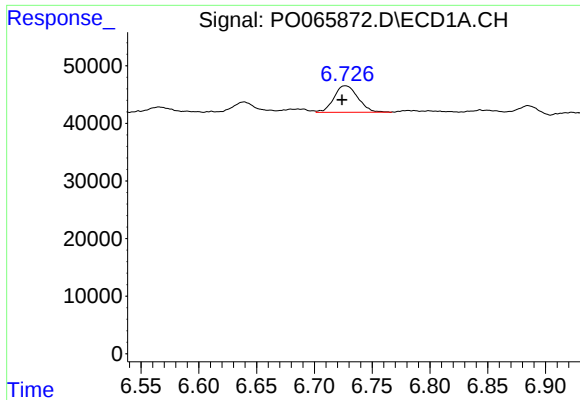


#28 AR-1254-3

R.T.: 6.727 min
Delta R.T.: 0.003 min
Response: 66304
Conc: 27.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020


Manual Integrations
APPROVED

mohammad
1/24/2020 1:52:45 PM

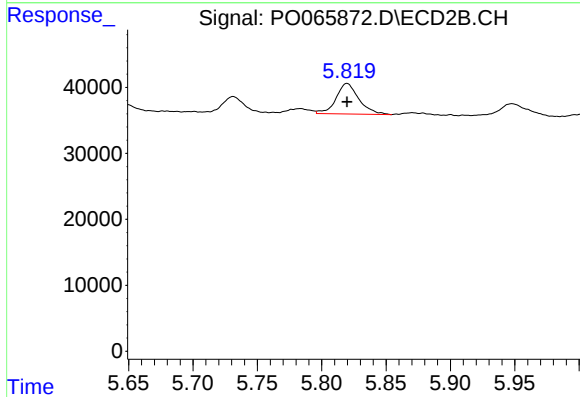


#28 AR-1254-3

R.T.: 5.820 min
Delta R.T.: 0.000 min
Response: 57527
Conc: 16.96 ng/ml

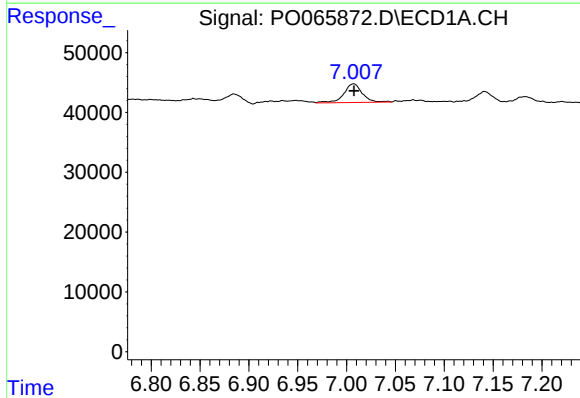


#29 AR-1254-4

R.T.: 7.007 min
Delta R.T.: 0.000 min
Response: 41204
Conc: 19.66 ng/ml

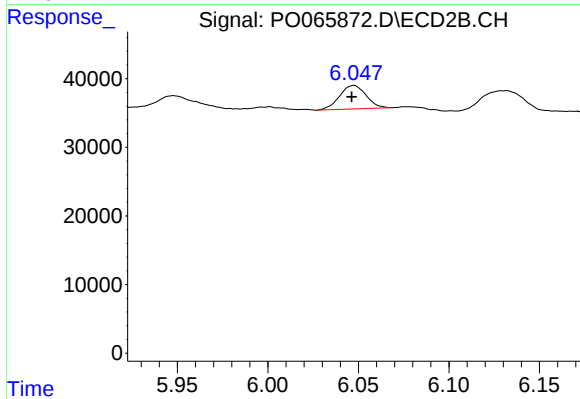

#29 AR-1254-4

R.T.: 6.047 min
Delta R.T.: 0.001 min
Response: 35098
Conc: 15.32 ng/ml

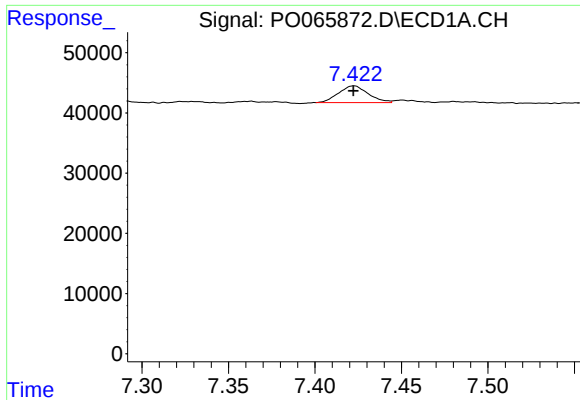


#30 AR-1254-5

R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 33265
Conc: 15.50 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT1-2020

Manual Integrations
APPROVED

mohammad
1/24/2020 1:52:45 PM

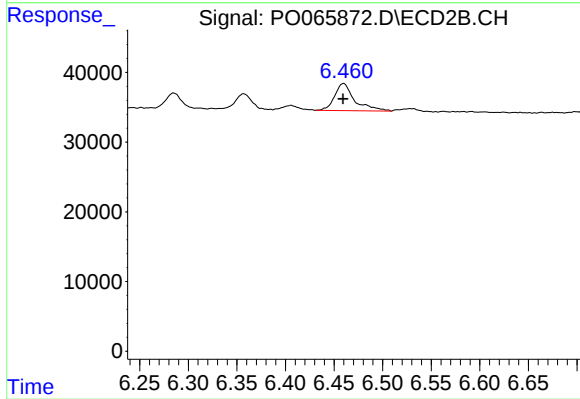

#30 AR-1254-5

R.T.: 6.460 min
Delta R.T.: 0.000 min
Response: 55482
Conc: 17.16 ng/ml