

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012323\
 Data File : P0092220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jan 2023 08:54
 Operator : YP/AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 04:43:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
27)	L6	AR-1254-2	6.795f	0.000	574592	0	3.535 N.D. #
29)	L6	AR-1254-4	7.398	0.000	295511	0	2.702 N.D. #
31)	L7	AR-1260-1	7.275	0.000	89202	0	0.677 N.D. #
32)	L7	AR-1260-2	7.542	0.000	702690	0	4.739 N.D. #
35)	L7	AR-1260-5	8.468	7.264	11977097	64377	53.937 0.452 #
37)	L8	AR-1262-2	8.468	7.264	11977097	64377	50.173 0.436 #
40)	L8	AR-1262-5	9.566	8.069f	1081662	130345	12.095 2.530 #
43)	L9	AR-1268-3	0.000	7.898f	0	369403	N.D. 2.488 #
44)	L9	AR-1268-4	9.566	8.069f	1081662	130345	10.349 2.076 #
45)	L9	AR-1268-5	9.961f	0.000	1869649	0	2.362 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO012323\
Data File : PO092220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jan 2023 08:54
Operator : YP/AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_0
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 04:43:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

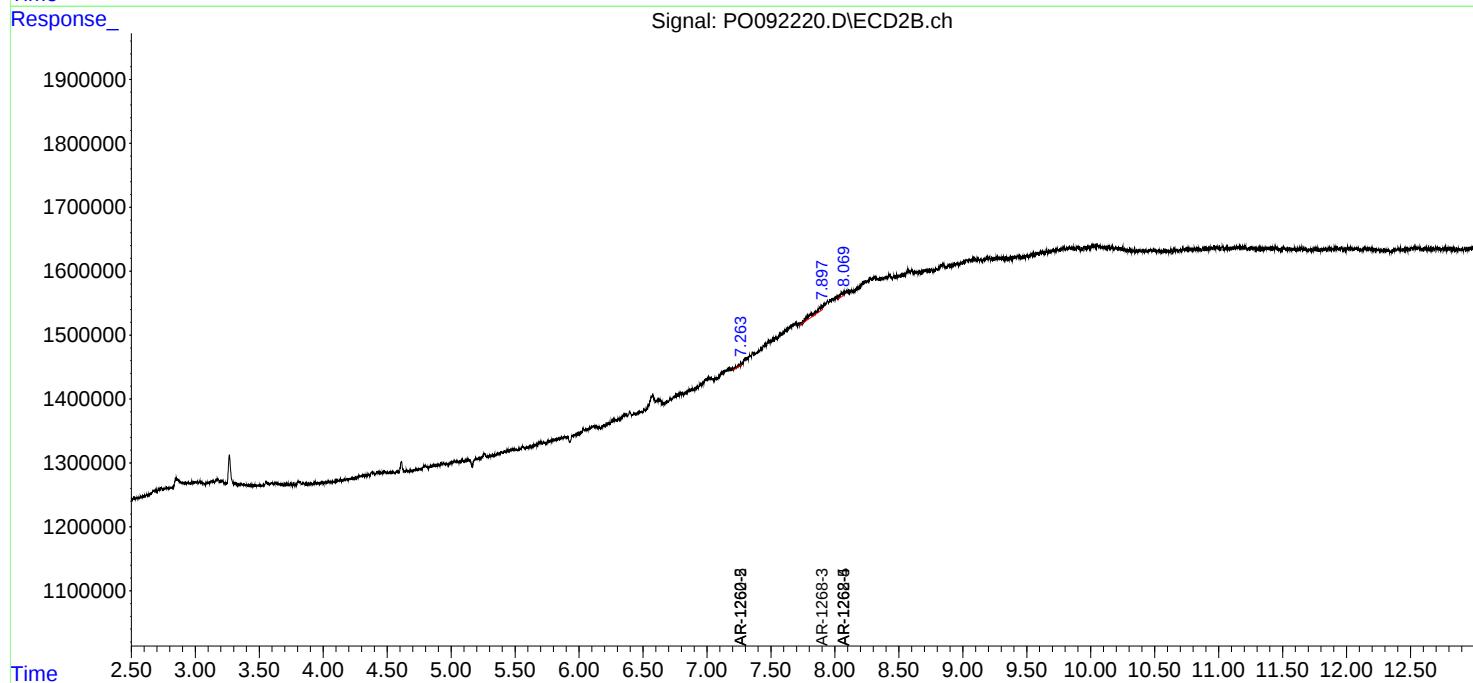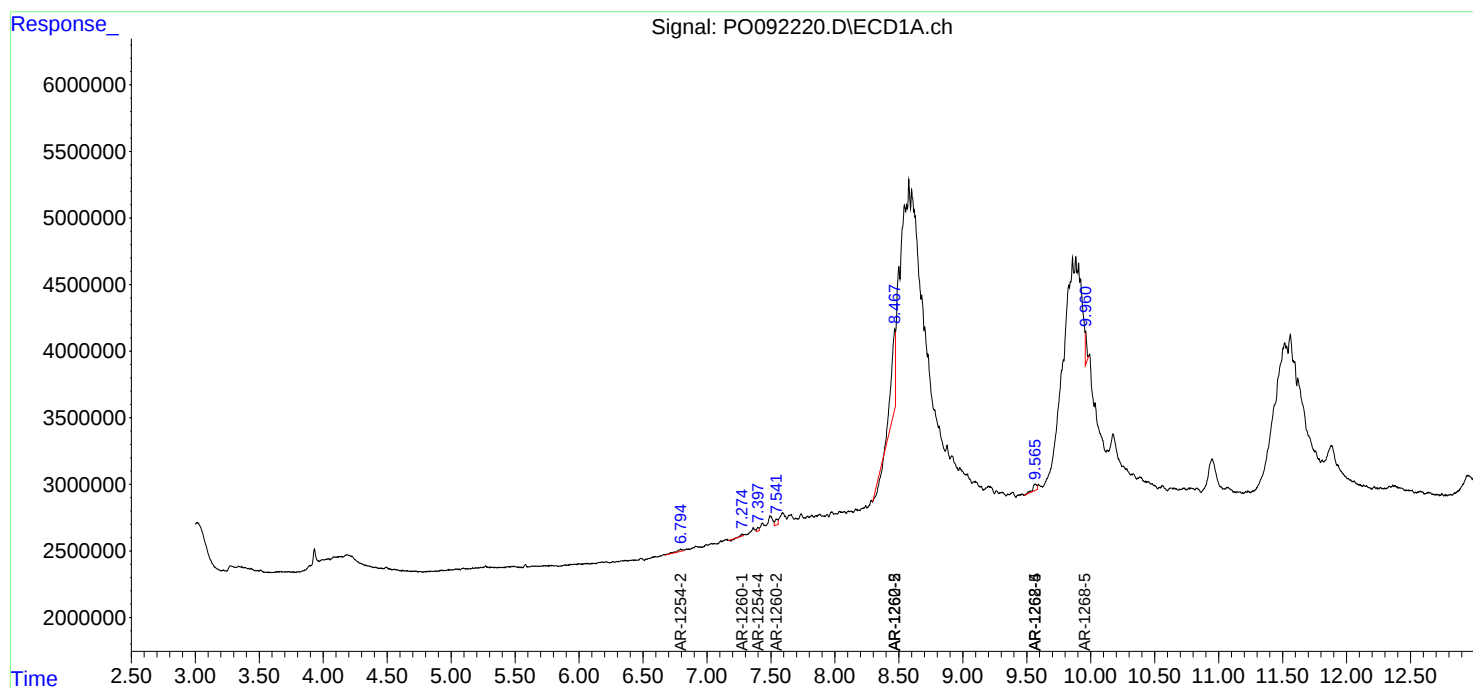


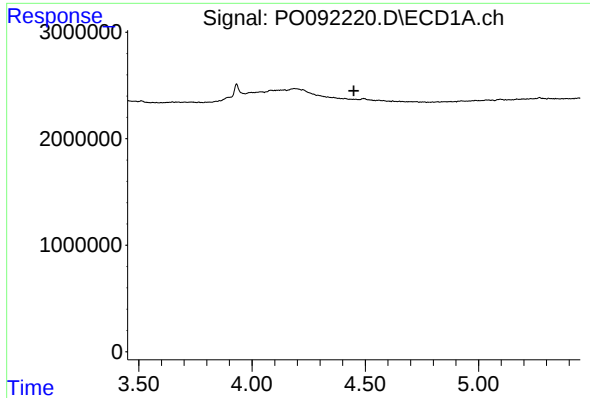

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

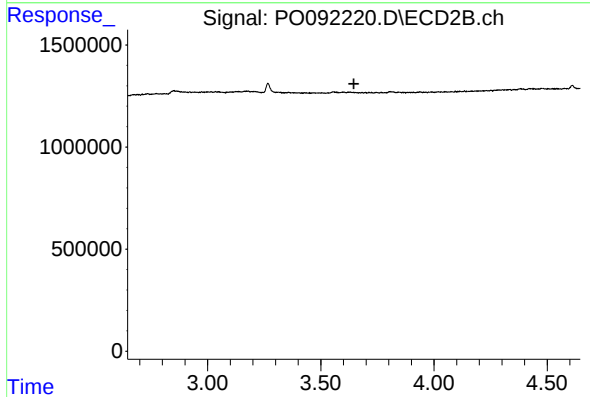


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.646 min
Response: 0
Conc: N.D.

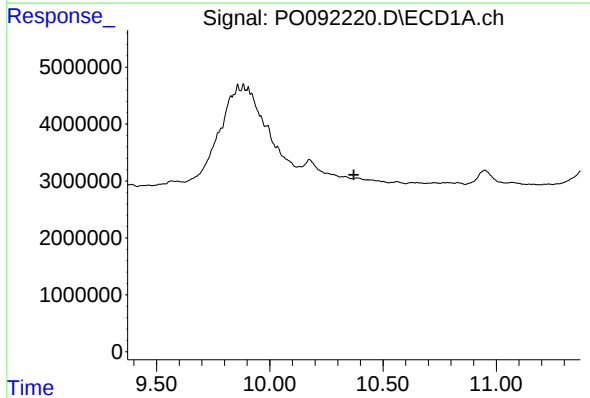


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.371 min
Response: 0
Conc: N.D.

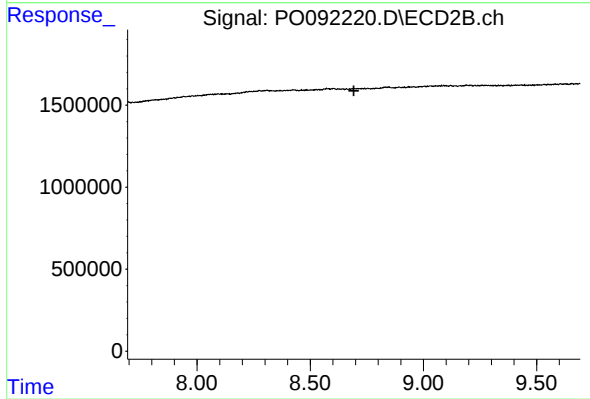

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.693 min
Response: 0
Conc: N.D.

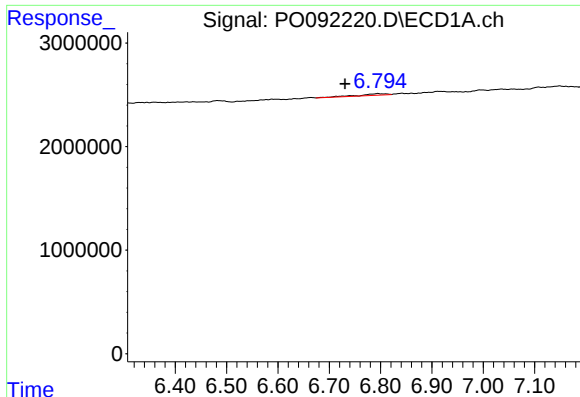

#27 AR-1254-2


R.T.: 6.795 min
Delta R.T.: 0.065 min
Response: 574592
Conc: 3.53 ng/ml

Instrument :
ECD_O
ClientSampleId :

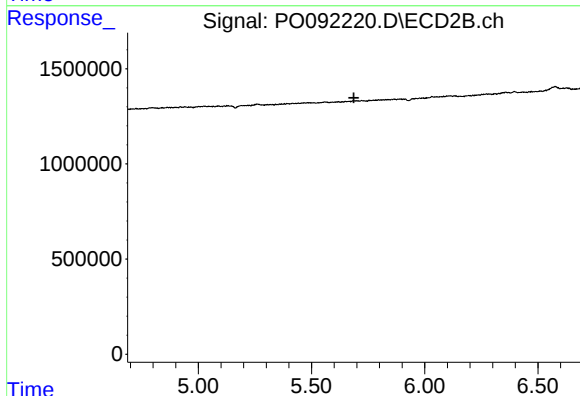


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.687 min
Response: 0
Conc: N.D.

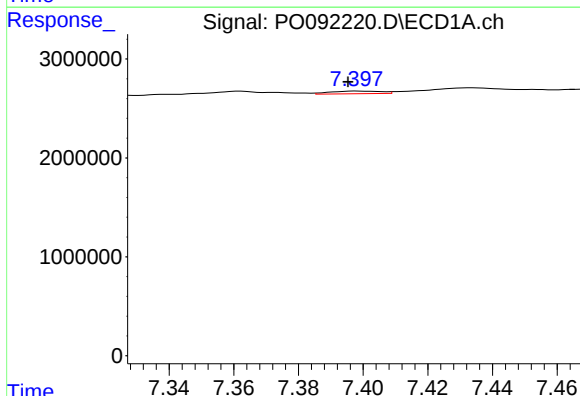


#29 AR-1254-4

R.T.: 7.398 min
Delta R.T.: 0.003 min
Response: 295511
Conc: 2.70 ng/ml

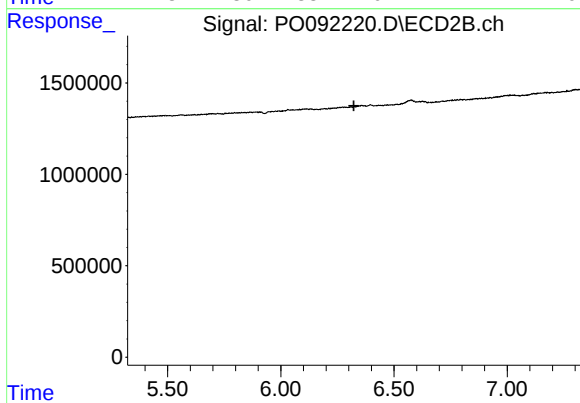

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.323 min
Response: 0
Conc: N.D.

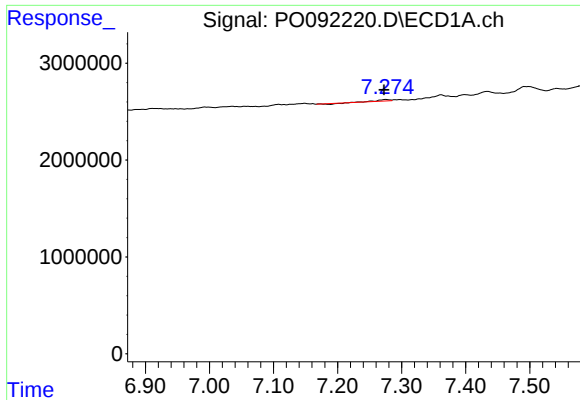

#31 AR-1260-1


R.T.: 7.275 min
Delta R.T.: 0.002 min
Response: 89202
Conc: 0.68 ng/ml

Instrument :
ECD_O
ClientSampleId :

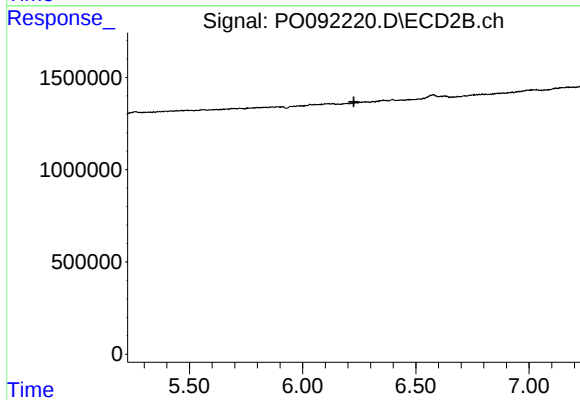


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.226 min
Response: 0
Conc: N.D.

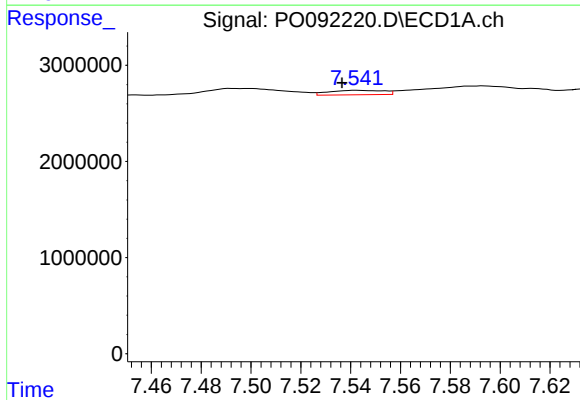


#32 AR-1260-2

R.T.: 7.542 min
Delta R.T.: 0.005 min
Response: 702690
Conc: 4.74 ng/ml

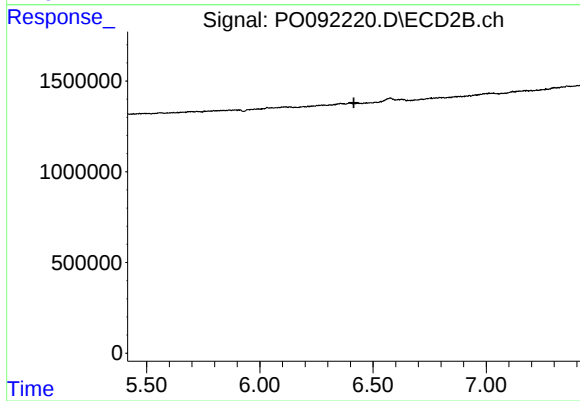

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.415 min
Response: 0
Conc: N.D.

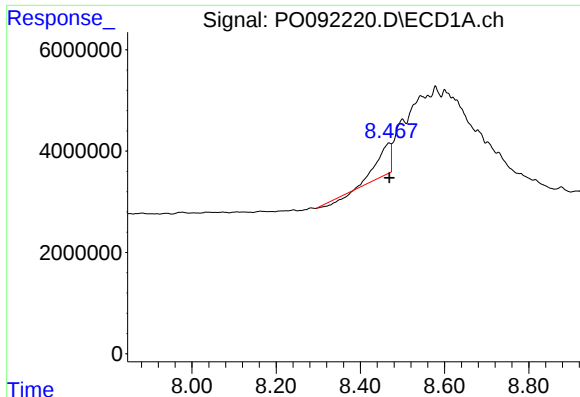

#35 AR-1260-5


R.T.: 8.468 min
Delta R.T.: 0.000 min
Response: 11977097
Conc: 53.94 ng/ml

Instrument :
ECD_O
ClientSampleId :

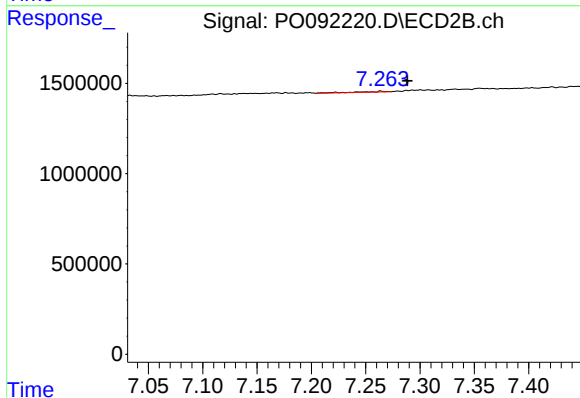


#35 AR-1260-5

R.T.: 7.264 min
Delta R.T.: -0.024 min
Response: 64377
Conc: 0.45 ng/ml

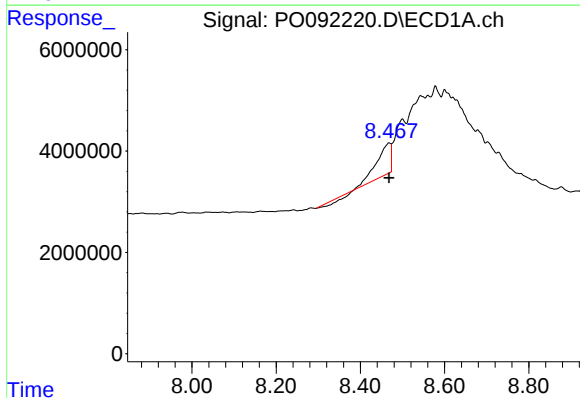


#37 AR-1262-2

R.T.: 8.468 min
Delta R.T.: 0.000 min
Response: 11977097
Conc: 50.17 ng/ml

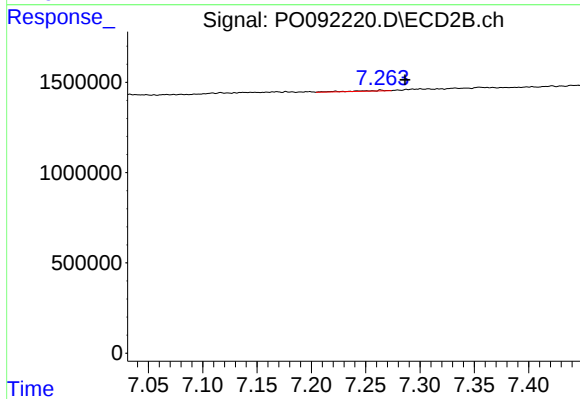

#37 AR-1262-2


R.T.: 7.264 min
Delta R.T.: -0.022 min
Response: 64377
Conc: 0.44 ng/ml

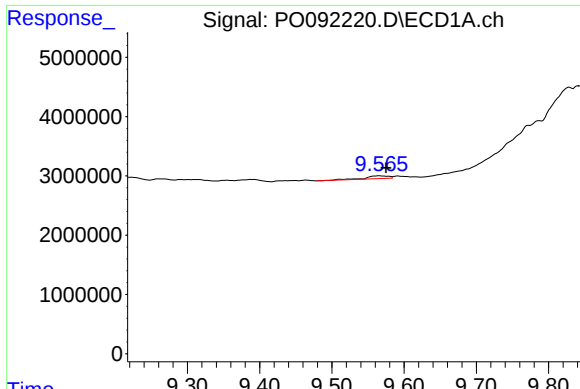

#40 AR-1262-5


R.T.: 9.566 min
Delta R.T.: -0.009 min
Response: 1081662
Conc: 12.10 ng/ml

Instrument :
ECD_O
ClientSampleId :

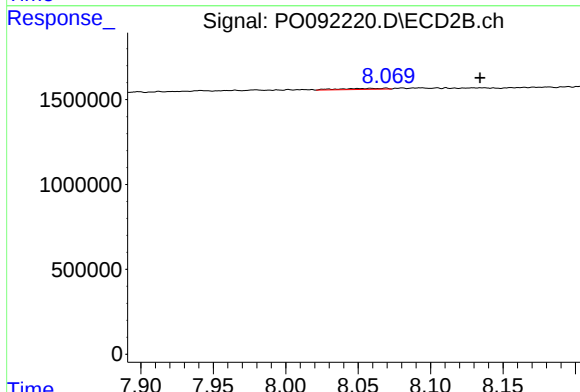


#40 AR-1262-5

R.T.: 8.069 min
Delta R.T.: -0.065 min
Response: 130345
Conc: 2.53 ng/ml

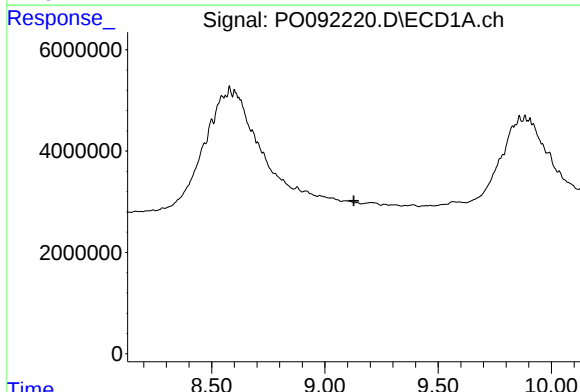


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 9.128 min
Response: 0
Conc: N.D.

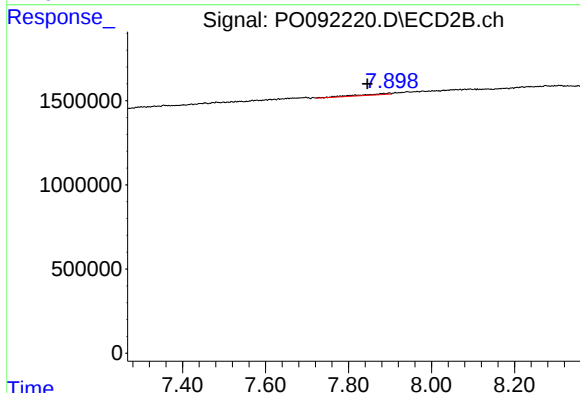

#43 AR-1268-3


R.T.: 7.898 min
Delta R.T.: 0.053 min
Response: 369403
Conc: 2.49 ng/ml

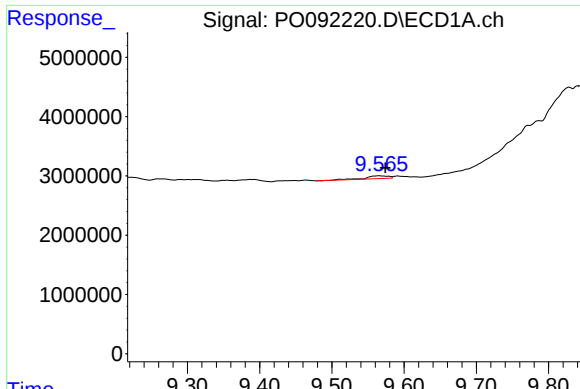

#44 AR-1268-4


R.T.: 9.566 min
Delta R.T.: -0.009 min
Response: 1081662
Conc: 10.35 ng/ml

Instrument :
ECD_O
ClientSampleId :

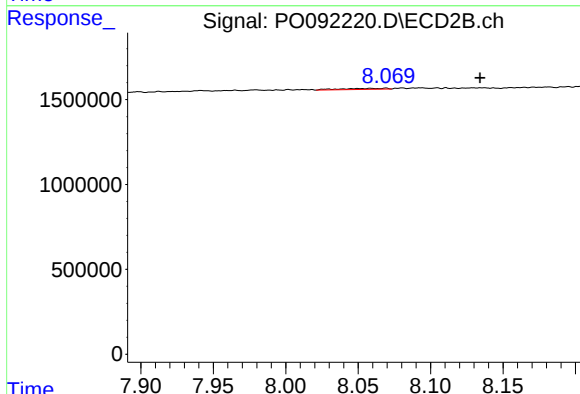


#44 AR-1268-4

R.T.: 8.069 min
Delta R.T.: -0.065 min
Response: 130345
Conc: 2.08 ng/ml

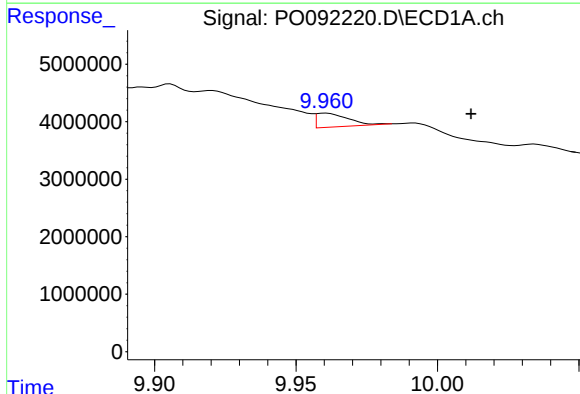

#45 AR-1268-5

R.T.: 9.961 min
Delta R.T.: -0.051 min
Response: 1869649
Conc: 2.36 ng/ml

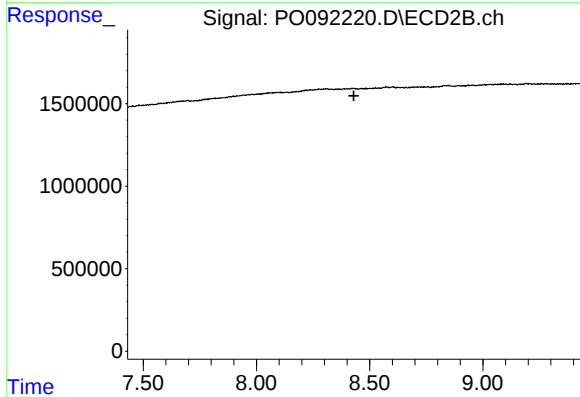

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 8.430 min
Response: 0
Conc: N.D.