

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012323\
 Data File : P0092229.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jan 2023 18:19
 Operator : YP/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 02:24:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 02:24:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.661	152.8E6	67739832	50.000	50.000
2) SA Decachlor...	10.369	8.706	104.9E6	56406677	50.000	50.000
Target Compounds						
8) L2 AR-1221-1	4.659	3.877	18902502	9465301	500.000	500.000
9) L2 AR-1221-2	4.746	3.962	13837241	7026989	500.000	500.000
10) L2 AR-1221-3	4.824	4.038	42191886	20937603	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012323\
Data File : PO092229.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jan 2023 18:19
Operator : YP/AJ
Sample : AR1221ICC500
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 02:24:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 02:24:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

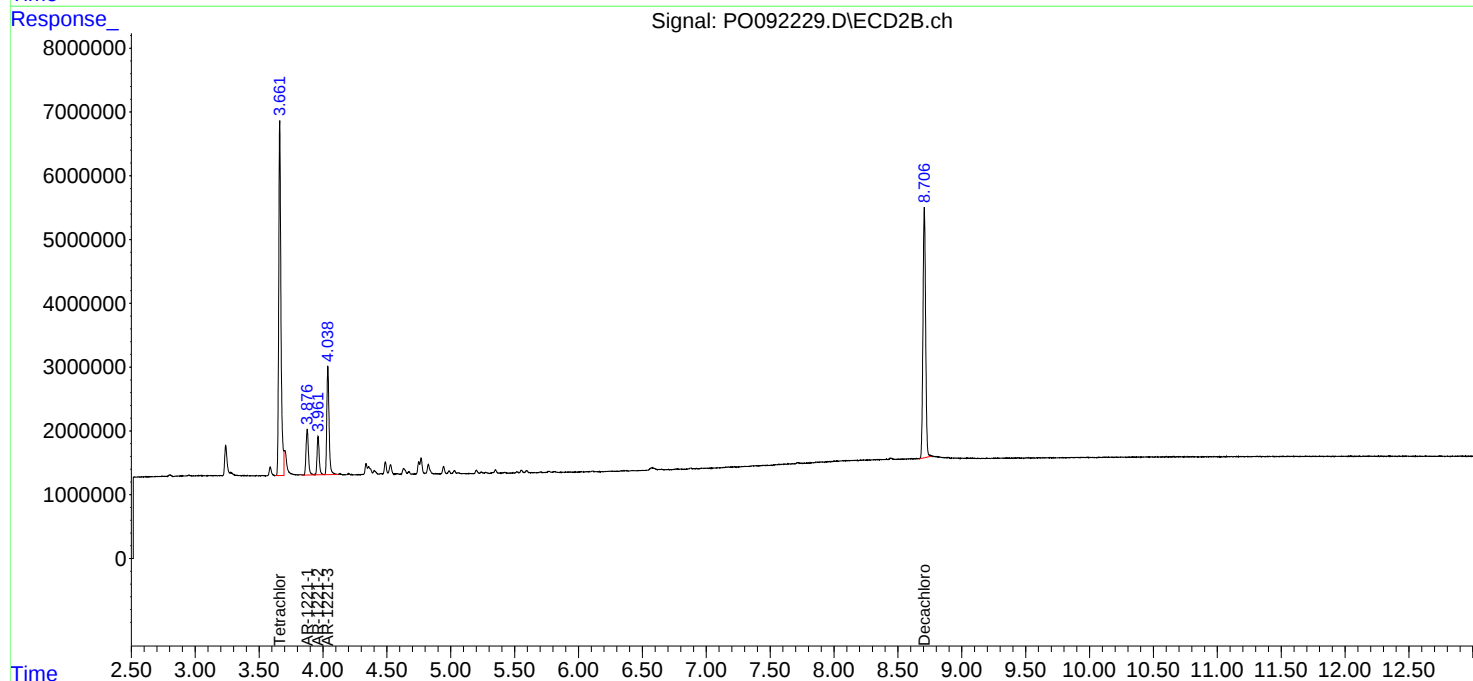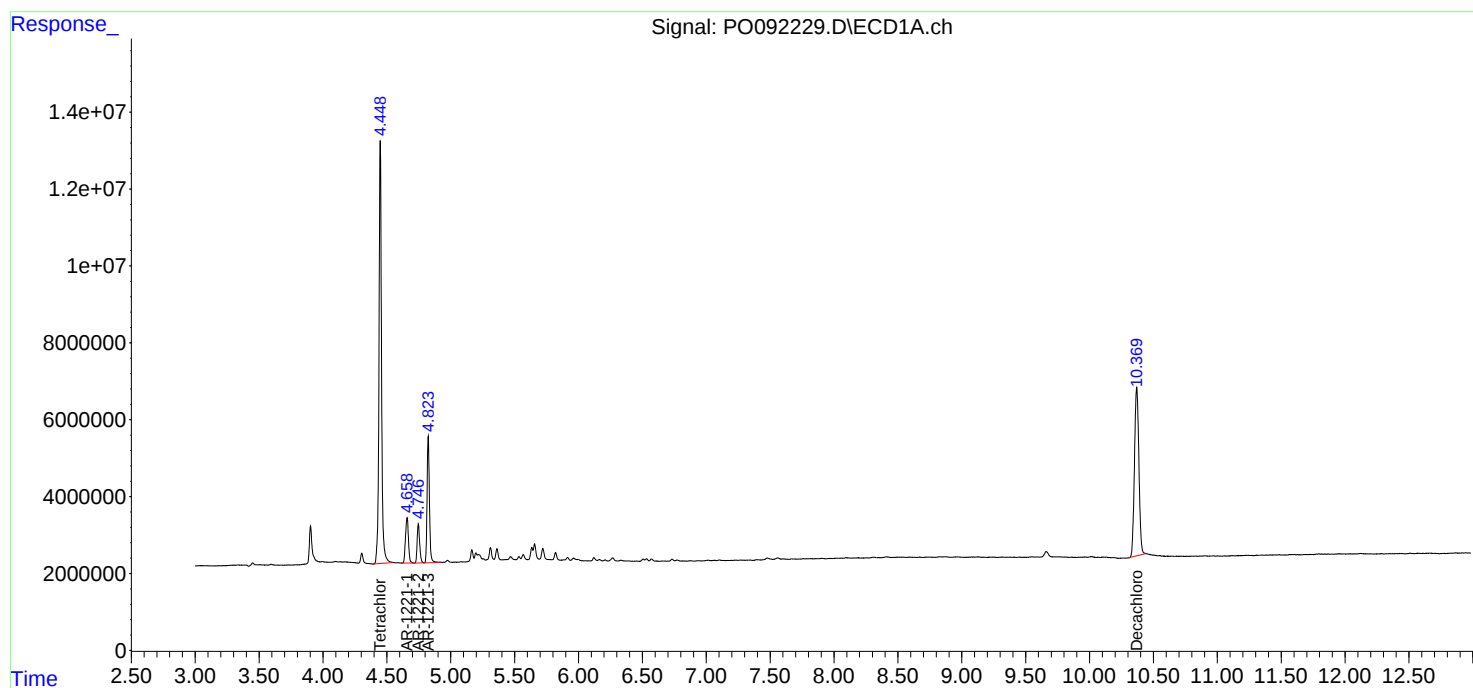


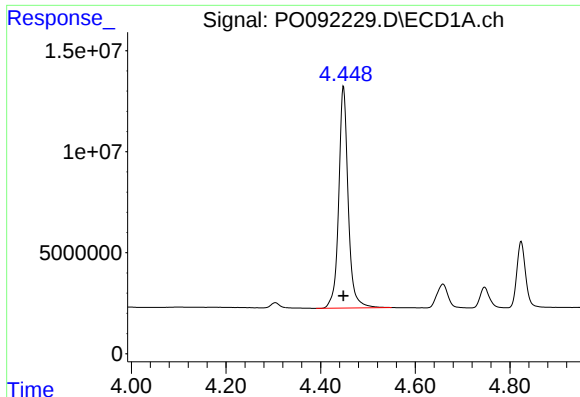

#1 Tetrachloro-m-xylene


R.T.: 4.448 min
Delta R.T.: 0.000 min
Response: 152796135
Conc: 50.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

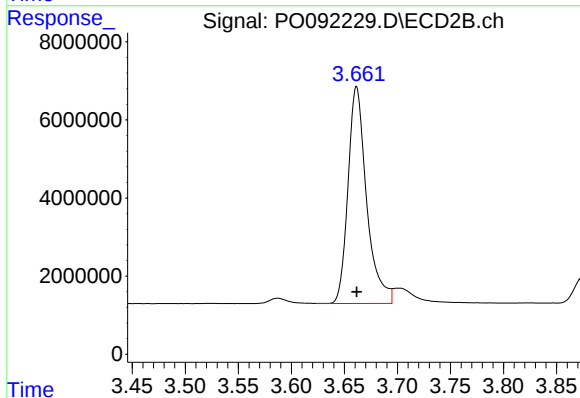


#1 Tetrachloro-m-xylene

R.T.: 3.661 min
Delta R.T.: 0.000 min
Response: 67739832
Conc: 50.00 ng/ml

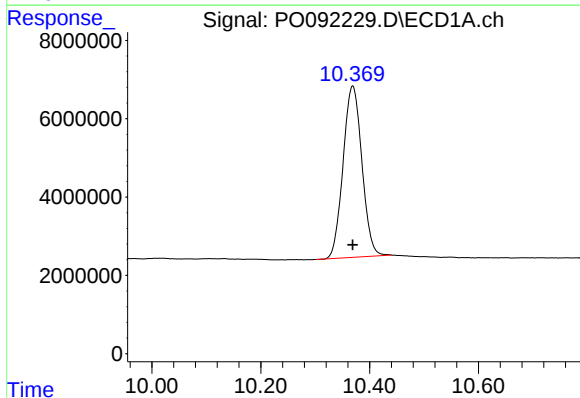


#2 Decachlorobiphenyl

R.T.: 10.369 min
Delta R.T.: 0.000 min
Response: 104919976
Conc: 50.00 ng/ml

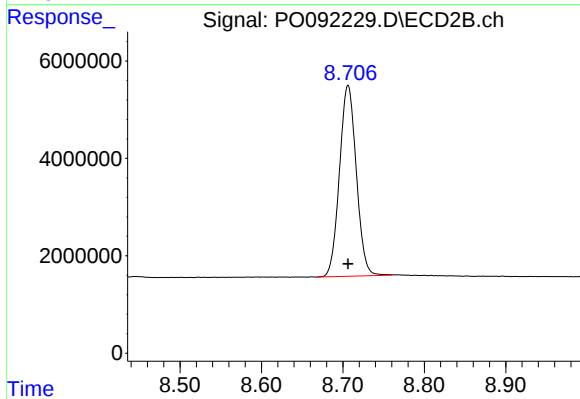

#2 Decachlorobiphenyl


R.T.: 8.706 min
Delta R.T.: 0.000 min
Response: 56406677
Conc: 50.00 ng/ml

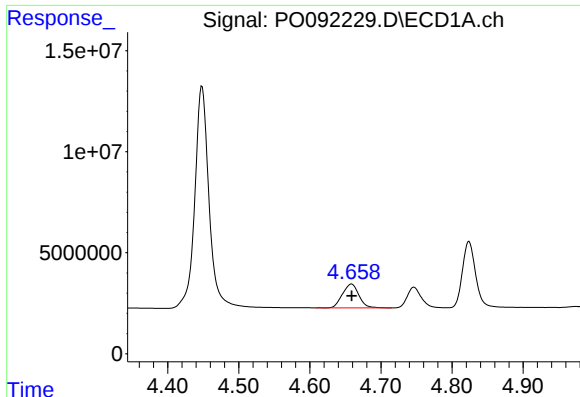

#8 AR-1221-1


R.T.: 4.659 min
Delta R.T.: 0.000 min
Response: 18902502
Conc: 500.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

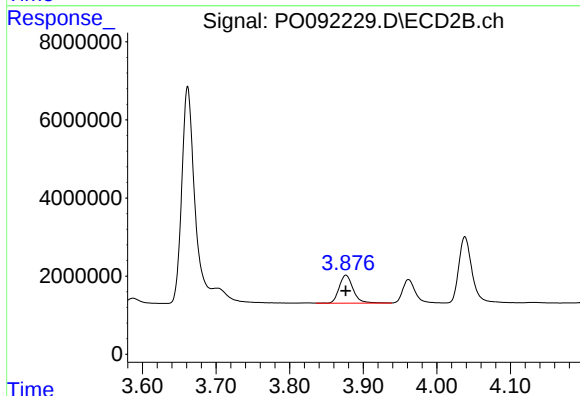


#8 AR-1221-1

R.T.: 3.877 min
Delta R.T.: 0.000 min
Response: 9465301
Conc: 500.00 ng/ml

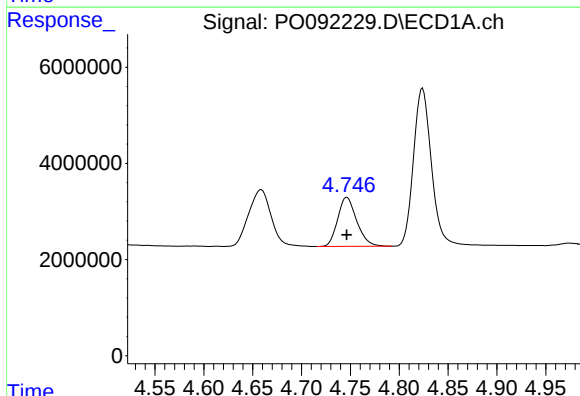


#9 AR-1221-2

R.T.: 4.746 min
Delta R.T.: 0.000 min
Response: 13837241
Conc: 500.00 ng/ml

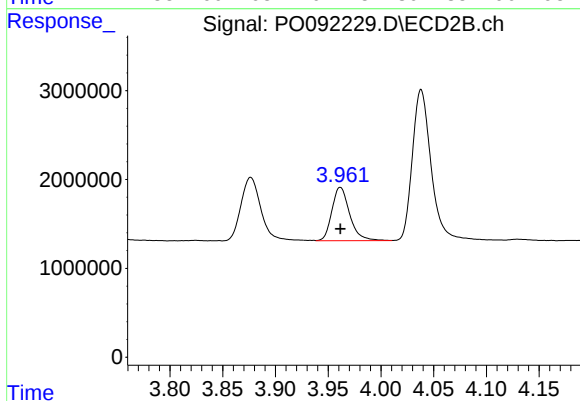

#9 AR-1221-2


R.T.: 3.962 min
Delta R.T.: 0.000 min
Response: 7026989
Conc: 500.00 ng/ml

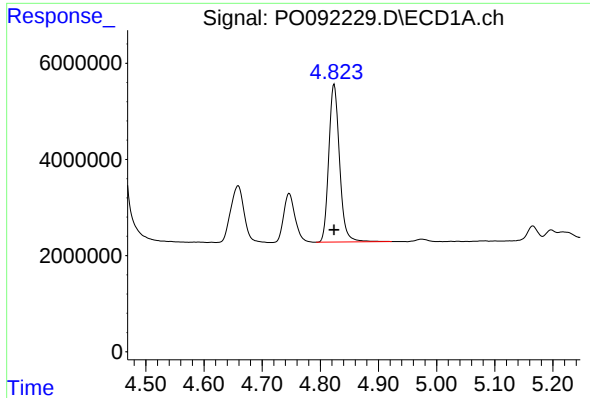

#10 AR-1221-3

R.T.: 4.824 min
Delta R.T.: 0.000 min
Response: 42191886
Conc: 500.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

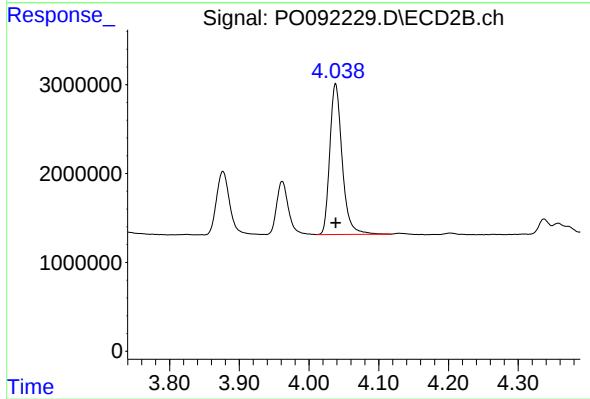

#10 AR-1221-3

R.T.: 4.038 min
Delta R.T.: 0.000 min
Response: 20937603
Conc: 500.00 ng/ml