

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012420\
 Data File : P0065891.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jan 2020 14:07
 Operator : DD\AJ
 Sample : L1230-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 14:59:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.153	3.431	574536	683310	24.777	25.726
2)	SA Decachlor...	9.647	8.327	921511	1139667	22.137	23.452
Target Compounds							
3)	L1 AR-1016-1	5.239	0.000	27827	0	25.338	N.D. #
9)	L2 AR-1221-2	0.000	3.724	0	11388	N.D.	44.815 #
16)	L4 AR-1242-1	5.239	0.000	27827	0	34.529	N.D. #
21)	L5 AR-1248-1	5.239	0.000	27827	0	45.061	N.D. #
28)	L6 AR-1254-3	6.731	0.000	15987	0	6.574	N.D. #
30)	L6 AR-1254-5	0.000	6.459	0	7837	N.D.	2.424 #
32)	L7 AR-1260-2	7.136	0.000	20290	0	7.738	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012420\
Data File : P0065891.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jan 2020 14:07
Operator : DD\AJ
Sample : L1230-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 14:59:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

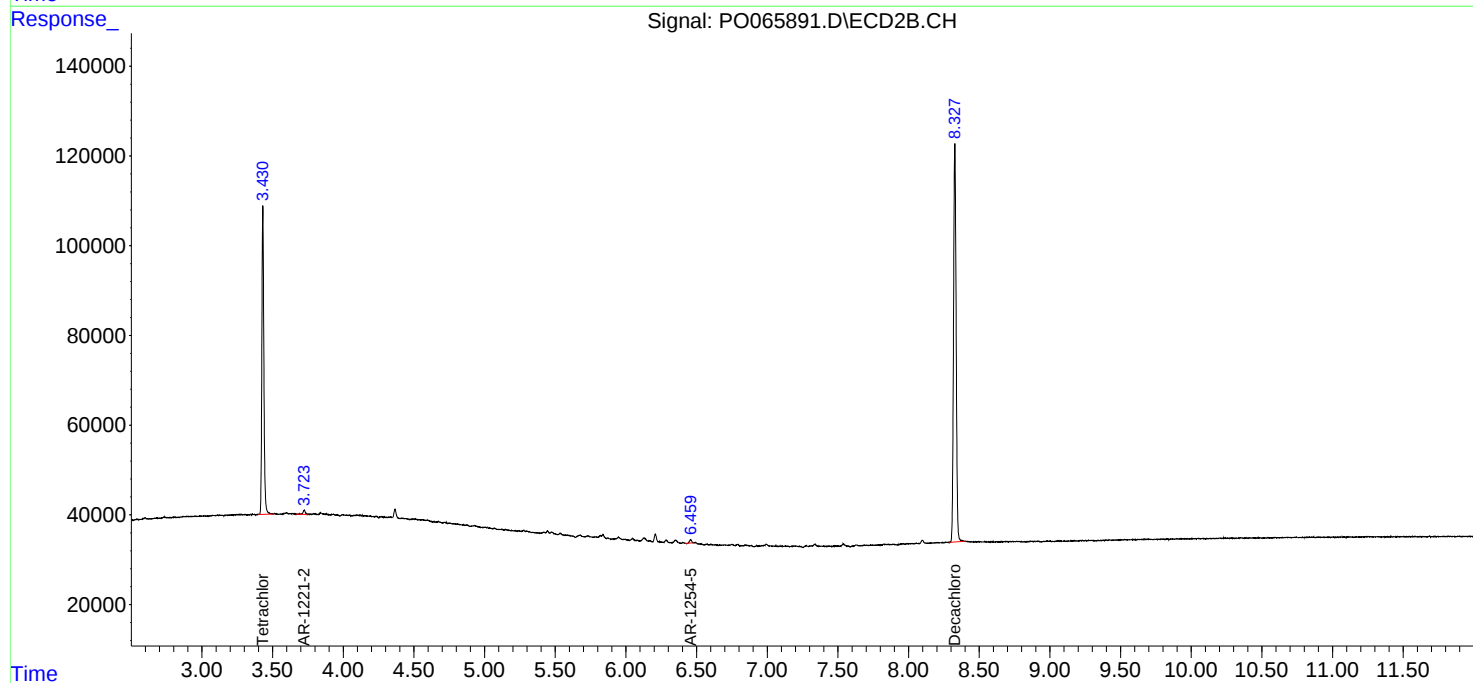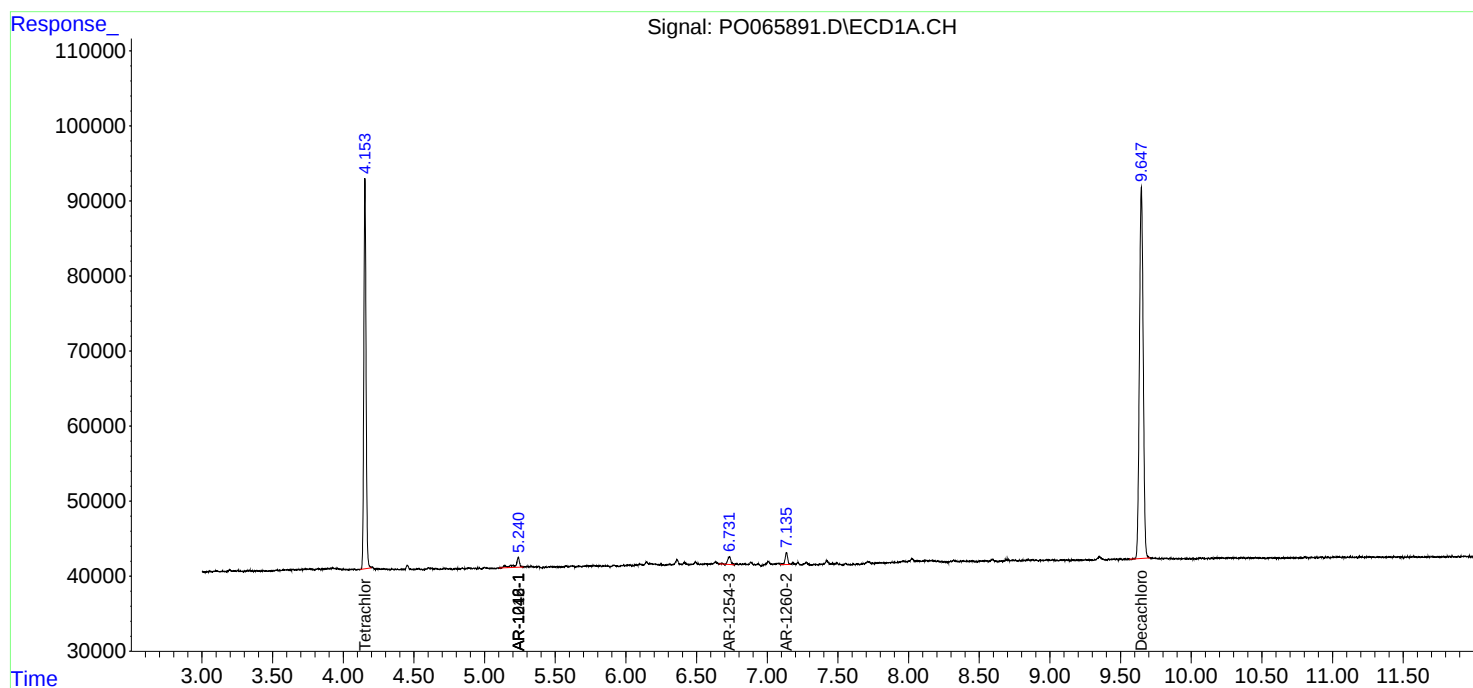


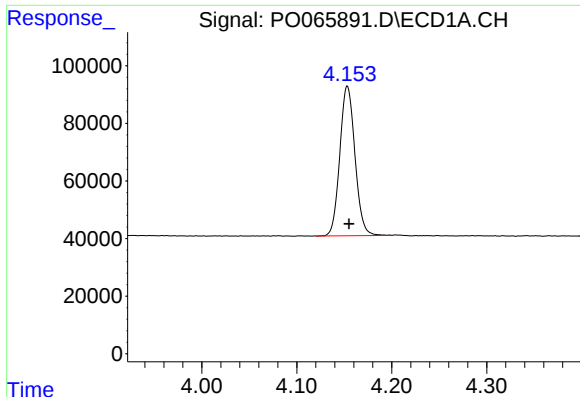

#1 Tetrachloro-m-xylene


R.T.: 4.153 min
Delta R.T.: -0.002 min
Response: 574536
Conc: 24.78 ng/ml

Instrument :
ECD_O
ClientSampleId :

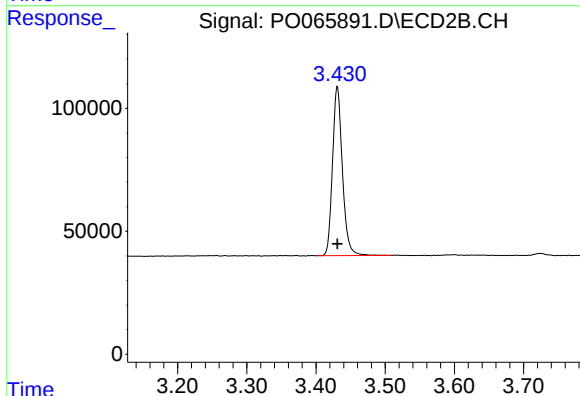


#1 Tetrachloro-m-xylene

R.T.: 3.431 min
Delta R.T.: 0.000 min
Response: 683310
Conc: 25.73 ng/ml

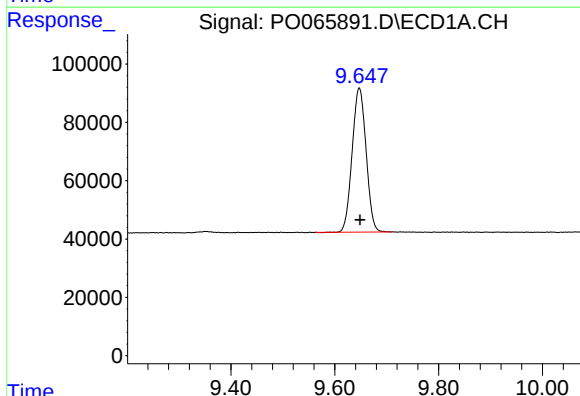


#2 Decachlorobiphenyl

R.T.: 9.647 min
Delta R.T.: -0.002 min
Response: 921511
Conc: 22.14 ng/ml

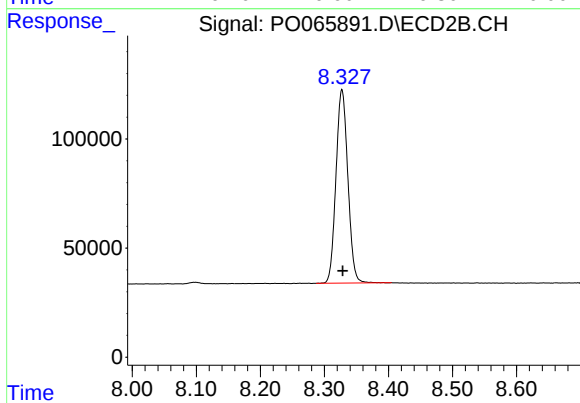

#2 Decachlorobiphenyl


R.T.: 8.327 min
Delta R.T.: -0.001 min
Response: 1139667
Conc: 23.45 ng/ml

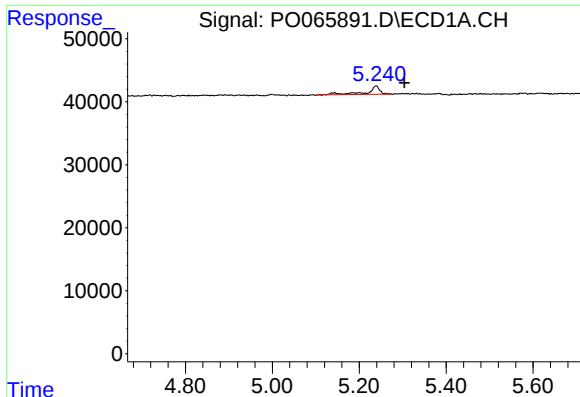

#3 AR-1016-1


R.T.: 5.239 min
Delta R.T.: -0.065 min
Response: 27827
Conc: 25.34 ng/ml

Instrument :
ECD_O
ClientSampleId :

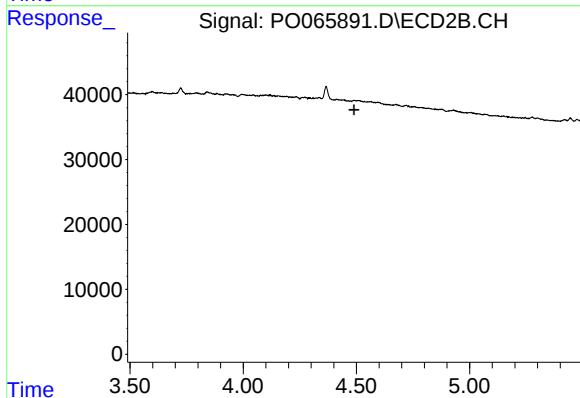


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.489 min
Response: 0
Conc: N.D.

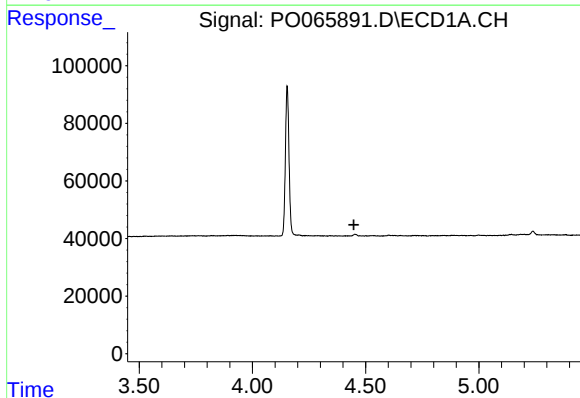


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.448 min
Response: 0
Conc: N.D.

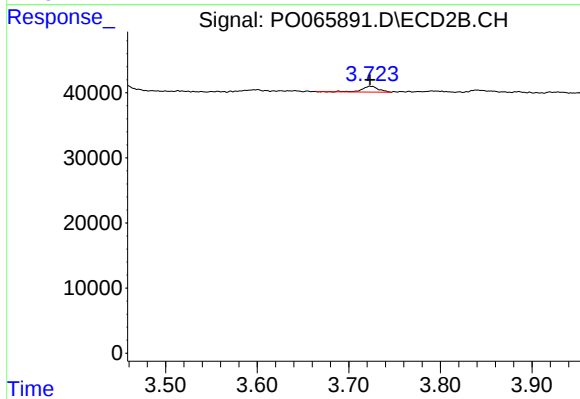

#9 AR-1221-2


R.T.: 3.724 min
Delta R.T.: 0.000 min
Response: 11388
Conc: 44.82 ng/ml

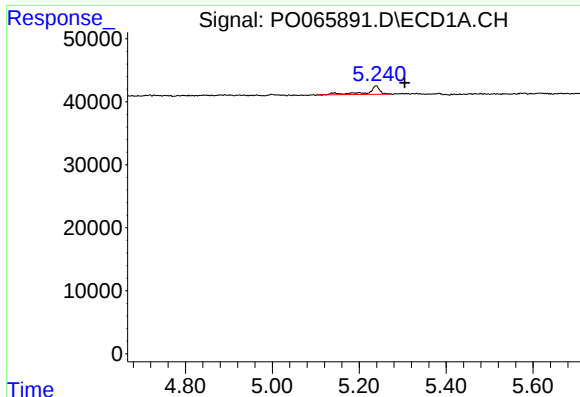

#16 AR-1242-1


R.T.: 5.239 min
Delta R.T.: -0.066 min
Response: 27827
Conc: 34.53 ng/ml

Instrument :
ECD_O
ClientSampleId :

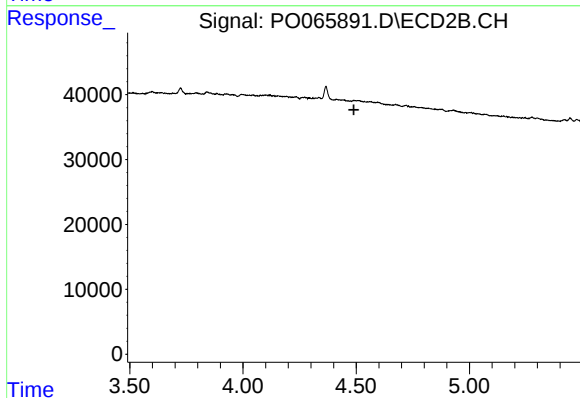


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

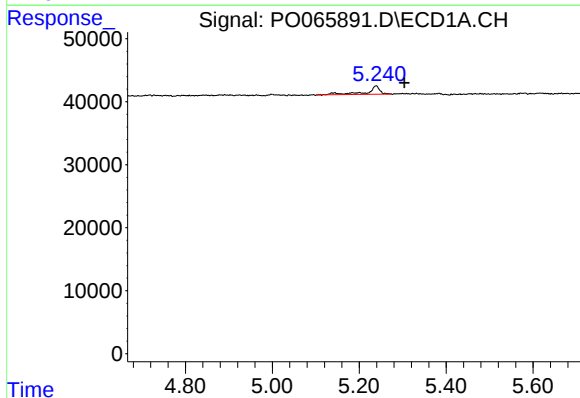


#21 AR-1248-1

R.T.: 5.239 min
Delta R.T.: -0.065 min
Response: 27827
Conc: 45.06 ng/ml

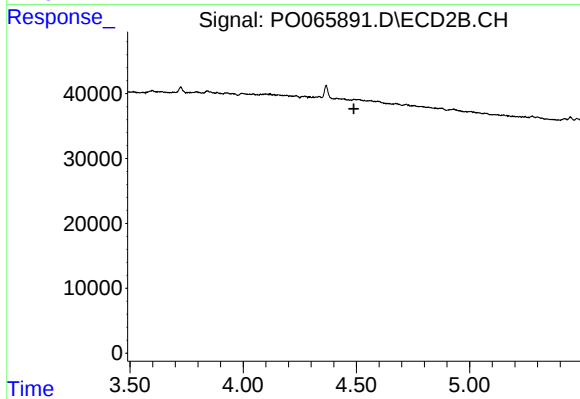

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T. : 4.489 min
Response: 0
Conc: N.D.

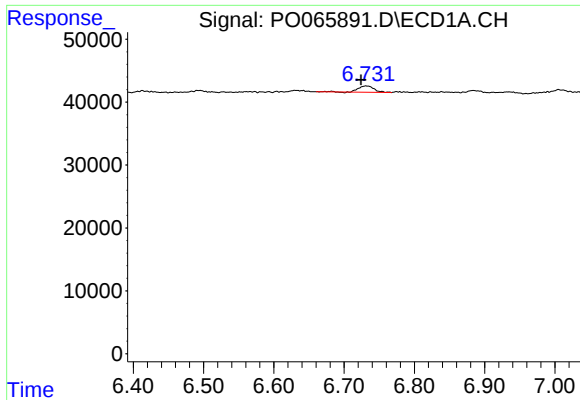

#28 AR-1254-3


R.T.: 6.731 min
Delta R.T.: 0.007 min
Response: 15987
Conc: 6.57 ng/ml

Instrument :
ECD_O
ClientSampleId :

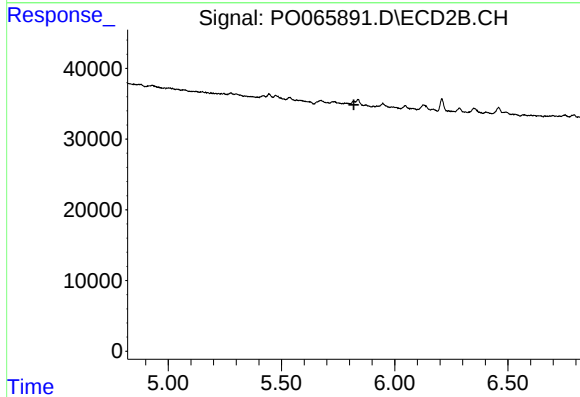


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 5.820 min
Response: 0
Conc: N.D.

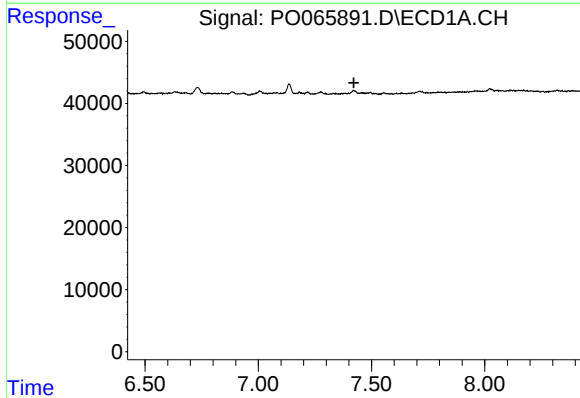


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.422 min
Response: 0
Conc: N.D.

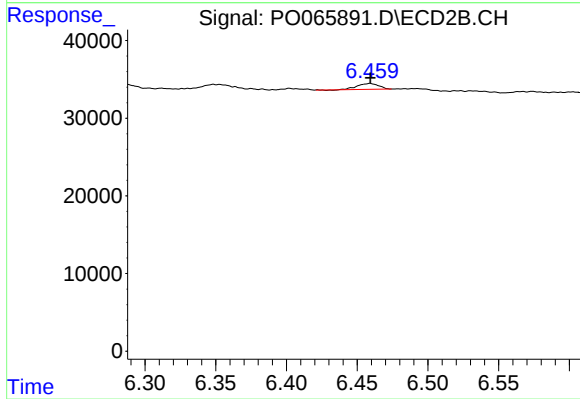

#30 AR-1254-5


R.T.: 6.459 min
Delta R.T.: 0.000 min
Response: 7837
Conc: 2.42 ng/ml

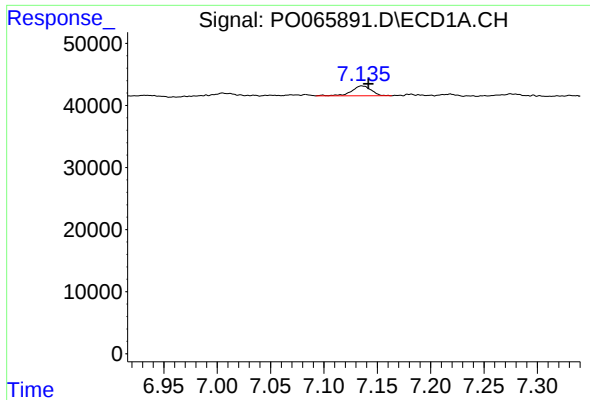

#32 AR-1260-2

R.T.: 7.136 min
Delta R.T.: -0.006 min
Response: 20290
Conc: 7.74 ng/ml

Instrument :
ECD_O
ClientSampleId :

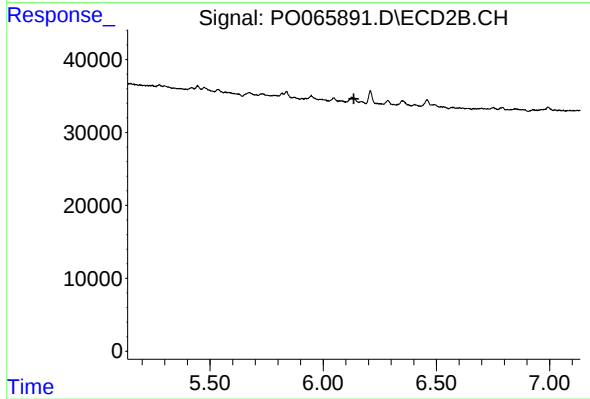

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.136 min
Response: 0
Conc: N.D.