

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012420\
 Data File : P0065917.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jan 2020 21:24
 Operator : DD\AJ
 Sample : L1173-05
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 22:22:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.156	3.433	463562	573152	19.992	21.578
2)	SA Decachlor...	9.647	8.328	735008	879928	17.657	18.107
Target Compounds							
3)	L1 AR-1016-1	5.239	0.000	57158	0	52.045	N.D. #
12)	L3 AR-1232-2	5.075	0.000	35482	0	122.853	N.D. #
16)	L4 AR-1242-1	5.239	0.000	57158	0	70.924	N.D. #
21)	L5 AR-1248-1	5.239	0.000	57158	0	92.556	N.D. #
27)	L6 AR-1254-2	6.326	0.000	10802	0	4.958	N.D. #
28)	L6 AR-1254-3	6.734	0.000	27416	0	11.274	N.D. #
32)	L7 AR-1260-2	0.000	6.123	0	23876	N.D.	7.535 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012420\
Data File : P0065917.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jan 2020 21:24
Operator : DD\AJ
Sample : L1173-05
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 22:22:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

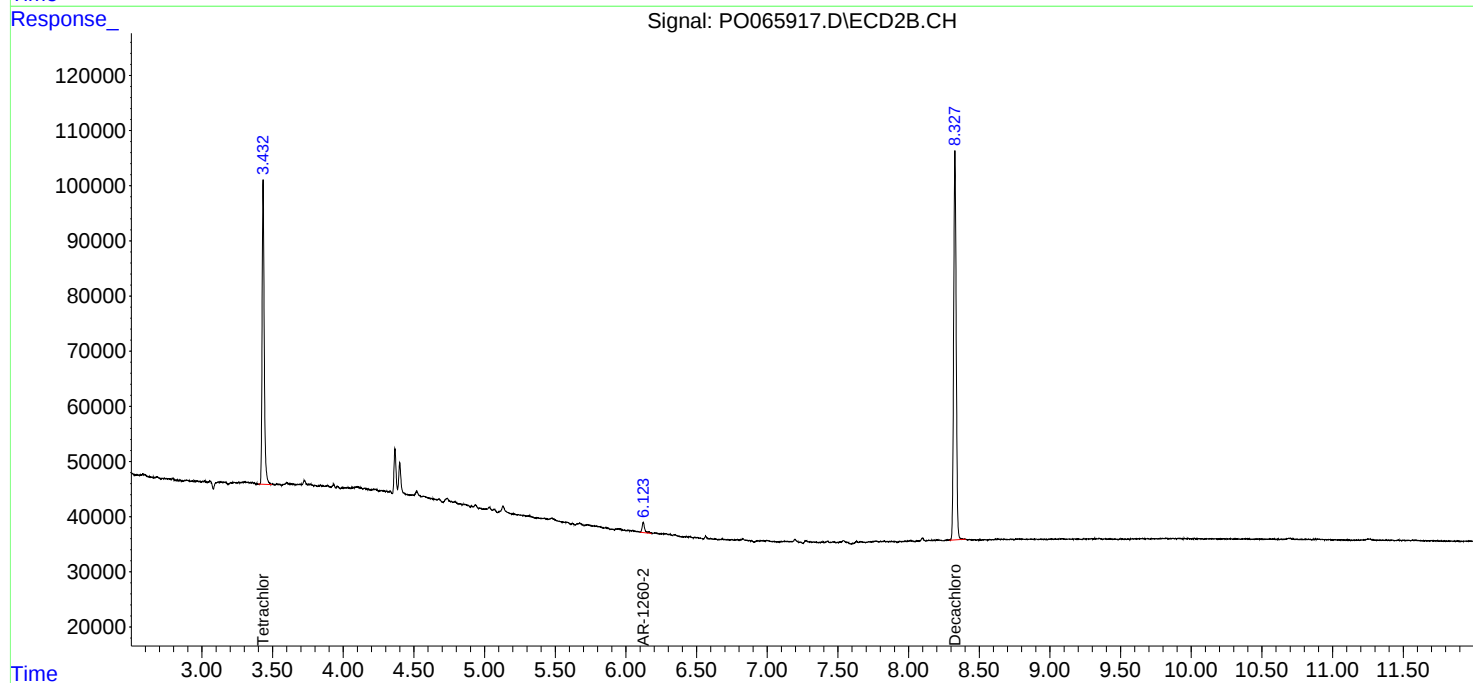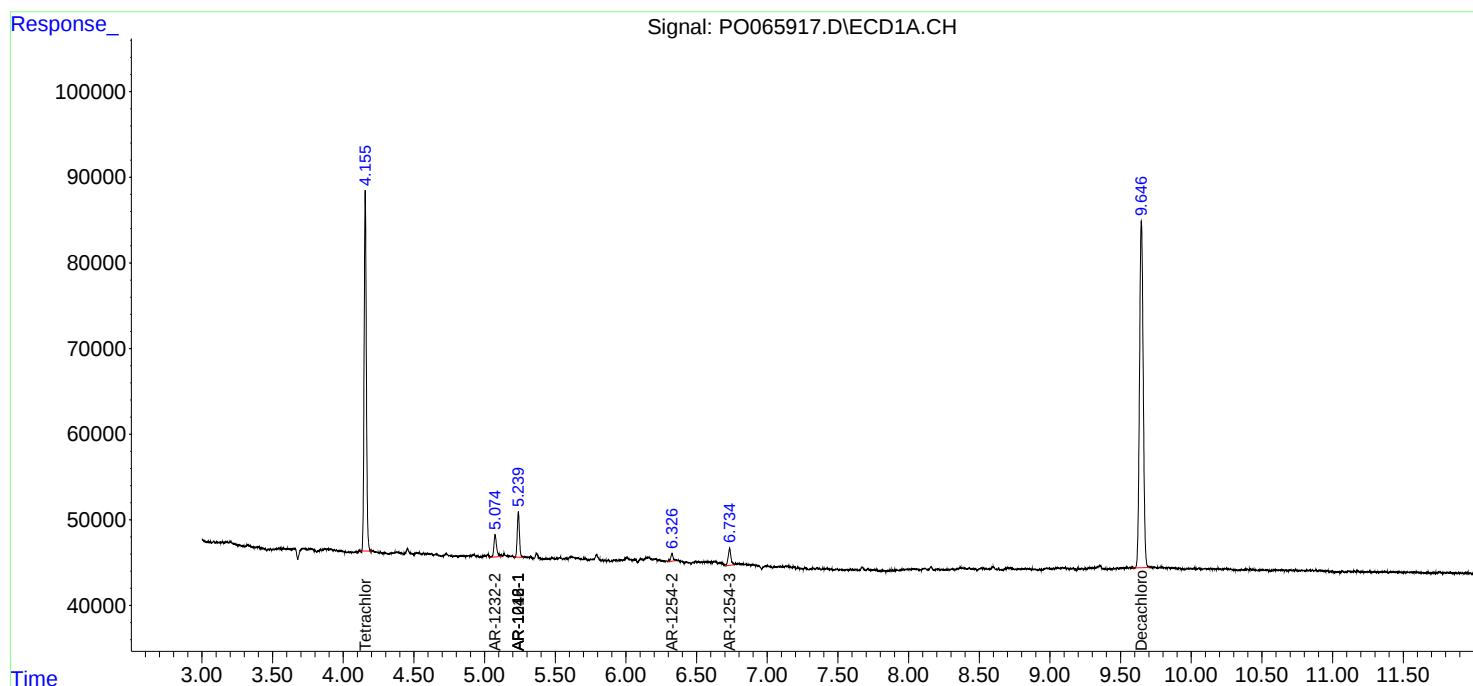


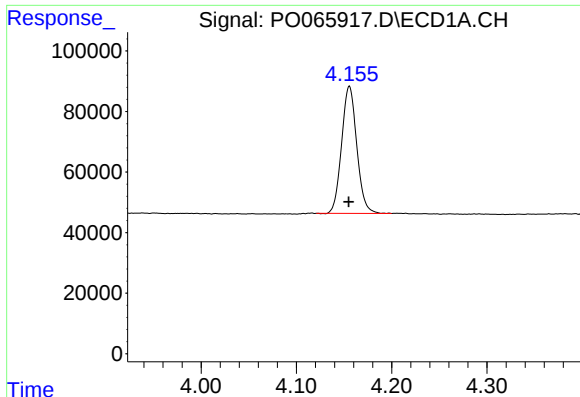

#1 Tetrachloro-m-xylene


R.T.: 4.156 min
Delta R.T.: 0.000 min
Response: 463562
Conc: 19.99 ng/ml

Instrument :
ECD_O
ClientSampleId :

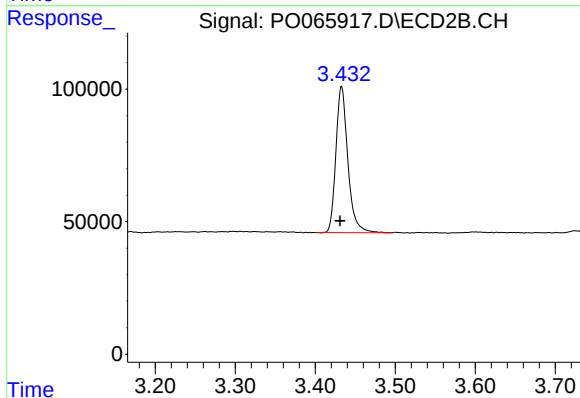


#1 Tetrachloro-m-xylene

R.T.: 3.433 min
Delta R.T.: 0.002 min
Response: 573152
Conc: 21.58 ng/ml

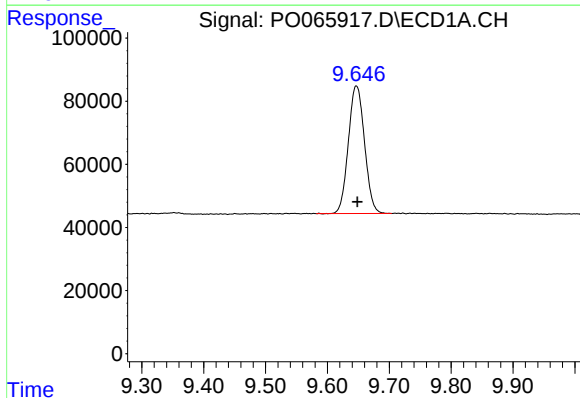


#2 Decachlorobiphenyl

R.T.: 9.647 min
Delta R.T.: -0.002 min
Response: 735008
Conc: 17.66 ng/ml

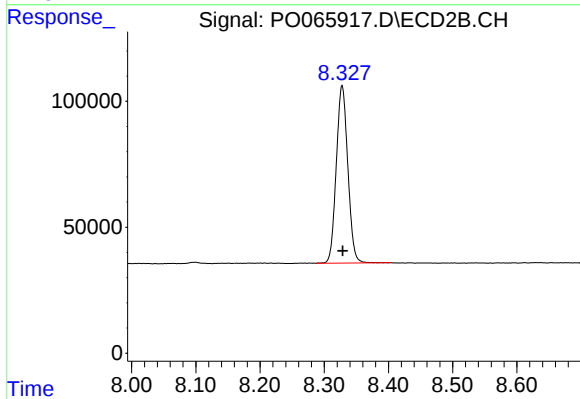

#2 Decachlorobiphenyl


R.T.: 8.328 min
Delta R.T.: 0.000 min
Response: 879928
Conc: 18.11 ng/ml

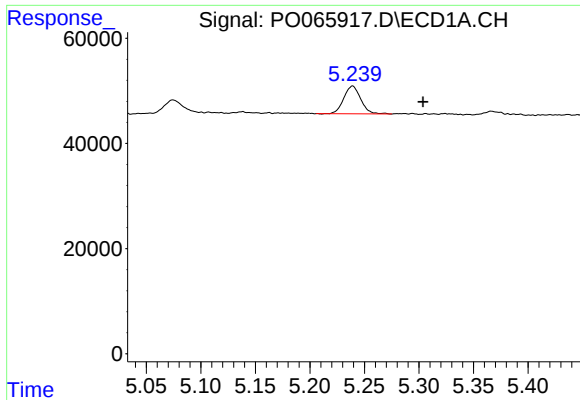

#3 AR-1016-1


R.T.: 5.239 min
Delta R.T.: -0.065 min
Response: 57158
Conc: 52.04 ng/ml

Instrument :
ECD_O
ClientSampleId :

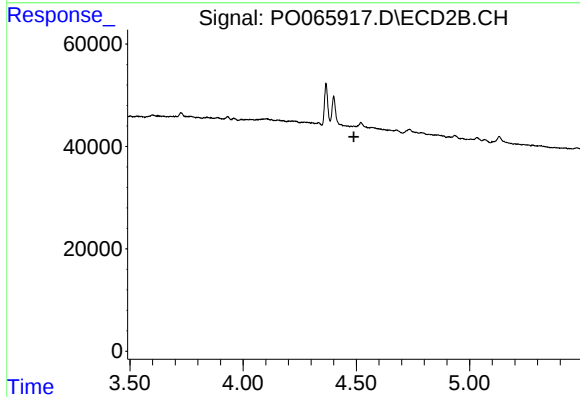


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.489 min
Response: 0
Conc: N.D.

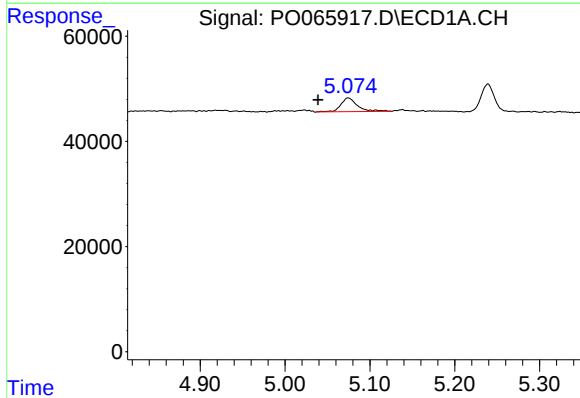


#12 AR-1232-2

R.T.: 5.075 min
Delta R.T.: 0.035 min
Response: 35482
Conc: 122.85 ng/ml

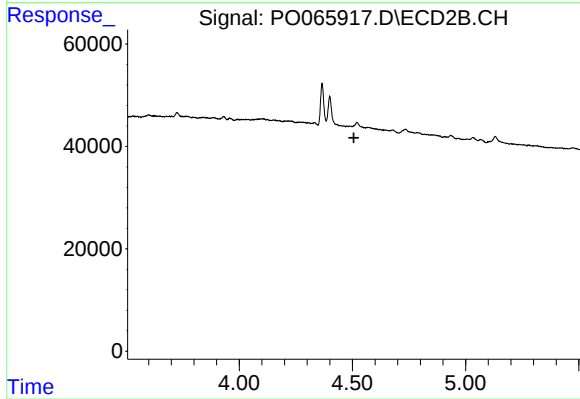

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.507 min
Response: 0
Conc: N.D.

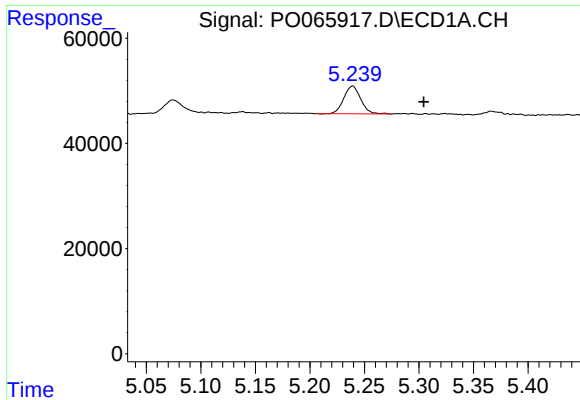

#16 AR-1242-1


R.T.: 5.239 min
Delta R.T.: -0.065 min
Response: 57158
Conc: 70.92 ng/ml

Instrument :
ECD_O
ClientSampleId :

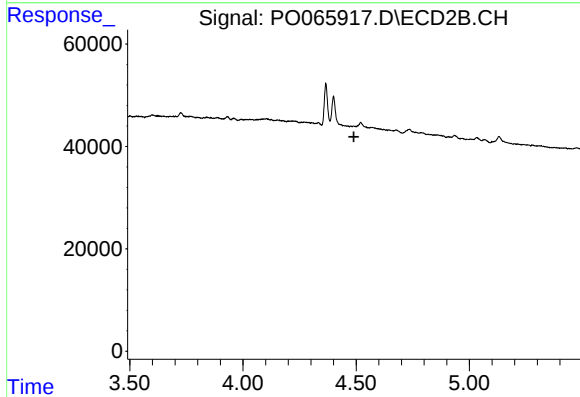


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.490 min
Response: 0
Conc: N.D.

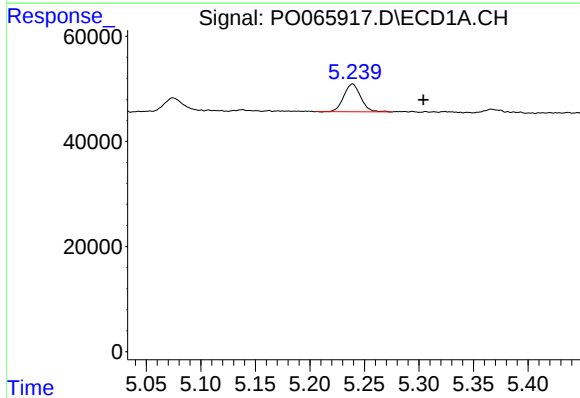


#21 AR-1248-1

R.T.: 5.239 min
Delta R.T.: -0.065 min
Response: 57158
Conc: 92.56 ng/ml

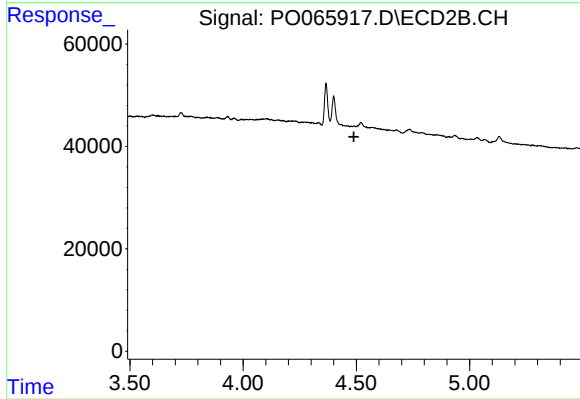

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T. : 4.489 min
Response: 0
Conc: N.D.

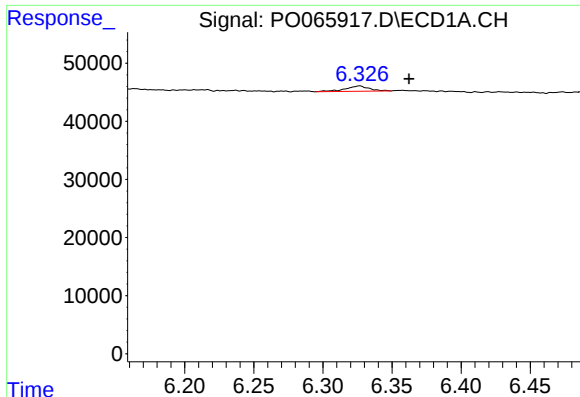

#27 AR-1254-2


R.T.: 6.326 min
Delta R.T.: -0.036 min
Response: 10802
Conc: 4.96 ng/ml

Instrument :
ECD_O
ClientSampleId :

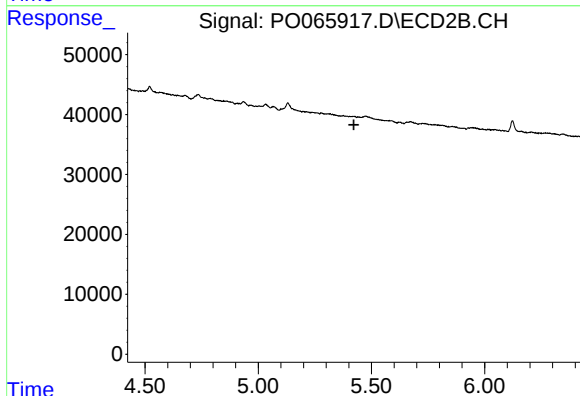


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.422 min
Response: 0
Conc: N.D.

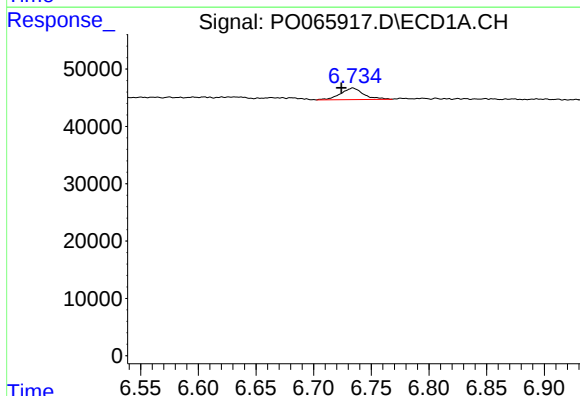


#28 AR-1254-3

R.T.: 6.734 min
Delta R.T.: 0.010 min
Response: 27416
Conc: 11.27 ng/ml

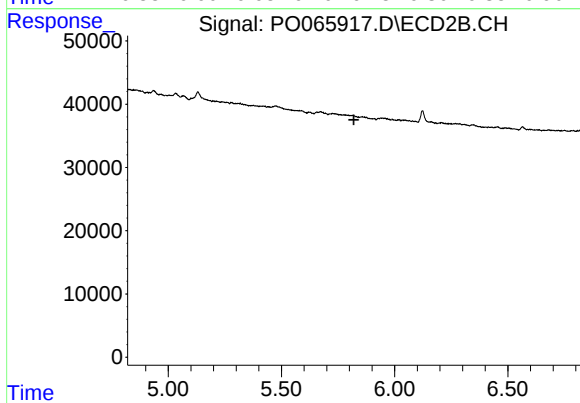

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 5.820 min
Response: 0
Conc: N.D.

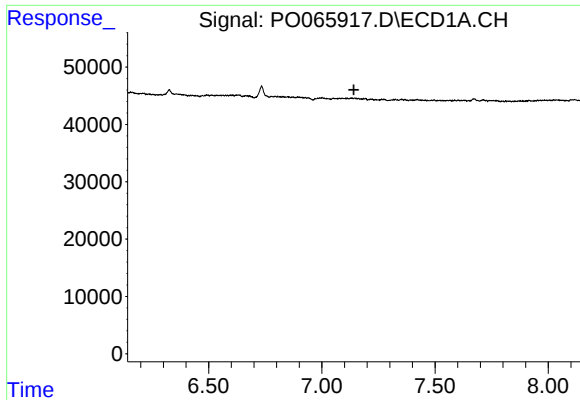

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.142 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

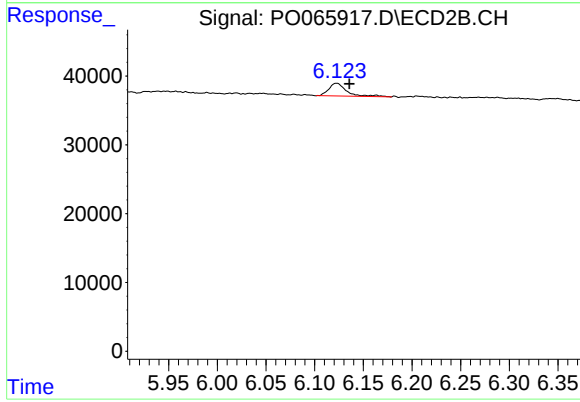

#32 AR-1260-2

R.T.: 6.123 min
Delta R.T.: -0.013 min
Response: 23876
Conc: 7.54 ng/ml