

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012420\
 Data File : P0065920.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jan 2020 22:14
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 23:56:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.154	3.431	440403	525195	18.993	19.773
2)	SA Decachlor...	9.648	8.328	703844	857030	16.908	17.636
Target Compounds							
7)	L1 AR-1016-5	0.000	4.932	0	211823	N.D.	196.471 #
15)	L3 AR-1232-5	0.000	4.932	0	211823	N.D.	531.581 #
20)	L4 AR-1242-5	6.150	5.300	119404	45339	143.399	40.956 #
24)	L5 AR-1248-4	6.150	4.932	119404	211823	88.620	165.994 #
25)	L5 AR-1248-5	6.150	5.300	119404	45339	92.386	32.484 #
26)	L6 AR-1254-1	6.150	5.300	119404	45339	89.960	20.277 #
28)	L6 AR-1254-3	6.733	5.786	17029	2662	7.003	0.785 #
32)	L7 AR-1260-2	0.000	6.122	0	14272	N.D.	4.504 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012420\
Data File : PO065920.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jan 2020 22:14
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 23:56:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

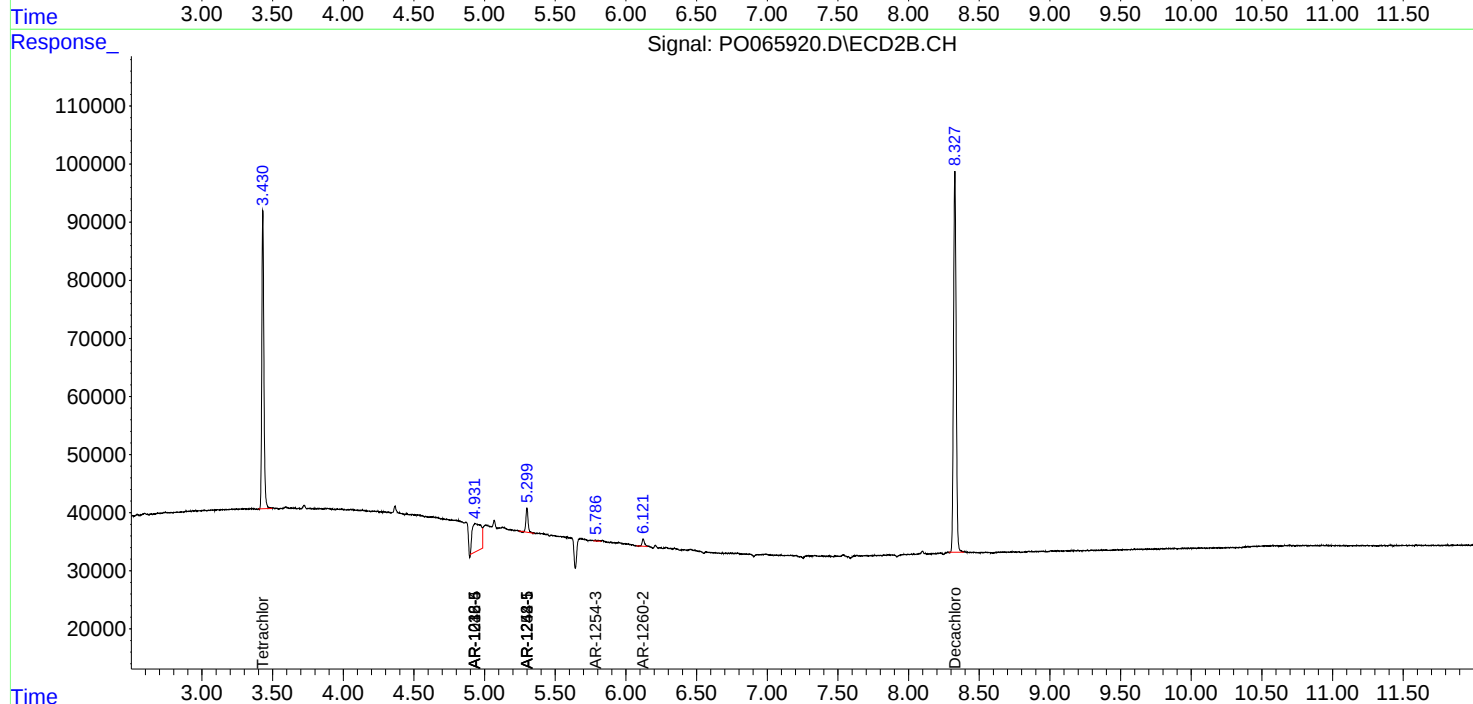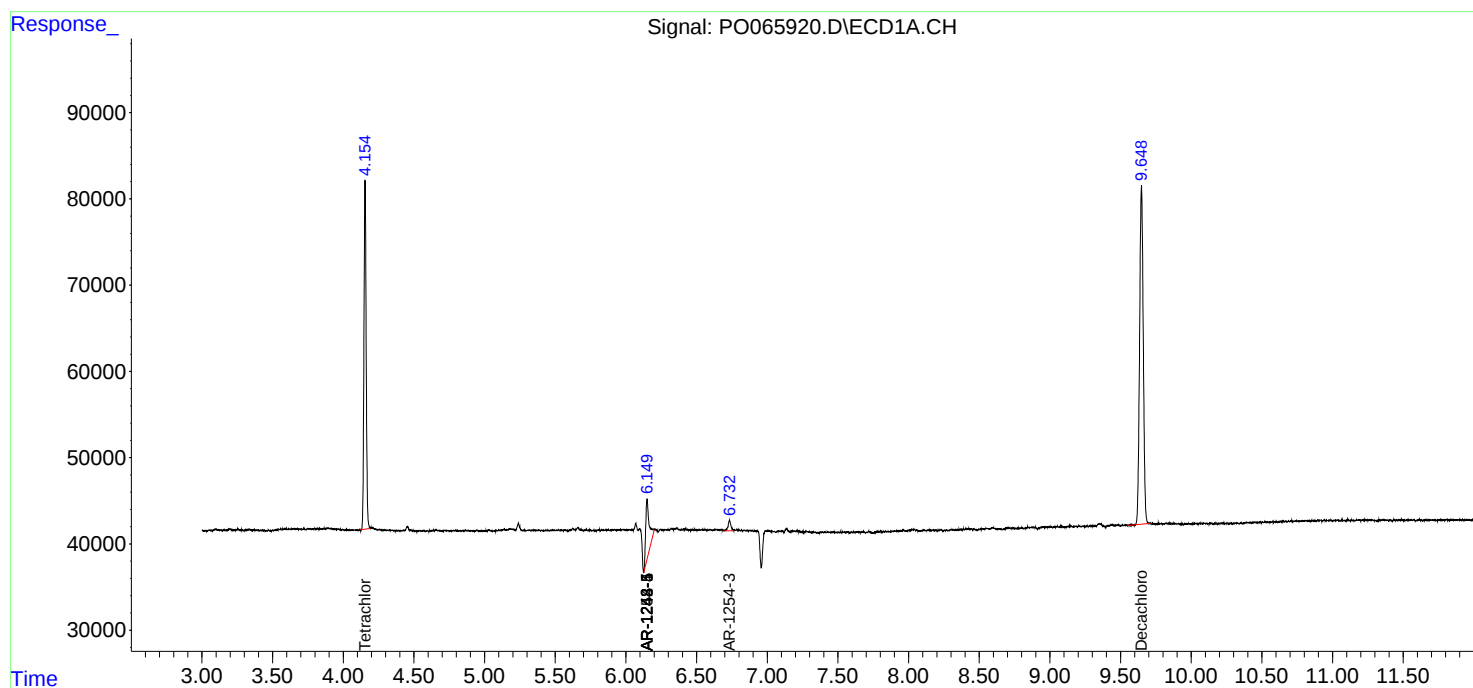


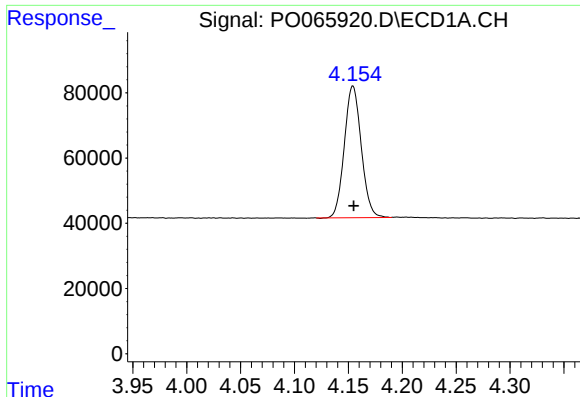

#1 Tetrachloro-m-xylene


R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 440403
Conc: 18.99 ng/ml

Instrument :
ECD_O
ClientSampleId :

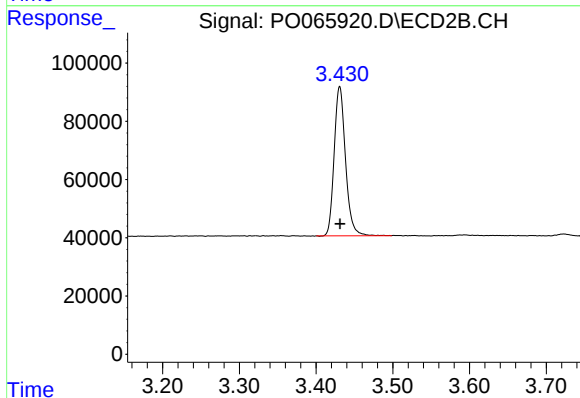


#1 Tetrachloro-m-xylene

R.T.: 3.431 min
Delta R.T.: 0.000 min
Response: 525195
Conc: 19.77 ng/ml

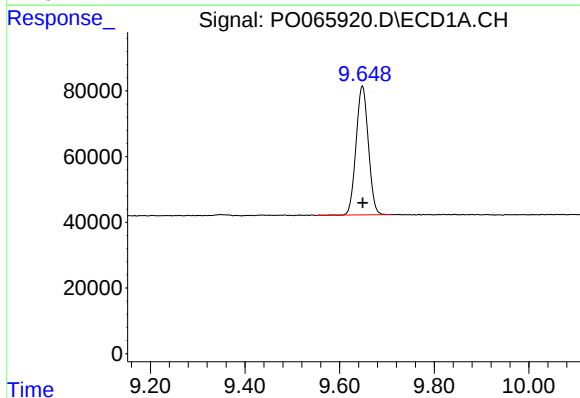


#2 Decachlorobiphenyl

R.T.: 9.648 min
Delta R.T.: 0.000 min
Response: 703844
Conc: 16.91 ng/ml

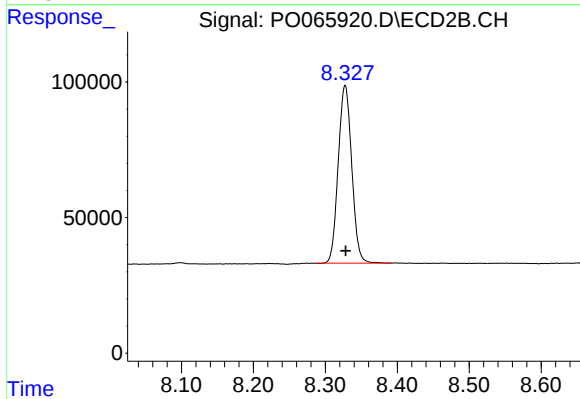

#2 Decachlorobiphenyl


R.T.: 8.328 min
Delta R.T.: -0.001 min
Response: 857030
Conc: 17.64 ng/ml

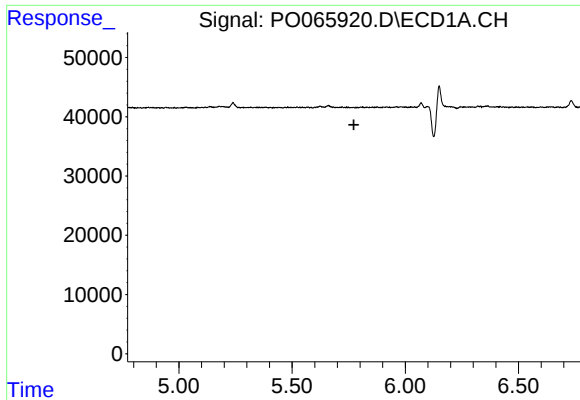

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

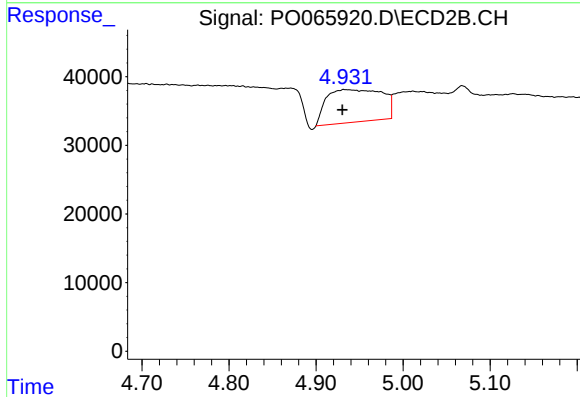


#7 AR-1016-5

R.T.: 4.932 min
Delta R.T.: 0.002 min
Response: 211823
Conc: 196.47 ng/ml

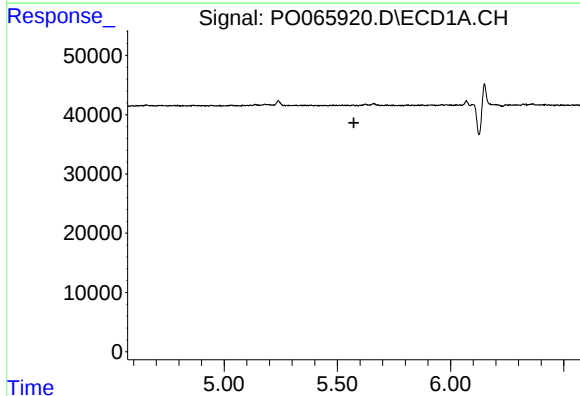


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 5.573 min
Response: 0
Conc: N.D.

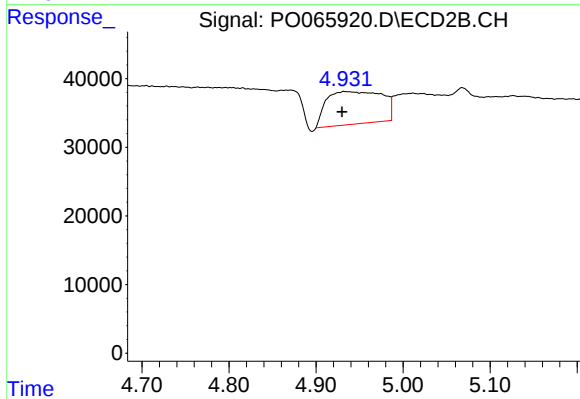

#15 AR-1232-5


R.T.: 4.932 min
Delta R.T.: 0.002 min
Response: 211823
Conc: 531.58 ng/ml

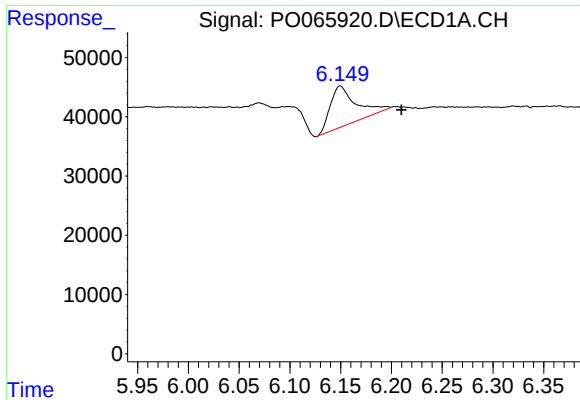

#20 AR-1242-5


R.T.: 6.150 min
Delta R.T.: -0.060 min
Response: 119404
Conc: 143.40 ng/ml

Instrument :
ECD_O
ClientSampleId :

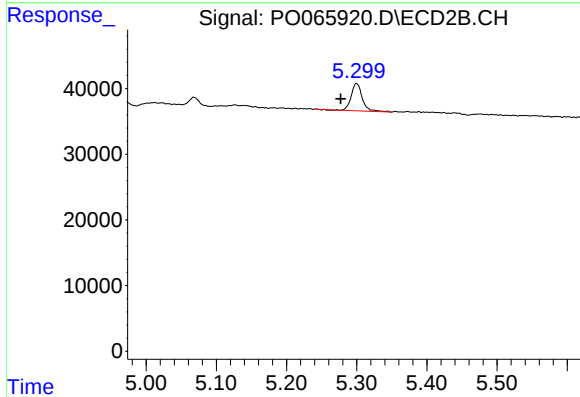


#20 AR-1242-5

R.T.: 5.300 min
Delta R.T.: 0.023 min
Response: 45339
Conc: 40.96 ng/ml

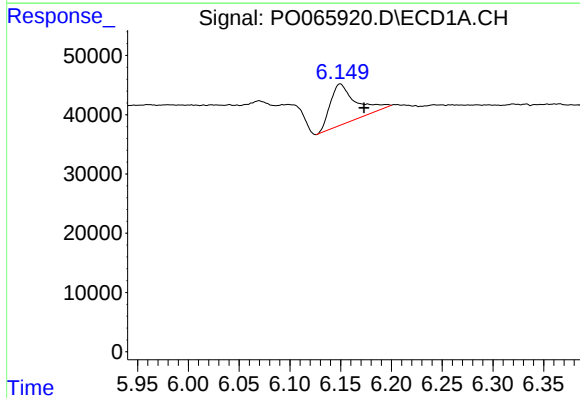


#24 AR-1248-4

R.T.: 6.150 min
Delta R.T.: -0.024 min
Response: 119404
Conc: 88.62 ng/ml

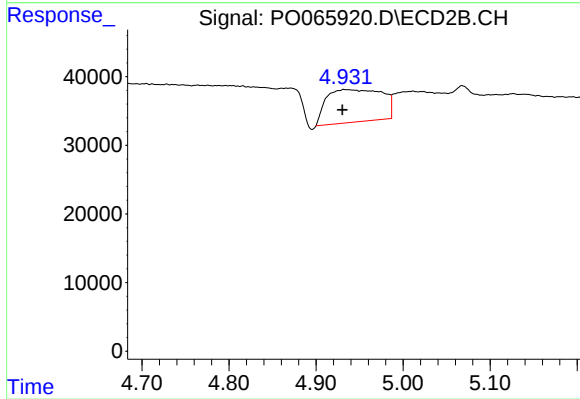

#24 AR-1248-4


R.T.: 4.932 min
Delta R.T.: 0.002 min
Response: 211823
Conc: 165.99 ng/ml

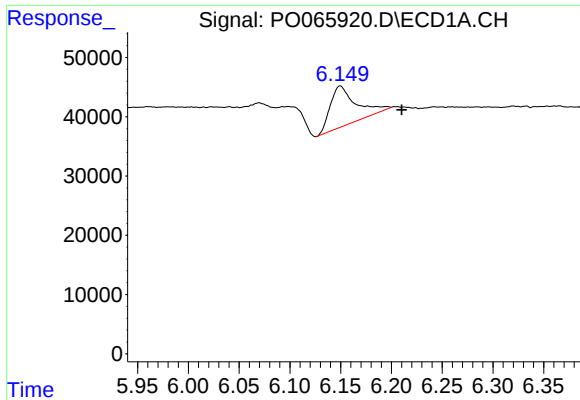

#25 AR-1248-5


R.T.: 6.150 min
Delta R.T.: -0.061 min
Response: 119404
Conc: 92.39 ng/ml

Instrument :
ECD_O
ClientSampleId :

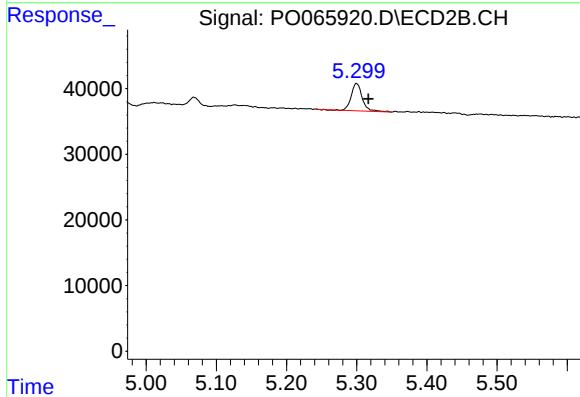


#25 AR-1248-5

R.T.: 5.300 min
Delta R.T.: -0.017 min
Response: 45339
Conc: 32.48 ng/ml

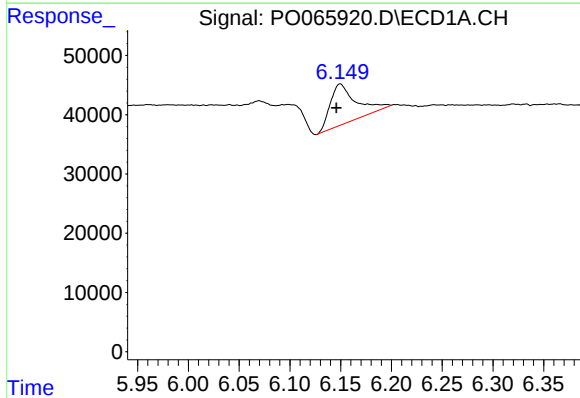


#26 AR-1254-1

R.T.: 6.150 min
Delta R.T.: 0.004 min
Response: 119404
Conc: 89.96 ng/ml

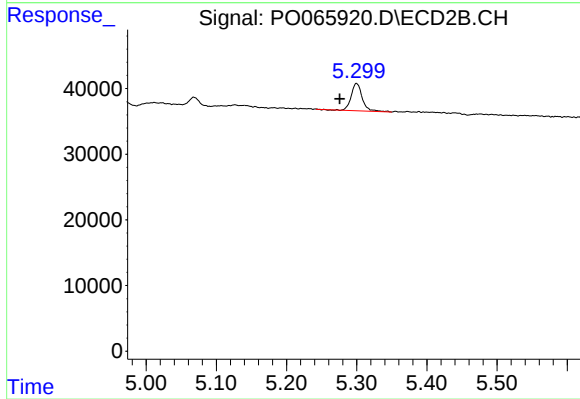

#26 AR-1254-1


R.T.: 5.300 min
Delta R.T.: 0.024 min
Response: 45339
Conc: 20.28 ng/ml

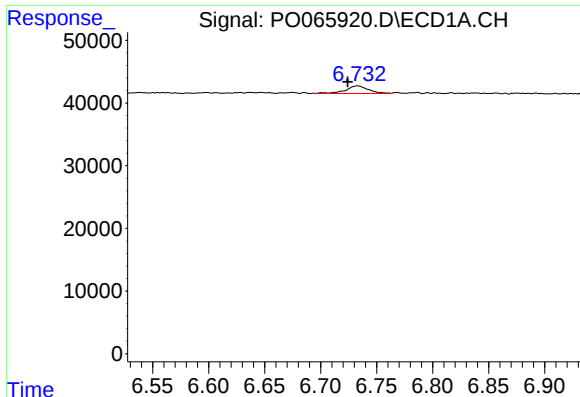

#28 AR-1254-3


R.T.: 6.733 min
Delta R.T.: 0.009 min
Response: 17029
Conc: 7.00 ng/ml

Instrument :
ECD_O
ClientSampleId :

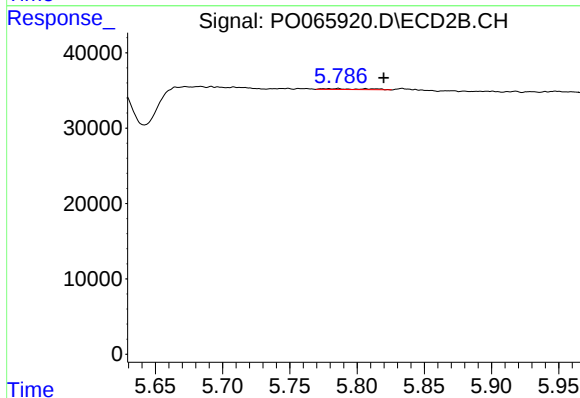


#28 AR-1254-3

R.T.: 5.786 min
Delta R.T.: -0.034 min
Response: 2662
Conc: 0.78 ng/ml

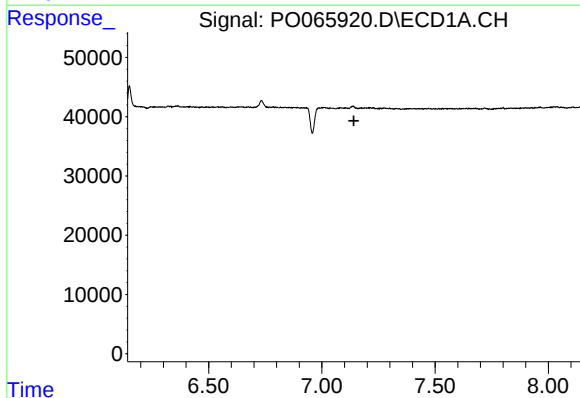

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.142 min
Response: 0
Conc: N.D.

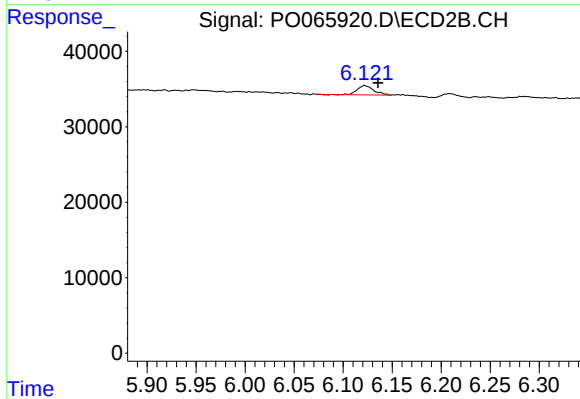

#32 AR-1260-2

R.T.: 6.122 min
Delta R.T.: -0.014 min
Response: 14272
Conc: 4.50 ng/ml