

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012420\
 Data File : P0065883.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jan 2020 11:36
 Operator : DD\AJ
 Sample : L1233-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 55-ST-25

Manual Integrations
 APPROVED

mohammad
 1/27/2020 5:51:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 13:41:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.154	3.432	604591	784076	26.074m	29.519
2) SA Decachlor...	9.647	8.326	878572	1023906	21.106	21.070

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012420\
Data File : P0065883.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jan 2020 11:36
Operator : DD\AJ
Sample : L1233-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
55-ST-25


Manual Integrations
APPROVED

mohammad
1/27/2020 5:51:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 13:41:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

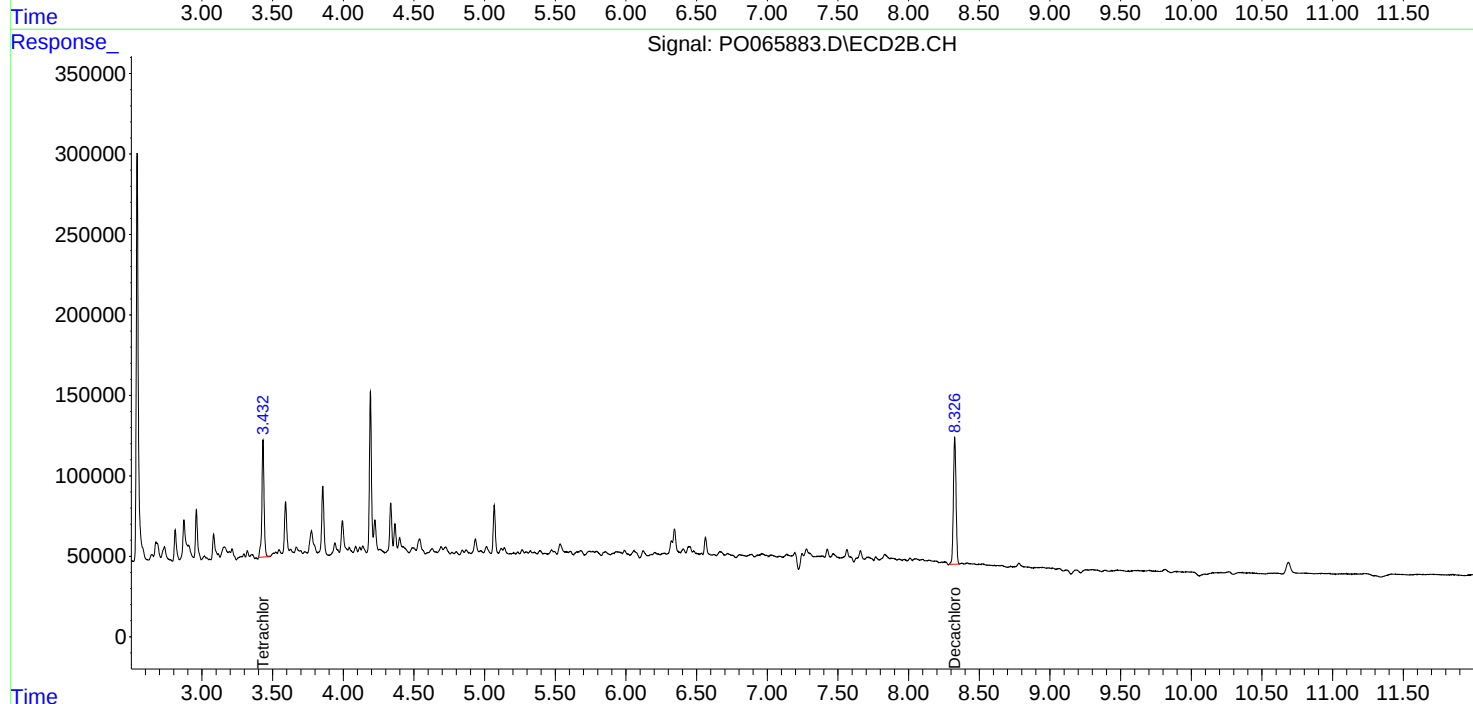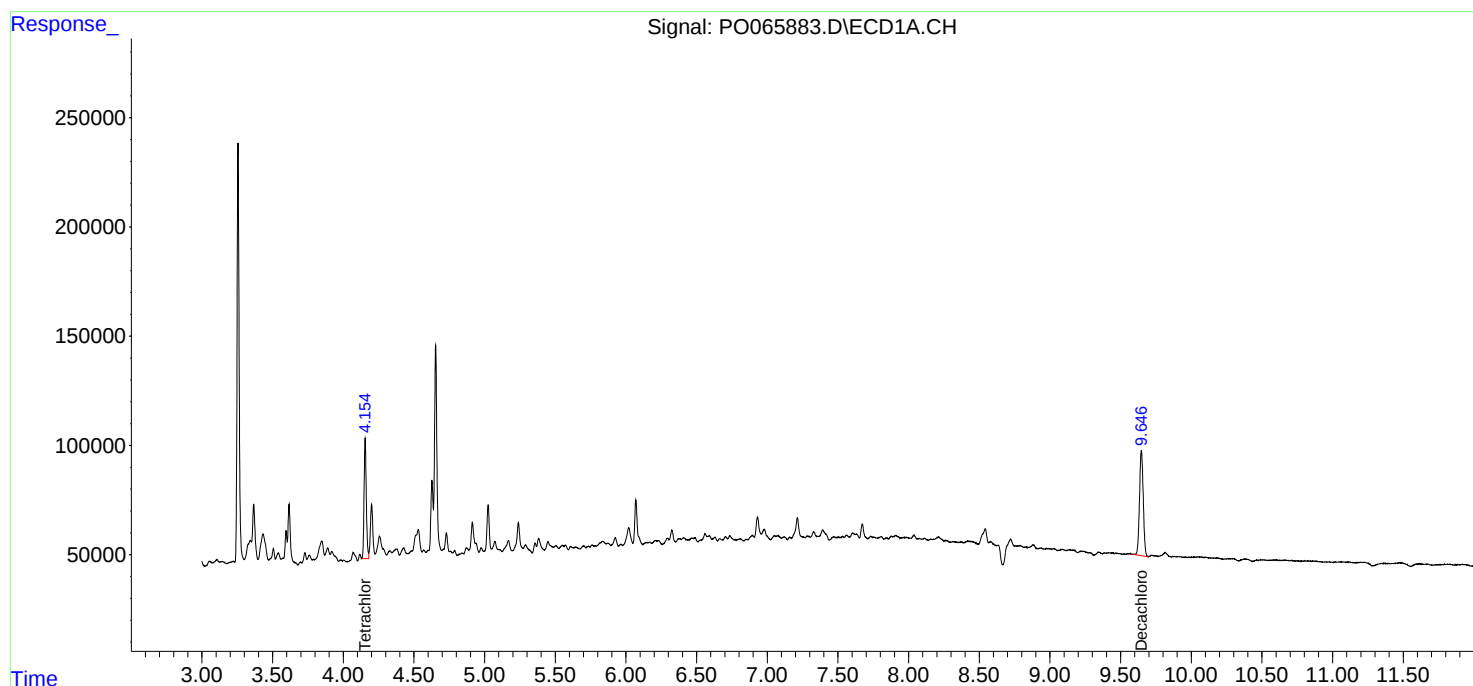

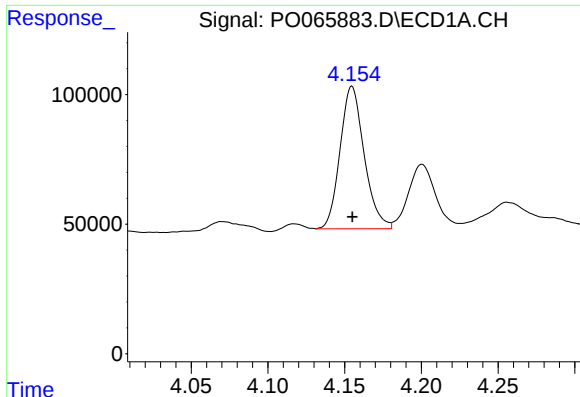


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 604591
Conc: 26.07 ng/ml m

Instrument :
ECD_O
ClientSampleId :
55-ST-25


Manual Integrations
APPROVED

mohammad
1/27/2020 5:51:53 PM

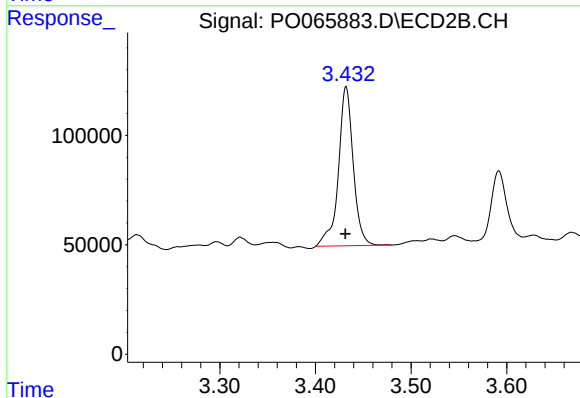


#1 Tetrachloro-m-xylene

R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 784076
Conc: 29.52 ng/ml

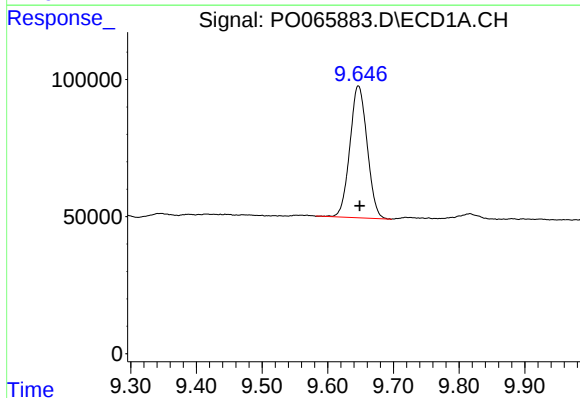

#2 Decachlorobiphenyl

R.T.: 9.647 min
Delta R.T.: -0.002 min
Response: 878572
Conc: 21.11 ng/ml

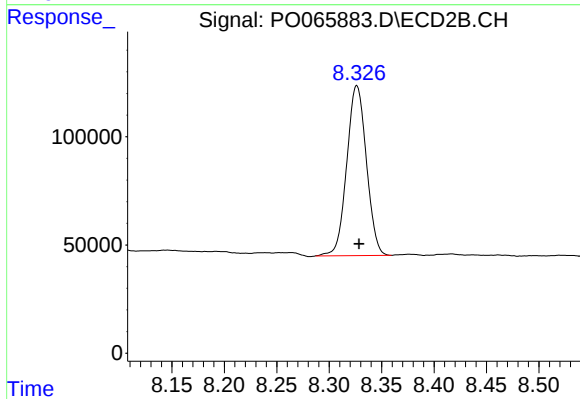

#2 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: -0.002 min
Response: 1023906
Conc: 21.07 ng/ml