

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012420\
 Data File : P0065897.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jan 2020 15:47
 Operator : DD\AJ
 Sample : L1234-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NS-TP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 22:15:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.155	3.432	999561	1614581	43.107	60.787 #
2) SA Decachlor...	9.648	8.328	670067	800471	16.097	16.472

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012420\
Data File : P0065897.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jan 2020 15:47
Operator : DD\AJ
Sample : L1234-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
NS-TP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 22:15:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

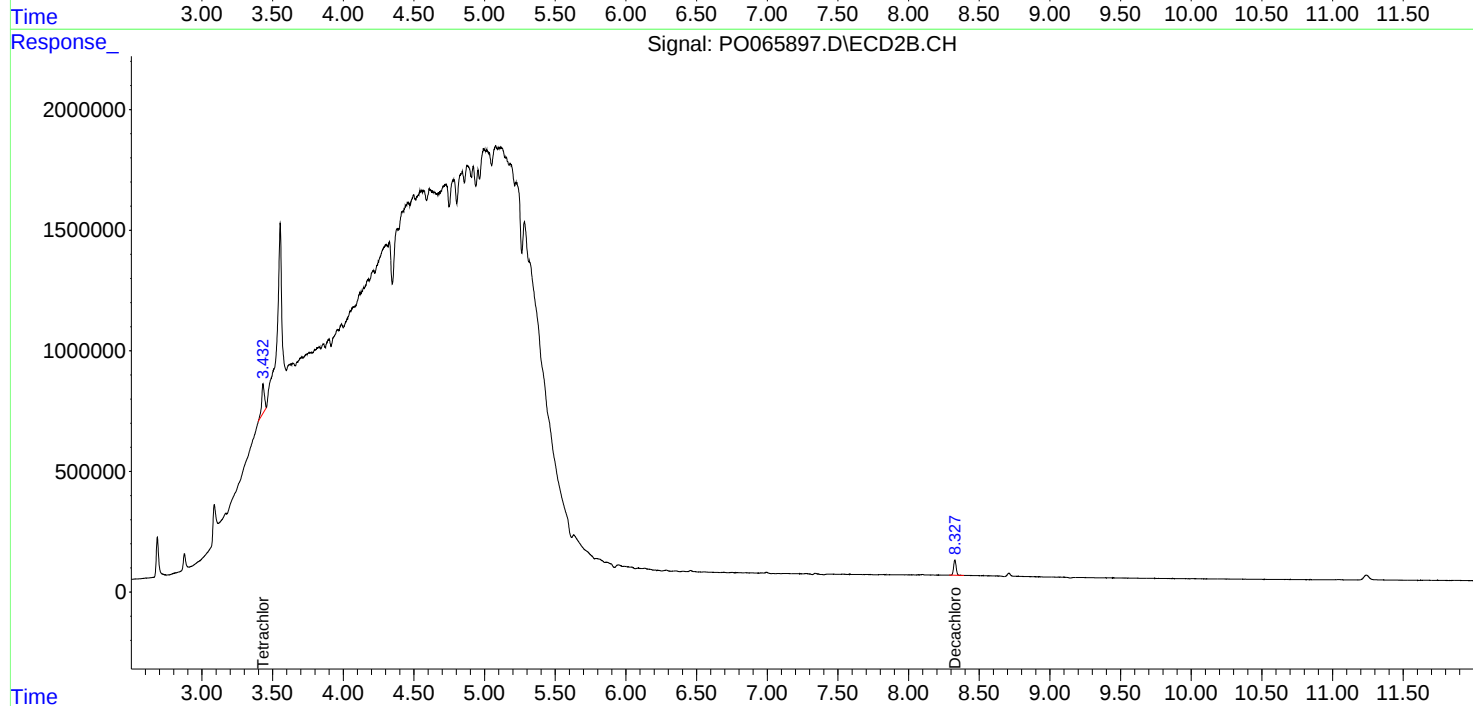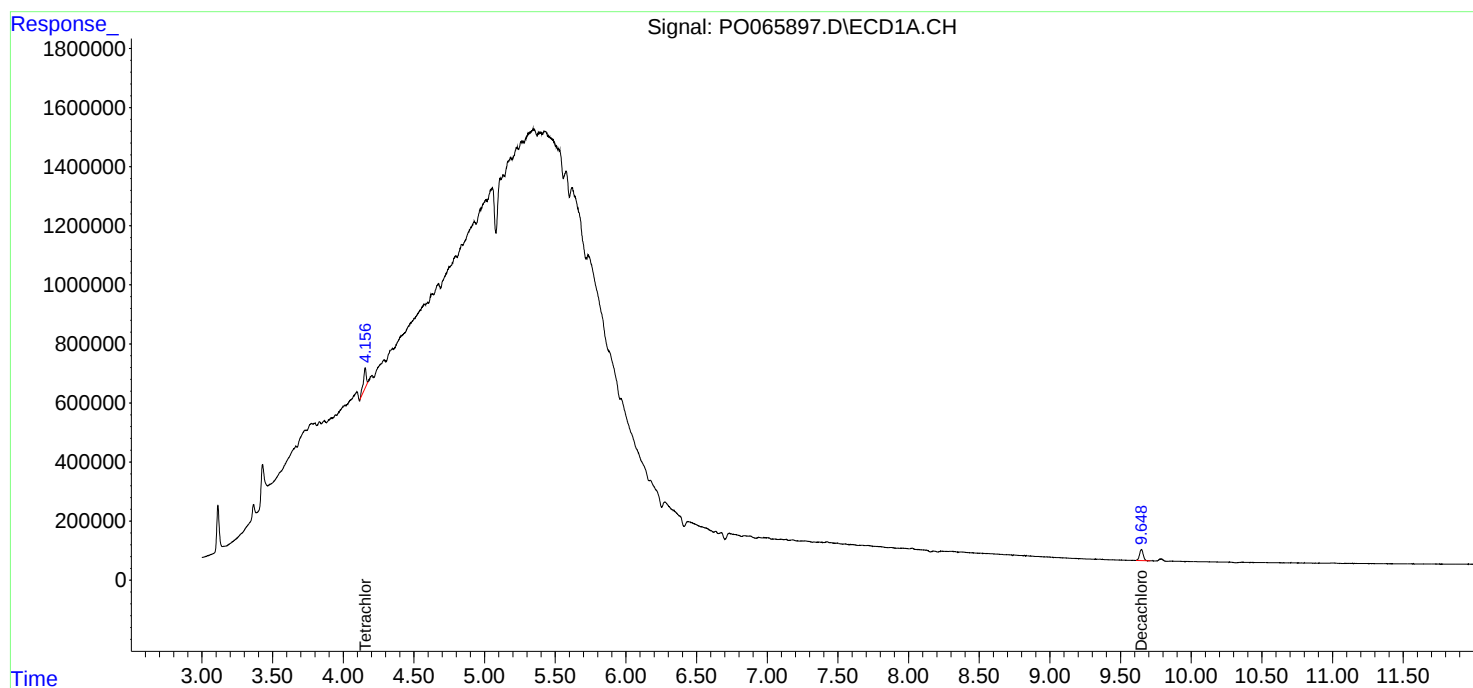


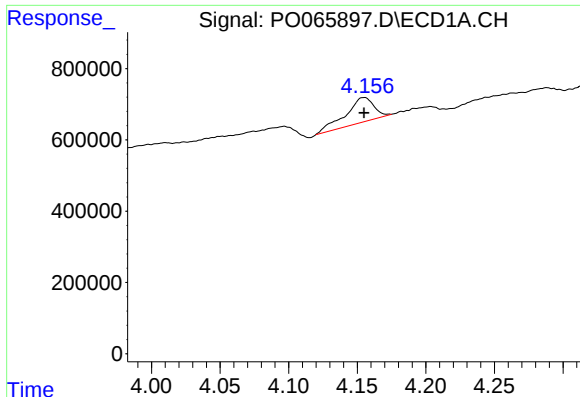

#1 Tetrachloro-m-xylene


R.T.: 4.155 min
Delta R.T.: 0.000 min
Response: 999561
Conc: 43.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
NS-TP

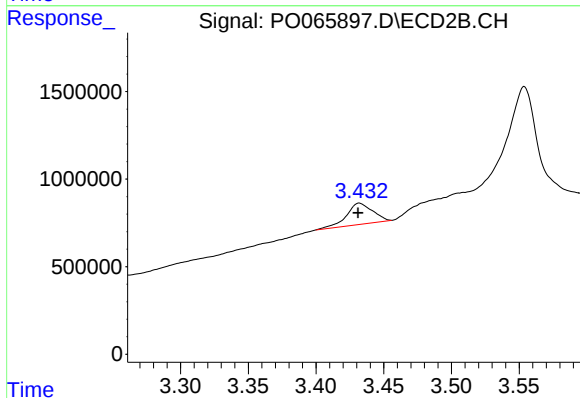


#1 Tetrachloro-m-xylene

R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 1614581
Conc: 60.79 ng/ml

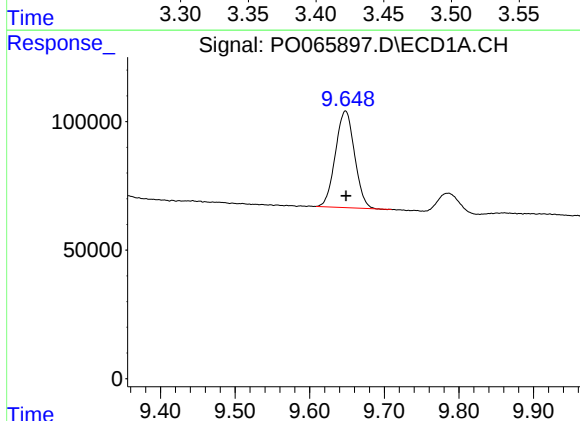

#2 Decachlorobiphenyl

R.T.: 9.648 min
Delta R.T.: 0.000 min
Response: 670067
Conc: 16.10 ng/ml

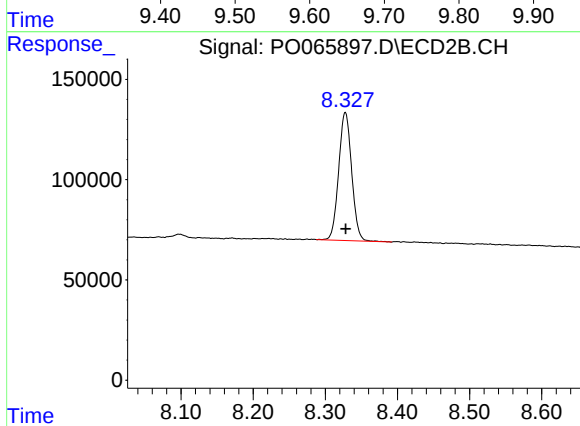

#2 Decachlorobiphenyl

R.T.: 8.328 min
Delta R.T.: 0.000 min
Response: 800471
Conc: 16.47 ng/ml