

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012420\
 Data File : P0065910.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jan 2020 19:26
 Operator : DD\AJ
 Sample : L1247-29
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-13-15-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 22:20:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.153	3.431	570961	624550	24.623	23.513
2) SA Decachlor...	9.647	8.327	1011380	1202073	24.296	24.736

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012420\
Data File : P0065910.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jan 2020 19:26
Operator : DD\AJ
Sample : L1247-29
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-13-15-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 22:20:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

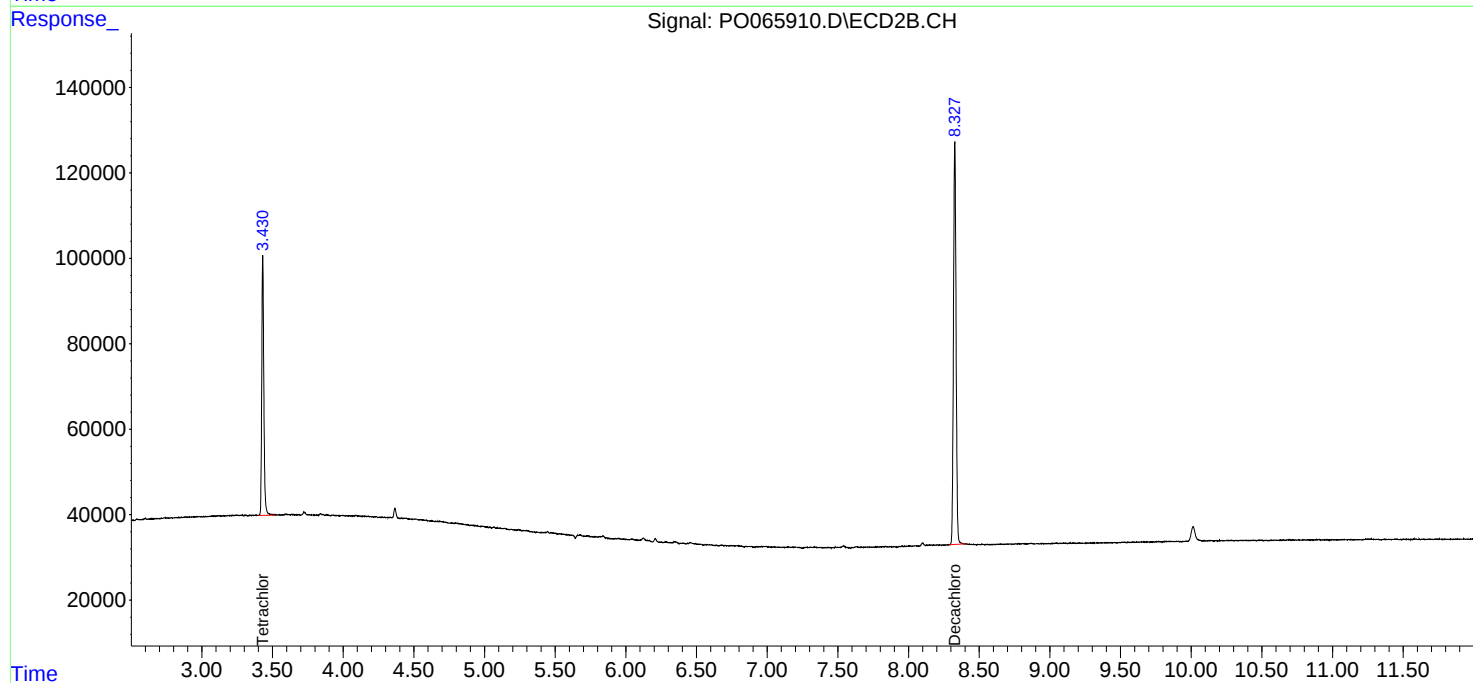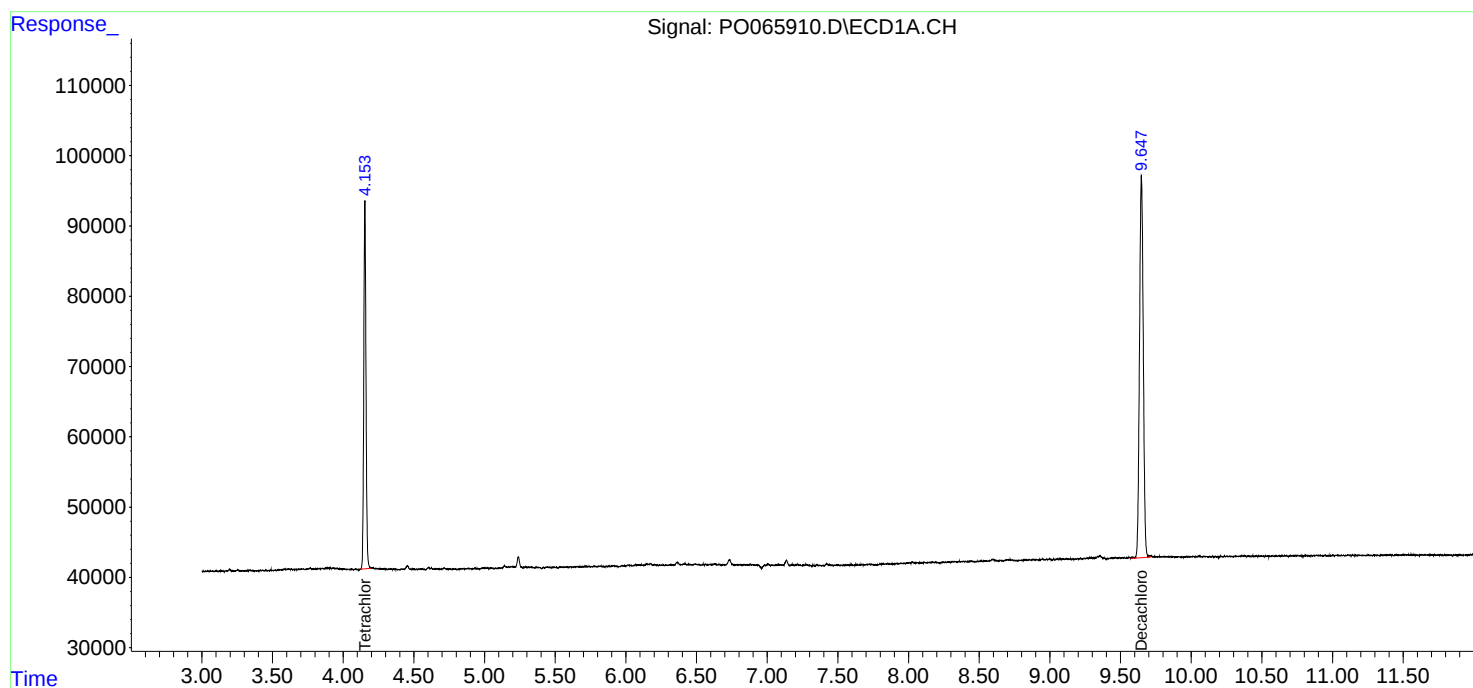


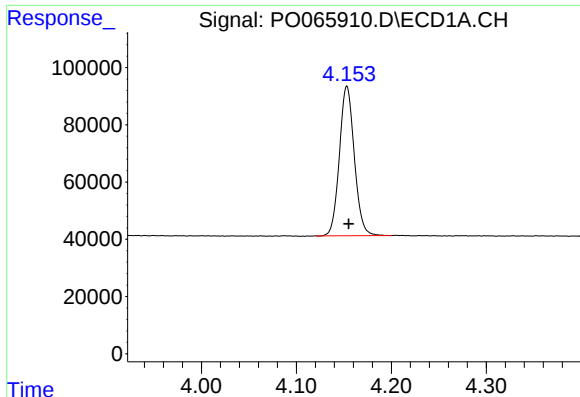

#1 Tetrachloro-m-xylene


R.T.: 4.153 min
Delta R.T.: -0.002 min
Response: 570961
Conc: 24.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-13-15-COMP

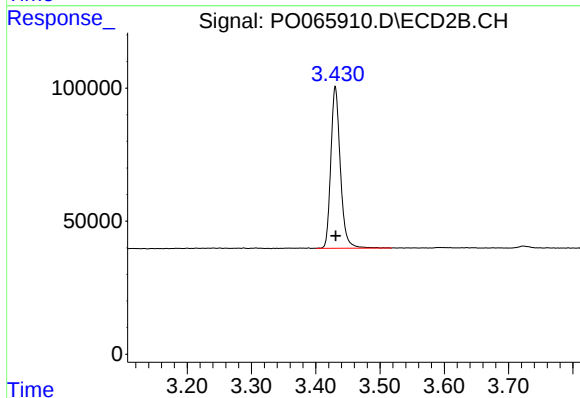


#1 Tetrachloro-m-xylene

R.T.: 3.431 min
Delta R.T.: 0.000 min
Response: 624550
Conc: 23.51 ng/ml

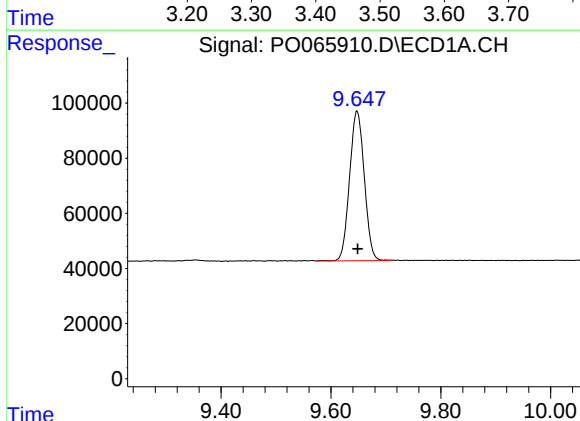

#2 Decachlorobiphenyl

R.T.: 9.647 min
Delta R.T.: -0.001 min
Response: 1011380
Conc: 24.30 ng/ml

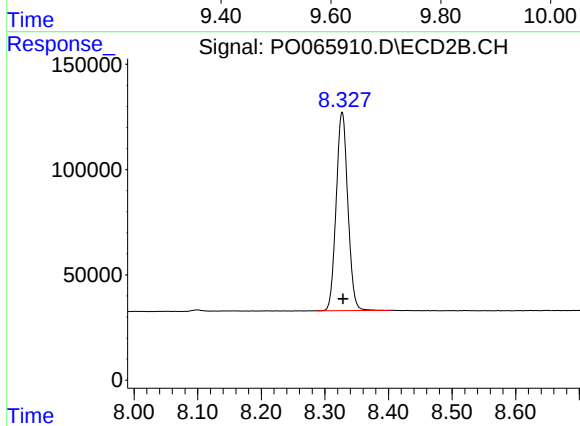

#2 Decachlorobiphenyl

R.T.: 8.327 min
Delta R.T.: -0.001 min
Response: 1202073
Conc: 24.74 ng/ml