

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012420\
 Data File : P0065922.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Jan 2020 23:37
 Operator : DD\AJ
 Sample : L1238-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLIFTON-POLES

Manual Integrations
 APPROVED

mohammad
 1/27/2020 5:52:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 23:56:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.144	3.454	2934702	2641070	126.562m	99.433m
2) SA Decachlor...	9.654	8.330	1000836	400135	24.043m	8.234 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012420\
Data File : P0065922.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Jan 2020 23:37
Operator : DD\AJ
Sample : L1238-01
Misc :
ALS Vial : 41 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
CLIFTON-POLES


Manual Integrations
APPROVED

mohammad
1/27/2020 5:52:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 23:56:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

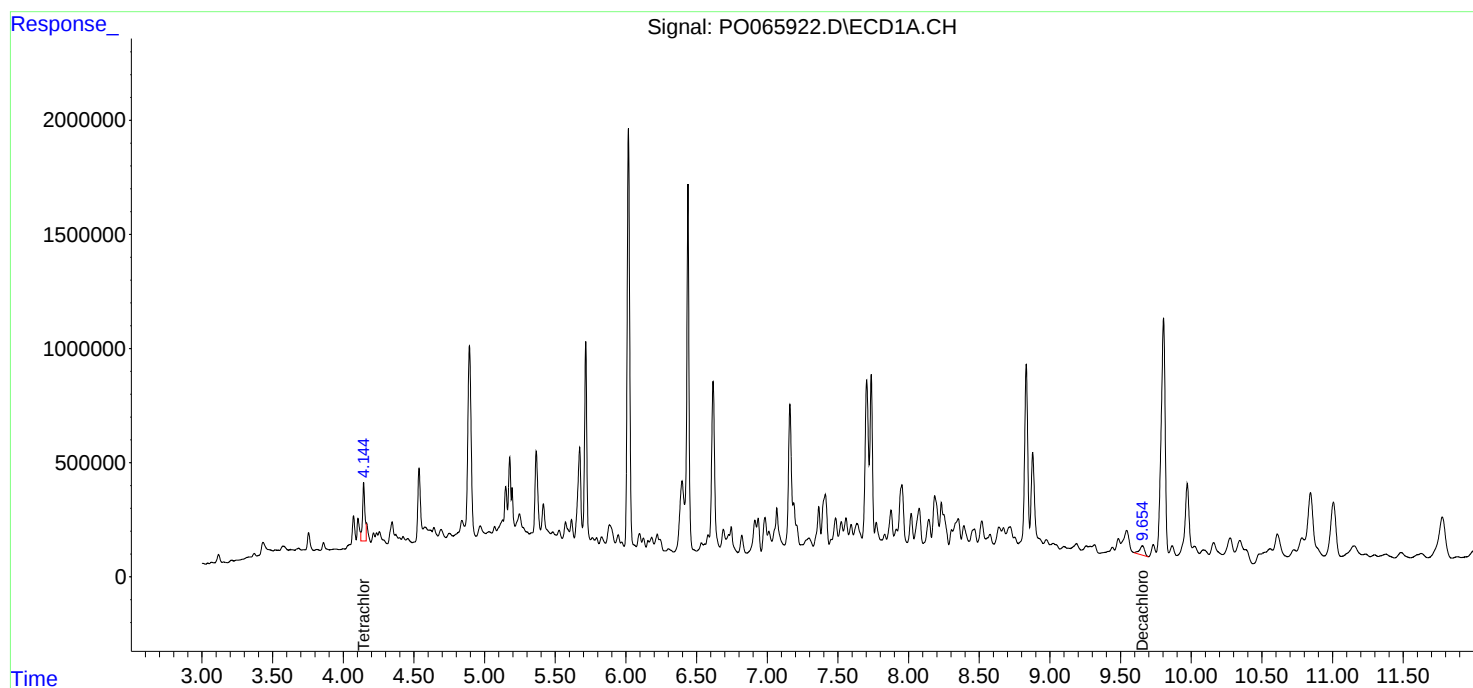

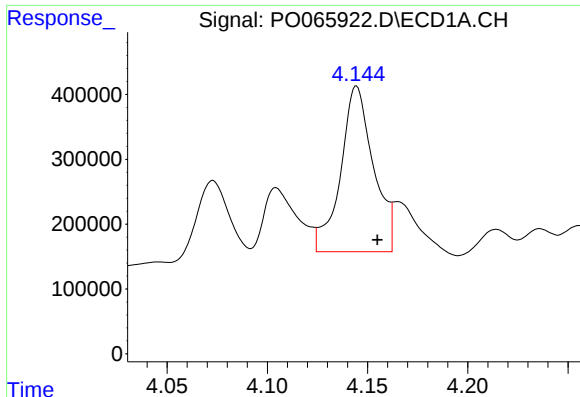


#1 Tetrachloro-m-xylene

R.T.: 4.144 min
Delta R.T.: -0.011 min
Response: 2934702
Conc: 126.56 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CLIFTON-POLES


Manual Integrations
APPROVED

mohammad
1/27/2020 5:52:20 PM

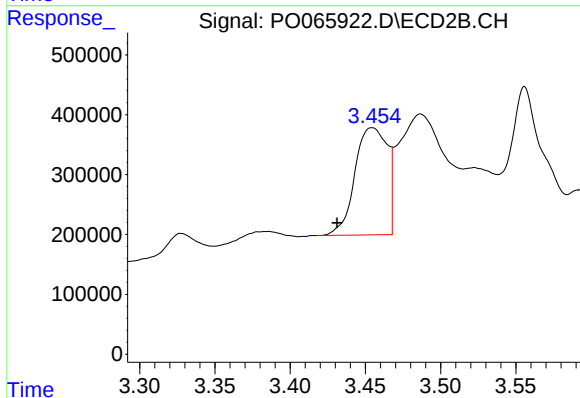


#1 Tetrachloro-m-xylene

R.T.: 3.454 min
Delta R.T.: 0.023 min
Response: 2641070
Conc: 99.43 ng/ml m

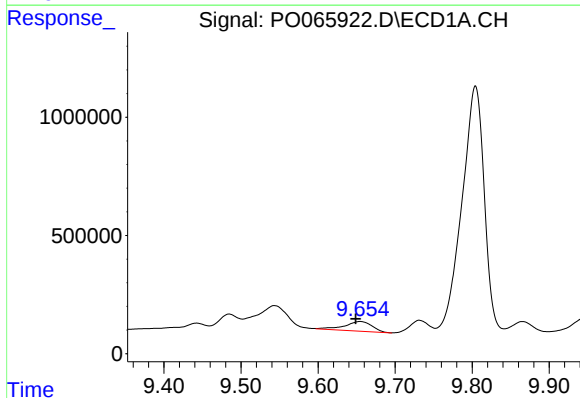

#2 Decachlorobiphenyl

R.T.: 9.654 min
Delta R.T.: 0.006 min
Response: 1000836
Conc: 24.04 ng/ml m

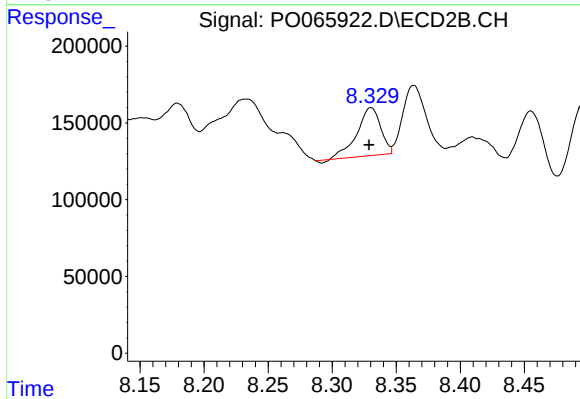

#2 Decachlorobiphenyl

R.T.: 8.330 min
Delta R.T.: 0.002 min
Response: 400135
Conc: 8.23 ng/ml