

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0012423\
 Data File : P0092270.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2023 11:39
 Operator : YP/AJ
 Sample : 01255-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 BORING-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/25/2023
 Supervised By :Ankita Jodhani 01/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 16:09:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.447	3.645	61286301	28752496	21.171	20.477
2) SA Decachlor...	10.363	8.688	39137020	20336405	18.962	18.014
Target Compounds						
26) L6 AR-1254-1	6.505	5.538	26558477	17279010	239.880	220.425
27) L6 AR-1254-2	6.728	5.686	39771890	16867114	244.668	243.777
28) L6 AR-1254-3	7.100	6.093	42615968	26417664	258.389	247.507
29) L6 AR-1254-4	7.393	6.322	27709047	14265423	253.316	242.221
30) L6 AR-1254-5	7.820	6.743	34548731	24961267	245.551m	274.253

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012423\
Data File : PO092270.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2023 11:39
Operator : YP/AJ
Sample : 01255-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BORING-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/25/2023
Supervised By :Ankita Jodhani 01/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 16:09:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

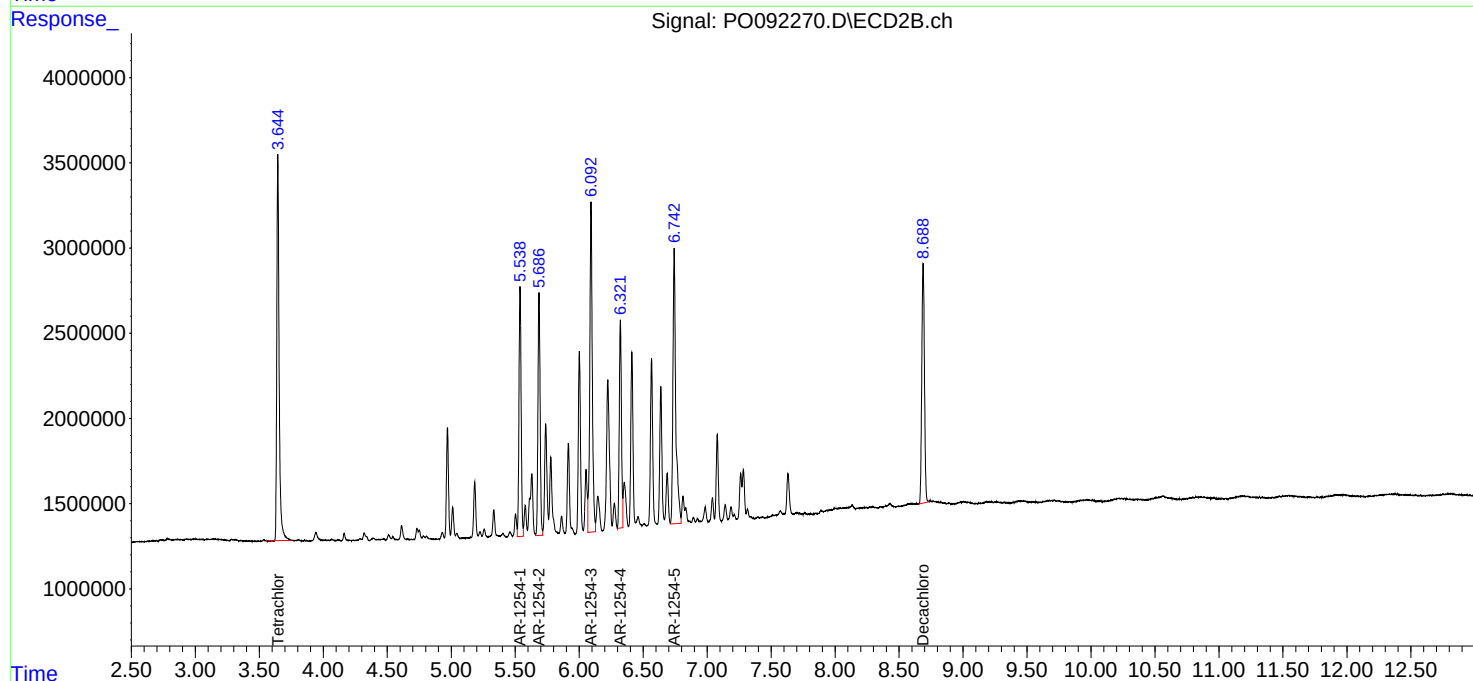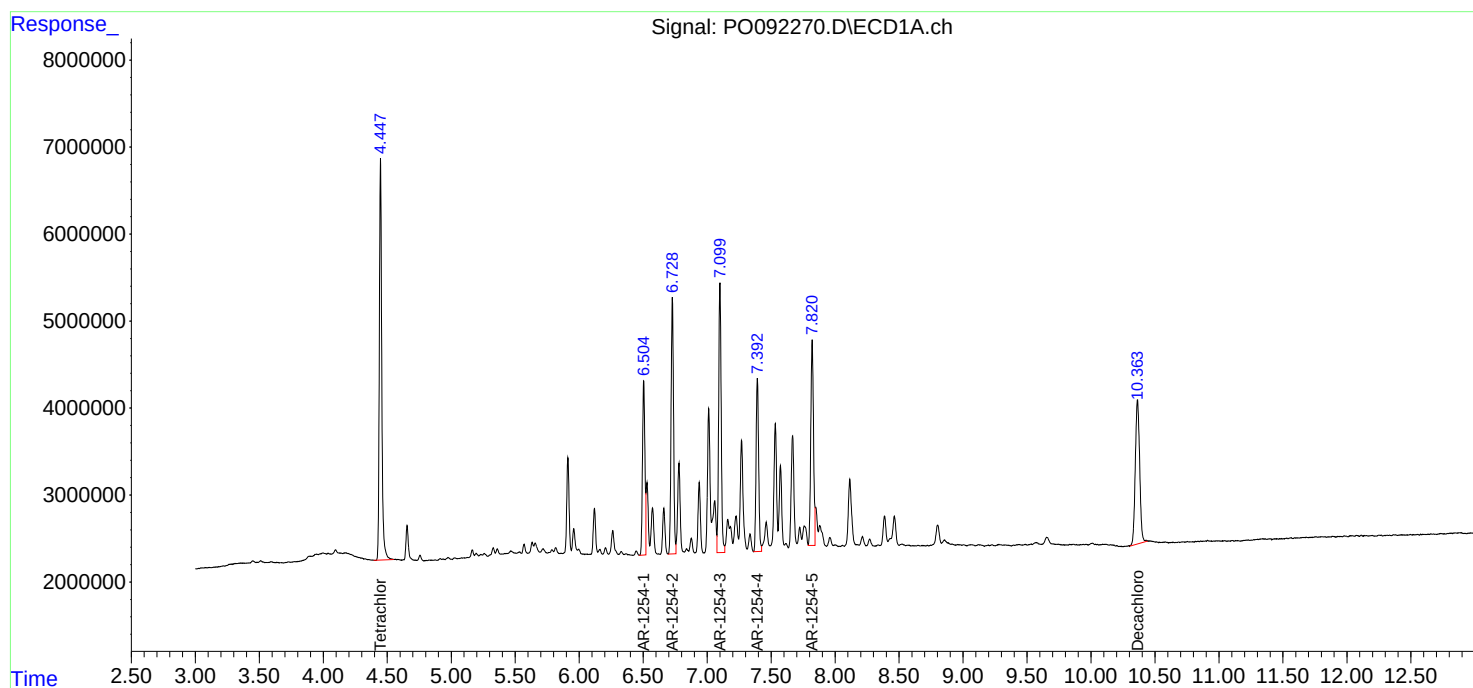

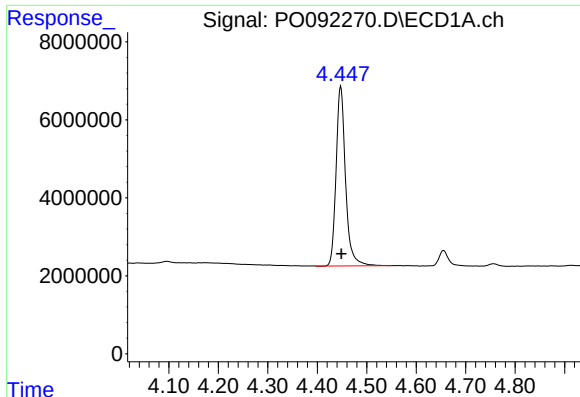


#1 Tetrachloro-m-xylene

R.T.: 4.447 min
Delta R.T.: -0.002 min
Response: 61286301
Conc: 21.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
BORING-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/25/2023
Supervised By :Ankita Jodhani 01/25/2023

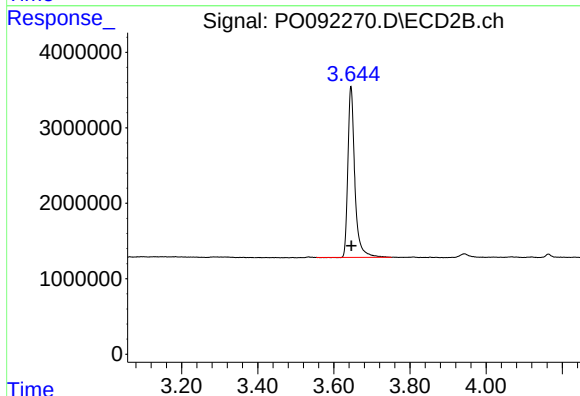


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.001 min
Response: 28752496
Conc: 20.48 ng/ml

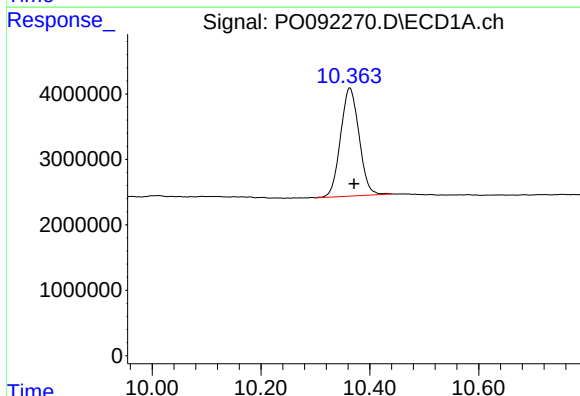


#2 Decachlorobiphenyl

R.T.: 10.363 min
Delta R.T.: -0.008 min
Response: 39137020
Conc: 18.96 ng/ml

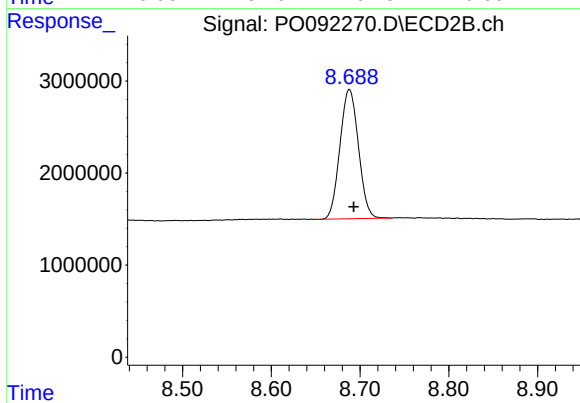

#2 Decachlorobiphenyl

R.T.: 8.688 min
Delta R.T.: -0.005 min
Response: 20336405
Conc: 18.01 ng/ml

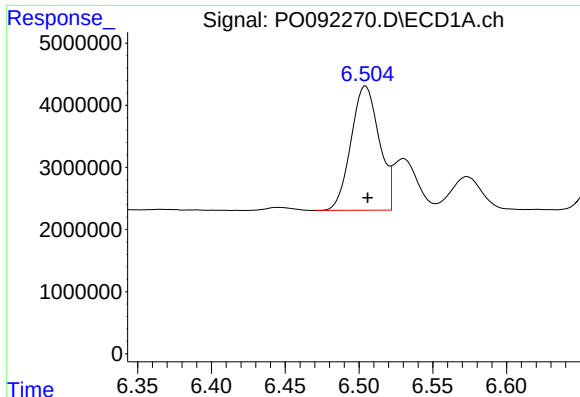


#26 AR-1254-1

R.T.: 6.505 min
Delta R.T.: -0.001 min
Response: 26558477
Conc: 239.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
BORING-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/25/2023
Supervised By :Ankita Jodhani 01/25/2023

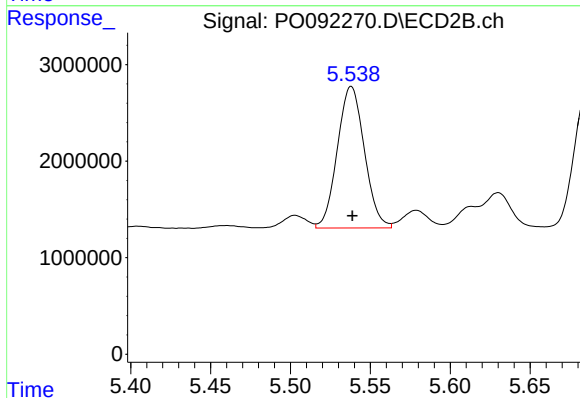


#26 AR-1254-1

R.T.: 5.538 min
Delta R.T.: 0.000 min
Response: 17279010
Conc: 220.42 ng/ml

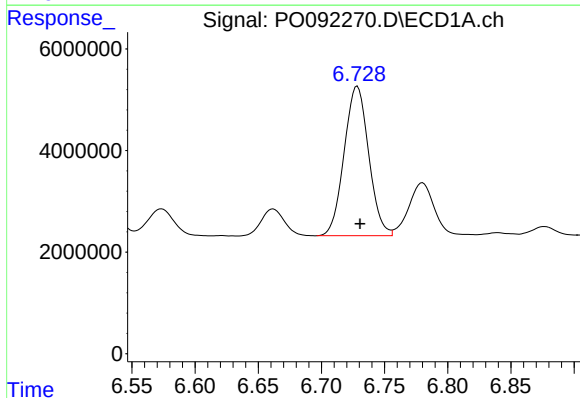


#27 AR-1254-2

R.T.: 6.728 min
Delta R.T.: -0.002 min
Response: 39771890
Conc: 244.67 ng/ml

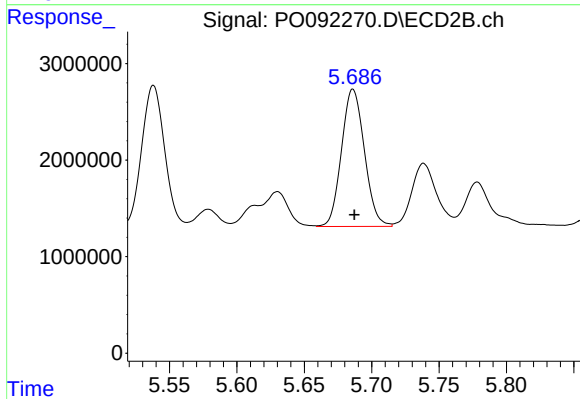

#27 AR-1254-2

R.T.: 5.686 min
Delta R.T.: -0.001 min
Response: 16867114
Conc: 243.78 ng/ml

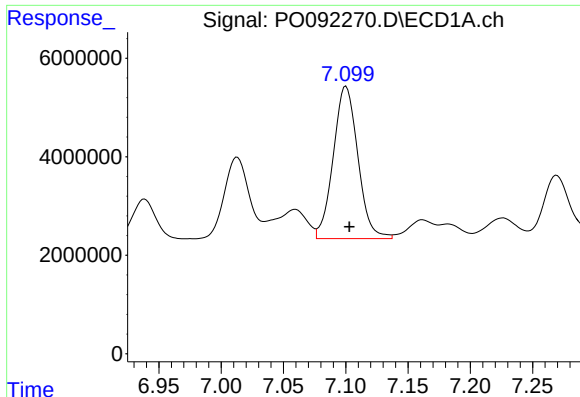


#28 AR-1254-3

R.T.: 7.100 min
Delta R.T.: -0.003 min
Response: 42615968
Conc: 258.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
BORING-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/25/2023
Supervised By :Ankita Jodhani 01/25/2023

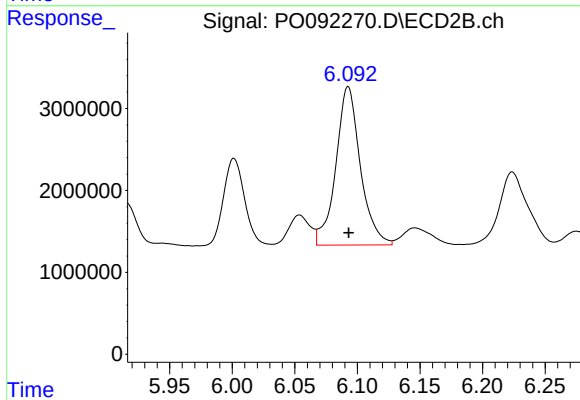


#28 AR-1254-3

R.T.: 6.093 min
Delta R.T.: 0.000 min
Response: 26417664
Conc: 247.51 ng/ml

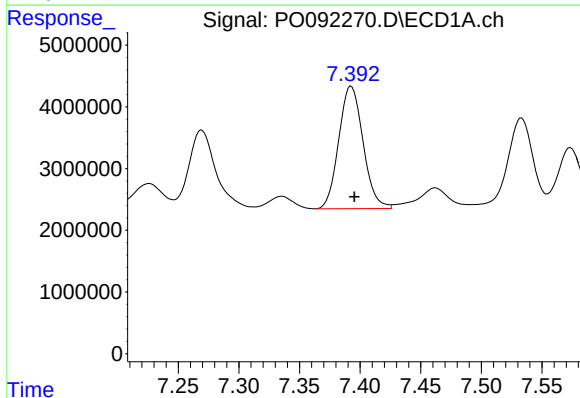


#29 AR-1254-4

R.T.: 7.393 min
Delta R.T.: -0.003 min
Response: 27709047
Conc: 253.32 ng/ml

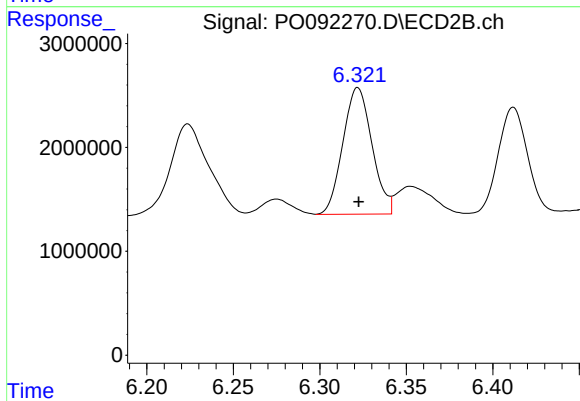

#29 AR-1254-4

R.T.: 6.322 min
Delta R.T.: 0.000 min
Response: 14265423
Conc: 242.22 ng/ml

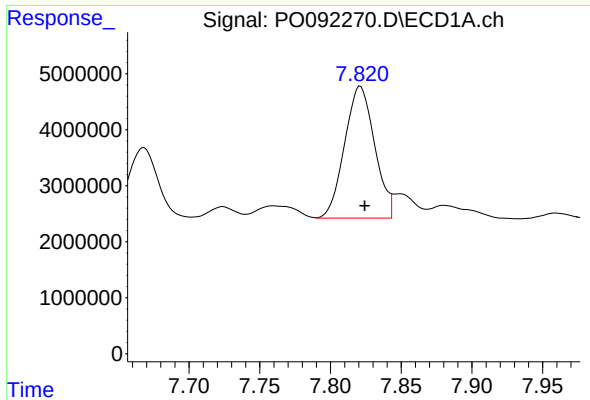


#30 AR-1254-5

R.T.: 7.820 min
Delta R.T.: -0.004 min
Response: 34548731
Conc: 245.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
BORING-1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/25/2023
Supervised By :Ankita Jodhani 01/25/2023

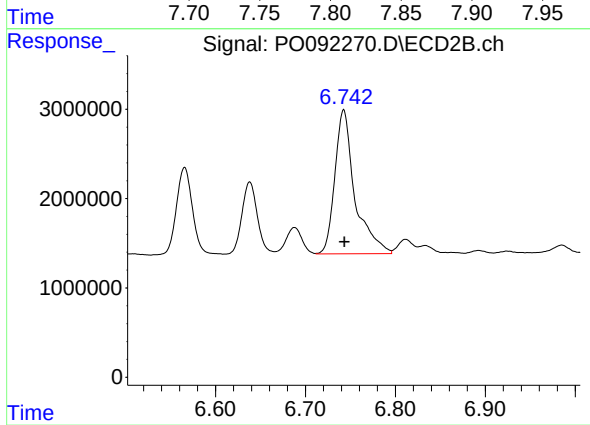

#30 AR-1254-5

R.T.: 6.743 min
Delta R.T.: 0.000 min
Response: 24961267
Conc: 274.25 ng/ml