

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0012423\
 Data File : P0092302.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2023 22:11
 Operator : YP/AJ
 Sample : 01251-07
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 COMP-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/25/2023
 Supervised By :Ankita Jodhani 01/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 01:42:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0012323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 24 04:40:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.645	60396810	29425449	20.863	20.956
2) SA Decachlor...	10.364	8.686	38710027	20489070	18.755	18.149
Target Compounds						
16) L4 AR-1242-1	5.633	4.732	1732375	870817	22.213	22.327
17) L4 AR-1242-2	5.655	4.751	3397800	1496689	30.185	27.558
18) L4 AR-1242-3	5.718	4.928	1328888	904036	18.306	31.041 #
19) L4 AR-1242-4	5.816	5.011	1420820	1097502	25.658m	34.120 #
20) L4 AR-1242-5	6.569	5.536	2555912	2160617	45.787	59.683m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012423\
Data File : PO092302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2023 22:11
Operator : YP/AJ
Sample : 01251-07
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/25/2023
Supervised By :Ankita Jodhani 01/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 01:42:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 24 04:40:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

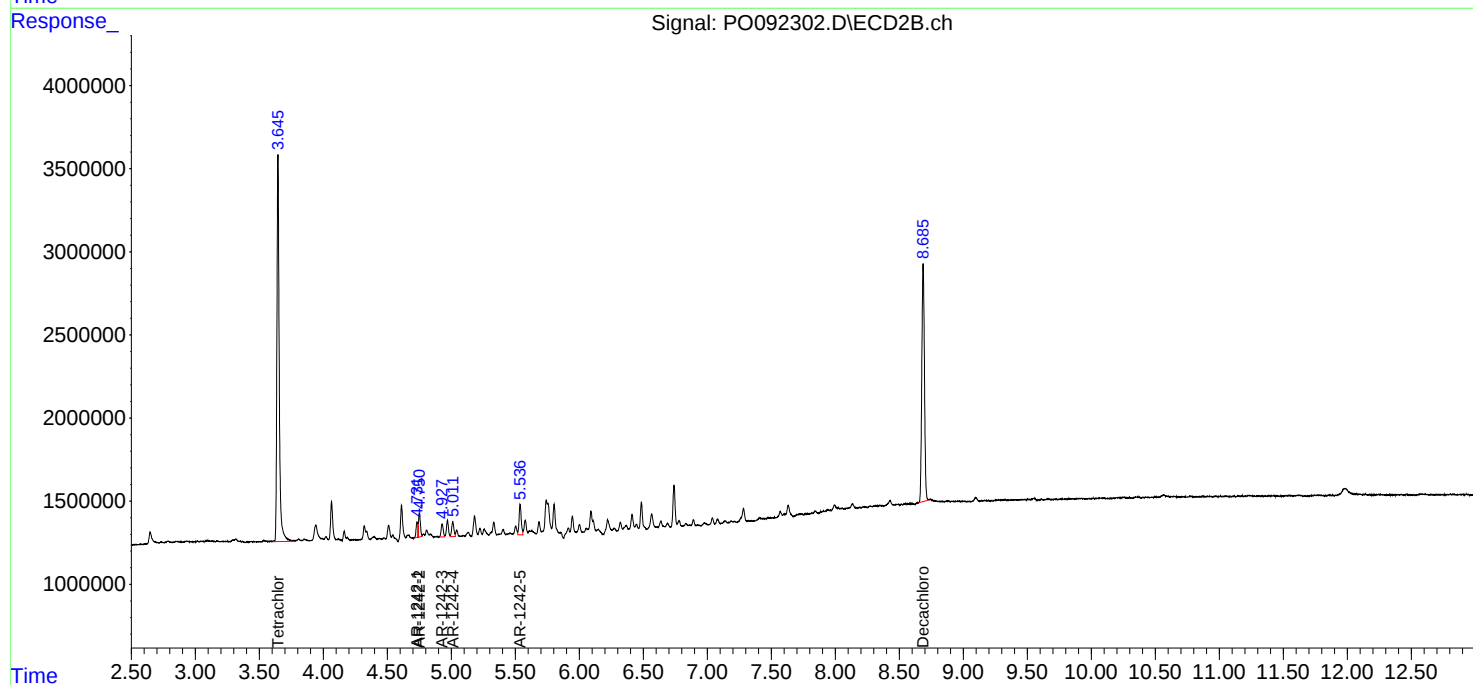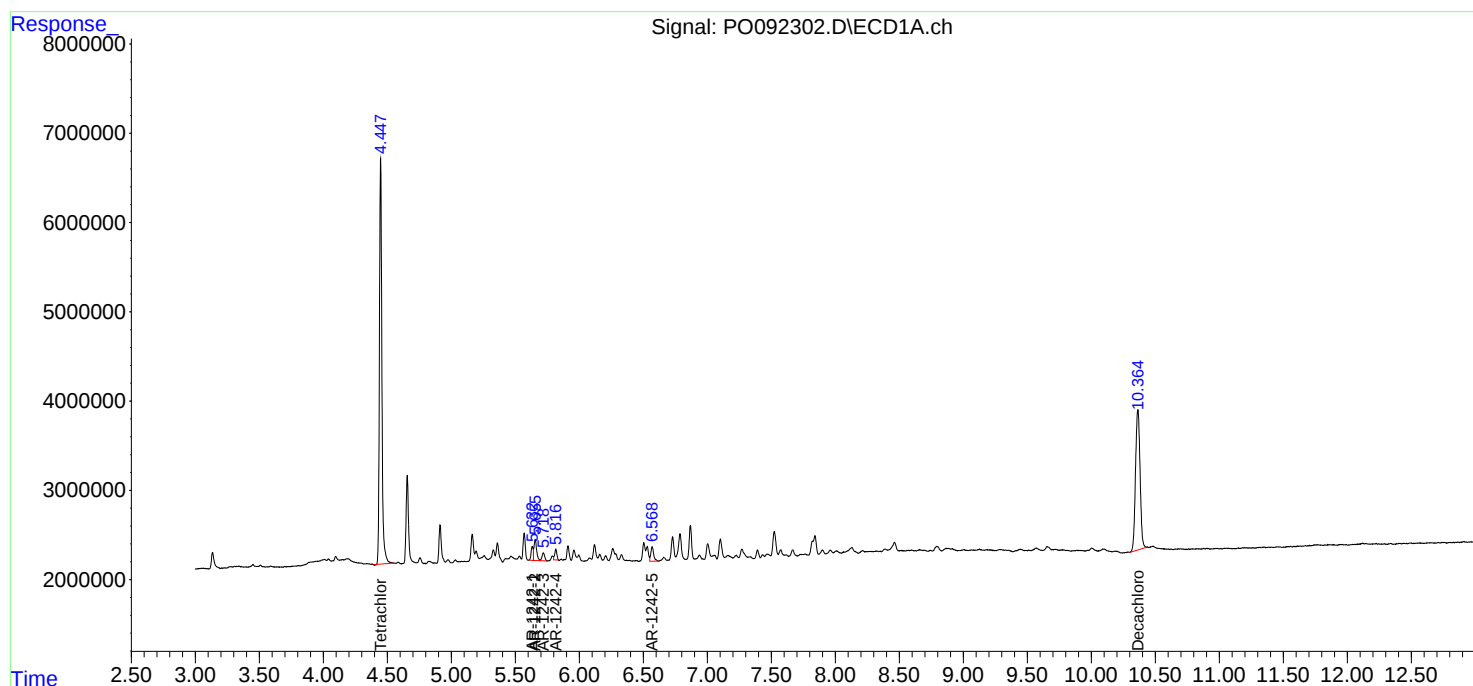

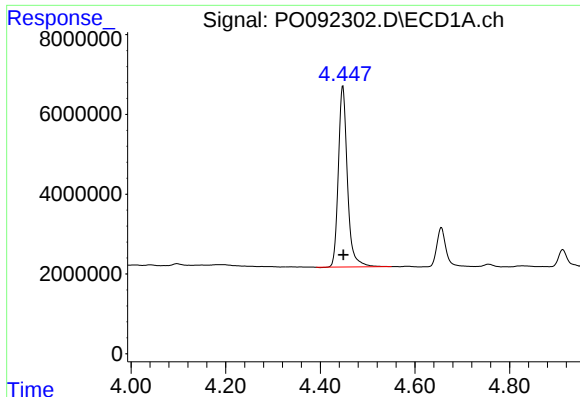


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: -0.001 min
Response: 60396810
Conc: 20.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/25/2023
Supervised By :Ankita Jodhani 01/25/2023

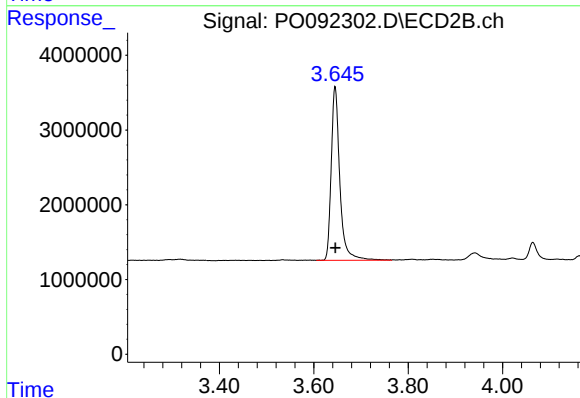


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: 0.000 min
Response: 29425449
Conc: 20.96 ng/ml

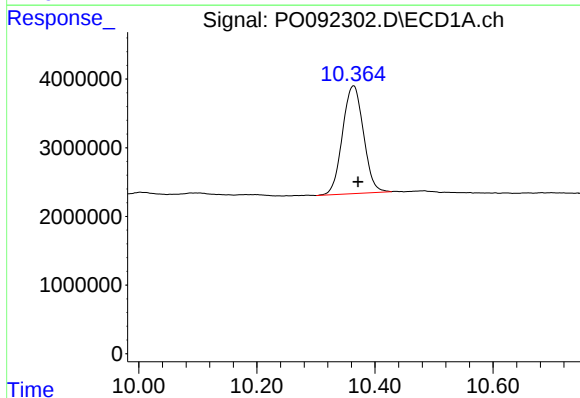


#2 Decachlorobiphenyl

R.T.: 10.364 min
Delta R.T.: -0.007 min
Response: 38710027
Conc: 18.76 ng/ml

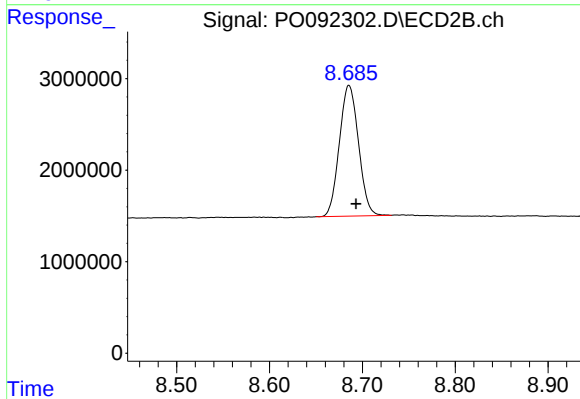

#2 Decachlorobiphenyl

R.T.: 8.686 min
Delta R.T.: -0.007 min
Response: 20489070
Conc: 18.15 ng/ml

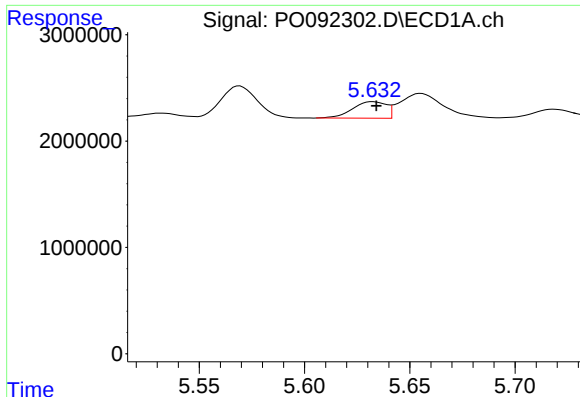


#16 AR-1242-1

R.T.: 5.633 min
Delta R.T.: -0.002 min
Response: 1732375
Conc: 22.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/25/2023
Supervised By :Ankita Jodhani 01/25/2023

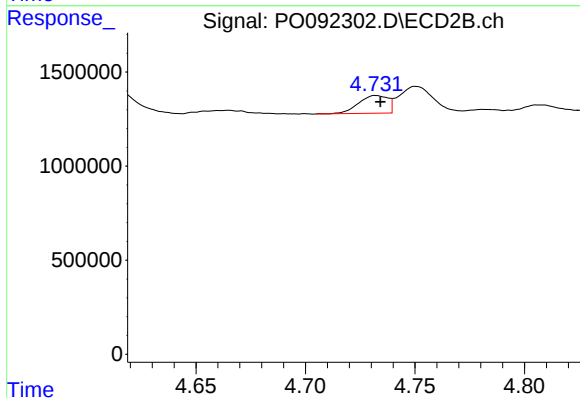


#16 AR-1242-1

R.T.: 4.732 min
Delta R.T.: -0.002 min
Response: 870817
Conc: 22.33 ng/ml

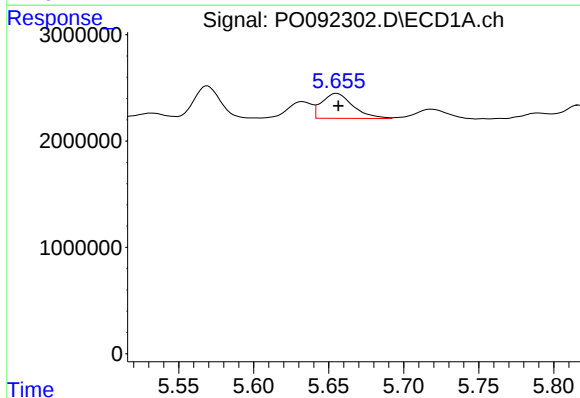


#17 AR-1242-2

R.T.: 5.655 min
Delta R.T.: -0.001 min
Response: 3397800
Conc: 30.19 ng/ml

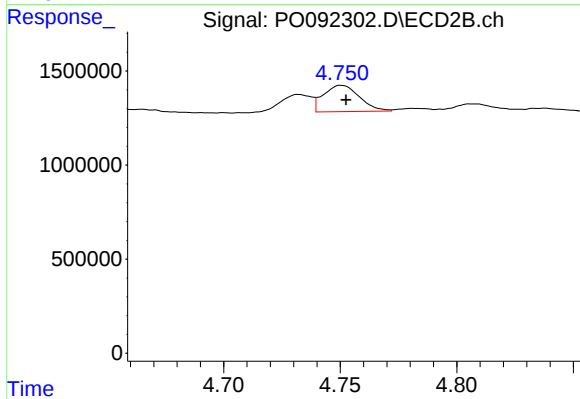

#17 AR-1242-2

R.T.: 4.751 min
Delta R.T.: -0.002 min
Response: 1496689
Conc: 27.56 ng/ml

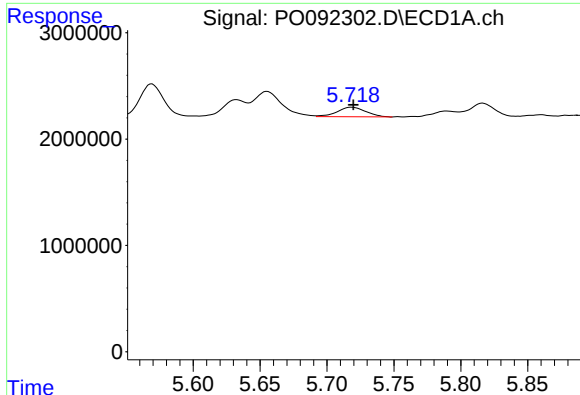


#18 AR-1242-3

R.T.: 5.718 min
Delta R.T.: -0.001 min
Response: 1328888
Conc: 18.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/25/2023
Supervised By :Ankita Jodhani 01/25/2023

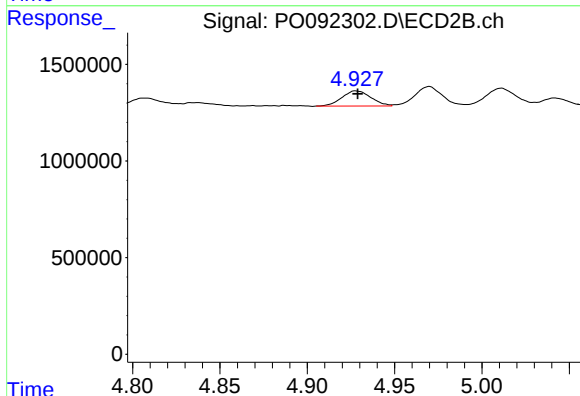


#18 AR-1242-3

R.T.: 4.928 min
Delta R.T.: 0.000 min
Response: 904036
Conc: 31.04 ng/ml

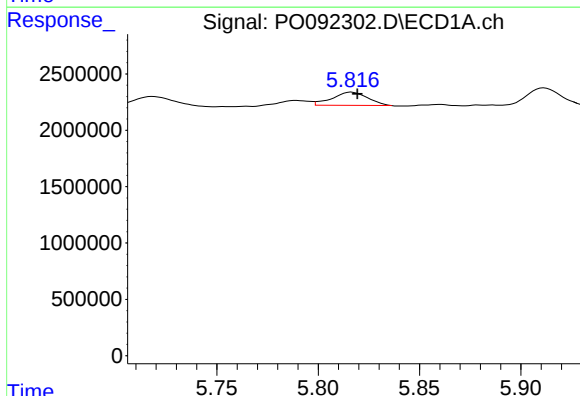


#19 AR-1242-4

R.T.: 5.816 min
Delta R.T.: -0.004 min
Response: 1420820
Conc: 25.66 ng/ml m

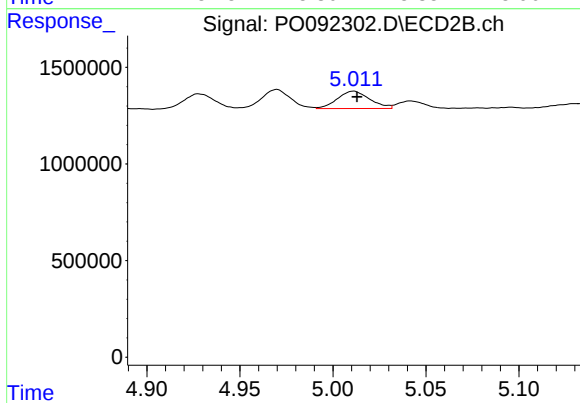

#19 AR-1242-4

R.T.: 5.011 min
Delta R.T.: -0.002 min
Response: 1097502
Conc: 34.12 ng/ml

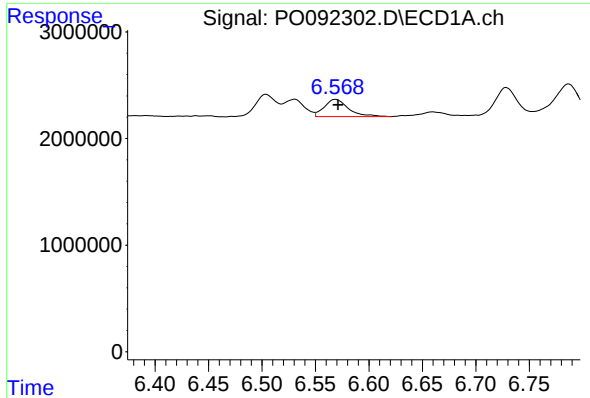


#20 AR-1242-5

R.T.: 6.569 min
Delta R.T.: -0.002 min
Response: 2555912
Conc: 45.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/25/2023
Supervised By :Ankita Jodhani 01/25/2023

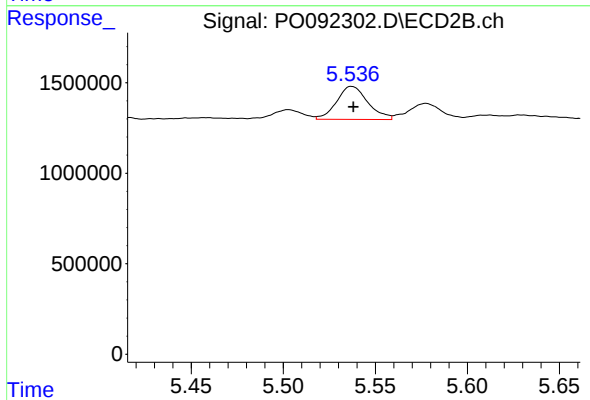

#20 AR-1242-5

R.T.: 5.536 min
Delta R.T.: -0.002 min
Response: 2160617
Conc: 59.68 ng/ml m