

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012521\
 Data File : P0075149.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2021 18:08
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 18:24:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.925	3.997	2149457	1023897	20.371	18.202
2)	SA Decachlor...	10.940	9.248	1994367	946254	19.650	17.235
Target Compounds							
26)	L6 AR-1254-1	7.165	0.000	33936	0	7.716	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012521\
Data File : P0075149.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2021 18:08
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 18:24:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

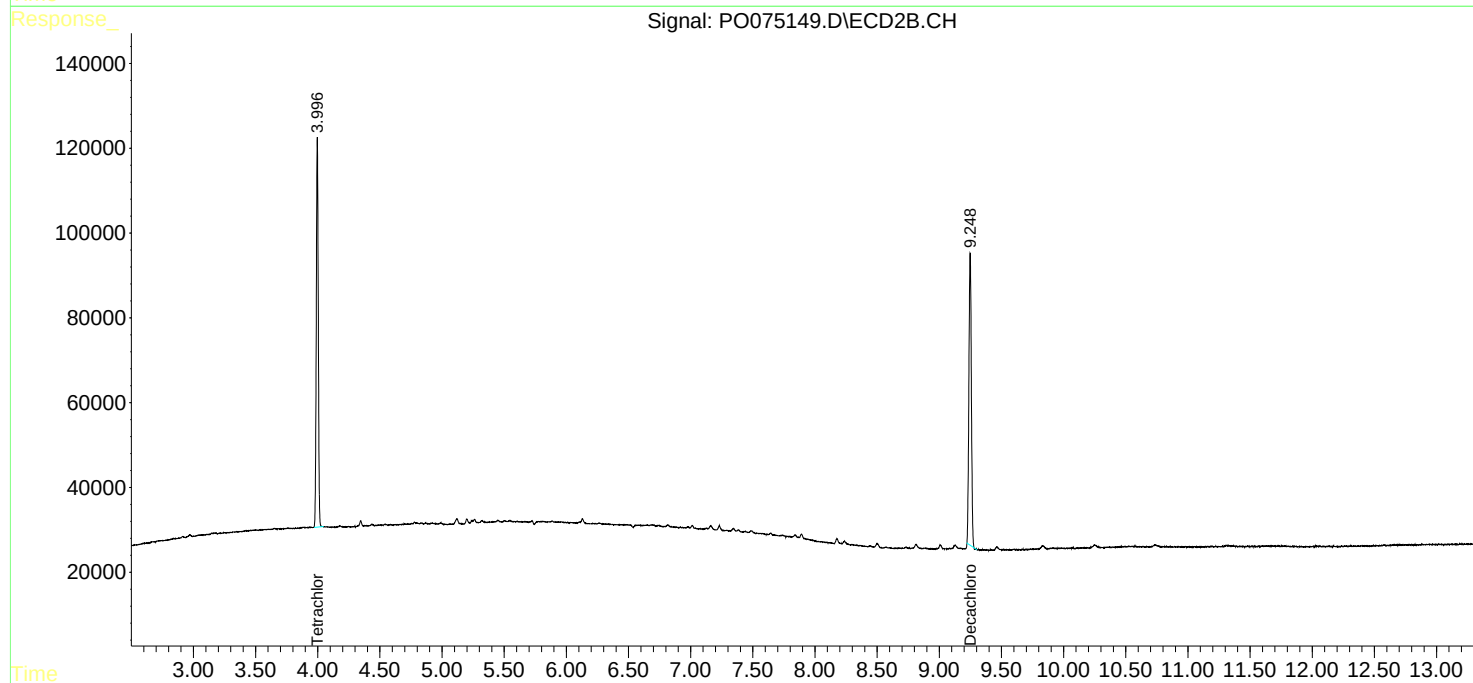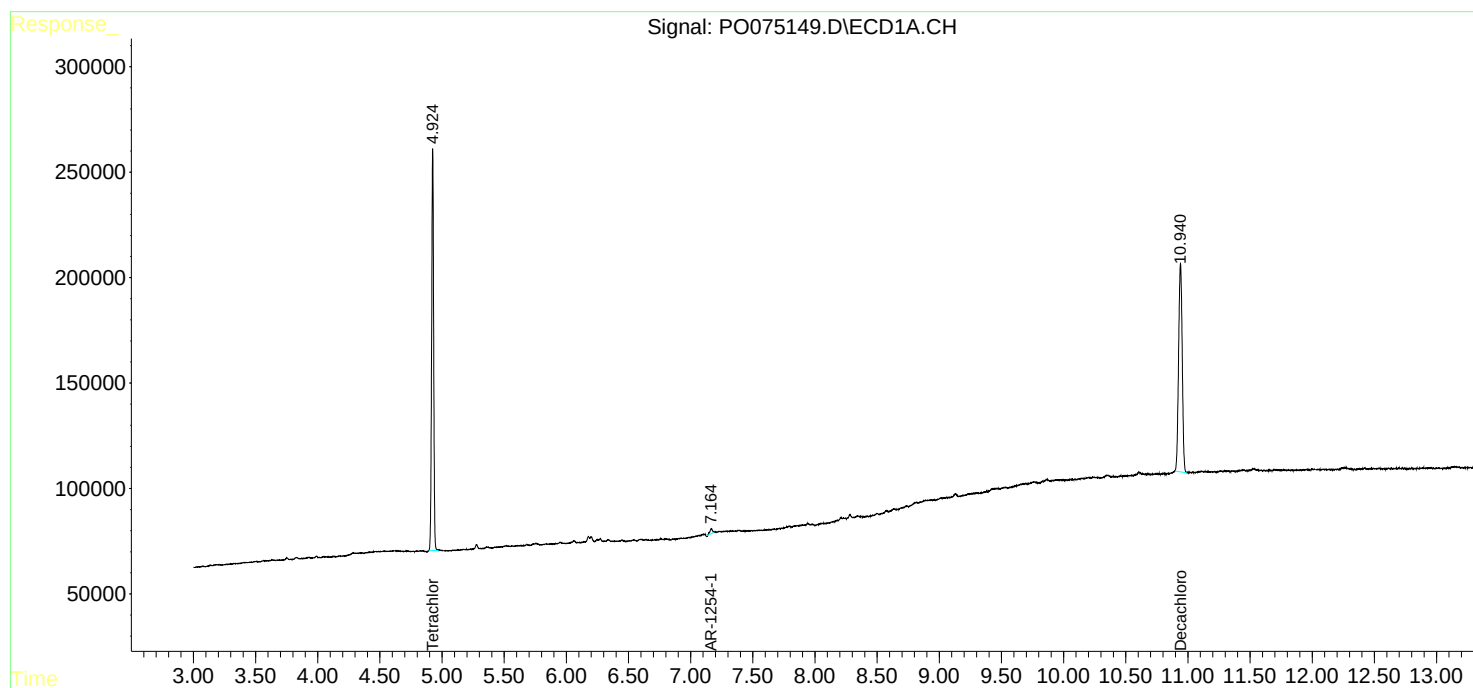


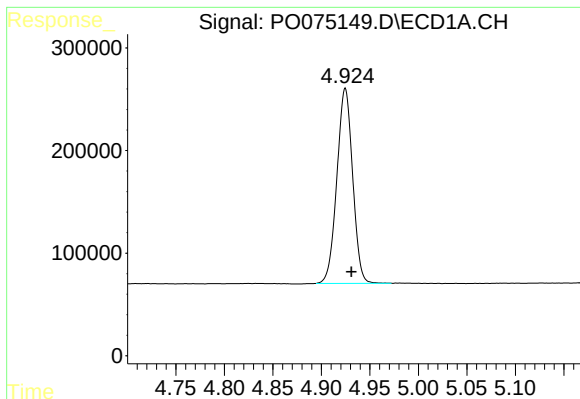

#1 Tetrachloro-m-xylene


R.T.: 4.925 min
Delta R.T.: -0.006 min
Response: 2149457
Conc: 20.37 ng/ml

Instrument :
ECD_O
ClientSampleId :

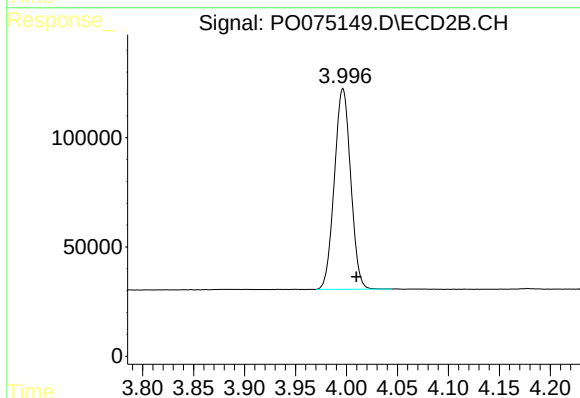


#1 Tetrachloro-m-xylene

R.T.: 3.997 min
Delta R.T.: -0.013 min
Response: 1023897
Conc: 18.20 ng/ml

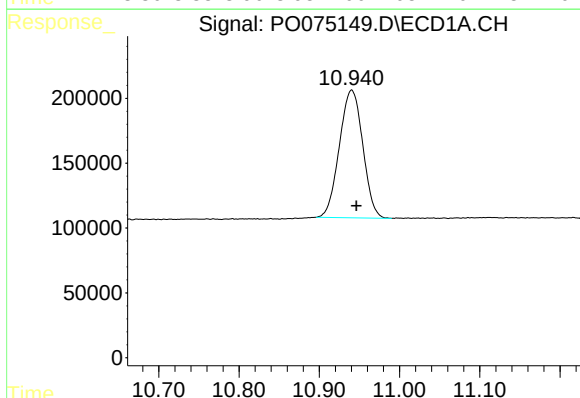


#2 Decachlorobiphenyl

R.T.: 10.940 min
Delta R.T.: -0.006 min
Response: 1994367
Conc: 19.65 ng/ml

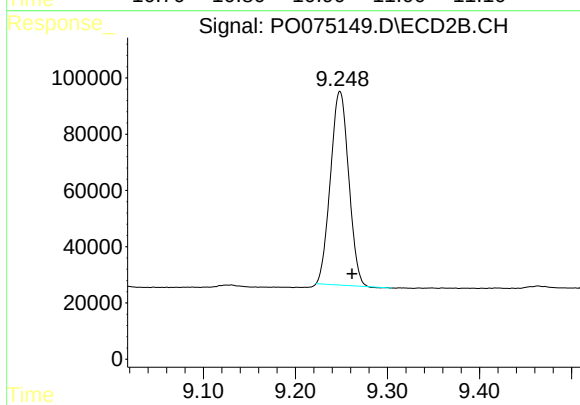

#2 Decachlorobiphenyl


R.T.: 9.248 min
Delta R.T.: -0.013 min
Response: 946254
Conc: 17.23 ng/ml

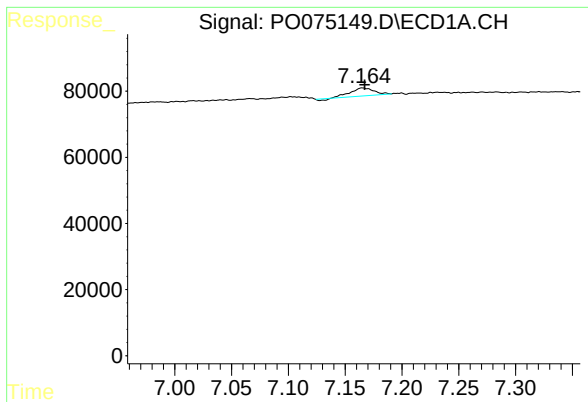

#26 AR-1254-1

R.T.: 7.165 min
Delta R.T.: -0.002 min
Response: 33936
Conc: 7.72 ng/ml

Instrument :
ECD_O
ClientSampleId :

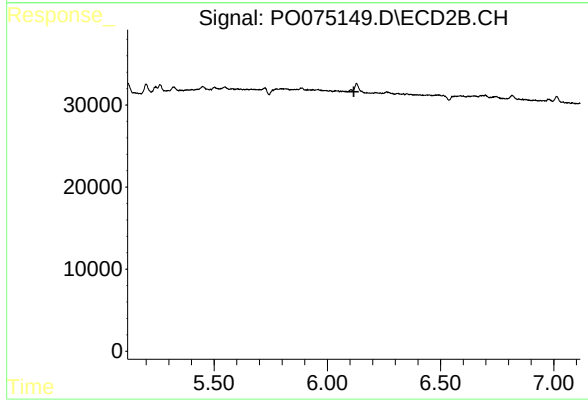

#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 6.117 min
Response: 0
Conc: N.D.