

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012521\
 Data File : P0075127.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2021 11:17
 Operator : AJ/MA
 Sample : M1187-07 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 UNKNOWN-MECHANIC-END-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 25 14:34:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.925	3.997	203830	110080	1.932	1.957
2)	SA Decachlor...	10.942	9.252	197544	93576	1.946	1.704

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012521\
Data File : P0075127.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2021 11:17
Operator : AJ/MA
Sample : M1187-07 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
UNKNOWN-MECHANIC-END-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 25 14:34:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

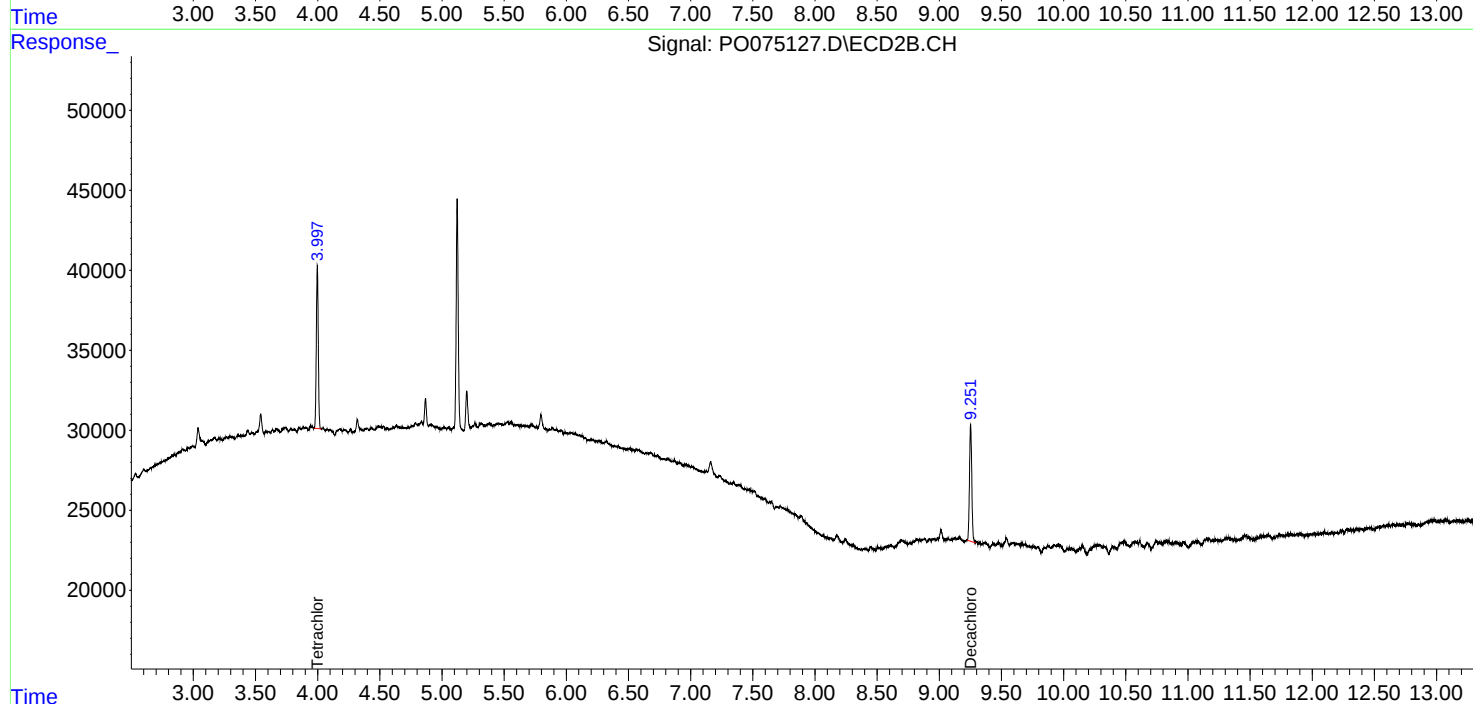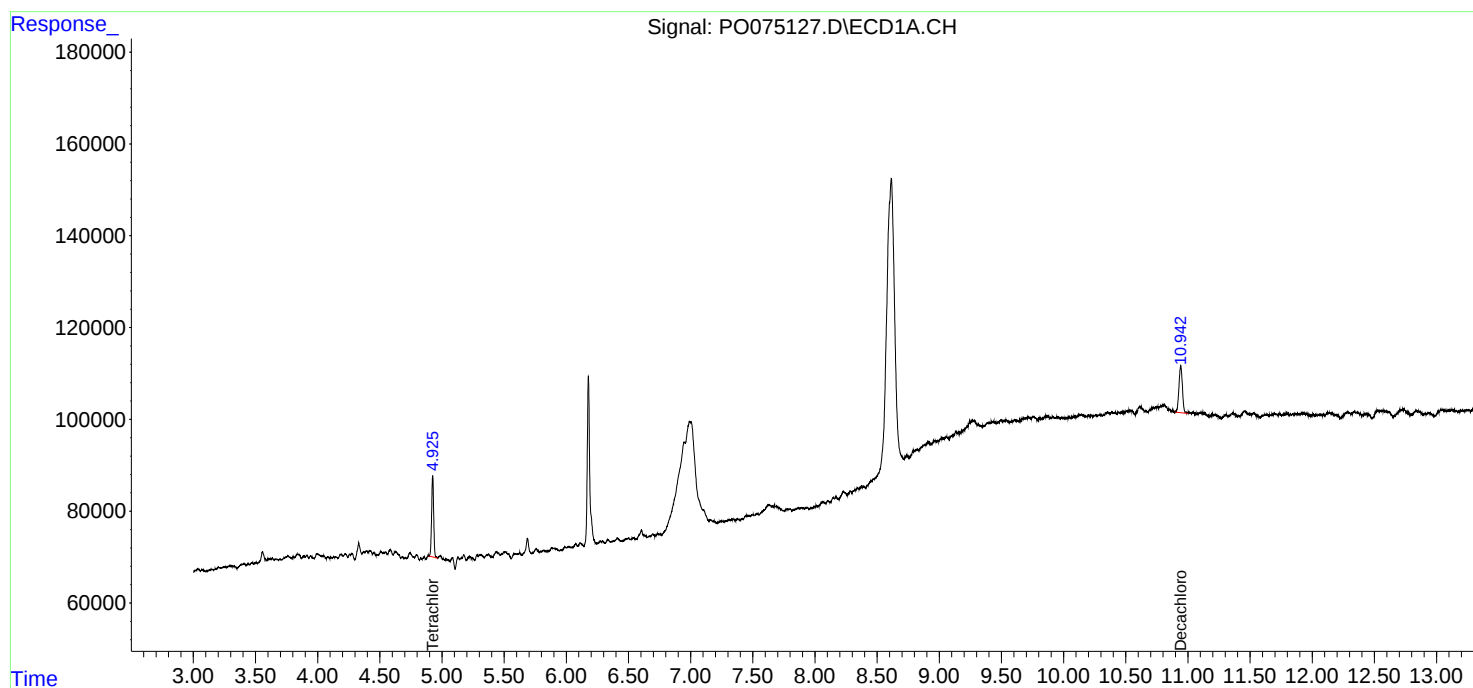


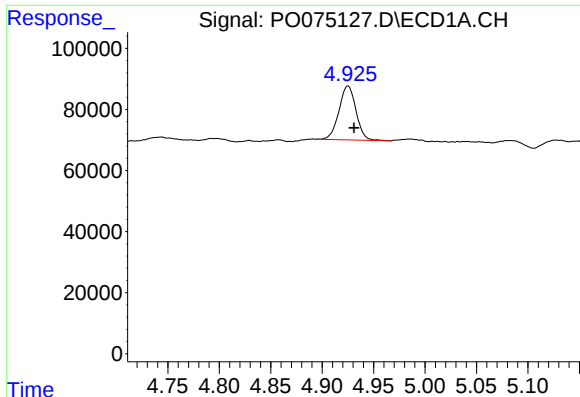

#1 Tetrachloro-m-xylene


R.T.: 4.925 min
Delta R.T.: -0.006 min
Response: 203830
Conc: 1.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
UNKNOWN-MECHANIC-END-1

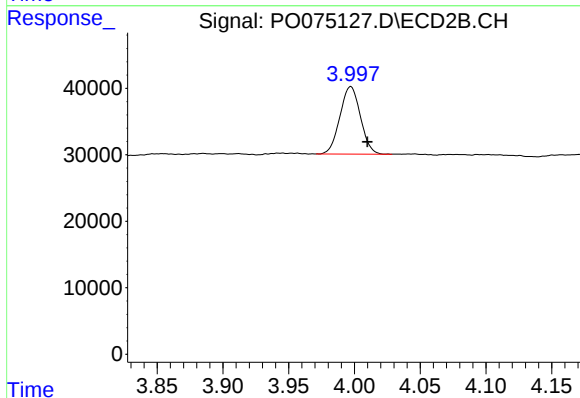


#1 Tetrachloro-m-xylene

R.T.: 3.997 min
Delta R.T.: -0.013 min
Response: 110080
Conc: 1.96 ng/ml

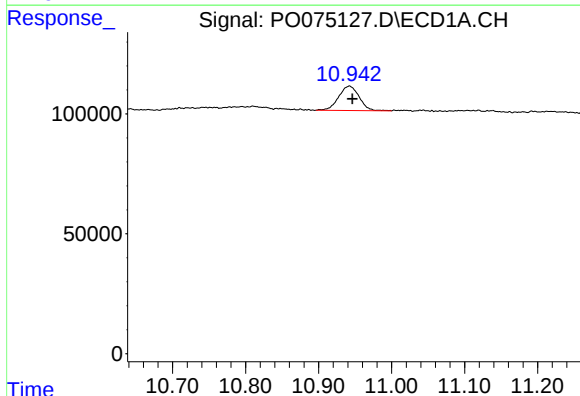

#2 Decachlorobiphenyl

R.T.: 10.942 min
Delta R.T.: -0.004 min
Response: 197544
Conc: 1.95 ng/ml

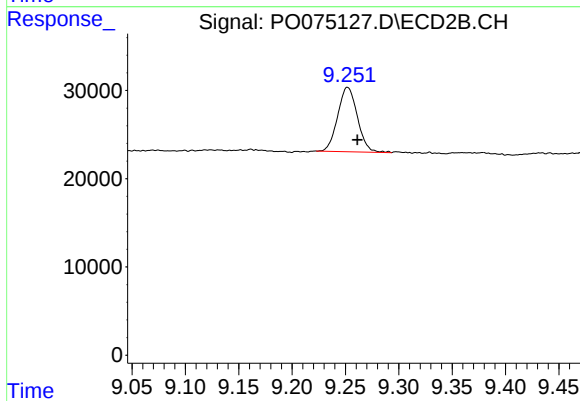

#2 Decachlorobiphenyl

R.T.: 9.252 min
Delta R.T.: -0.009 min
Response: 93576
Conc: 1.70 ng/ml