

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012521\
 Data File : P0075156.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2021 20:07
 Operator : AJ/MA
 Sample : M1226-06
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0046-051-COMP-H

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 01:01:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.925	3.996	2367416	1102662	22.436	19.602
2) SA Decachlor...	10.939	9.248	2034343	992567	20.044	18.078m

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012521\
Data File : P0075156.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2021 20:07
Operator : AJ/MA
Sample : M1226-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
0046-051-COMP-H

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 01:01:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

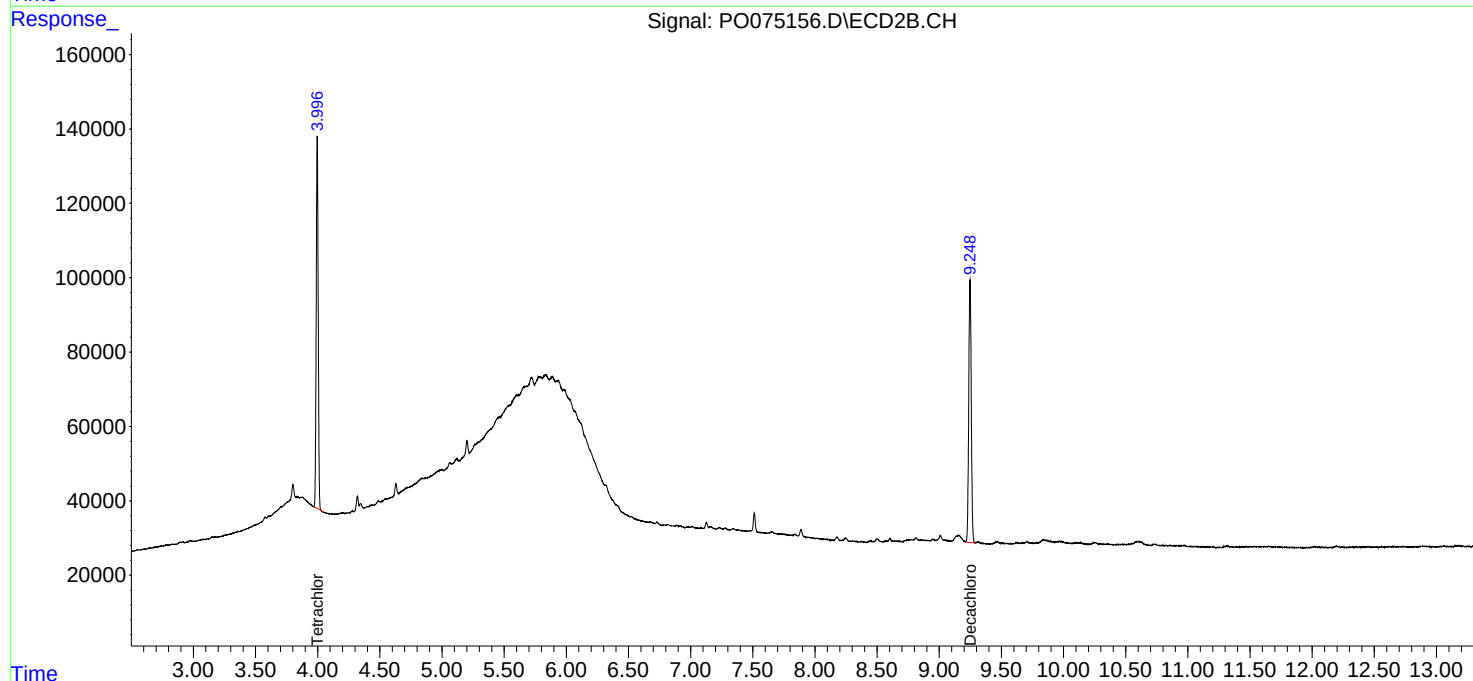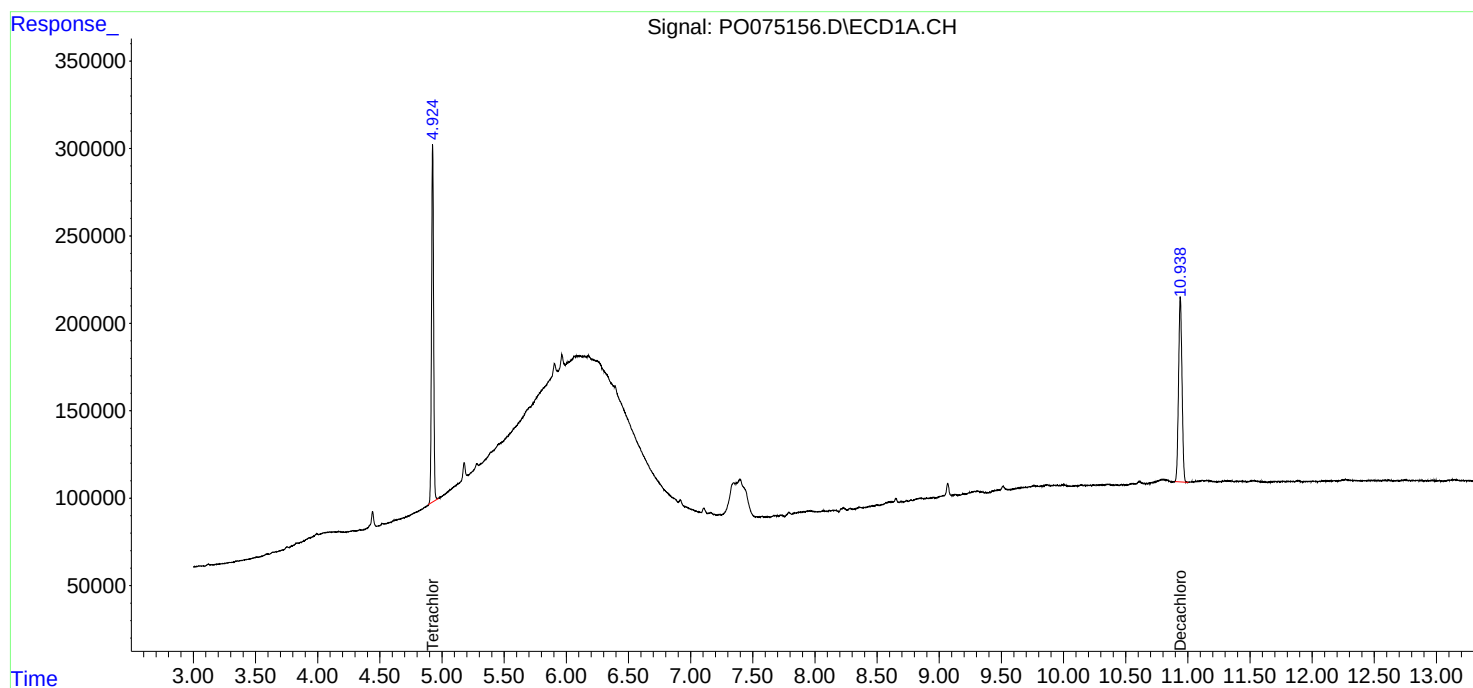


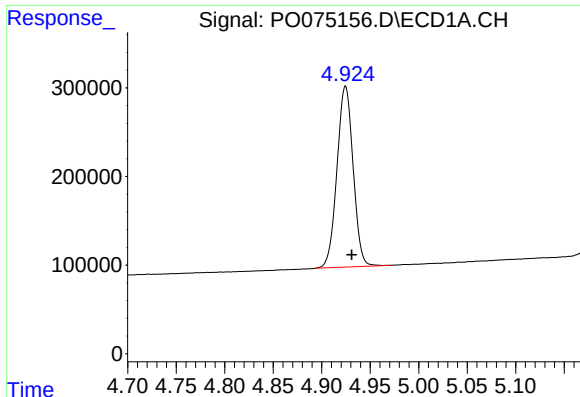

#1 Tetrachloro-m-xylene


R.T.: 4.925 min
Delta R.T.: -0.006 min
Response: 2367416
Conc: 22.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
0046-051-COMP-H

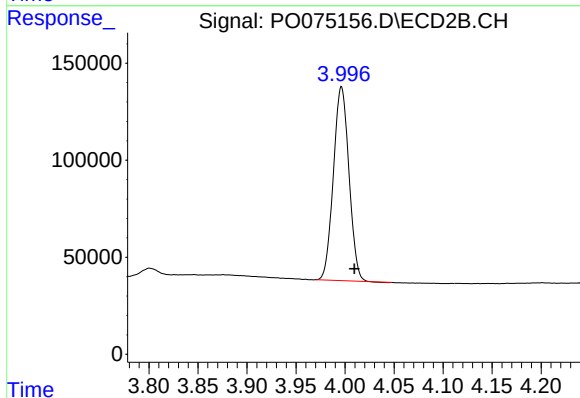


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: -0.013 min
Response: 1102662
Conc: 19.60 ng/ml

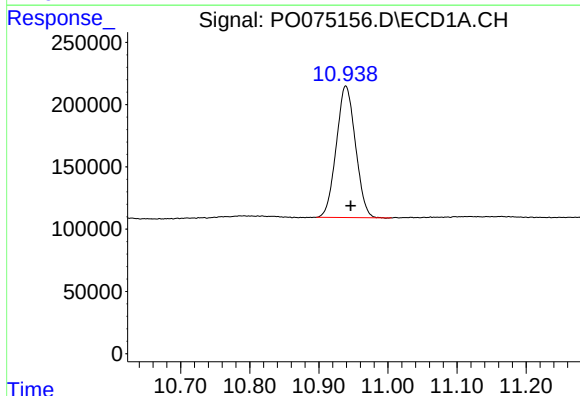

#2 Decachlorobiphenyl

R.T.: 10.939 min
Delta R.T.: -0.007 min
Response: 2034343
Conc: 20.04 ng/ml

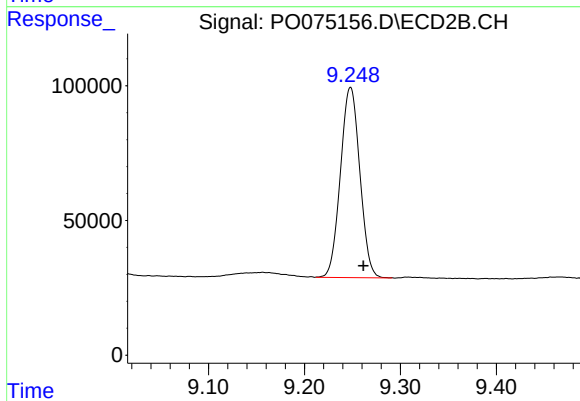

#2 Decachlorobiphenyl

R.T.: 9.248 min
Delta R.T.: -0.014 min
Response: 992567
Conc: 18.08 ng/ml m