

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012521\
 Data File : P0075163.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2021 22:41
 Operator : AJ/MA
 Sample : M1217-17
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1723-1724

Manual Integrations
 APPROVED

Ankita
 1/26/2021 2:38:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 01:04:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.924	3.996	3063093	1417486	29.029	25.199
2) SA Decachlor...	10.938	9.246	3023288	1481678	29.788	26.986m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012521\
Data File : P0075163.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2021 22:41
Operator : AJ/MA
Sample : M1217-17
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1723-1724


Manual Integrations
APPROVED

Ankita
1/26/2021 2:38:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 01:04:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

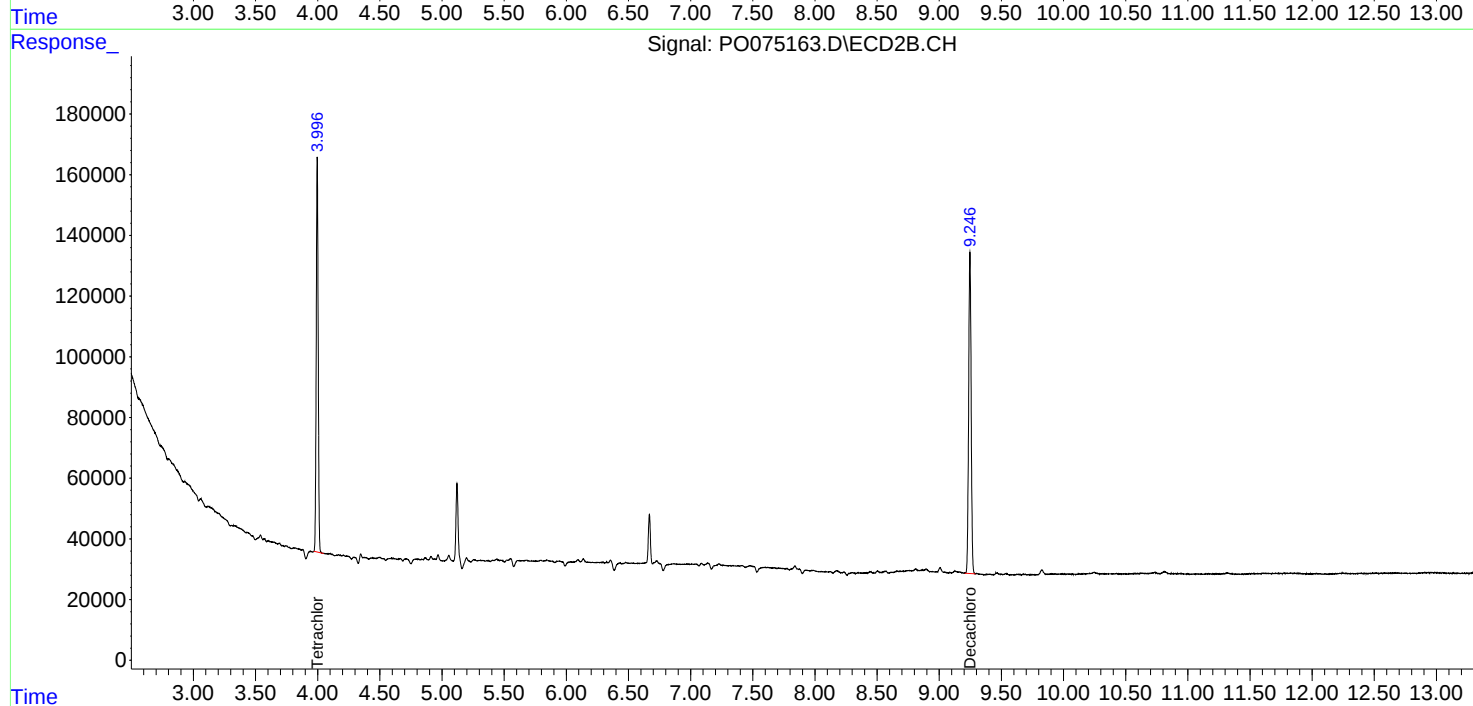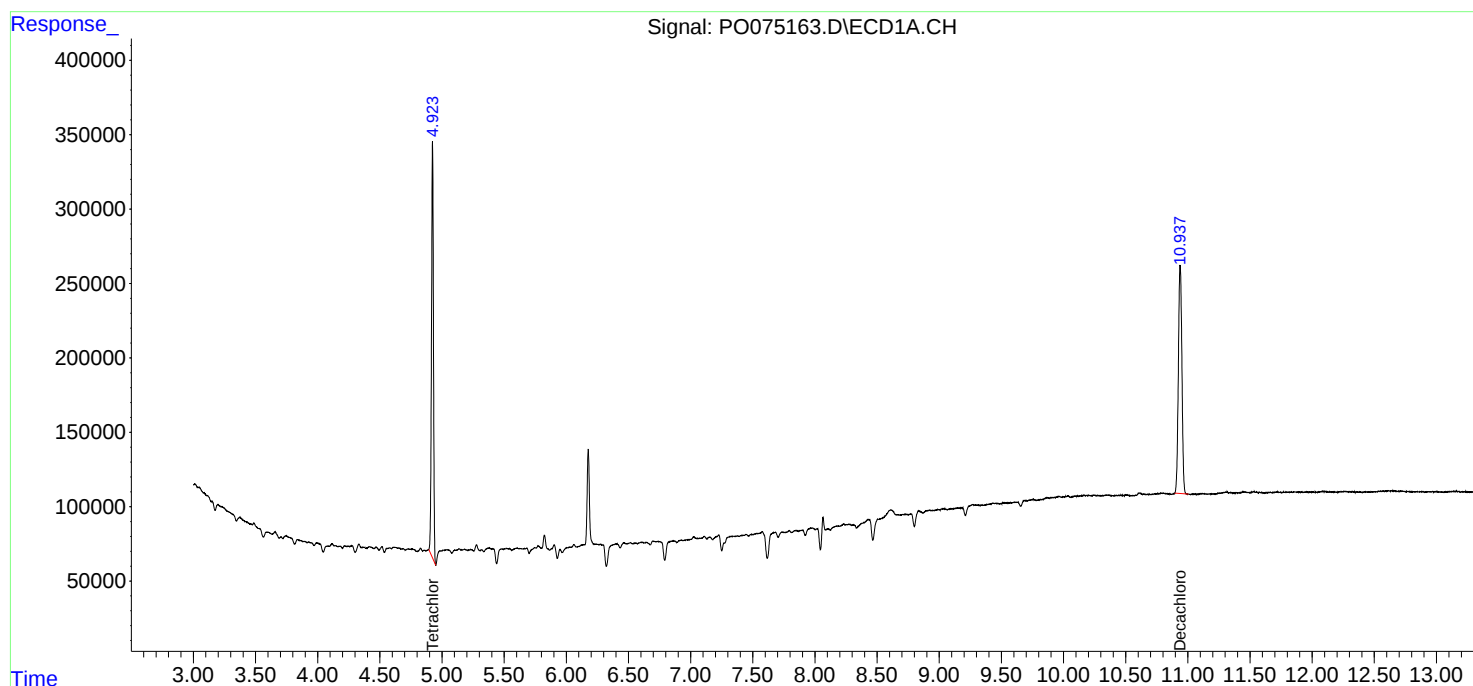

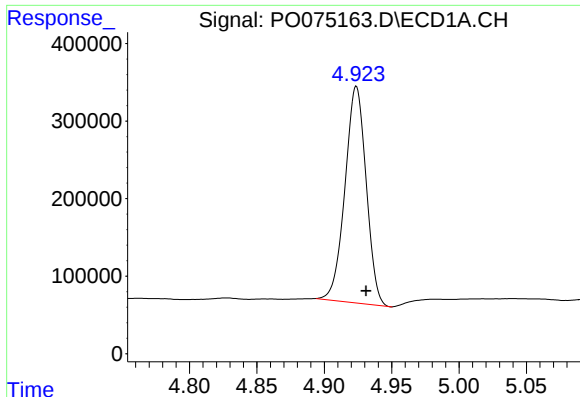


#1 Tetrachloro-m-xylene

R.T.: 4.924 min
Delta R.T.: -0.007 min
Response: 3063093
Conc: 29.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
1723-1724


Manual Integrations
APPROVED

Ankita
1/26/2021 2:38:42 PM

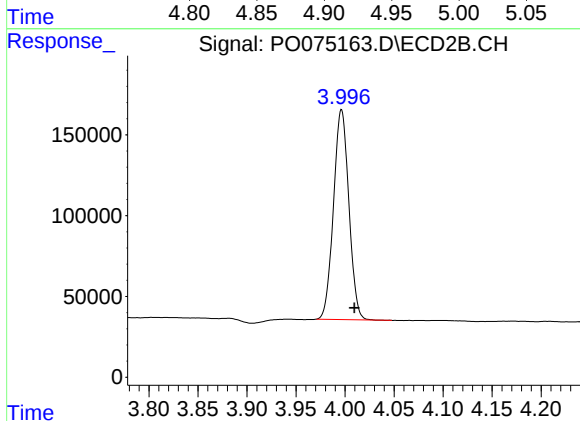


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: -0.013 min
Response: 1417486
Conc: 25.20 ng/ml

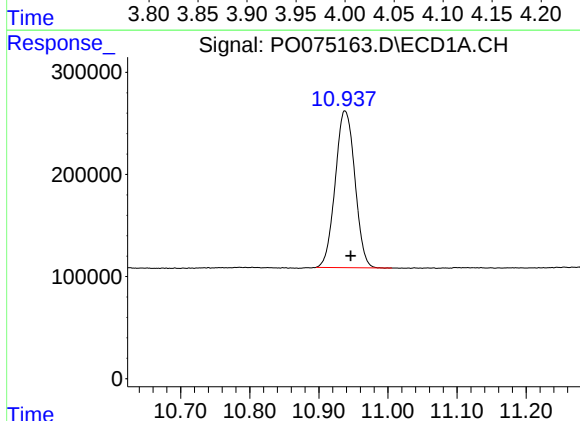

#2 Decachlorobiphenyl

R.T.: 10.938 min
Delta R.T.: -0.008 min
Response: 3023288
Conc: 29.79 ng/ml

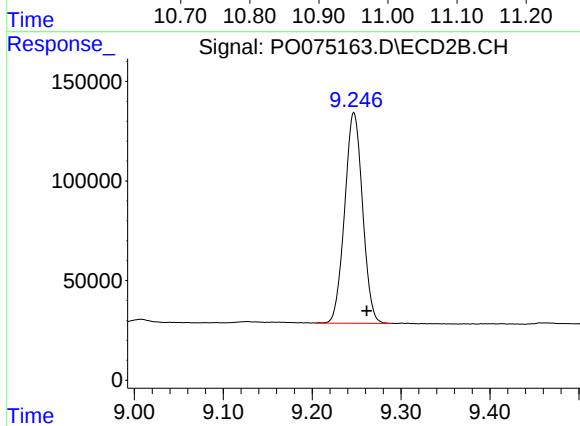

#2 Decachlorobiphenyl

R.T.: 9.246 min
Delta R.T.: -0.015 min
Response: 1481678
Conc: 26.99 ng/ml m