

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012521\
 Data File : P0075164.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 25 Jan 2021 22:59
 Operator : AJ/MA
 Sample : M1217-18
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1726-1727

Manual Integrations
 APPROVED

Ankita
 1/26/2021 2:38:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 01:05:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.924	3.998	2511863	1365489	23.805	24.274
2) SA Decachlor...	10.939	9.248	3012328	1398225	29.680	25.466m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012521\
Data File : PO075164.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 25 Jan 2021 22:59
Operator : AJ/MA
Sample : M1217-18
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1726-1727


Manual Integrations
APPROVED

Ankita
1/26/2021 2:38:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 01:05:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

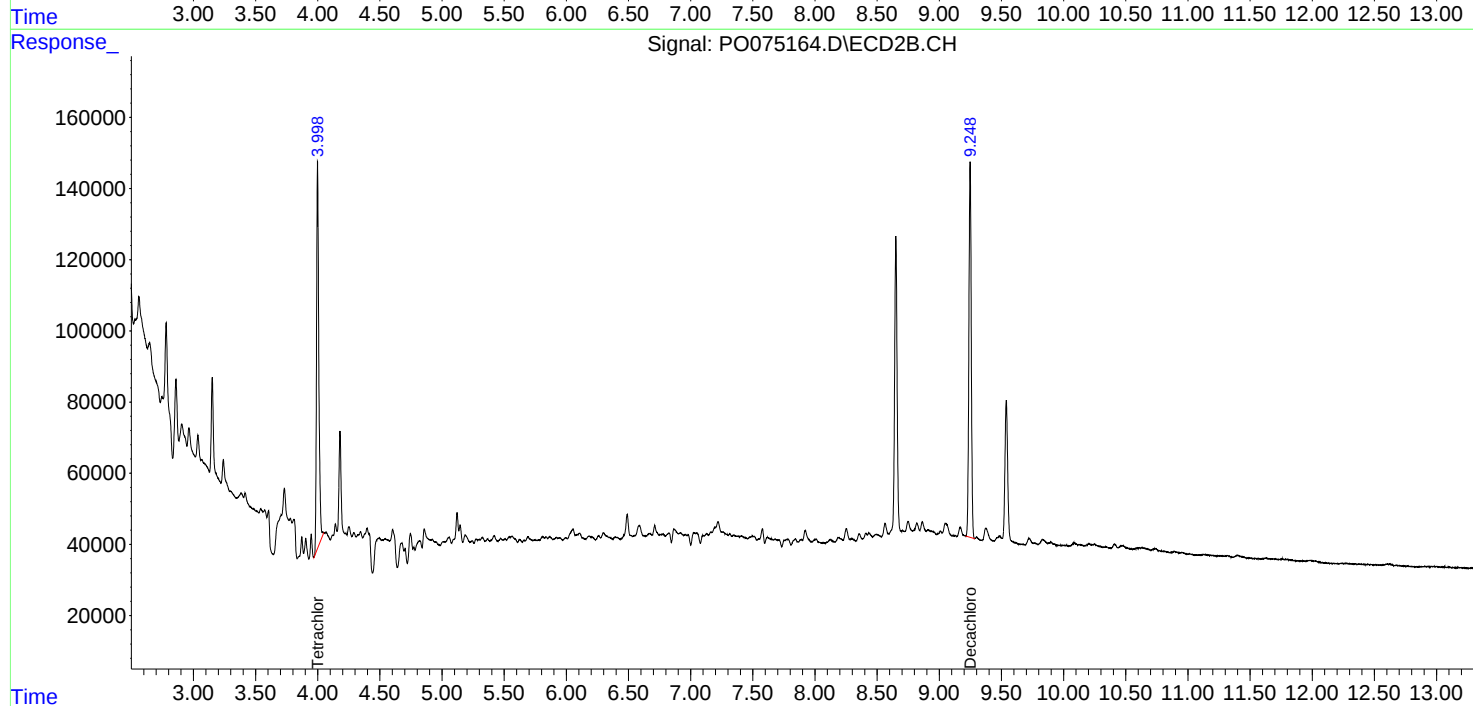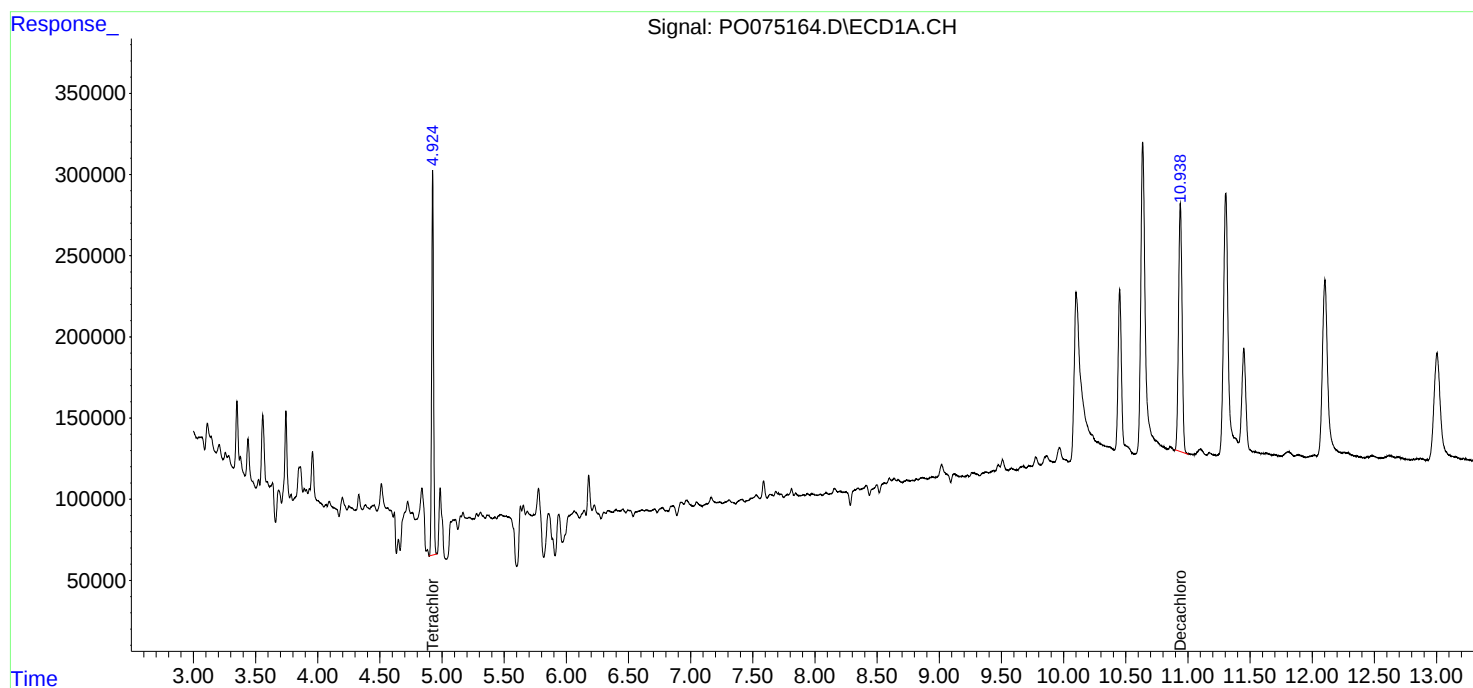

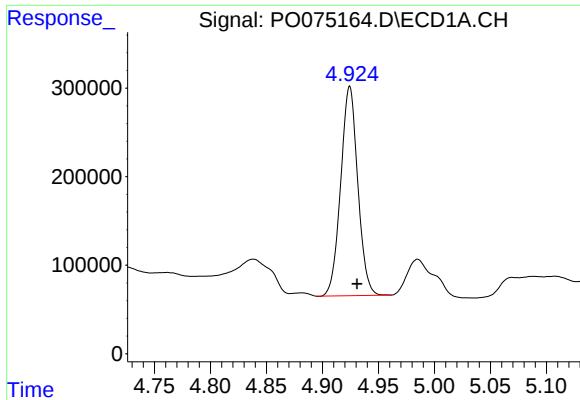


#1 Tetrachloro-m-xylene

R.T.: 4.924 min
Delta R.T.: -0.007 min
Response: 2511863
Conc: 23.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
1726-1727


Manual Integrations
APPROVED

Ankita
1/26/2021 2:38:44 PM

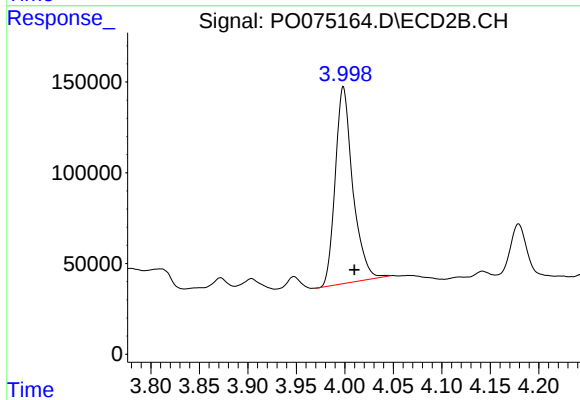


#1 Tetrachloro-m-xylene

R.T.: 3.998 min
Delta R.T.: -0.011 min
Response: 1365489
Conc: 24.27 ng/ml

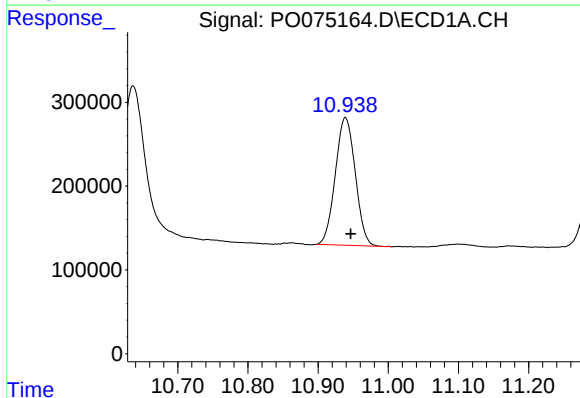

#2 Decachlorobiphenyl

R.T.: 10.939 min
Delta R.T.: -0.007 min
Response: 3012328
Conc: 29.68 ng/ml

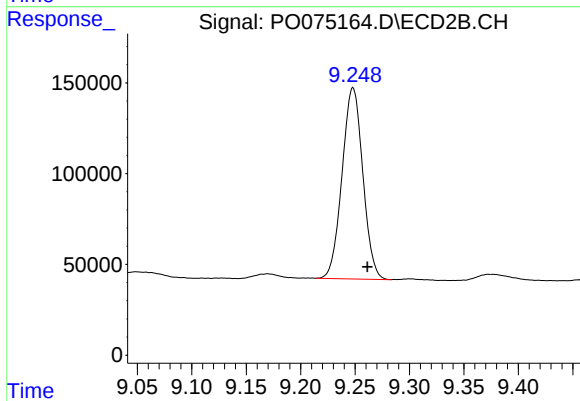

#2 Decachlorobiphenyl

R.T.: 9.248 min
Delta R.T.: -0.014 min
Response: 1398225
Conc: 25.47 ng/ml m