

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012524\
 Data File : P0101302.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jan 2024 09:44
 Operator : YP/AJ
 Sample : P1204-01 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMA895G-1-1

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/25/2024
 Supervised By :Sohil Jodhani 01/25/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 24 11:44:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 24 04:51:39 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.332	3.630	6548804	4358514	1.706m	1.687m
2) SA Decachlor...	10.058	8.675	4980475	3661947	2.137m	1.932m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012524\
Data File : PO101302.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jan 2024 09:44
Operator : YP/AJ
Sample : P1204-01 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMA895G-1-1


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/25/2024
Supervised By :Sohil Jodhani 01/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 24 11:44:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012424.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 24 04:51:39 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

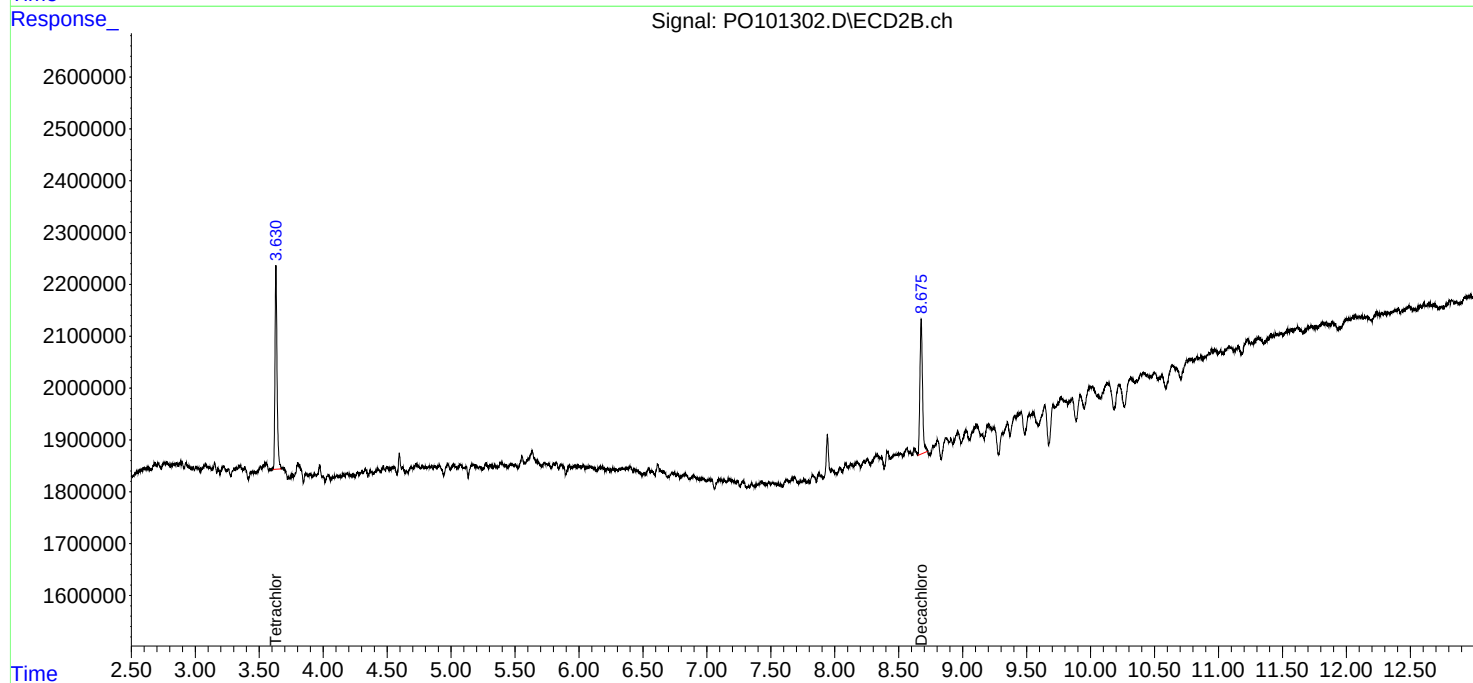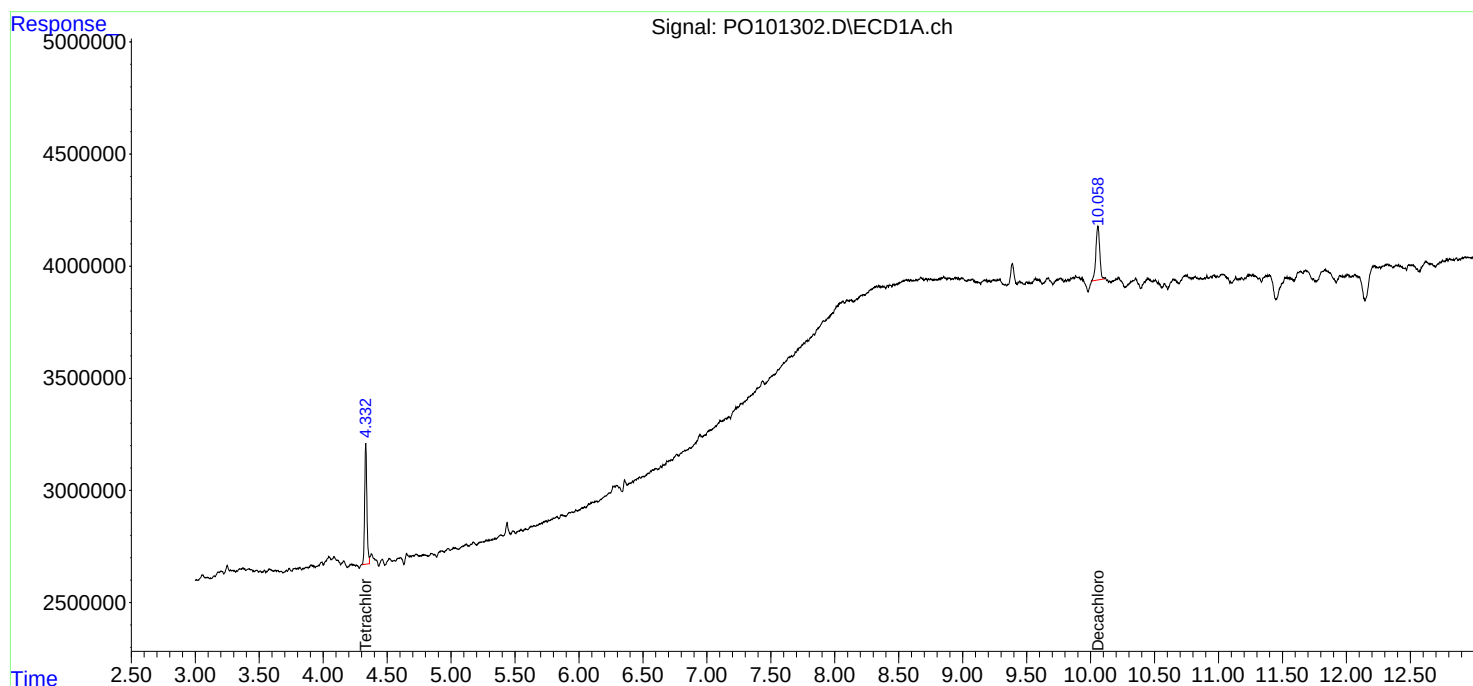

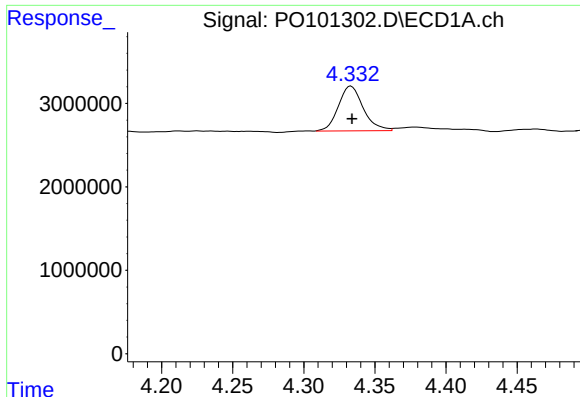


#1 Tetrachloro-m-xylene

R.T.: 4.332 min
Delta R.T.: -0.002 min
Response: 6548804
Conc: 1.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMA895G-1-1


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/25/2024
Supervised By :Sohil Jodhani 01/25/2024

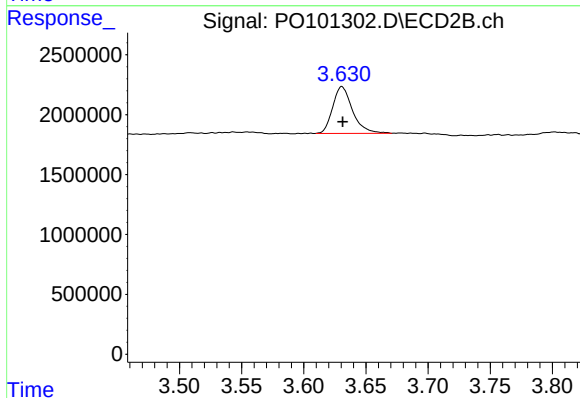


#1 Tetrachloro-m-xylene

R.T.: 3.630 min
Delta R.T.: -0.001 min
Response: 4358514
Conc: 1.69 ng/ml m

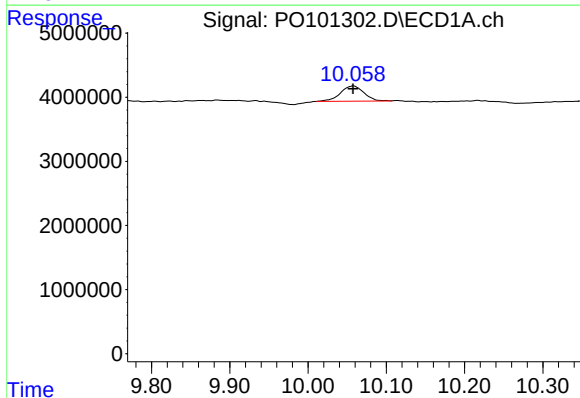

#2 Decachlorobiphenyl

R.T.: 10.058 min
Delta R.T.: 0.000 min
Response: 4980475
Conc: 2.14 ng/ml m

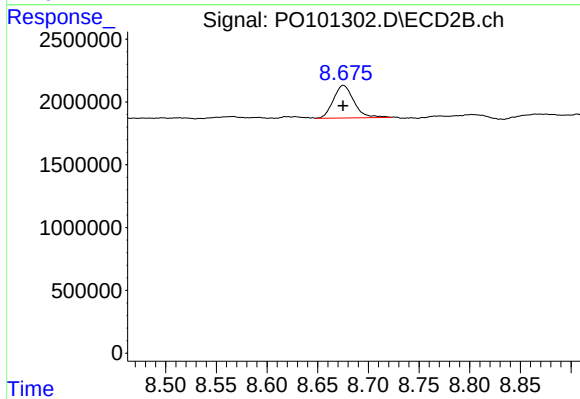

#2 Decachlorobiphenyl

R.T.: 8.675 min
Delta R.T.: 0.000 min
Response: 3661947
Conc: 1.93 ng/ml m