

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012621\
 Data File : P0075173.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jan 2021 10:02
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

mohammad
 1/27/2021 5:25:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:53:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.928	3.996	2251779	1078747	21.340	19.177
2)	SA Decachlor...	10.942	9.248	2123411	1121168	20.922	20.420m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012621\
Data File : P0075173.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jan 2021 10:02
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

mohammad
1/27/2021 5:25:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:53:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

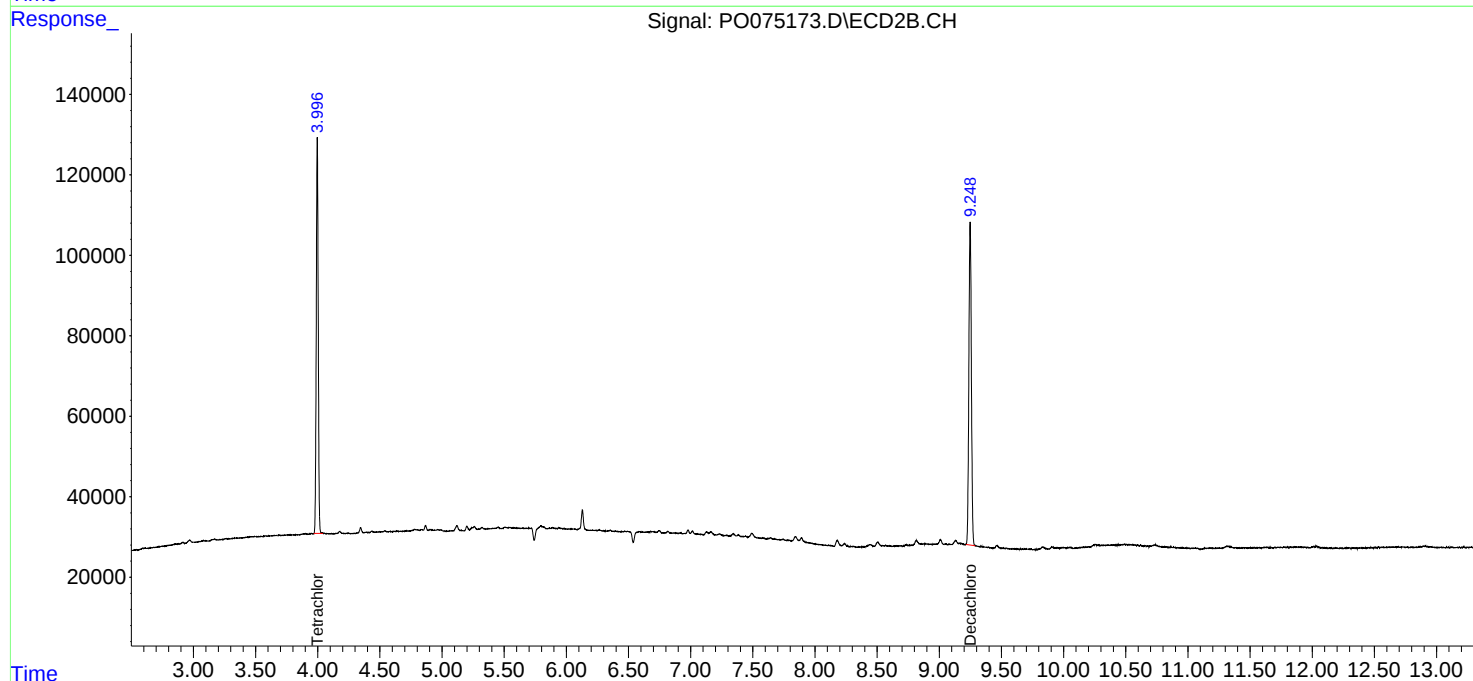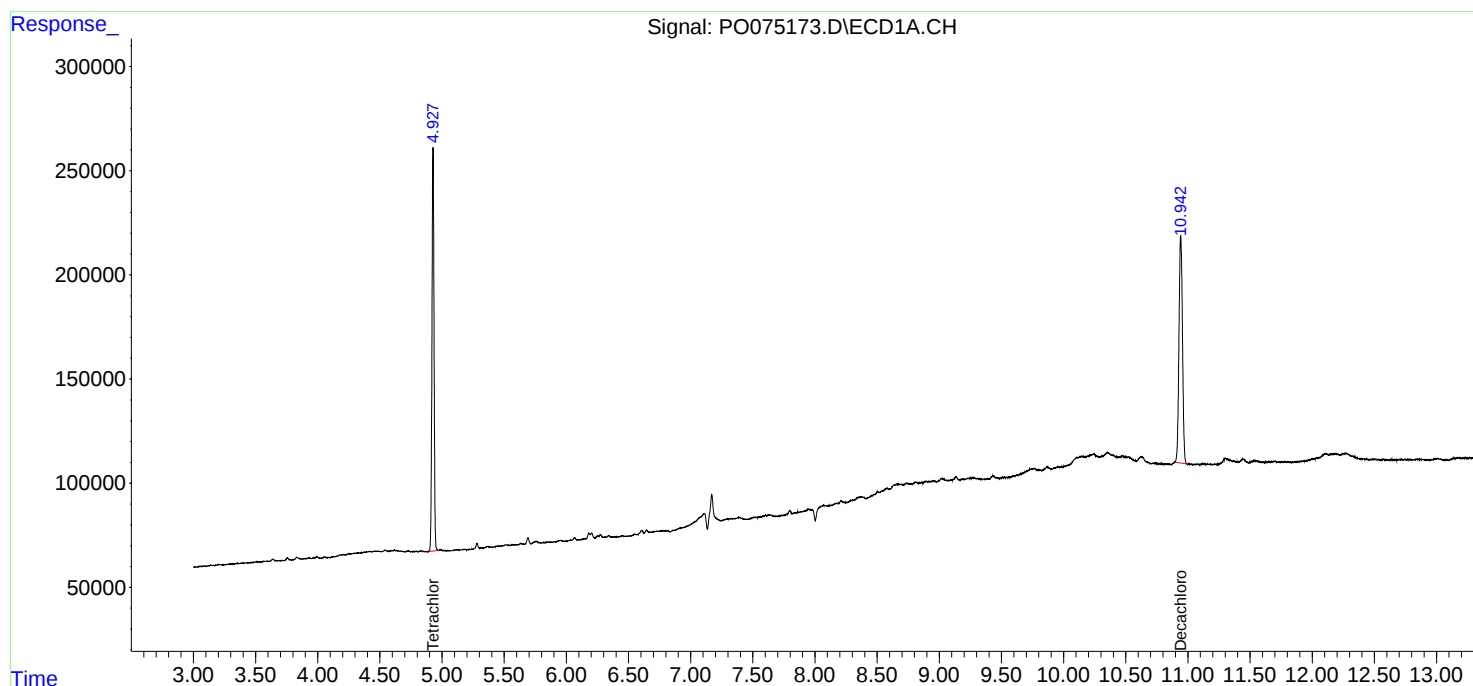

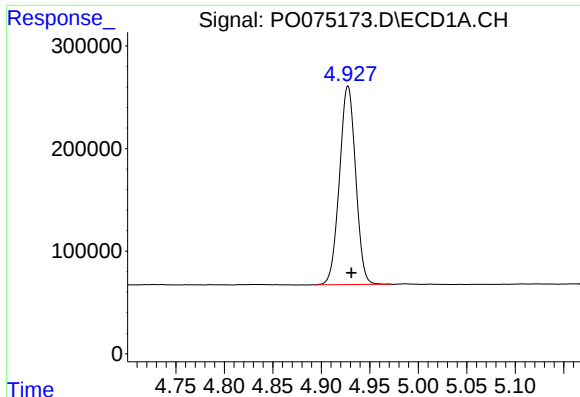


#1 Tetrachloro-m-xylene

R.T.: 4.928 min
Delta R.T.: -0.003 min
Response: 2251779
Conc: 21.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

mohammad
1/27/2021 5:25:58 PM

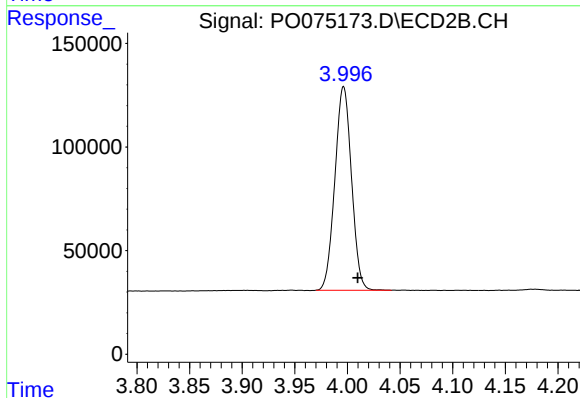


#1 Tetrachloro-m-xylene

R.T.: 3.996 min
Delta R.T.: -0.013 min
Response: 1078747
Conc: 19.18 ng/ml

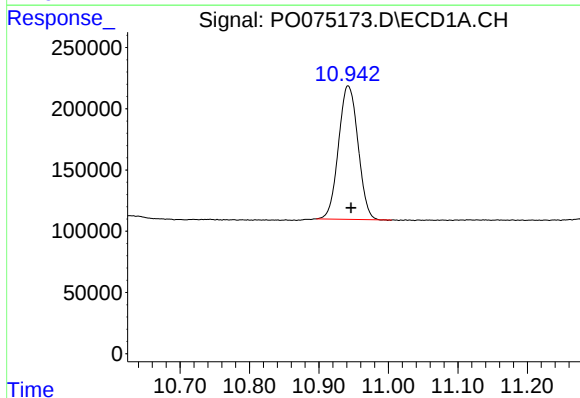

#2 Decachlorobiphenyl

R.T.: 10.942 min
Delta R.T.: -0.004 min
Response: 2123411
Conc: 20.92 ng/ml

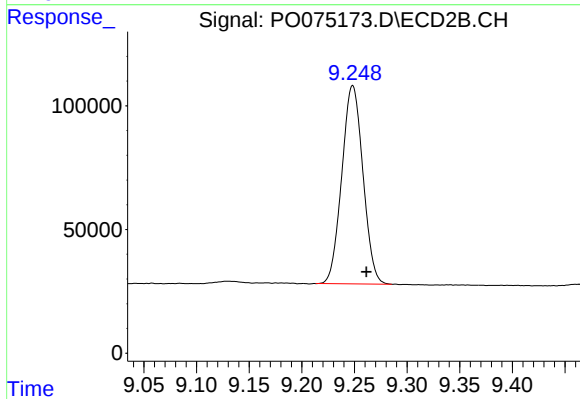

#2 Decachlorobiphenyl

R.T.: 9.248 min
Delta R.T.: -0.014 min
Response: 1121168
Conc: 20.42 ng/ml m