

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012621\
 Data File : P0075182.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jan 2021 12:36
 Operator : AJ/MA
 Sample : PB134327BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB134327BL

Manual Integrations
 APPROVED

mohammad
 1/27/2021 5:27:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:56:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.925	3.997	2390199	1136514	22.652	20.204
2) SA Decachlor...	10.940	9.248	2270103	1170761	22.367	21.324m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012621\
Data File : P0075182.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jan 2021 12:36
Operator : AJ/MA
Sample : PB134327BL
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB134327BL


Manual Integrations
APPROVED

mohammad
1/27/2021 5:27:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:56:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

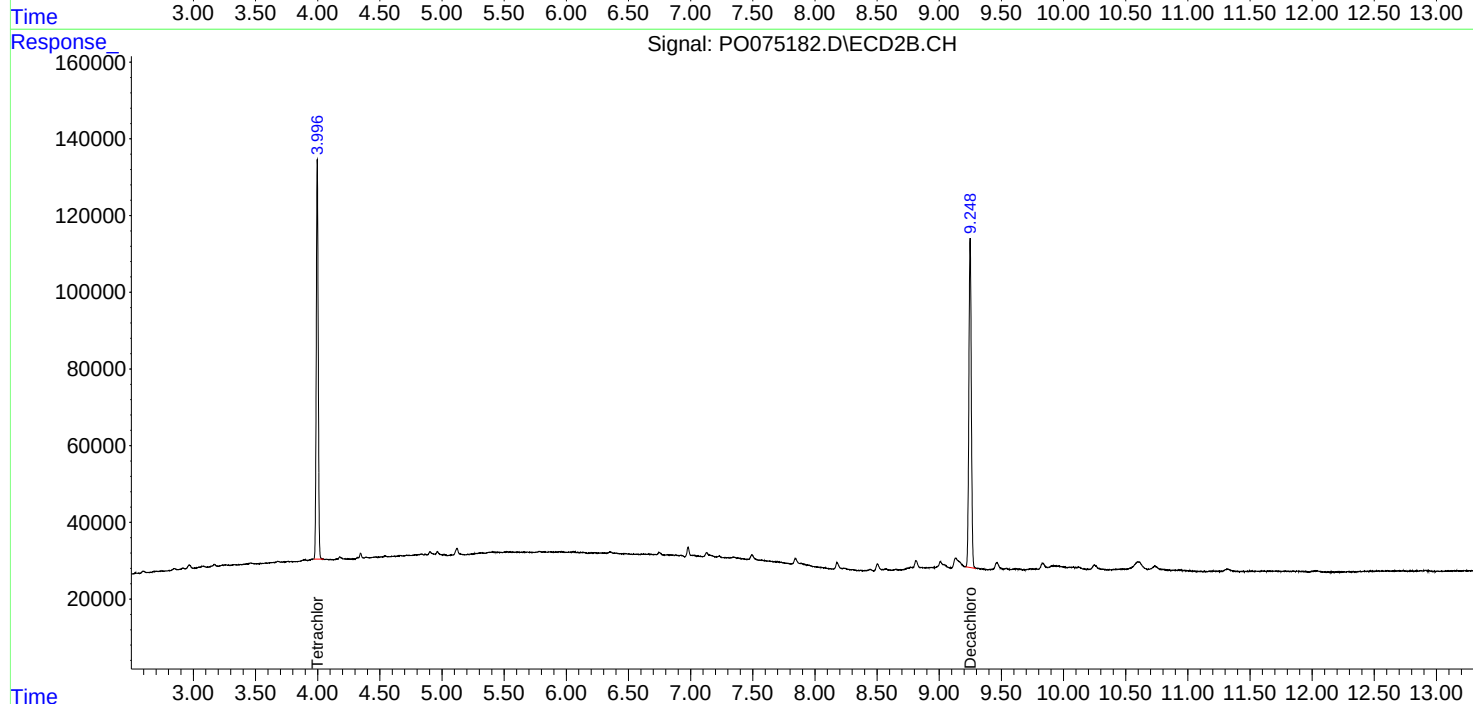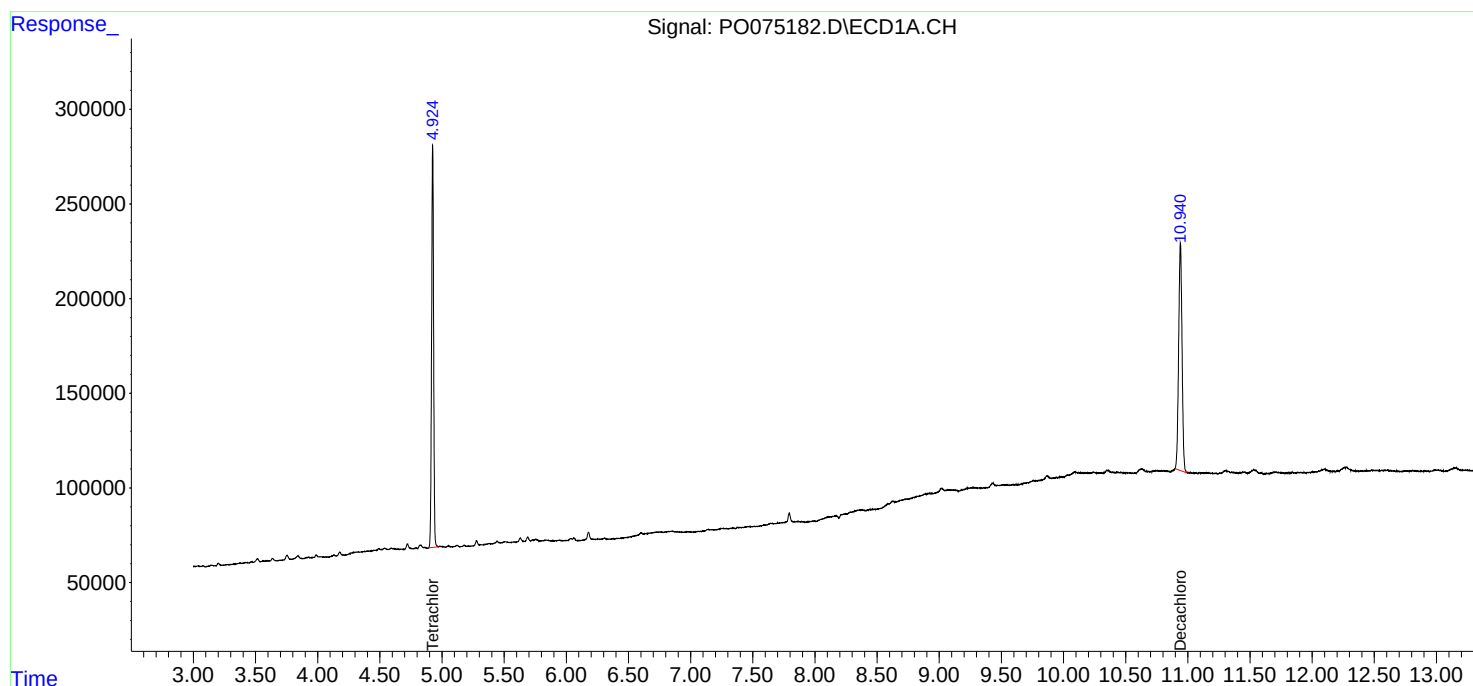

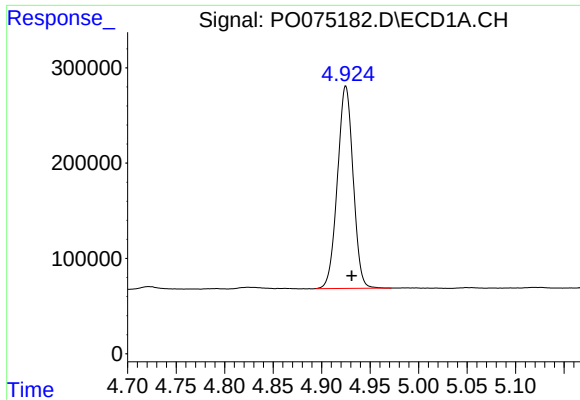


#1 Tetrachloro-m-xylene

R.T.: 4.925 min
Delta R.T.: -0.006 min
Response: 2390199
Conc: 22.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB134327BL


Manual Integrations
APPROVED

mohammad
1/27/2021 5:27:42 PM

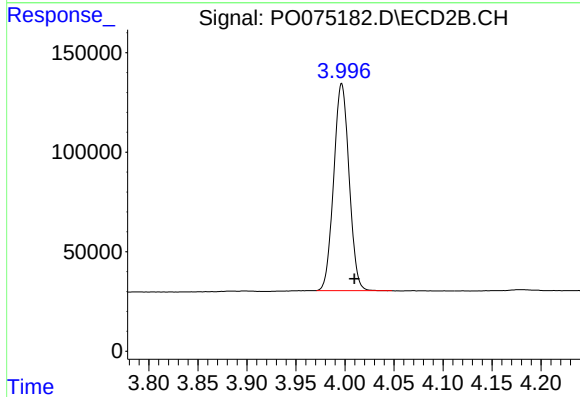


#1 Tetrachloro-m-xylene

R.T.: 3.997 min
Delta R.T.: -0.013 min
Response: 1136514
Conc: 20.20 ng/ml

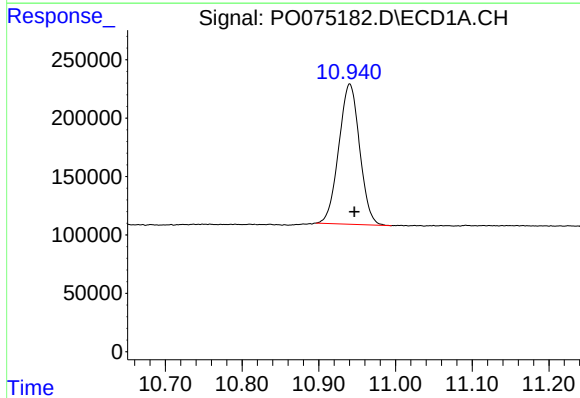

#2 Decachlorobiphenyl

R.T.: 10.940 min
Delta R.T.: -0.006 min
Response: 2270103
Conc: 22.37 ng/ml

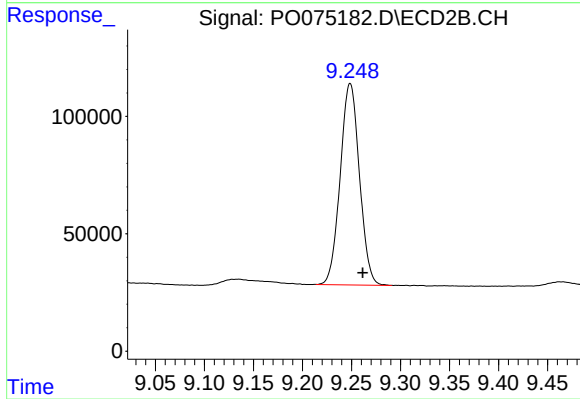

#2 Decachlorobiphenyl

R.T.: 9.248 min
Delta R.T.: -0.013 min
Response: 1170761
Conc: 21.32 ng/ml m