

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012621\
 Data File : P0075189.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jan 2021 14:36
 Operator : AJ/MA
 Sample : M1235-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-SF-SAMPLE-1

Manual Integrations
 APPROVED

Ankita
 1/28/2021 2:54:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:58:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.926	3.998	1890520	1037402	17.917	18.442
2) SA Decachlor...	10.942	9.250	1798099	849922	17.717	15.480m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012621\
Data File : P0075189.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jan 2021 14:36
Operator : AJ/MA
Sample : M1235-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-SF-SAMPLE-1


Manual Integrations
APPROVED

Ankita
1/28/2021 2:54:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:58:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

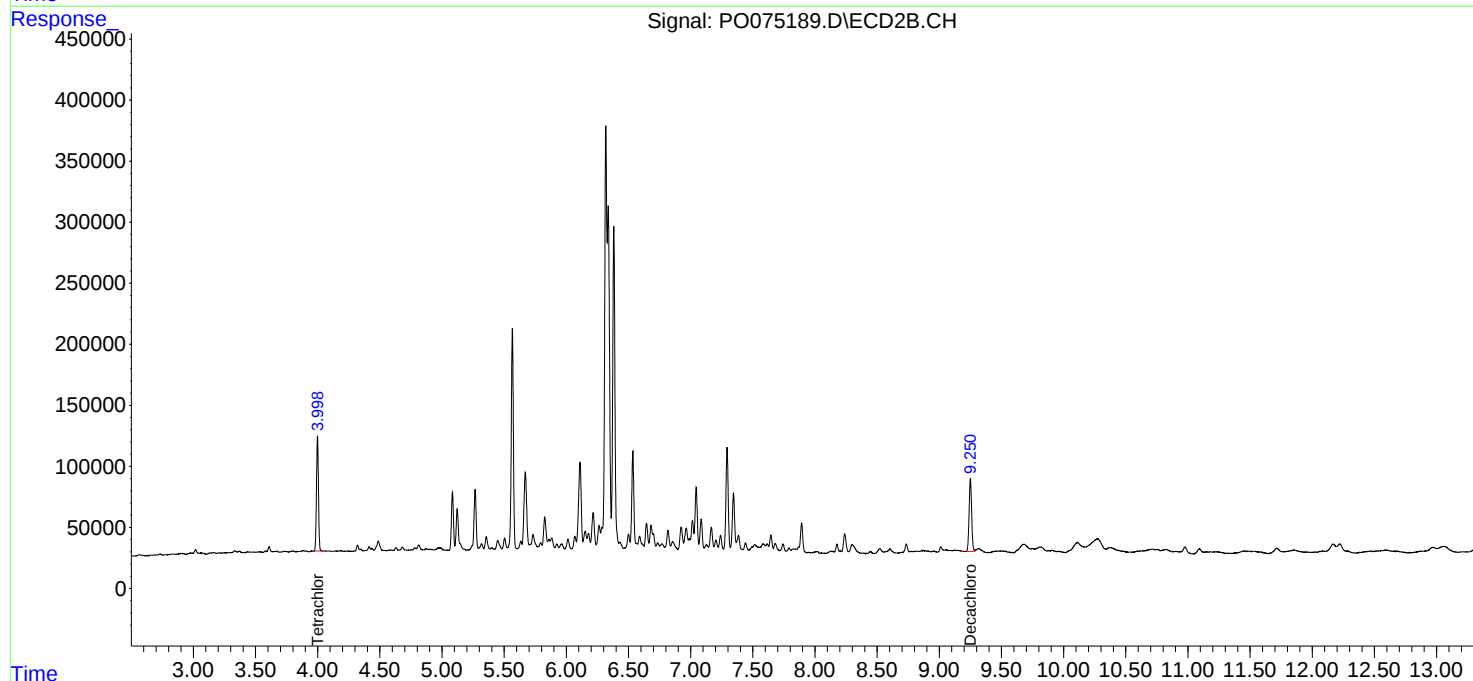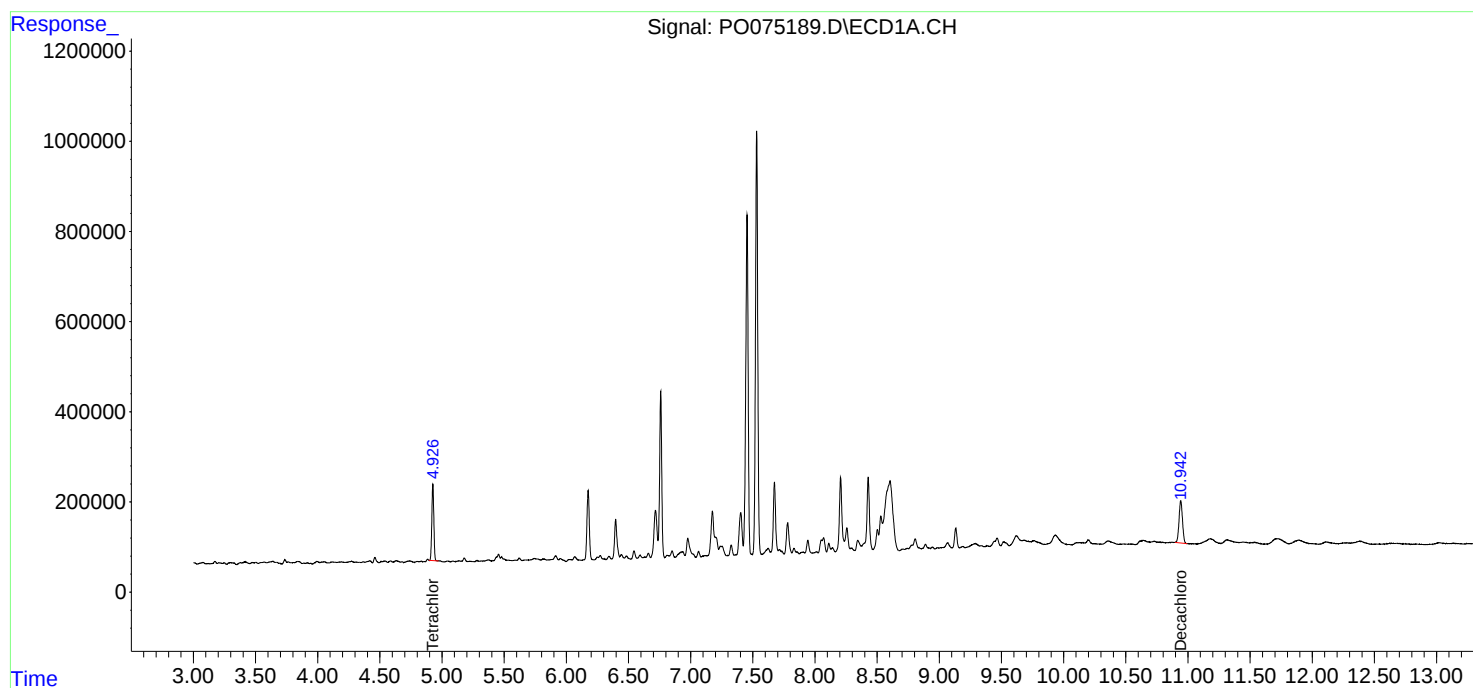

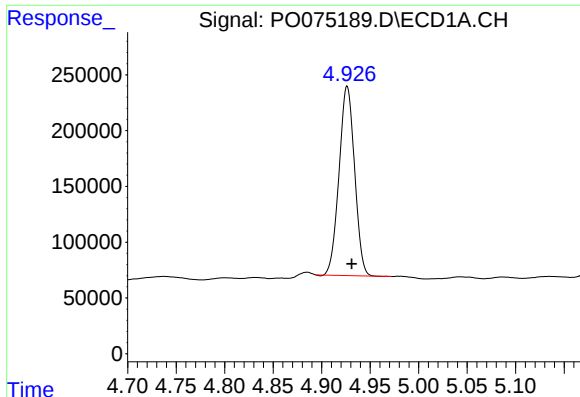


#1 Tetrachloro-m-xylene

R.T.: 4.926 min
Delta R.T.: -0.005 min
Response: 1890520
Conc: 17.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-SF-SAMPLE-1


Manual Integrations
APPROVED

Ankita
1/28/2021 2:54:25 PM

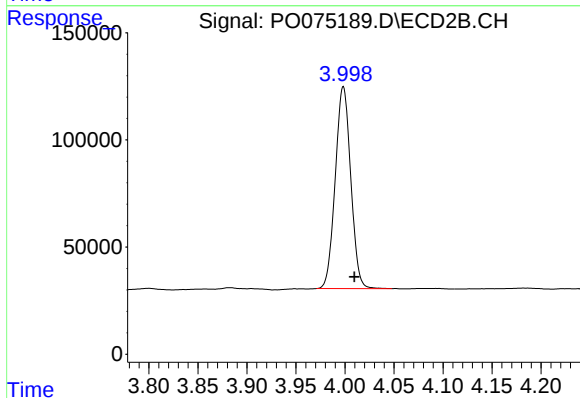


#1 Tetrachloro-m-xylene

R.T.: 3.998 min
Delta R.T.: -0.011 min
Response: 1037402
Conc: 18.44 ng/ml

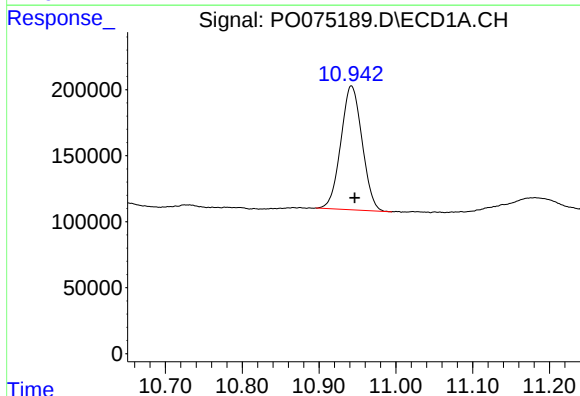

#2 Decachlorobiphenyl

R.T.: 10.942 min
Delta R.T.: -0.004 min
Response: 1798099
Conc: 17.72 ng/ml

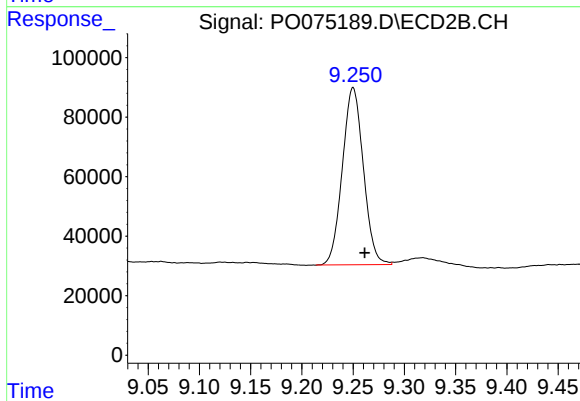

#2 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.012 min
Response: 849922
Conc: 15.48 ng/ml m