

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012621\
 Data File : P0075192.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jan 2021 15:27
 Operator : AJ/MA
 Sample : M1230-01 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NWB-1501

Manual Integrations
 APPROVED

Ankita
 1/28/2021 4:35:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 00:59:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.926	3.999	148504	95497	1.407m	1.698m
2) SA Decachlor...	10.950	9.259	405711	221472	3.997	4.034

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012621\
Data File : P0075192.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jan 2021 15:27
Operator : AJ/MA
Sample : M1230-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NWB-1501


Manual Integrations
APPROVED

Ankita
1/28/2021 4:35:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 00:59:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

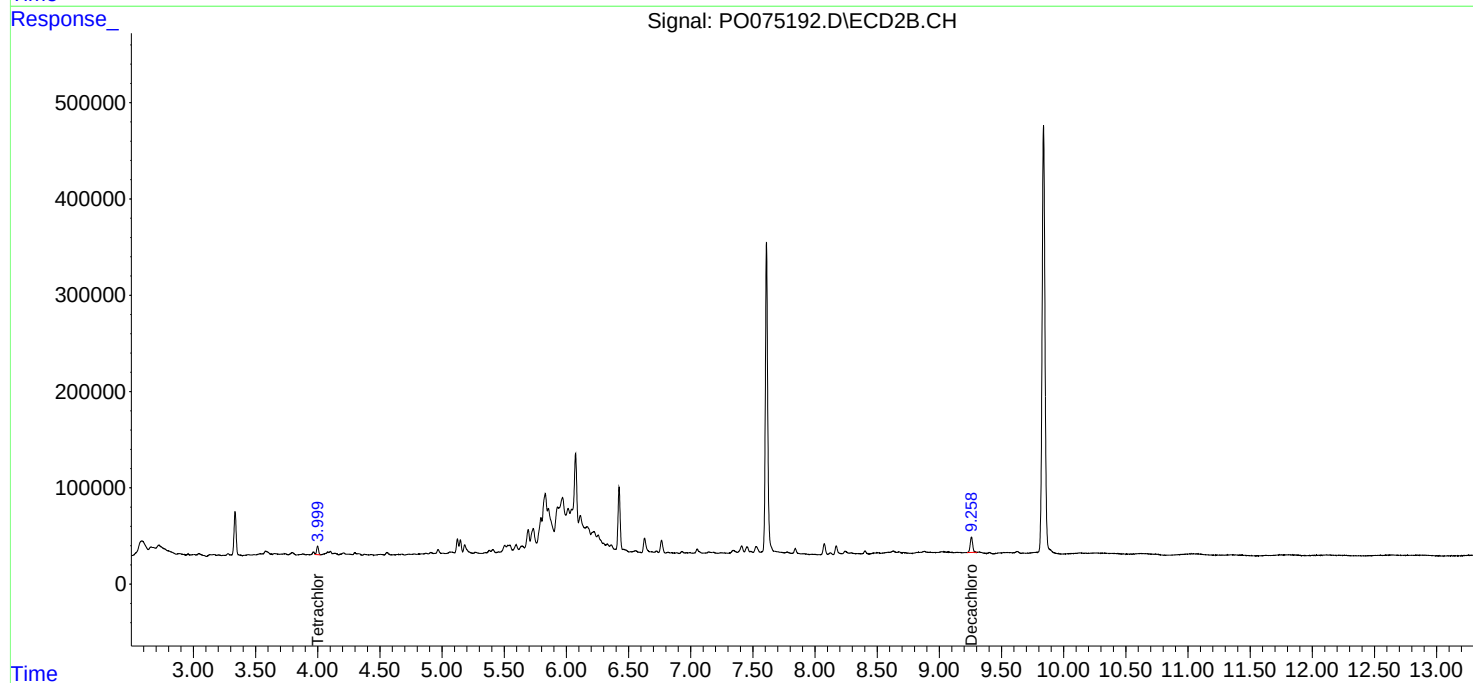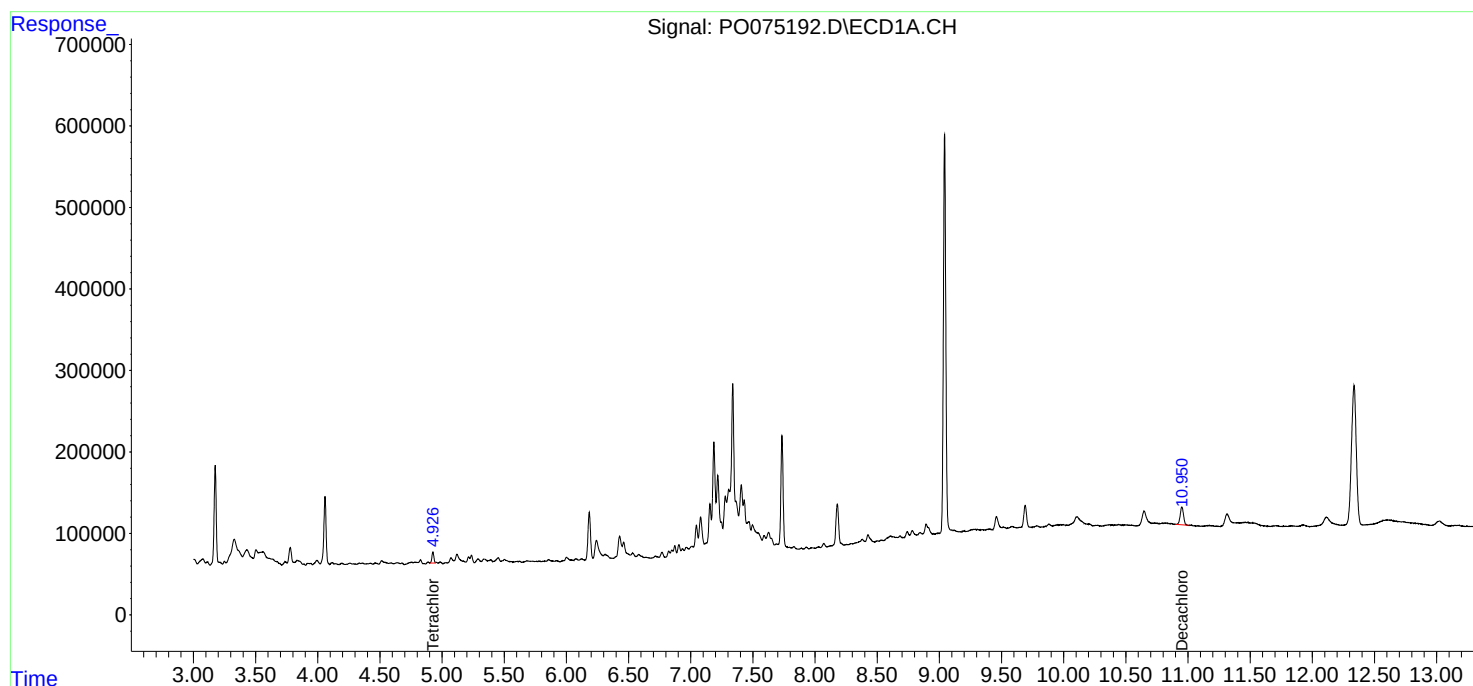

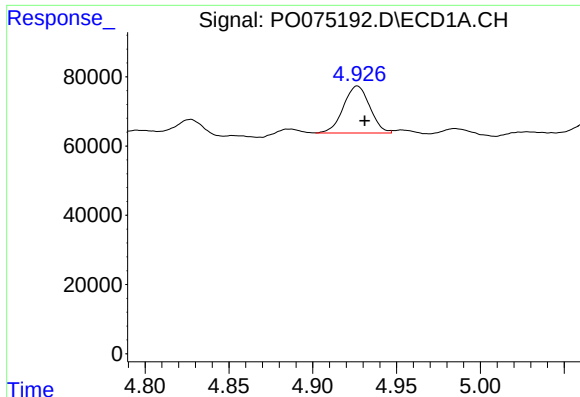


#1 Tetrachloro-m-xylene

R.T.: 4.926 min
Delta R.T.: -0.005 min
Response: 148504
Conc: 1.41 ng/ml m

Instrument :
ECD_O
ClientSampleId :
NWB-1501


Manual Integrations
APPROVED

Ankita
1/28/2021 4:35:00 PM

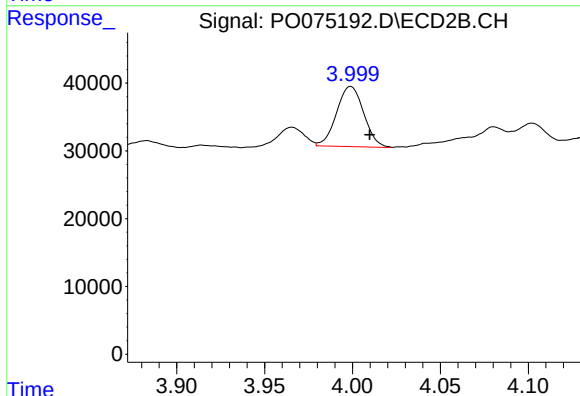


#1 Tetrachloro-m-xylene

R.T.: 3.999 min
Delta R.T.: -0.011 min
Response: 95497
Conc: 1.70 ng/ml m

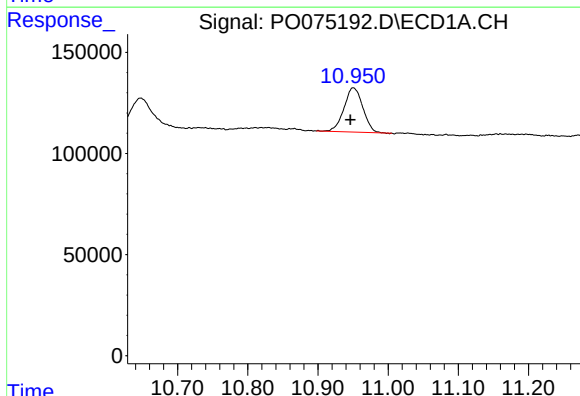

#2 Decachlorobiphenyl

R.T.: 10.950 min
Delta R.T.: 0.004 min
Response: 405711
Conc: 4.00 ng/ml

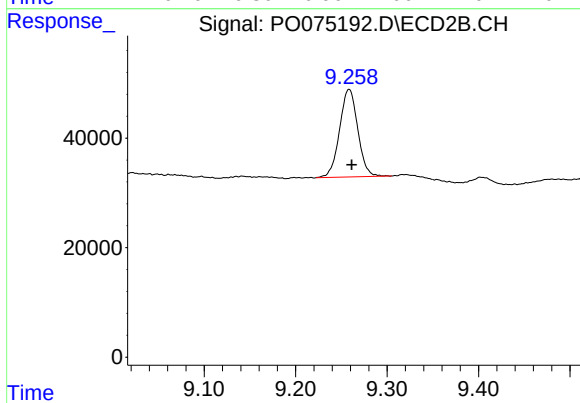

#2 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.003 min
Response: 221472
Conc: 4.03 ng/ml