

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012621\
 Data File : P0075195.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 Jan 2021 17:25
 Operator : AJ/MA
 Sample : PB134352BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB134352BL

Manual Integrations
 APPROVED

mohammad
 1/27/2021 5:28:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 01:00:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.926	3.998	2226867	1033656	21.104	18.375
2) SA Decachlor...	10.944	9.250	1775988	892886	17.499	16.263m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012621\
Data File : P0075195.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Jan 2021 17:25
Operator : AJ/MA
Sample : PB134352BL
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB134352BL


Manual Integrations
APPROVED

mohammad
1/27/2021 5:28:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 01:00:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

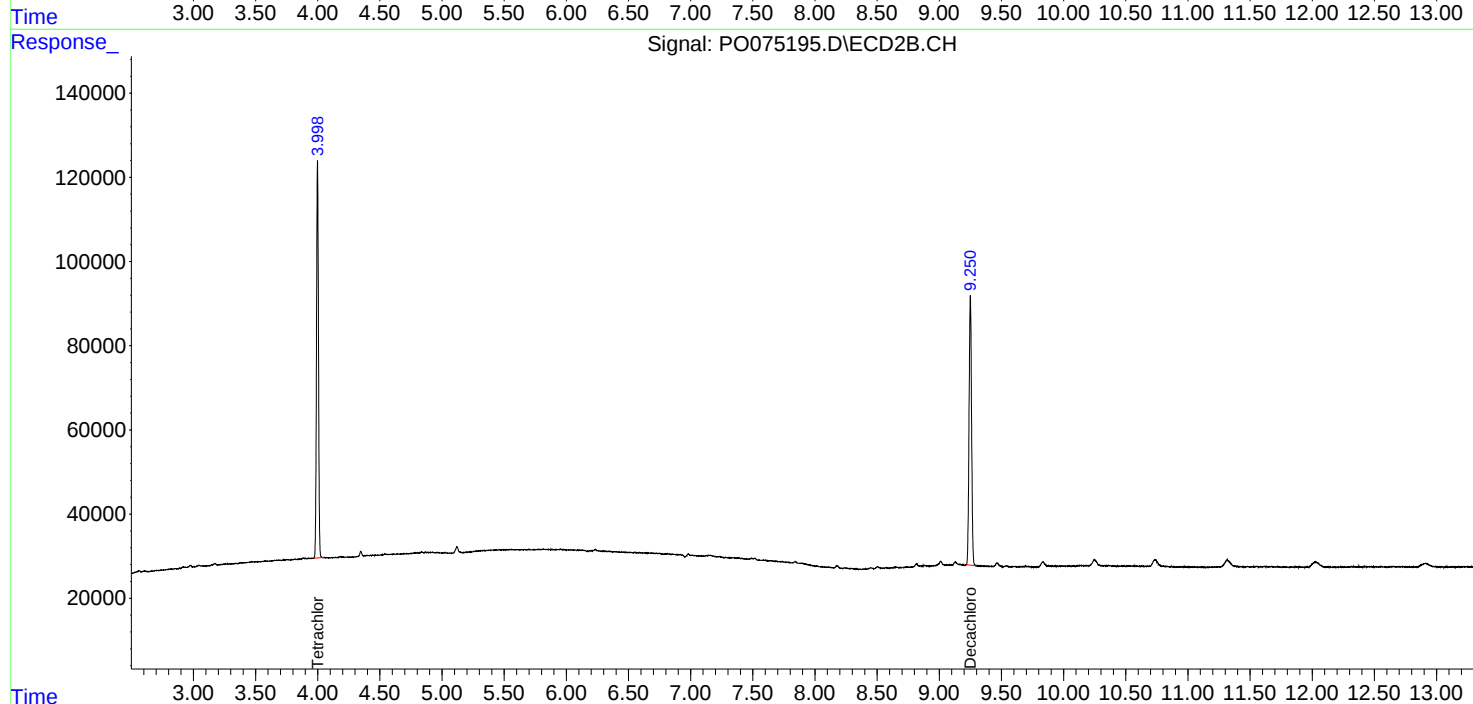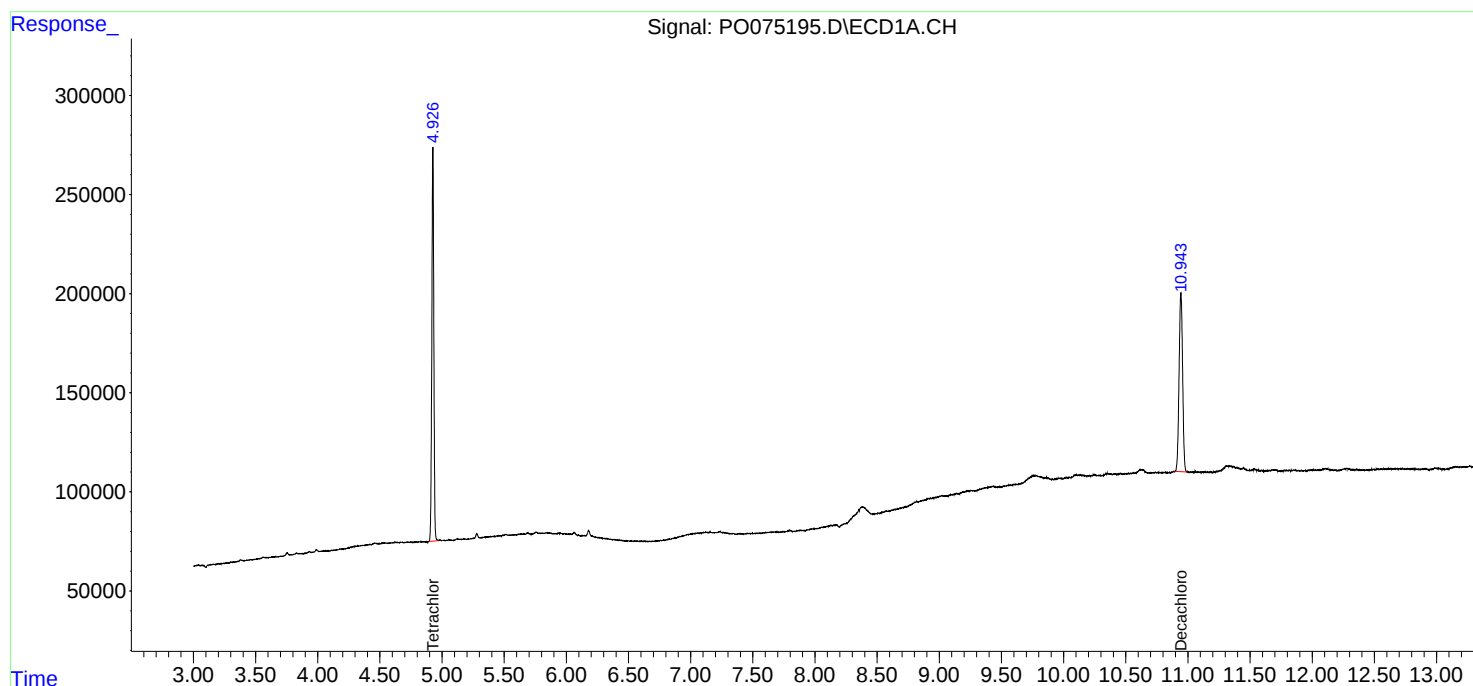

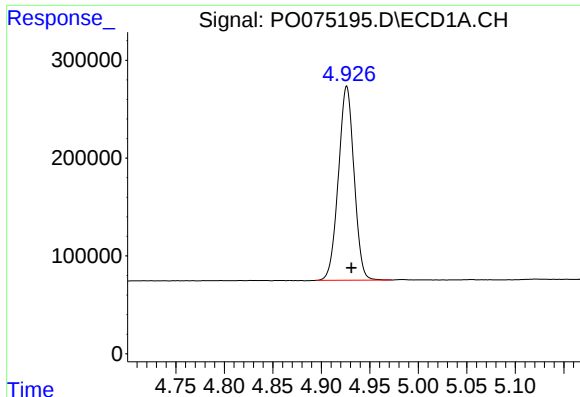


#1 Tetrachloro-m-xylene

R.T.: 4.926 min
Delta R.T.: -0.005 min
Response: 2226867
Conc: 21.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB134352BL


Manual Integrations
APPROVED

mohammad
1/27/2021 5:28:13 PM

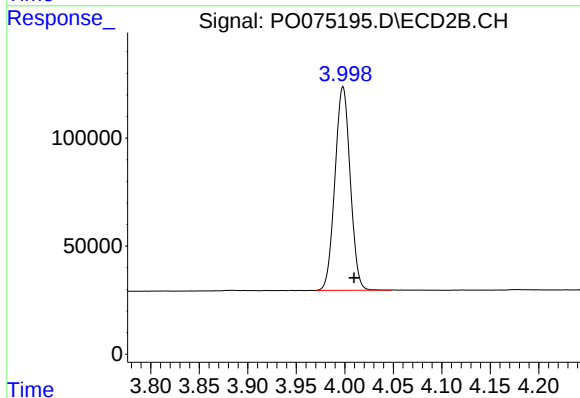


#1 Tetrachloro-m-xylene

R.T.: 3.998 min
Delta R.T.: -0.012 min
Response: 1033656
Conc: 18.38 ng/ml

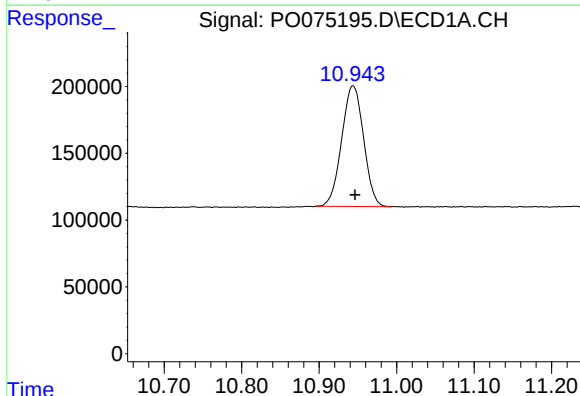

#2 Decachlorobiphenyl

R.T.: 10.944 min
Delta R.T.: -0.003 min
Response: 1775988
Conc: 17.50 ng/ml

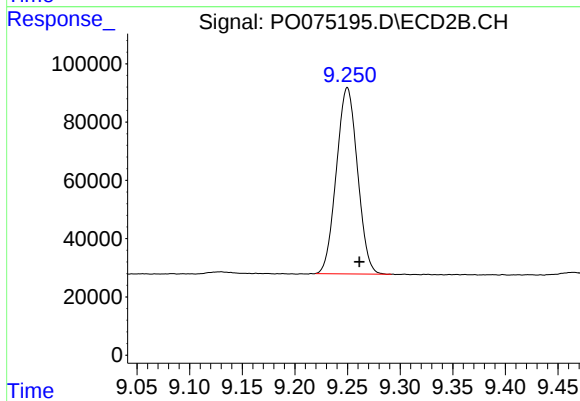

#2 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.012 min
Response: 892886
Conc: 16.26 ng/ml m