

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012621\
 Data File : P0075232.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jan 2021 4:50
 Operator : AJ/MA
 Sample : M1247-05
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 250EM-017-0002

Manual Integrations
 APPROVED

mohammad
 1/27/2021 5:29:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 05:45:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.925	3.997	2235116	1107753	21.182	19.693
2) SA Decachlor...	10.941	9.248	1430042	907063	14.090m	16.521

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012621\
Data File : P0075232.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jan 2021 4:50
Operator : AJ/MA
Sample : M1247-05
Misc :
ALS Vial : 52 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleID :
250EM-017-0002


Manual Integrations
APPROVED

mohammad
1/27/2021 5:29:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 05:45:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

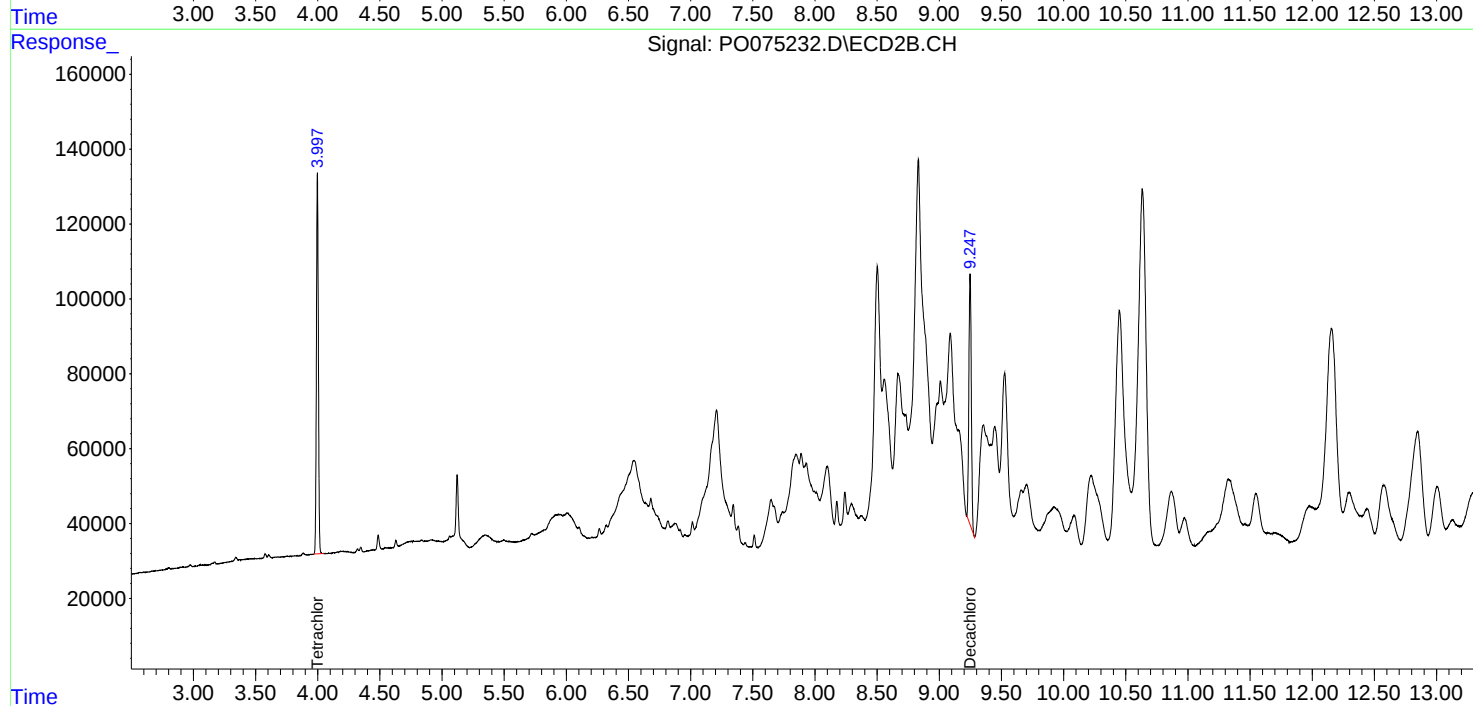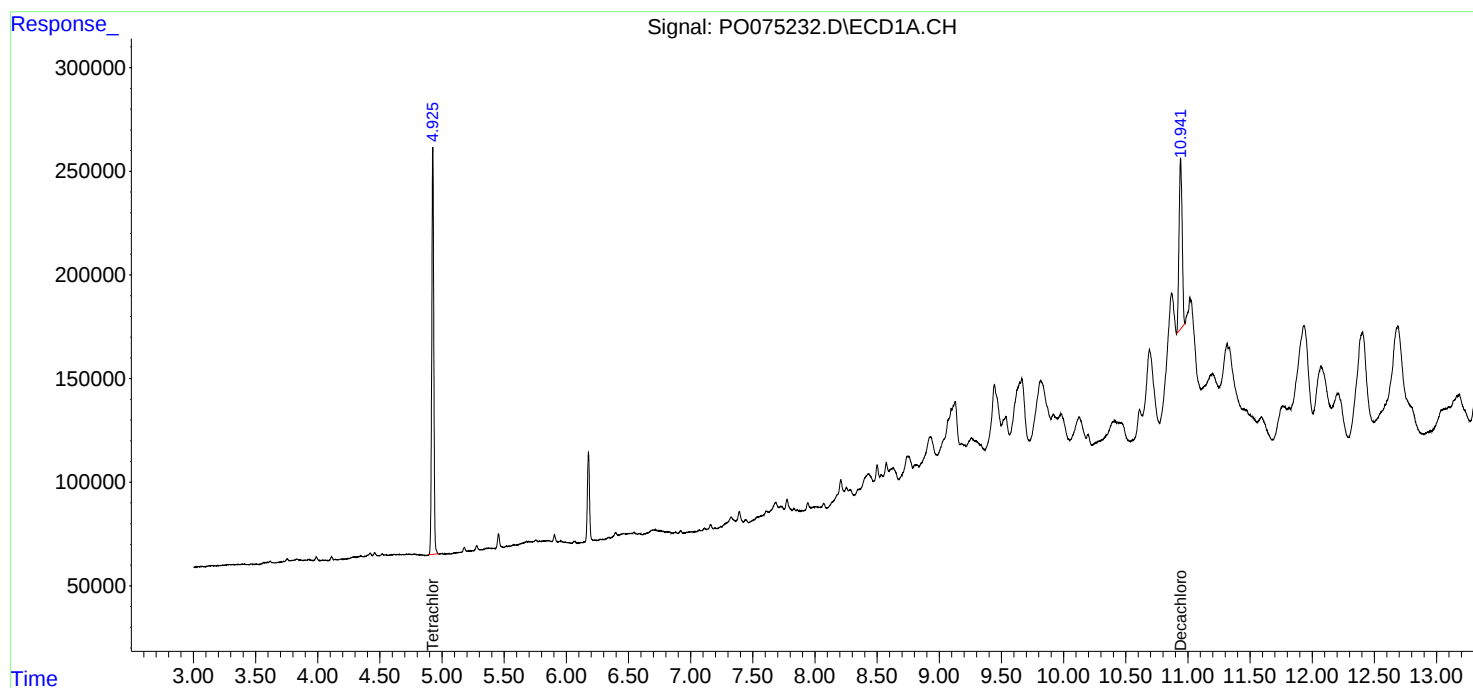

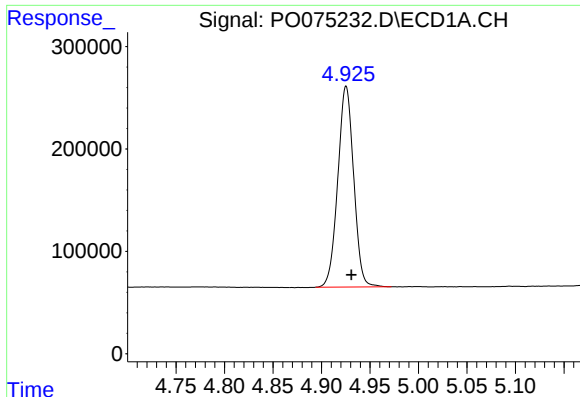


#1 Tetrachloro-m-xylene

R.T.: 4.925 min
Delta R.T.: -0.006 min
Response: 2235116
Conc: 21.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
250EM-017-0002


Manual Integrations
APPROVED

mohammad
1/27/2021 5:29:16 PM

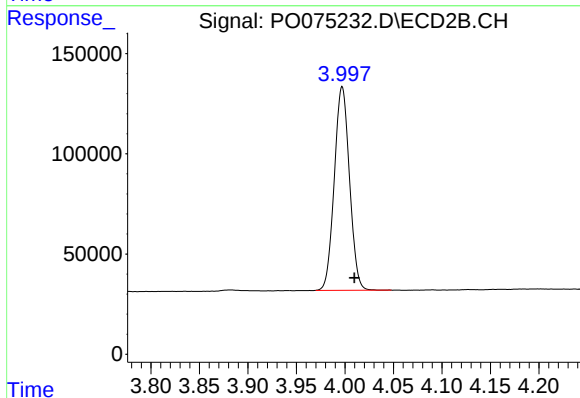


#1 Tetrachloro-m-xylene

R.T.: 3.997 min
Delta R.T.: -0.013 min
Response: 1107753
Conc: 19.69 ng/ml

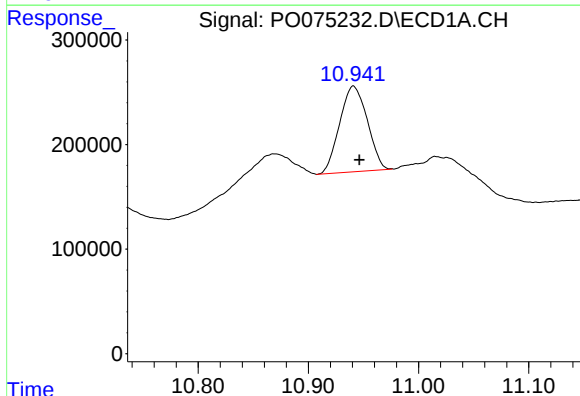

#2 Decachlorobiphenyl

R.T.: 10.941 min
Delta R.T.: -0.006 min
Response: 1430042
Conc: 14.09 ng/ml m

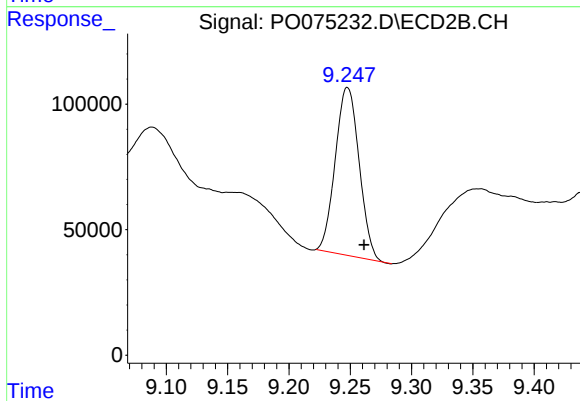

#2 Decachlorobiphenyl

R.T.: 9.248 min
Delta R.T.: -0.014 min
Response: 907063
Conc: 16.52 ng/ml