

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012720\
 Data File : P0065973.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Jan 2020 1:13
 Operator : DD\AJ
 Sample : L1269-13
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-25-24-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 04:11:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.154	3.430	763712	914780	32.936	34.440
2)	SA Decachlor...	9.653	8.331	679563	872378	16.325	17.952
Target Compounds							
7)	L1 AR-1016-5	0.000	4.926	0	28021	N.D.	25.990 #
9)	L2 AR-1221-2	0.000	3.722	0	11512	N.D.	45.303 #
15)	L3 AR-1232-5	0.000	4.926	0	28021	N.D.	70.319 #
20)	L4 AR-1242-5	6.150	5.301	47264	36422	56.762	32.901 #
24)	L5 AR-1248-4	6.150	4.926	47264	28021	35.079	21.958 #
25)	L5 AR-1248-5	6.150	5.301	47264	36422	36.569	26.095 #
26)	L6 AR-1254-1	6.150	5.301	47264	36422	35.609	16.289 #
45)	L9 AR-1268-5	0.000	8.103	0	8881	N.D.	0.492 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012720\
Data File : P0065973.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Jan 2020 1:13
Operator : DD\AJ
Sample : L1269-13
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-25-24-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 04:11:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

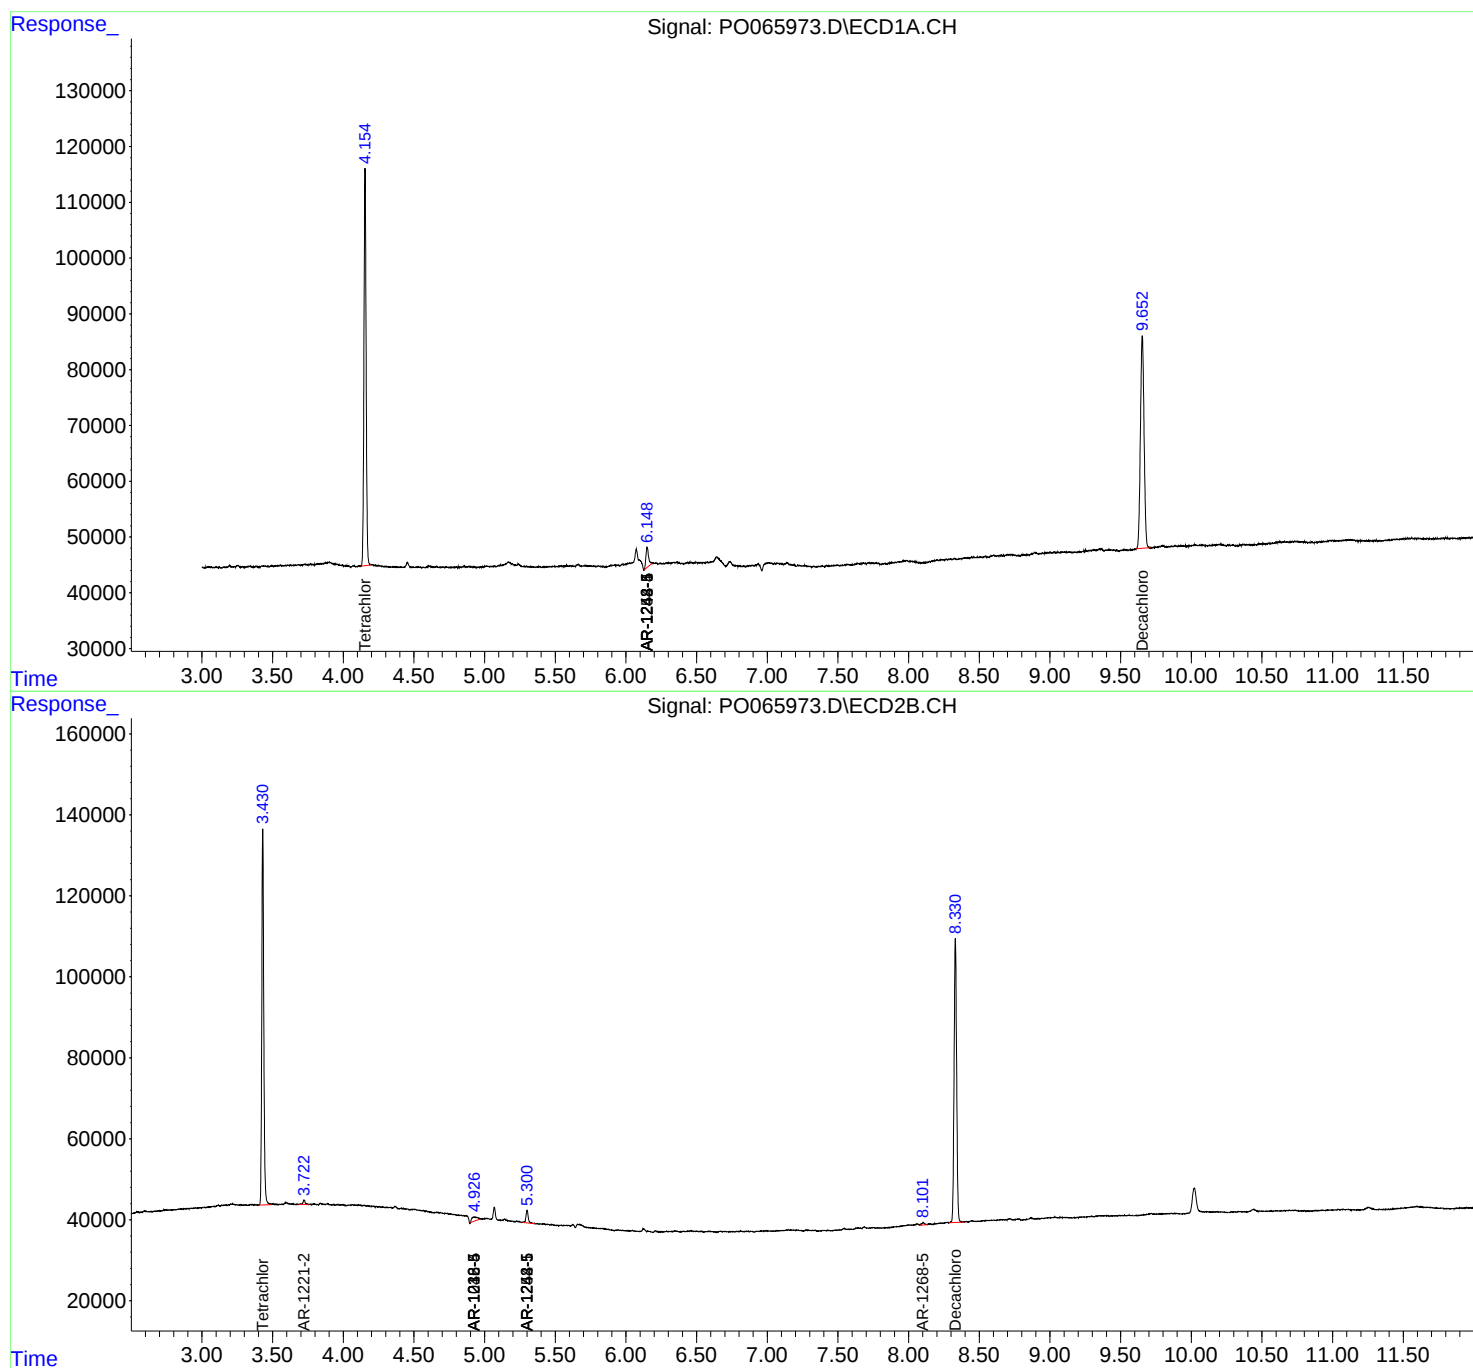


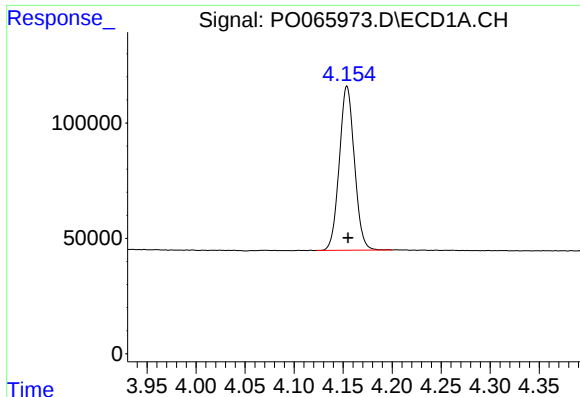

#1 Tetrachloro-m-xylene


R.T.: 4.154 min
Delta R.T.: -0.001 min
Response: 763712
Conc: 32.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-25-24-COMP

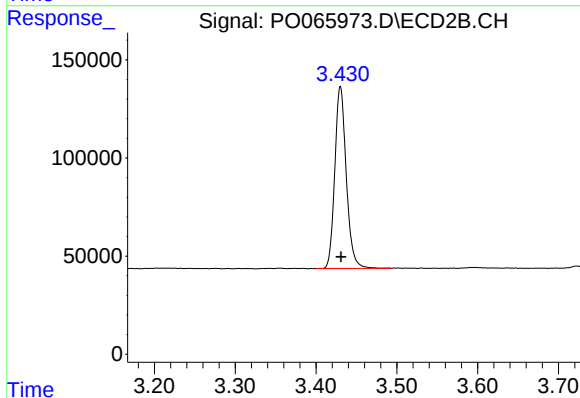


#1 Tetrachloro-m-xylene

R.T.: 3.430 min
Delta R.T.: 0.000 min
Response: 914780
Conc: 34.44 ng/ml

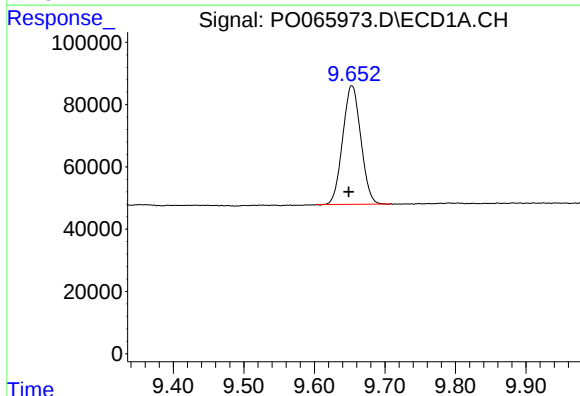


#2 Decachlorobiphenyl

R.T.: 9.653 min
Delta R.T.: 0.004 min
Response: 679563
Conc: 16.32 ng/ml

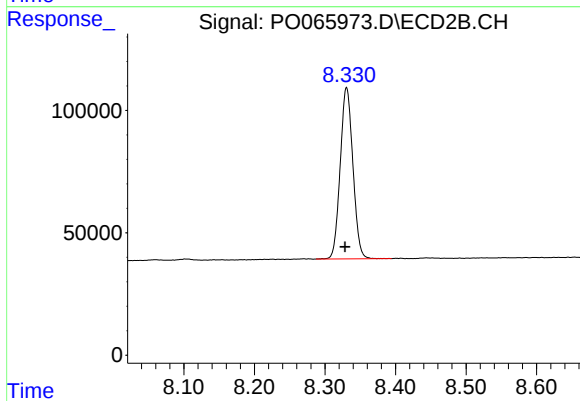

#2 Decachlorobiphenyl


R.T.: 8.331 min
Delta R.T.: 0.002 min
Response: 872378
Conc: 17.95 ng/ml

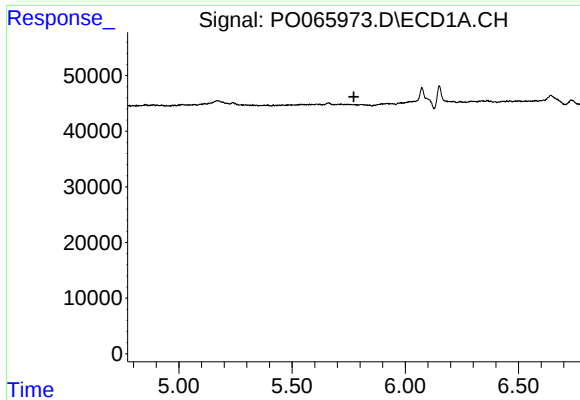

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T. : 5.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-25-24-COMP

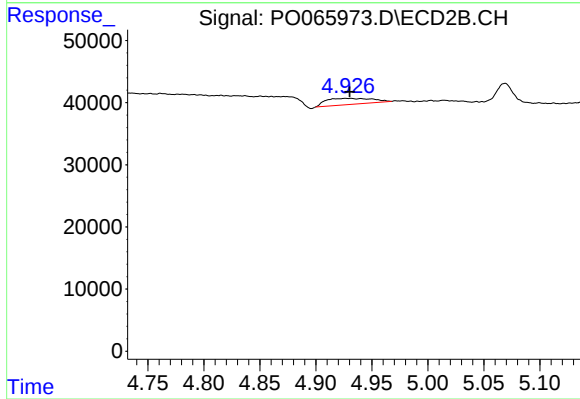


#7 AR-1016-5

R.T.: 4.926 min
Delta R.T.: -0.004 min
Response: 28021
Conc: 25.99 ng/ml

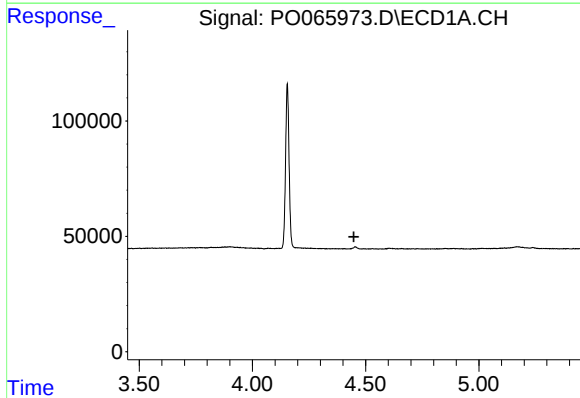


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.448 min
Response: 0
Conc: N.D.

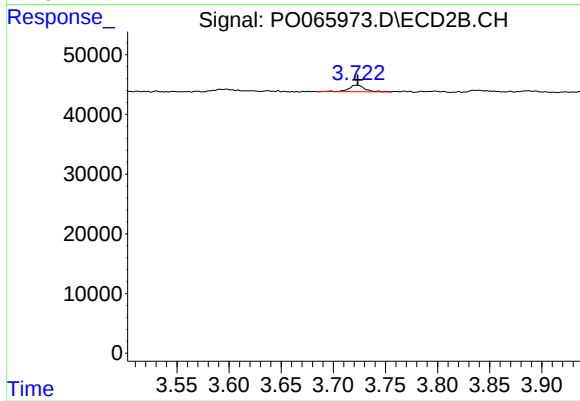

#9 AR-1221-2


R.T.: 3.722 min
Delta R.T.: -0.001 min
Response: 11512
Conc: 45.30 ng/ml

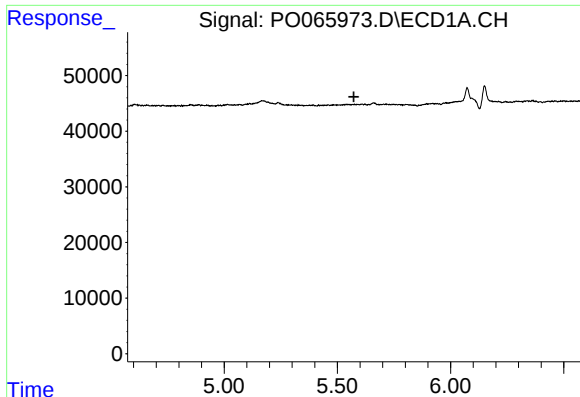

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-25-24-COMP

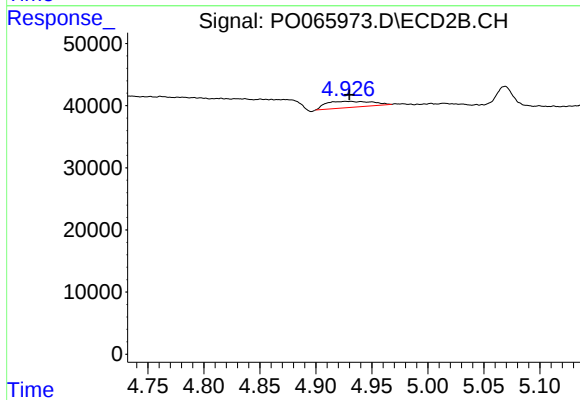


#15 AR-1232-5

R.T.: 4.926 min
Delta R.T.: -0.003 min
Response: 28021
Conc: 70.32 ng/ml

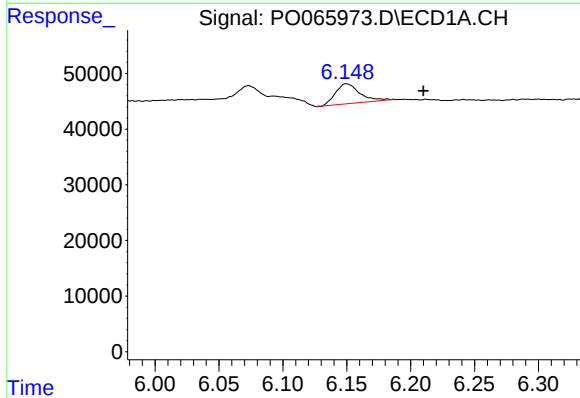


#20 AR-1242-5

R.T.: 6.150 min
Delta R.T.: -0.060 min
Response: 47264
Conc: 56.76 ng/ml

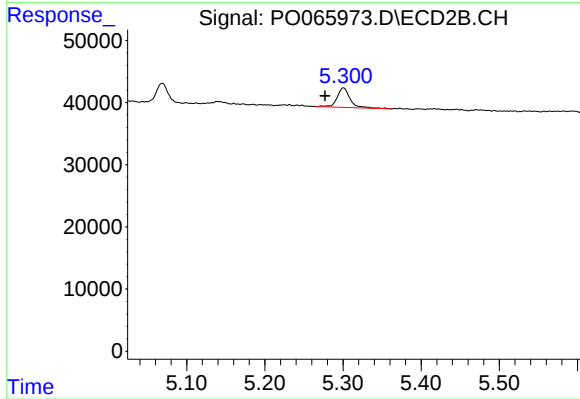

#20 AR-1242-5


R.T.: 5.301 min
Delta R.T.: 0.023 min
Response: 36422
Conc: 32.90 ng/ml

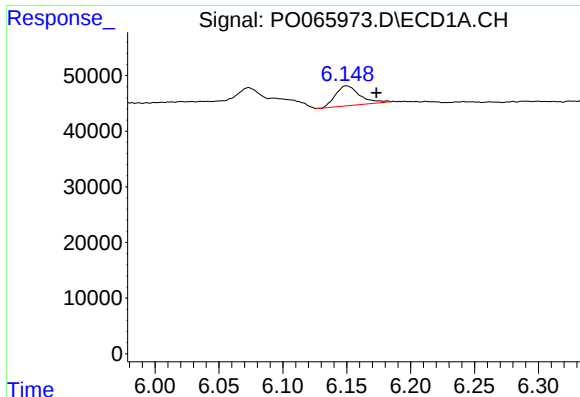

#24 AR-1248-4


R.T.: 6.150 min
Delta R.T.: -0.023 min
Response: 47264
Conc: 35.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-25-24-COMP

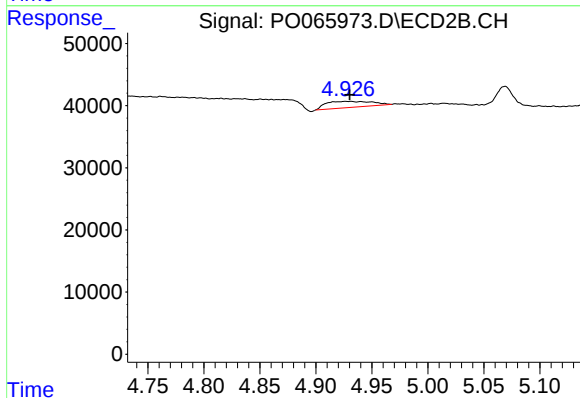


#24 AR-1248-4

R.T.: 4.926 min
Delta R.T.: -0.004 min
Response: 28021
Conc: 21.96 ng/ml

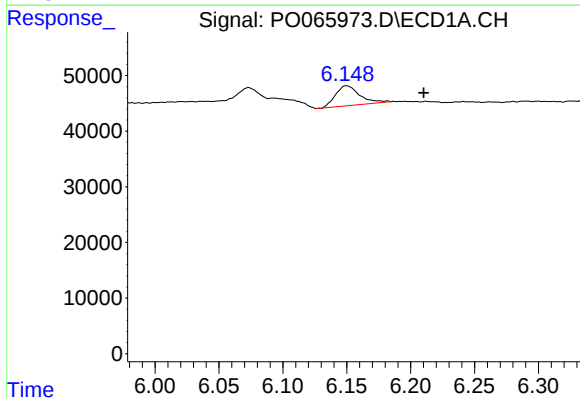


#25 AR-1248-5

R.T.: 6.150 min
Delta R.T.: -0.060 min
Response: 47264
Conc: 36.57 ng/ml

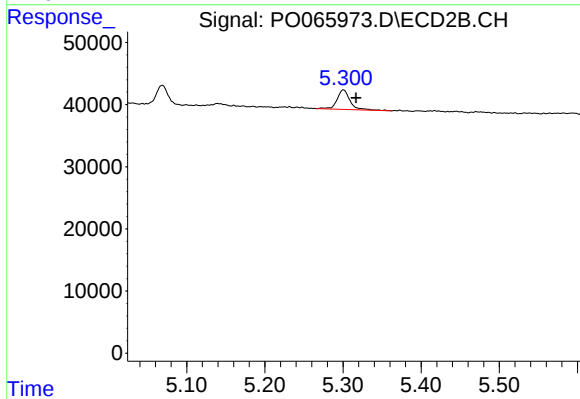

#25 AR-1248-5


R.T.: 5.301 min
Delta R.T.: -0.016 min
Response: 36422
Conc: 26.10 ng/ml

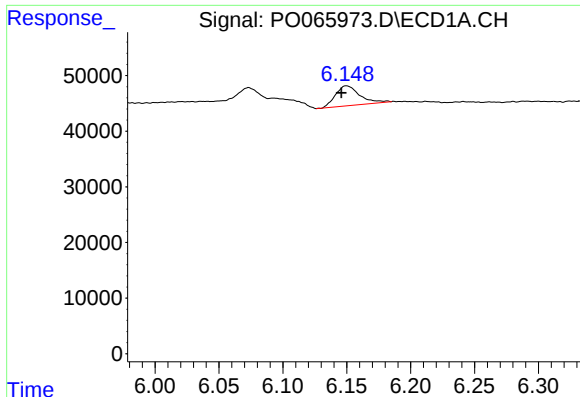

#26 AR-1254-1


R.T.: 6.150 min
Delta R.T.: 0.004 min
Response: 47264
Conc: 35.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-25-24-COMP

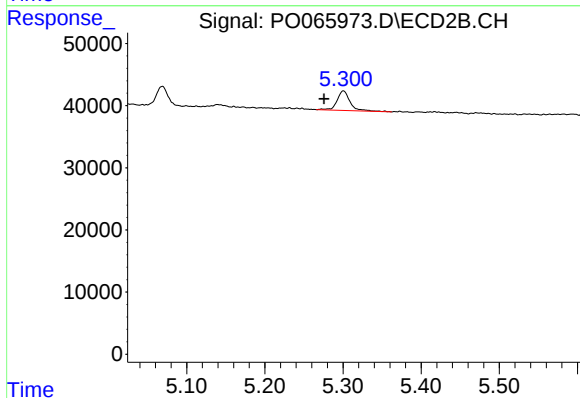


#26 AR-1254-1

R.T.: 5.301 min
Delta R.T.: 0.025 min
Response: 36422
Conc: 16.29 ng/ml

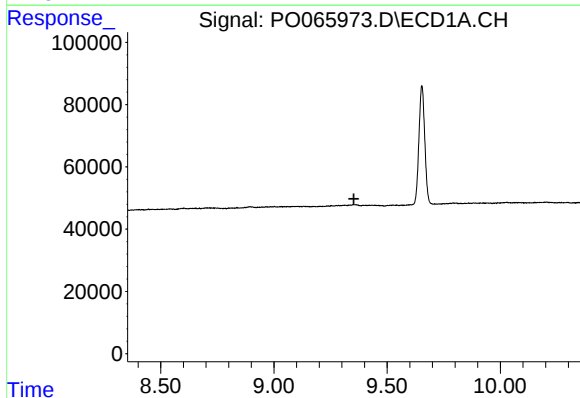

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.353 min
Response: 0
Conc: N.D.

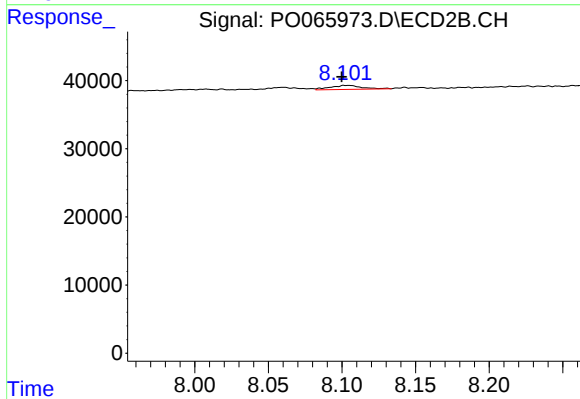

#45 AR-1268-5

R.T.: 8.103 min
Delta R.T.: 0.003 min
Response: 8881
Conc: 0.49 ng/ml