

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012720\
 Data File : P0065936.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jan 2020 12:18
 Operator : DD\AJ
 Sample : L1238-01RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLIFTON-POLESRE

Manual Integrations
 APPROVED

mohammad
 1/28/2020 2:40:12 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 01:11:44 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.145	3.449	2348808	1944971	101.295m	73.225m#
2) SA Decachlor...	9.663	8.335	996492	475193	23.938	9.778m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO012720\
Data File : PO065936.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jan 2020 12:18
Operator : DD\AJ
Sample : L1238-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CLIFTON-POLESRE


Manual Integrations
APPROVED

mohammad
1/28/2020 2:40:12 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 01:11:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

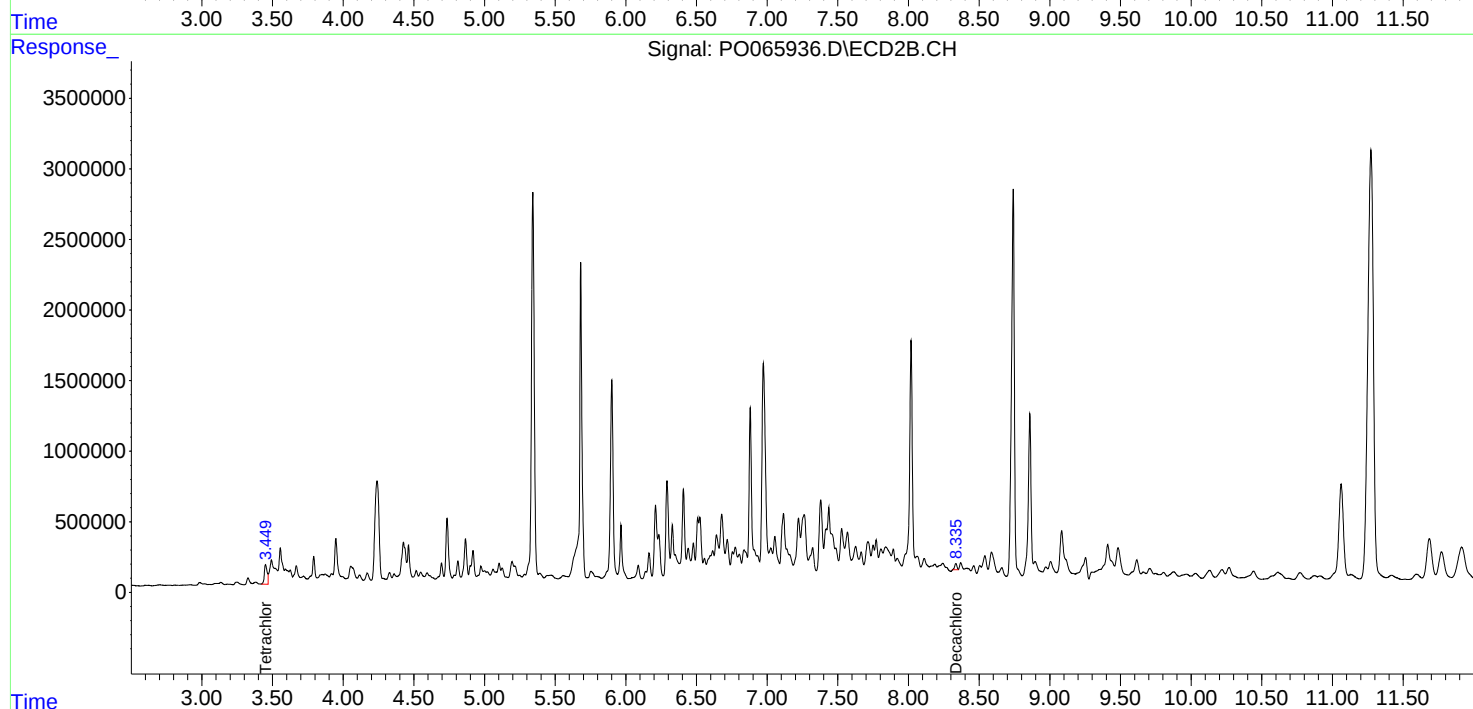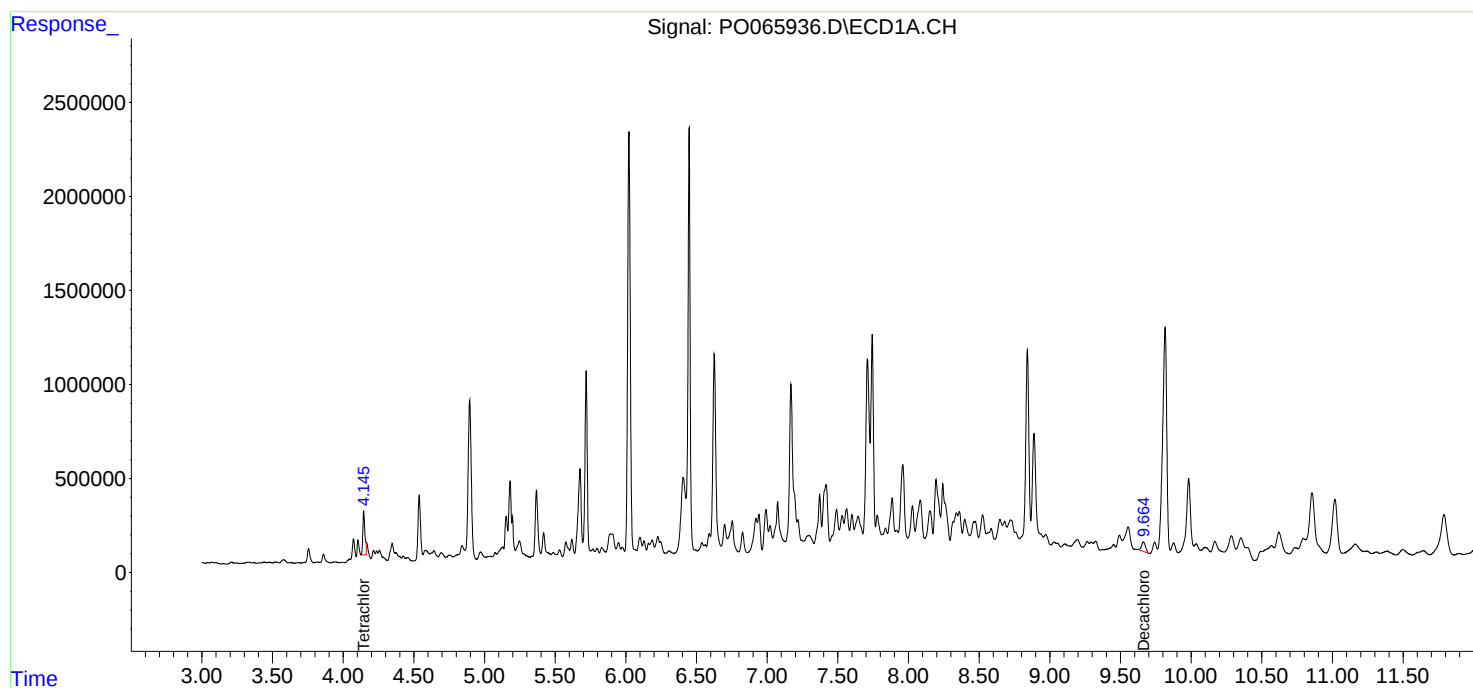

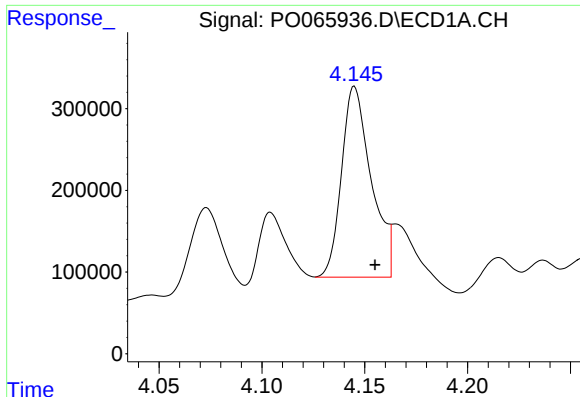


#1 Tetrachloro-m-xylene

R.T.: 4.145 min
Delta R.T.: -0.010 min
Response: 2348808
Conc: 101.29 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CLIFTON-POLESRE


Manual Integrations
APPROVED

mohammad
1/28/2020 2:40:12 PM

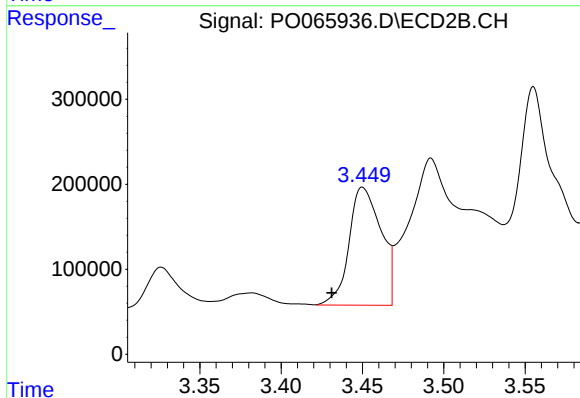


#1 Tetrachloro-m-xylene

R.T.: 3.449 min
Delta R.T.: 0.018 min
Response: 1944971
Conc: 73.23 ng/ml m

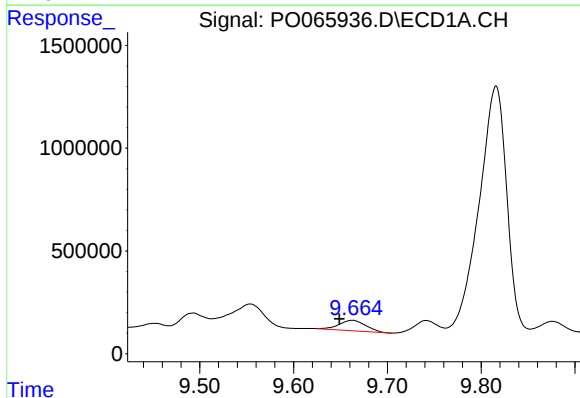

#2 Decachlorobiphenyl

R.T.: 9.663 min
Delta R.T.: 0.014 min
Response: 996492
Conc: 23.94 ng/ml

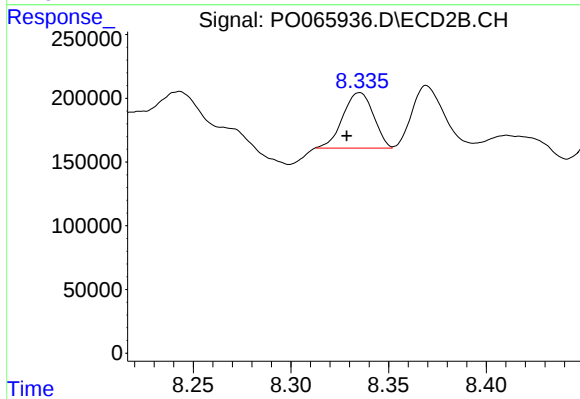

#2 Decachlorobiphenyl

R.T.: 8.335 min
Delta R.T.: 0.006 min
Response: 475193
Conc: 9.78 ng/ml m