

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012720\
 Data File : P0065940.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Jan 2020 13:31
 Operator : DD\AJ
 Sample : L1007-19RE
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 JC-03-012320-CRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 28 02:40:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 24 03:54:38 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.165	3.433	824406	1055650	35.553	39.744
2) SA Decachlor...	9.668	8.338	577159	826797	13.865	17.014

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0012720\
Data File : P0065940.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Jan 2020 13:31
Operator : DD\AJ
Sample : L1007-19RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
JC-03-012320-CRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 28 02:40:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0012320.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 24 03:54:38 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

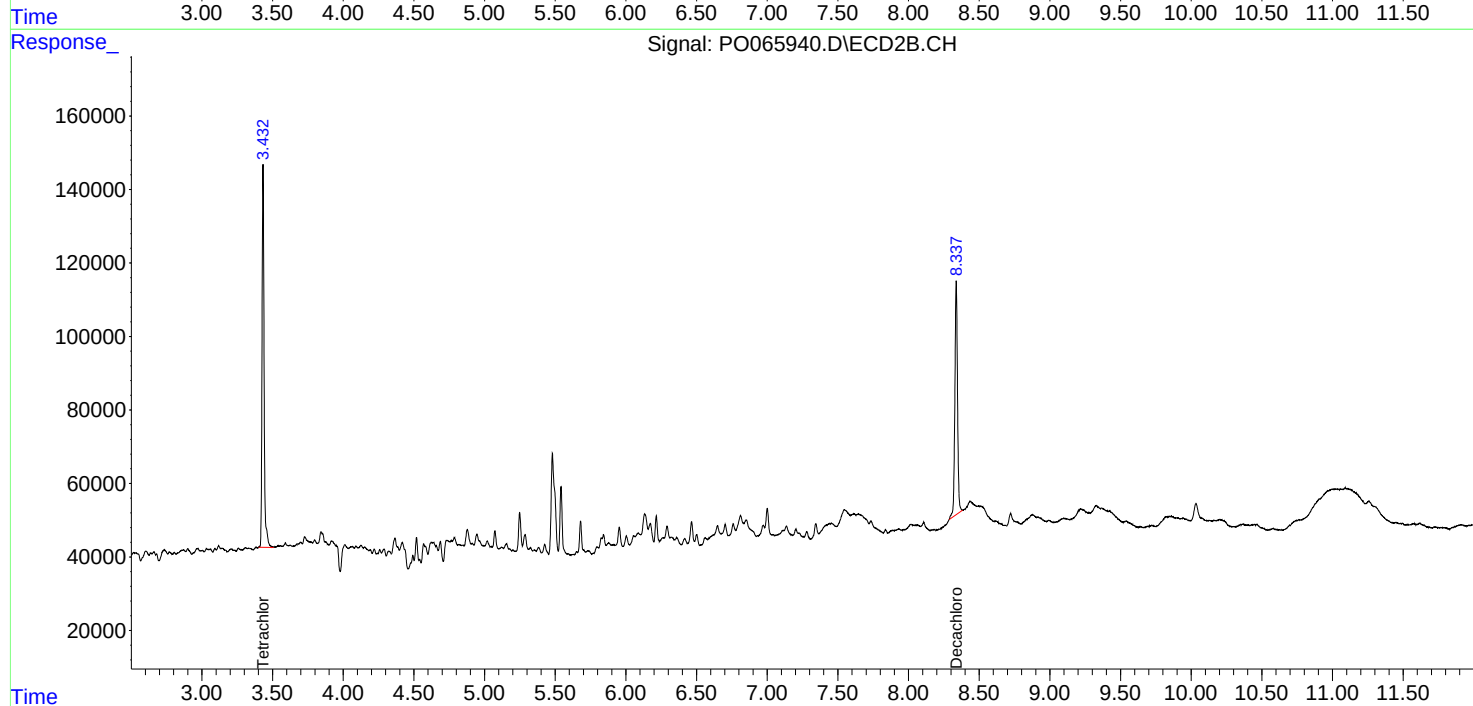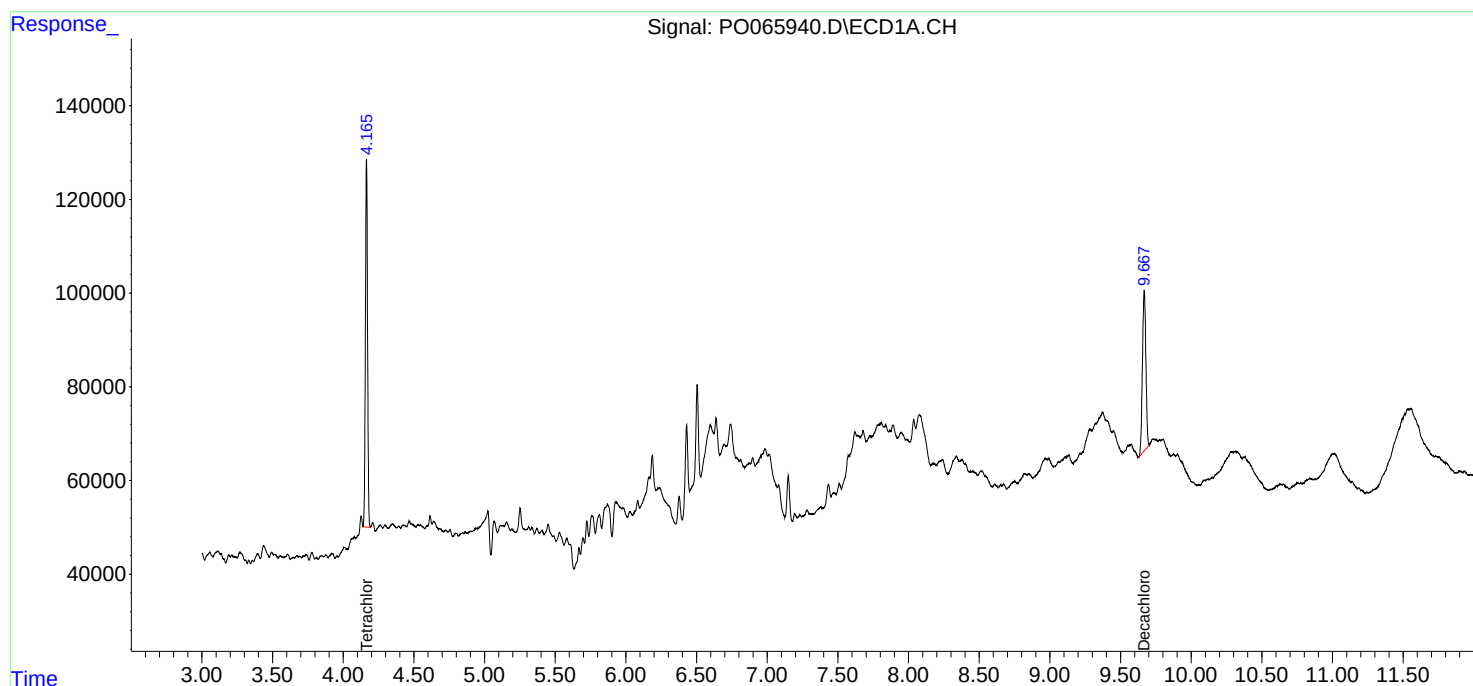


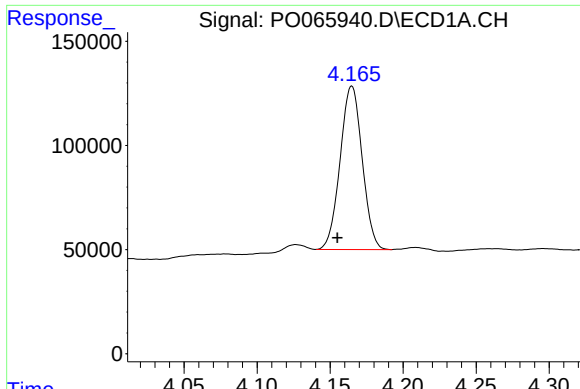

#1 Tetrachloro-m-xylene


R.T.: 4.165 min
Delta R.T.: 0.010 min
Response: 824406
Conc: 35.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
JC-03-012320-CRE

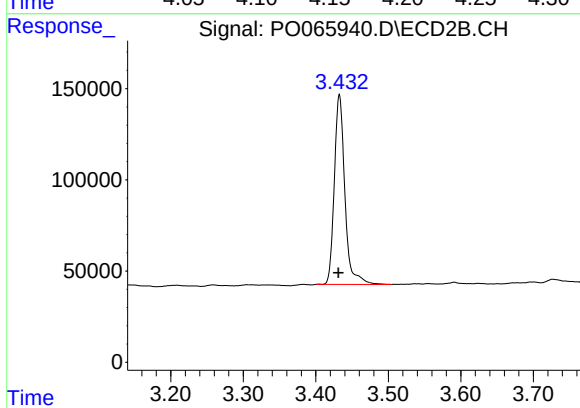


#1 Tetrachloro-m-xylene

R.T.: 3.433 min
Delta R.T.: 0.002 min
Response: 1055650
Conc: 39.74 ng/ml

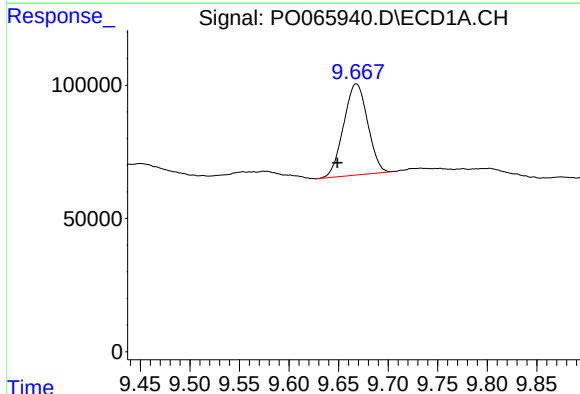

#2 Decachlorobiphenyl

R.T.: 9.668 min
Delta R.T.: 0.019 min
Response: 577159
Conc: 13.86 ng/ml

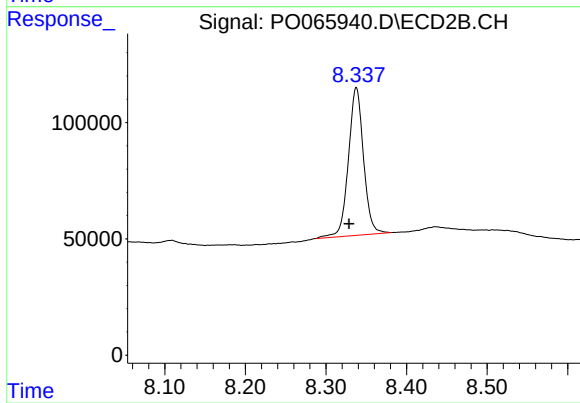

#2 Decachlorobiphenyl

R.T.: 8.338 min
Delta R.T.: 0.009 min
Response: 826797
Conc: 17.01 ng/ml